

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043021\
 Data File : PL066602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 12:44
 Operator : AR\AJ
 Sample : M2217-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HTCVRV2-GRAB-CF02-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 01:08:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.154	51169233	51438119	13.580	14.646
28)	SA Decachlor...	8.167	9.357	51452224	46730083	13.419	15.105
Target Compounds							
23)	Chlordane-1	4.279	0.000	1847657	0	10.931	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043021\
Data File : PL066602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2021 12:44
Operator : AR\AJ
Sample : M2217-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HTCRV2-GRAB-CF02-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 01:08:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

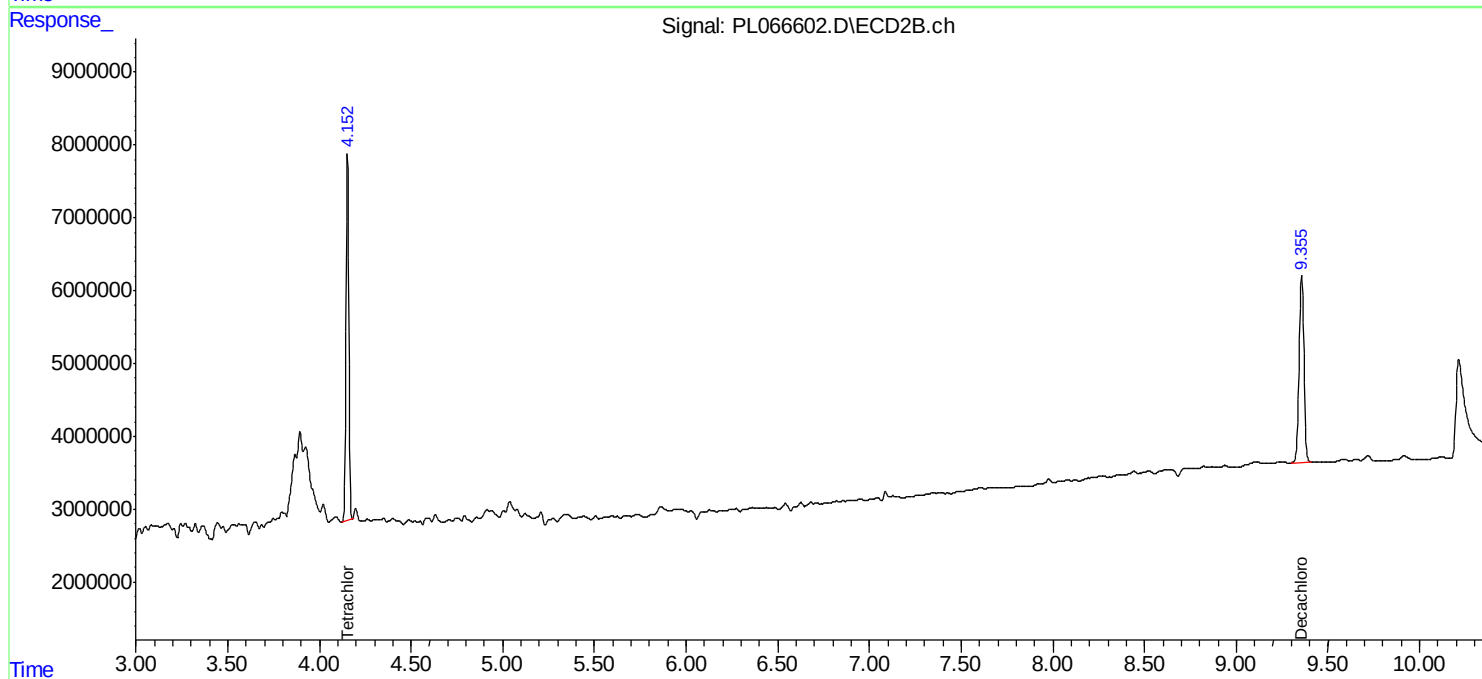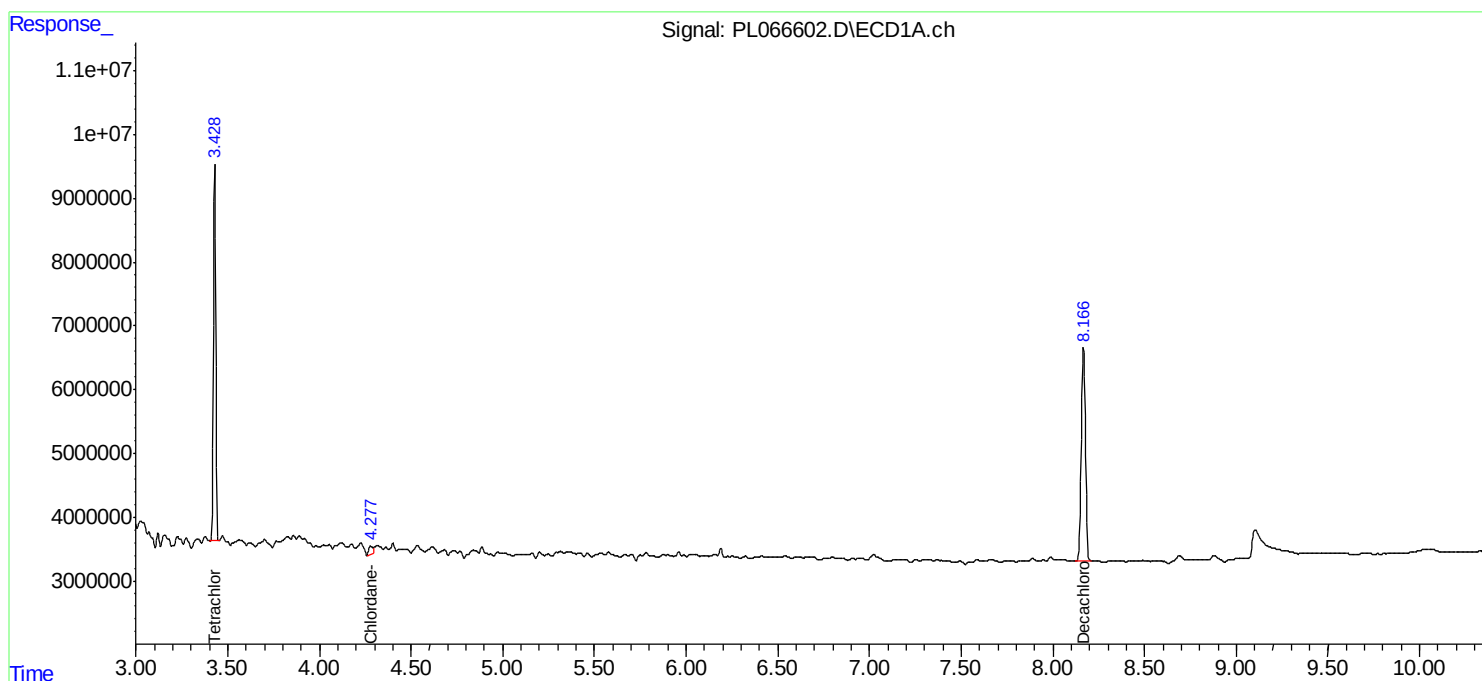


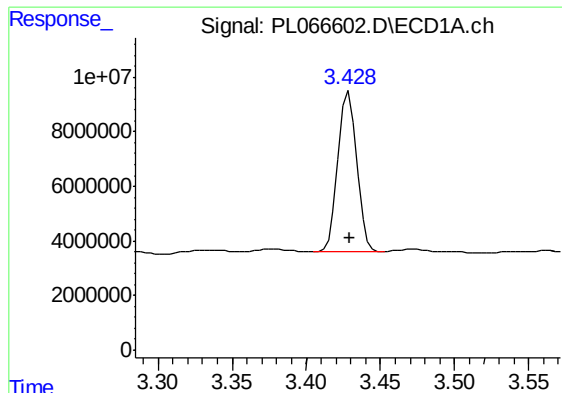

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 51169233
Conc: 13.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
HTCRV2-GRAB-CF02-01

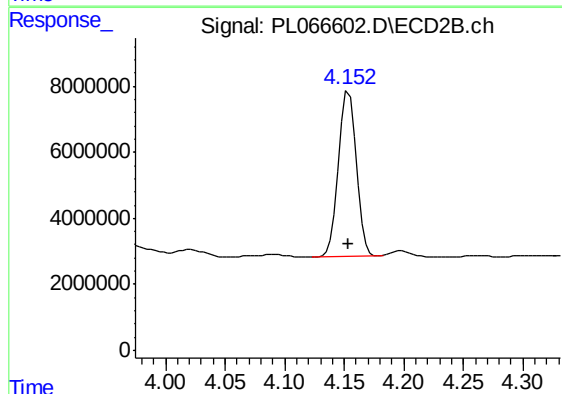


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 51438119
Conc: 14.65 ng/ml

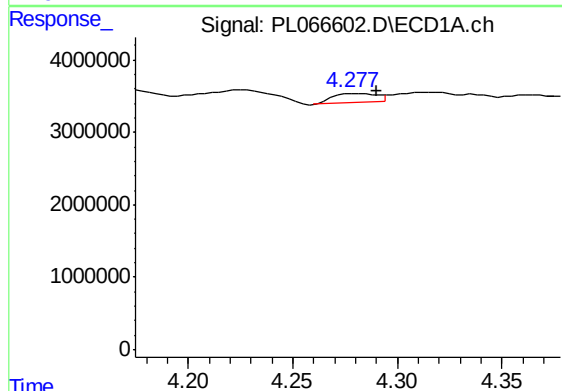


#23 Chlordane-1

R.T.: 4.279 min
Delta R.T.: -0.011 min
Response: 1847657
Conc: 10.93 ng/ml

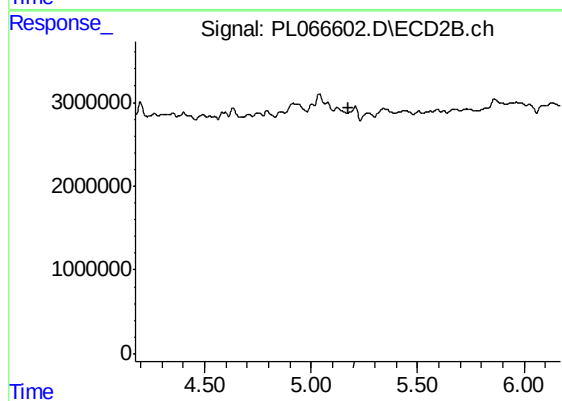

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

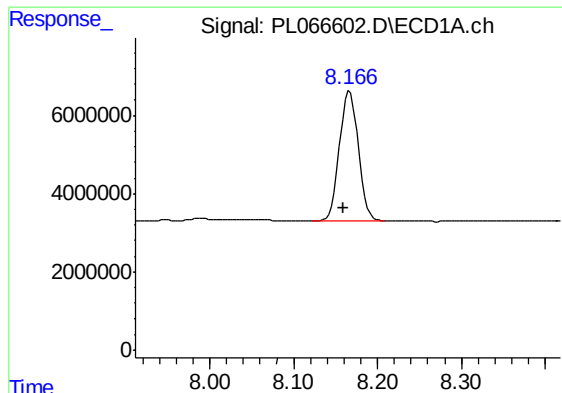

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.008 min
Response: 51452224
Conc: 13.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
HTCRV2-GRAB-CF02-01

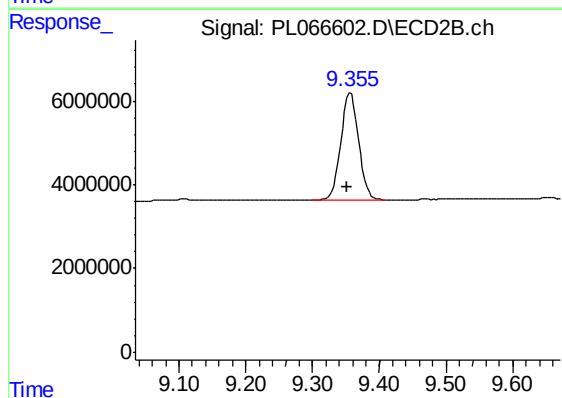

#28 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: 0.005 min
Response: 46730083
Conc: 15.11 ng/ml