

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043021\
 Data File : PL066604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 13:12
 Operator : AR\AJ
 Sample : M2219-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-071

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 01:08:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.155	41572989	43207047	11.033	12.303
28)	SA Decachlor...	8.165	9.356	25180595	23483714	6.567	7.591
Target Compounds							
11)	B alpha-Chl...	5.408	6.385	2759336	3941472	0.560	0.950 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043021\
Data File : PL066604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2021 13:12
Operator : AR\AJ
Sample : M2219-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-071

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 01:08:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

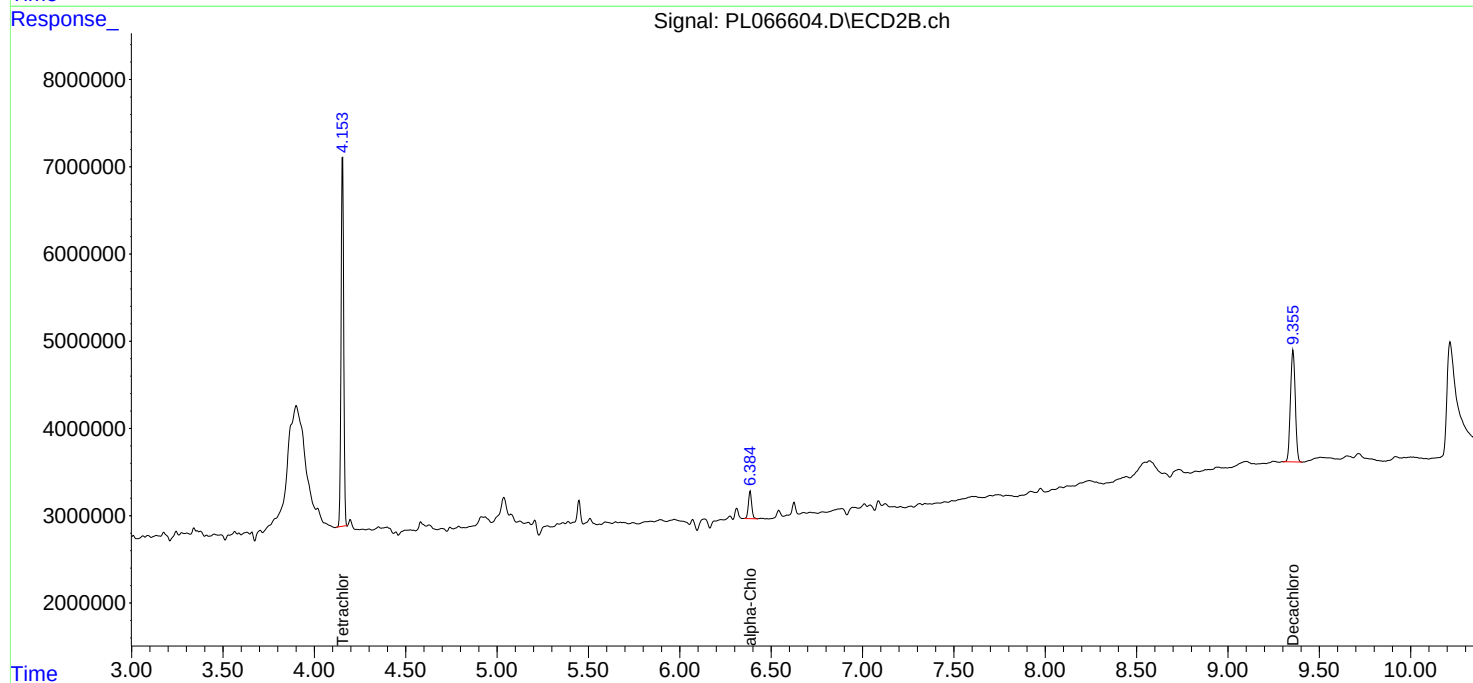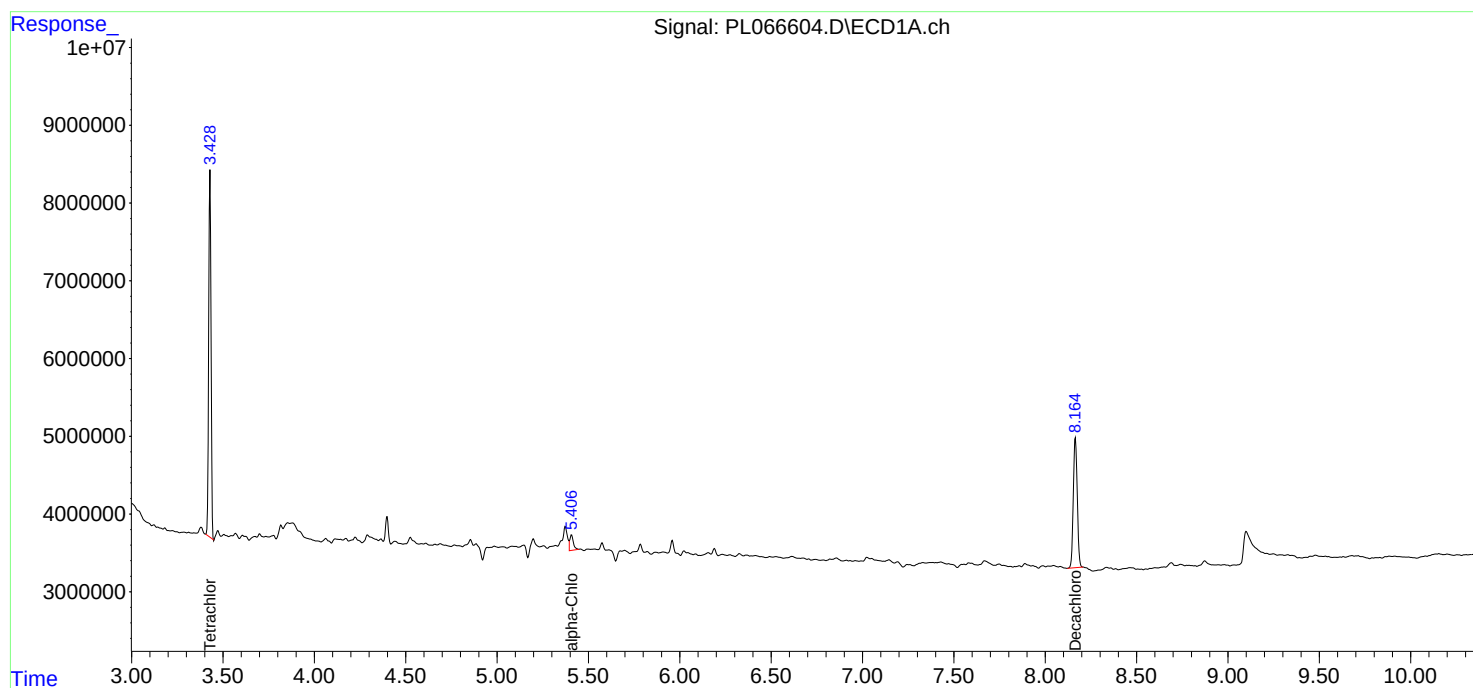


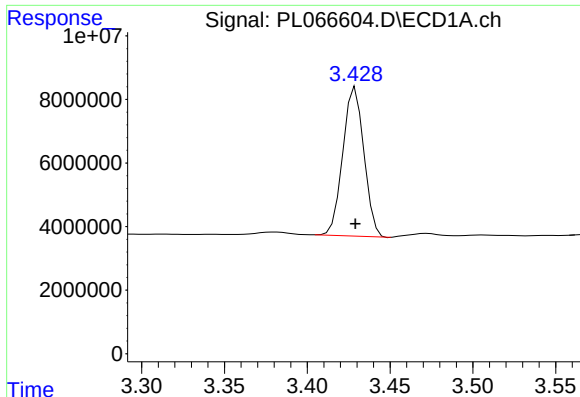

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 41572989
Conc: 11.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-071

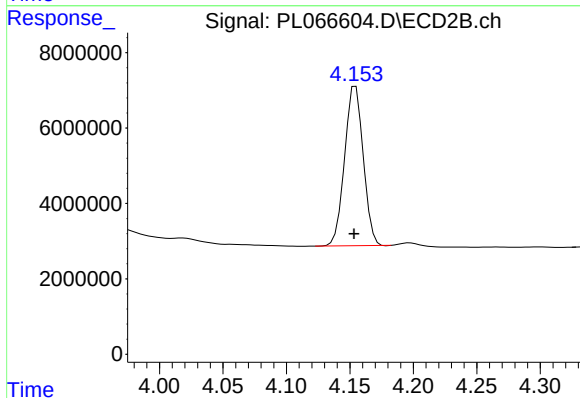


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.001 min
Response: 43207047
Conc: 12.30 ng/ml

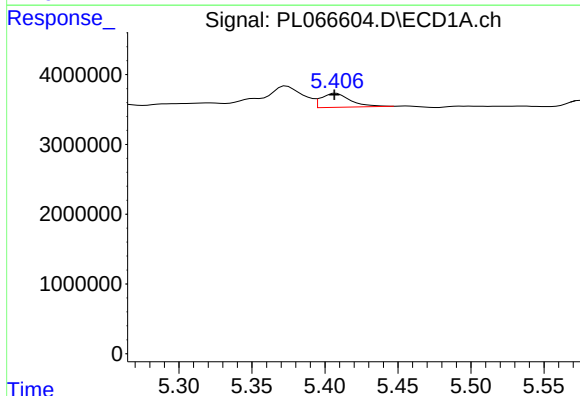


#11 alpha-Chlordane

R.T.: 5.408 min
Delta R.T.: 0.001 min
Response: 2759336
Conc: 0.56 ng/ml

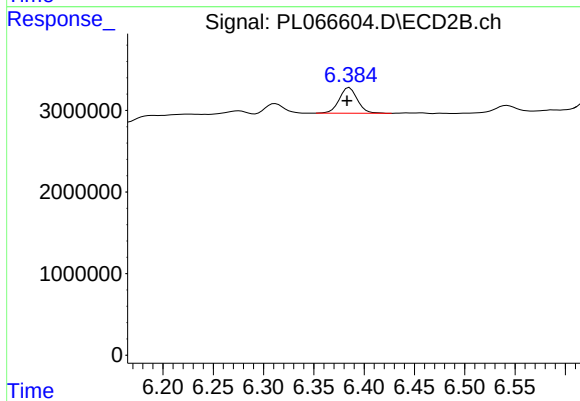

#11 alpha-Chlordane


R.T.: 6.385 min
Delta R.T.: 0.002 min
Response: 3941472
Conc: 0.95 ng/ml

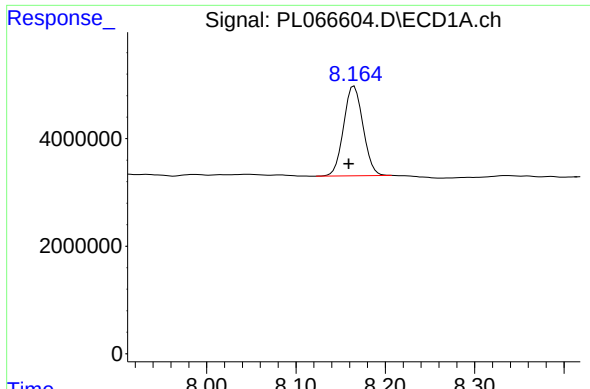

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: 0.006 min
Response: 25180595
Conc: 6.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-071

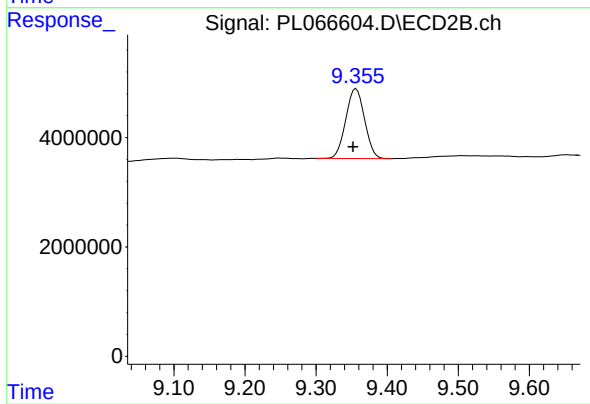

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.004 min
Response: 23483714
Conc: 7.59 ng/ml