

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043025\
 Data File : PL095457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2025 21:30
 Operator : AR\AJ
 Sample : Q1895-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 08:47:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.592	2.904	63486276	63202530	19.446	19.877
28)	SA Decachlor...	9.113	8.081	53088104	57909458	19.160	19.569
Target Compounds							
10)	B gamma-Chl...	0.000	5.164f	0	6014501	N.D.	1.484 #
13)	MA Dieldrin	0.000	5.522	0	8461019	N.D.	2.080 #
14)	MA Endrin	6.615	0.000	12928466	0	4.059	N.D. #
15)	B Endosulfa...	0.000	6.088	0	25050255	N.D.	6.976 #
16)	A 4,4'-DDD	6.748	0.000	21043664	0	7.433	N.D. #
17)	MA 4,4'-DDT	0.000	6.191	0	11376140	N.D.	3.311 #
25)	Chlordane-3	0.000	5.164	0	6014501	N.D.	11.642 #
27)	Chlordane-5	0.000	6.088f	0	25050255	N.D.	135.598 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043025\
Data File : PL095457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2025 21:30
Operator : AR\AJ
Sample : Q1895-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 08:47:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

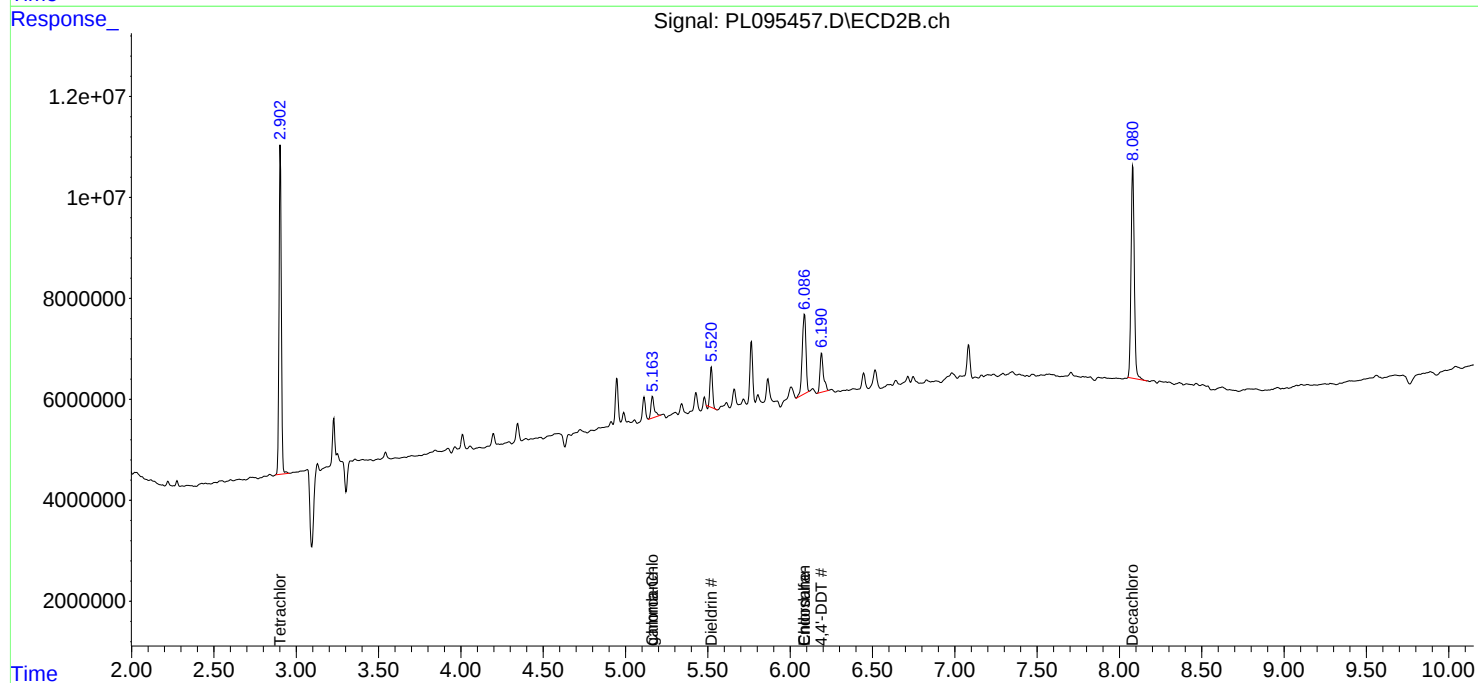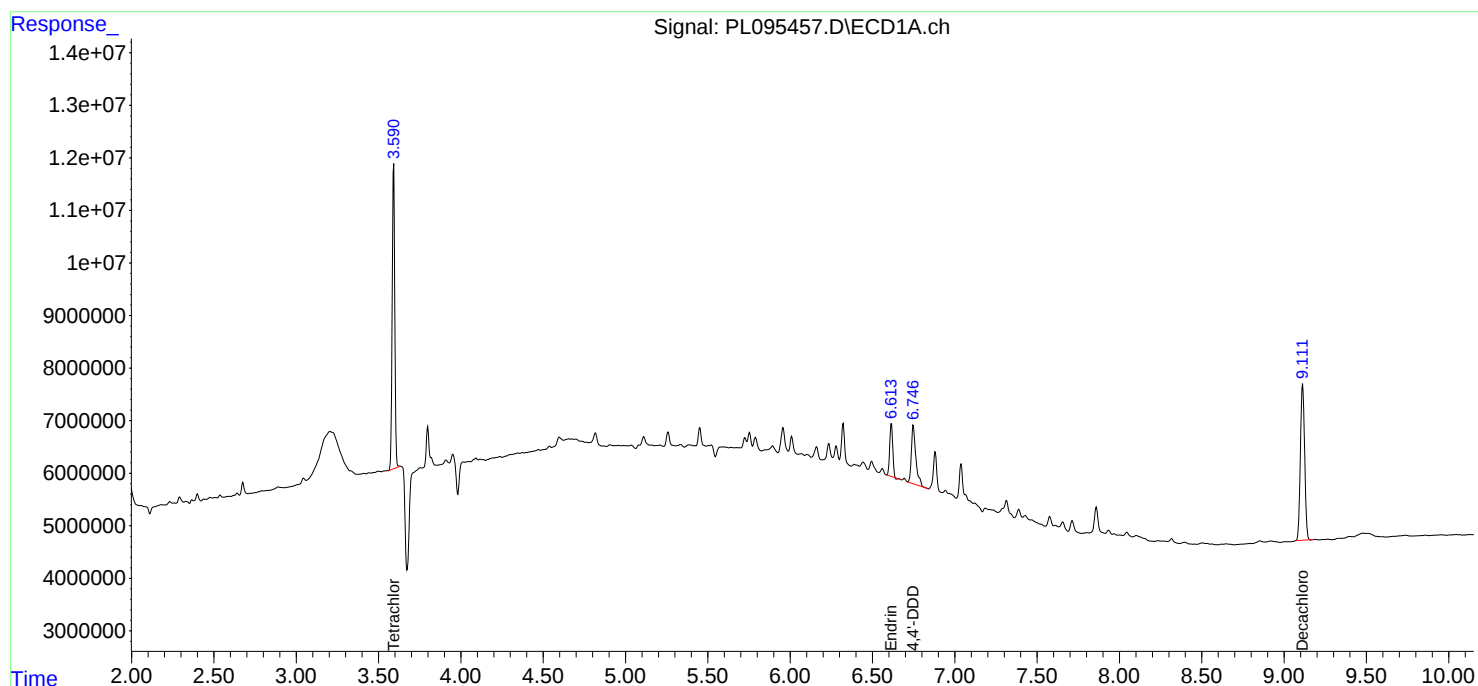


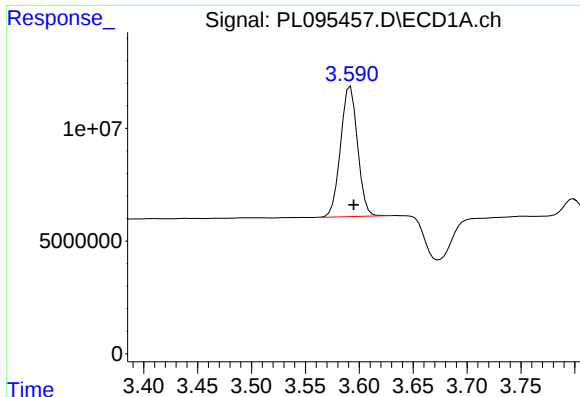

#1 Tetrachloro-m-xylene


R.T.: 3.592 min
Delta R.T.: -0.003 min
Response: 63486276
Conc: 19.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

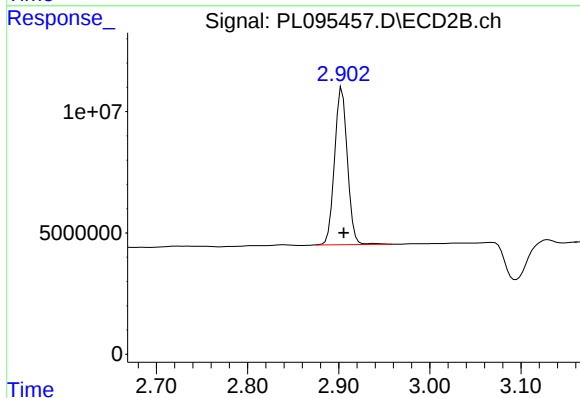


#1 Tetrachloro-m-xylene

R.T.: 2.904 min
Delta R.T.: -0.002 min
Response: 63202530
Conc: 19.88 ng/ml

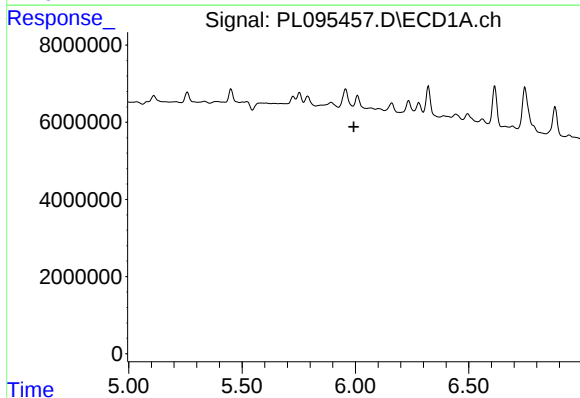


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.994 min
Response: 0
Conc: N.D.

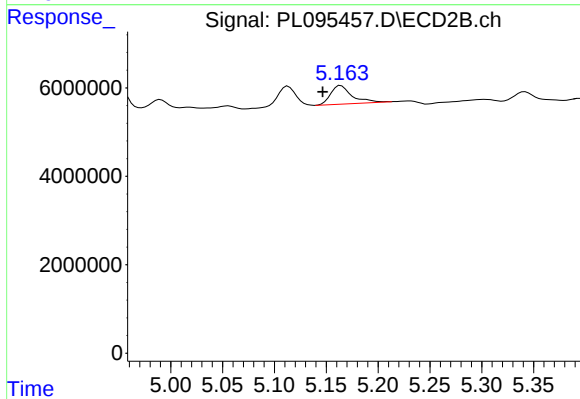

#10 gamma-Chlordane


R.T.: 5.164 min
Delta R.T.: 0.017 min
Response: 6014501
Conc: 1.48 ng/ml

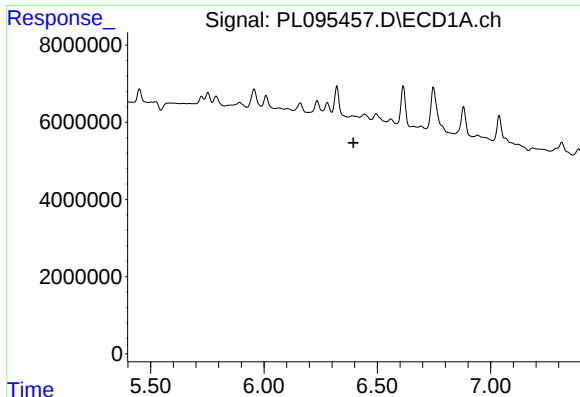

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-3

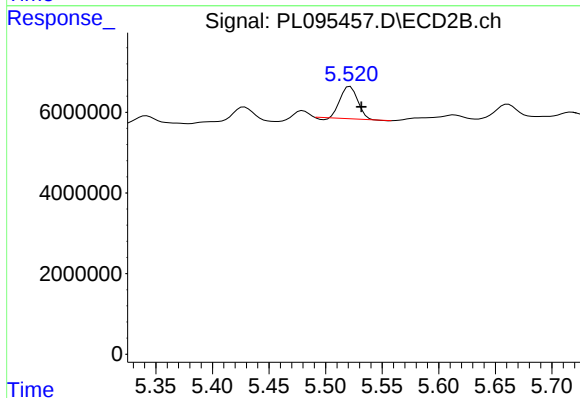


#13 Dieldrin

R.T.: 5.522 min
Delta R.T.: -0.010 min
Response: 8461019
Conc: 2.08 ng/ml

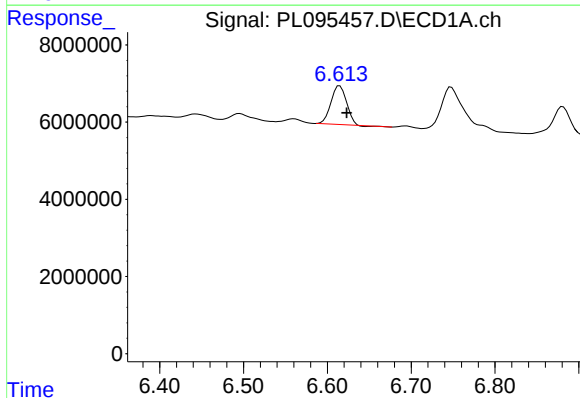


#14 Endrin

R.T.: 6.615 min
Delta R.T.: -0.008 min
Response: 12928466
Conc: 4.06 ng/ml

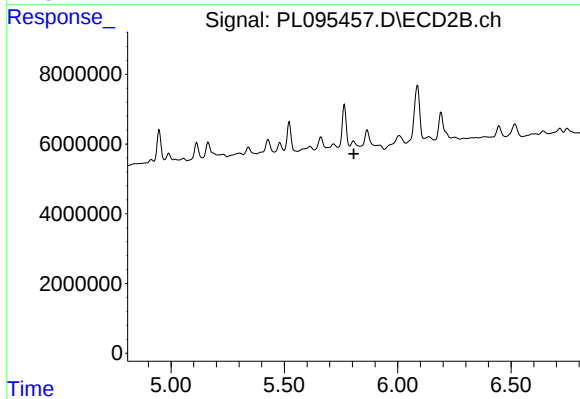

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.807 min
Response: 0
Conc: N.D.

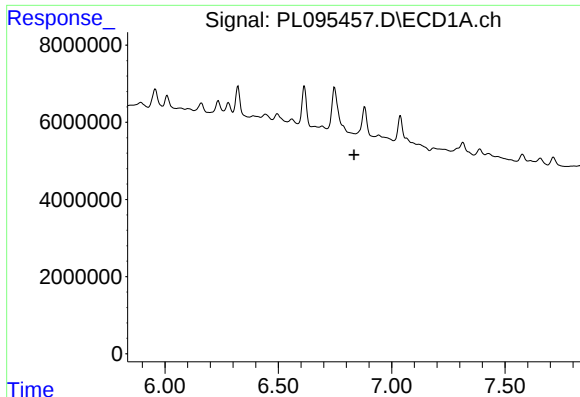

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.835 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-3

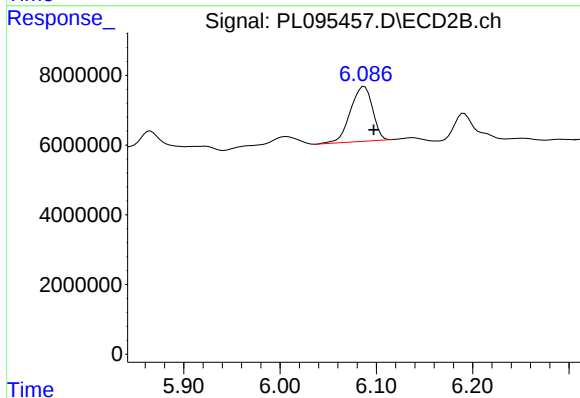


#15 Endosulfan II

R.T.: 6.088 min
Delta R.T.: -0.010 min
Response: 25050255
Conc: 6.98 ng/ml

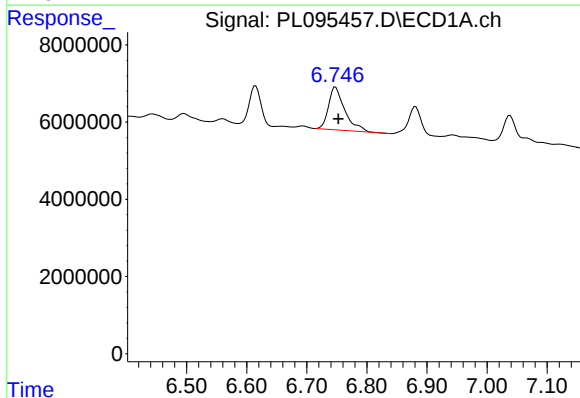


#16 4,4'-DDD

R.T.: 6.748 min
Delta R.T.: -0.005 min
Response: 21043664
Conc: 7.43 ng/ml

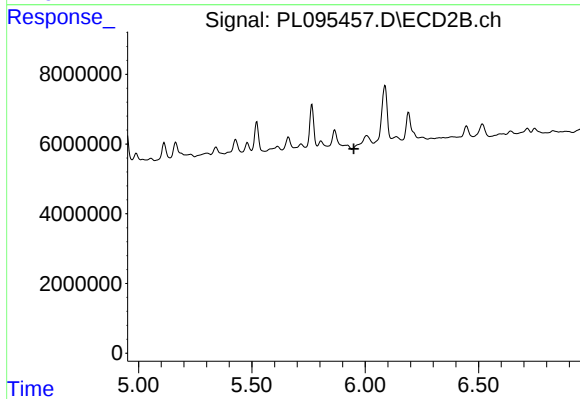

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

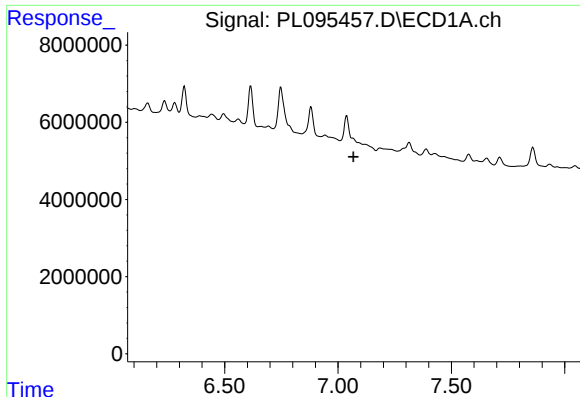

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-3

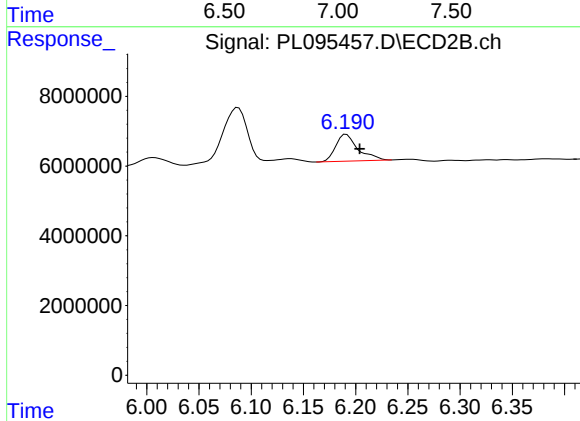


#17 4,4'-DDT

R.T.: 6.191 min
Delta R.T.: -0.013 min
Response: 11376140
Conc: 3.31 ng/ml

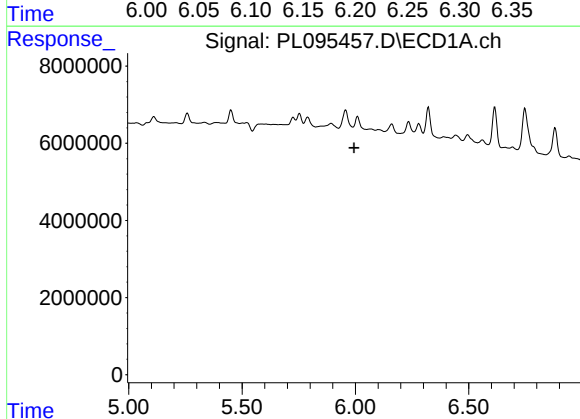


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.994 min
Response: 0
Conc: N.D.

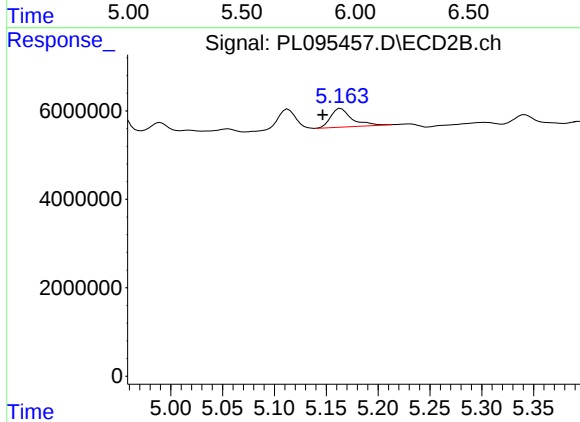

#25 Chlordane-3


R.T.: 5.164 min
Delta R.T.: 0.017 min
Response: 6014501
Conc: 11.64 ng/ml

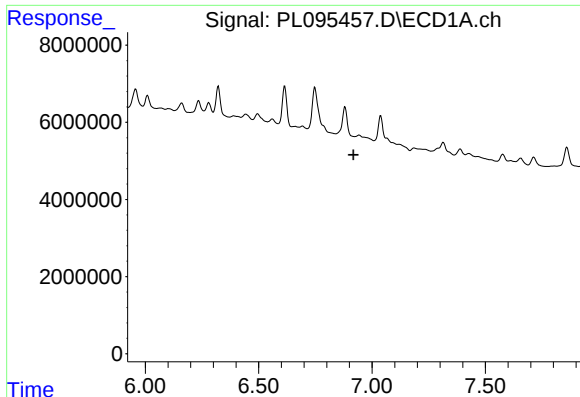

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-3

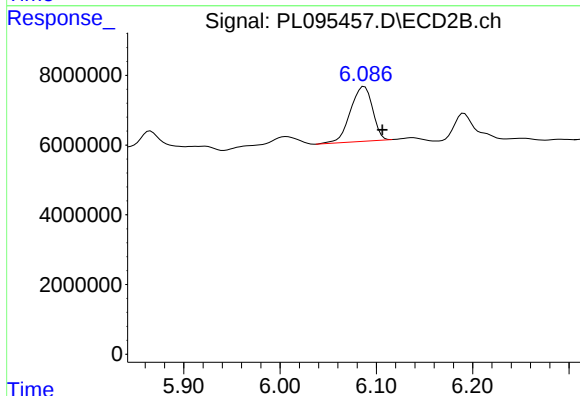


#27 Chlordane-5

R.T.: 6.088 min
Delta R.T.: -0.019 min
Response: 25050255
Conc: 135.60 ng/ml

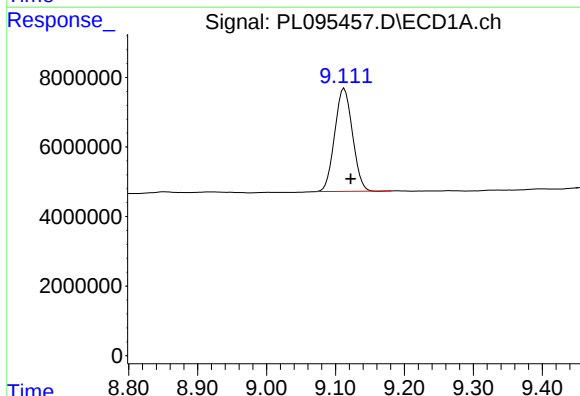

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: -0.010 min
Response: 53088104
Conc: 19.16 ng/ml

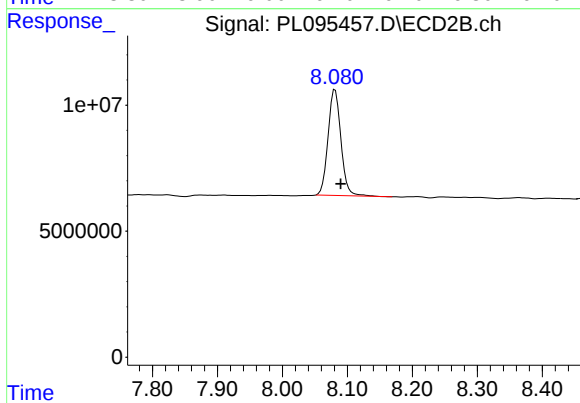

#28 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: -0.008 min
Response: 57909458
Conc: 19.57 ng/ml