

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050119\
 Data File : PL048085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2019 19:32
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 09:30:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:29:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	802.6E6	193.0E6	73.555	74.289
28)	SA Decachlor...	7.996	8.976	747.6E6	191.1E6	72.511	71.447
Target Compounds							
23)	Chlordane-1	4.170	4.927	358.4E6	95621200	749.346	759.507
24)	Chlordane-2	4.660	5.395	385.7E6	95730827	730.541	724.433
25)	Chlordane-3	5.216	6.039	1244.8E6	337.0E6	740.078	752.477
26)	Chlordane-4	5.270	6.112	1140.2E6	395.9E6	747.589	745.655
27)	Chlordane-5	6.093	6.914	365.3E6	77620602	757.652	744.472



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050119\
Data File : PL048085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2019 19:32
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 09:30:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:29:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

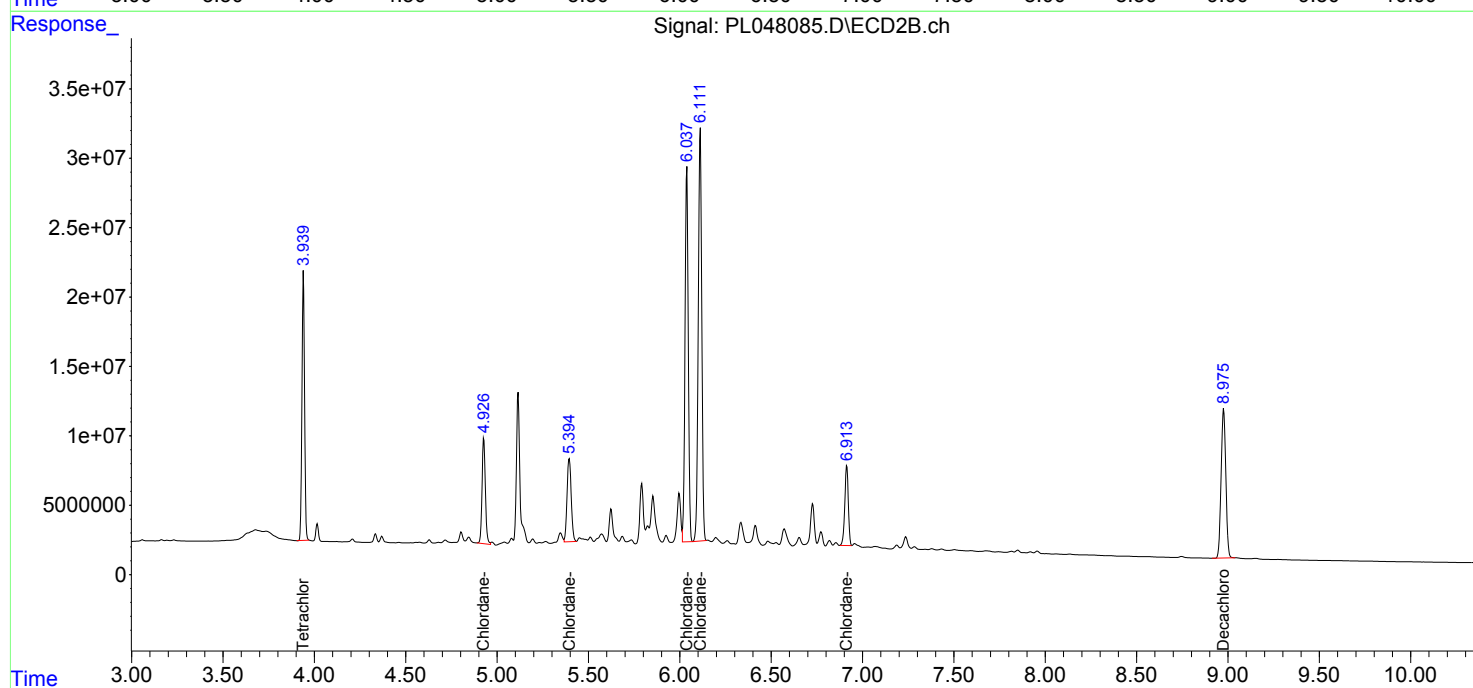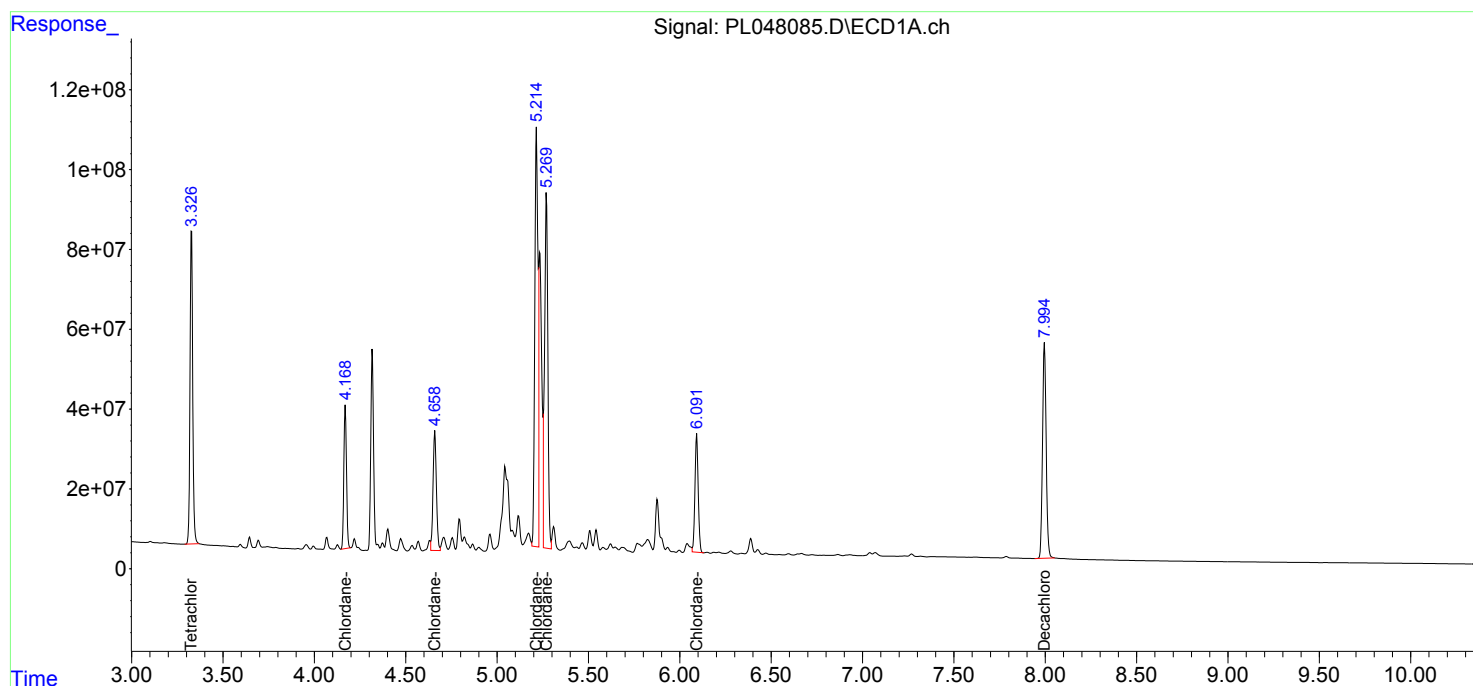


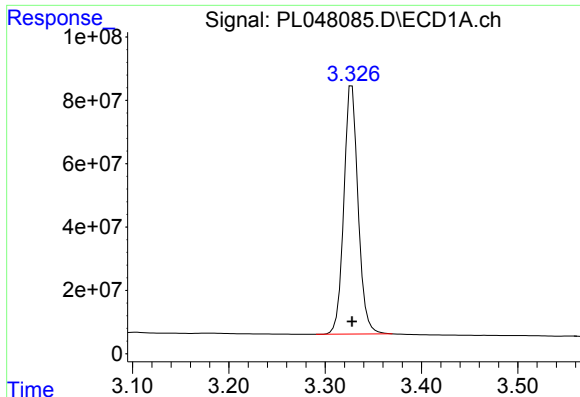

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 802615751
Conc: 73.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

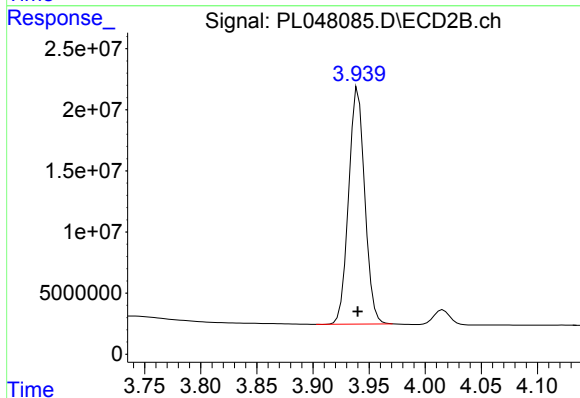


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 192979269
Conc: 74.29 ng/ml

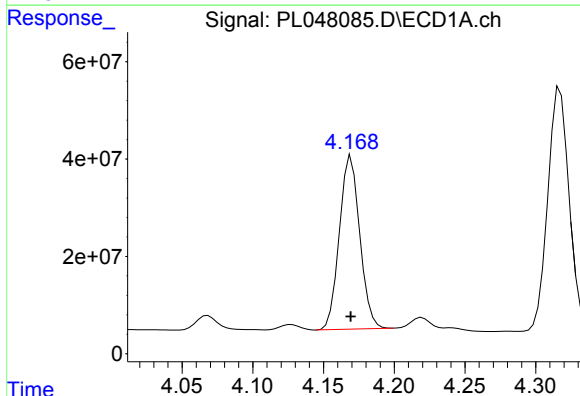


#23 Chlordane-1

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 358433376
Conc: 749.35 ng/ml

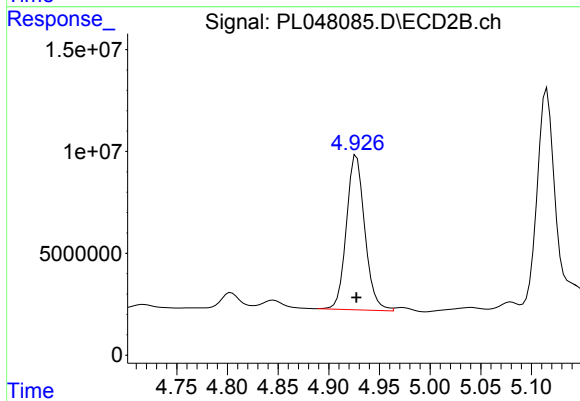

#23 Chlordane-1


R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 95621200
Conc: 759.51 ng/ml

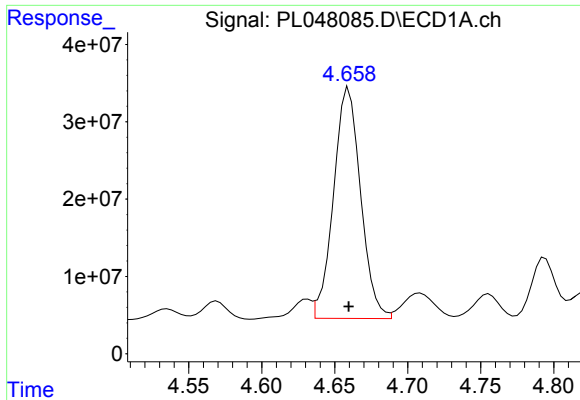

#24 Chlordane-2


R.T.: 4.660 min
Delta R.T.: 0.000 min
Response: 385678123
Conc: 730.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

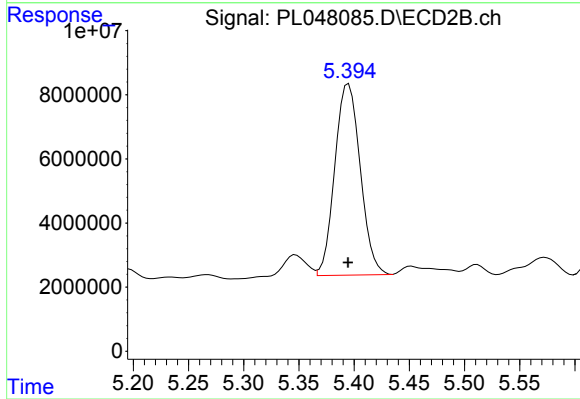


#24 Chlordane-2

R.T.: 5.395 min
Delta R.T.: 0.000 min
Response: 95730827
Conc: 724.43 ng/ml

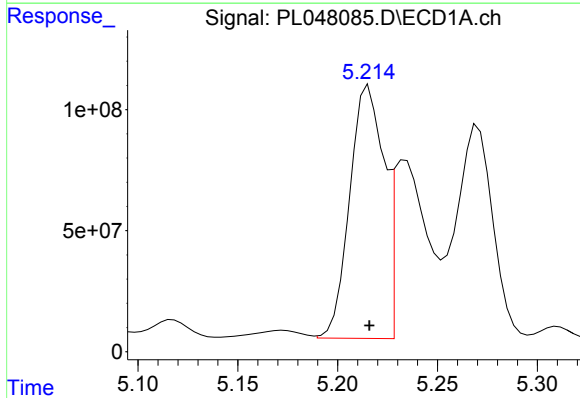


#25 Chlordane-3

R.T.: 5.216 min
Delta R.T.: 0.000 min
Response: 1244775004
Conc: 740.08 ng/ml

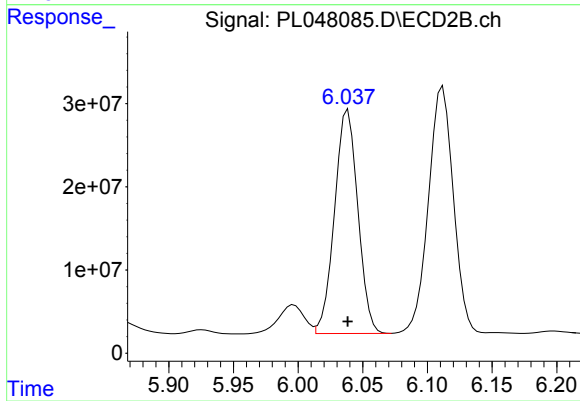

#25 Chlordane-3


R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 337015681
Conc: 752.48 ng/ml

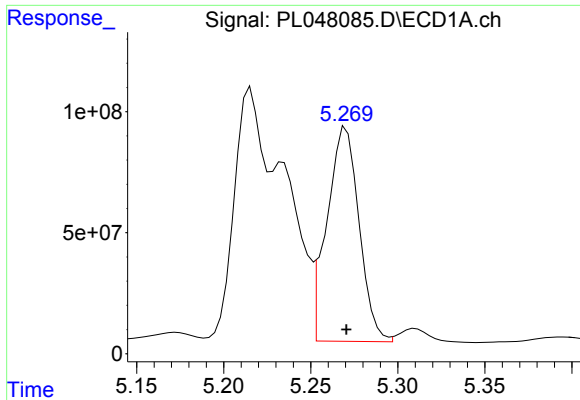

#26 Chlordane-4


R.T.: 5.270 min
Delta R.T.: 0.000 min
Response: 1140224475
Conc: 747.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

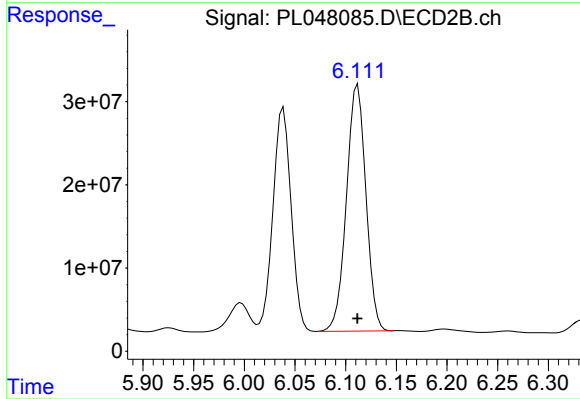


#26 Chlordane-4

R.T.: 6.112 min
Delta R.T.: 0.000 min
Response: 395902784
Conc: 745.65 ng/ml

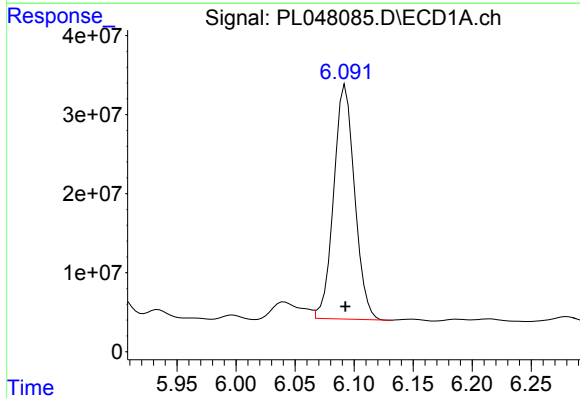


#27 Chlordane-5

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 365320315
Conc: 757.65 ng/ml

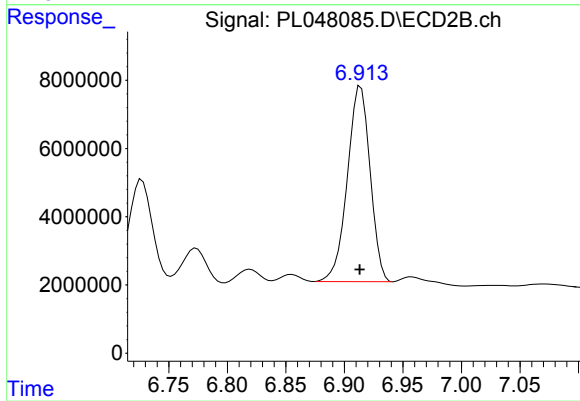

#27 Chlordane-5


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 77620602
Conc: 744.47 ng/ml

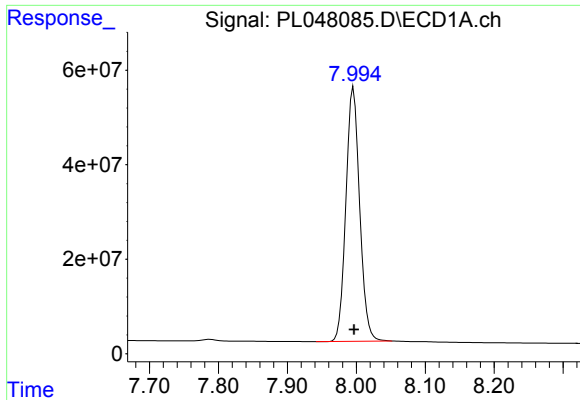

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 747632632
Conc: 72.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

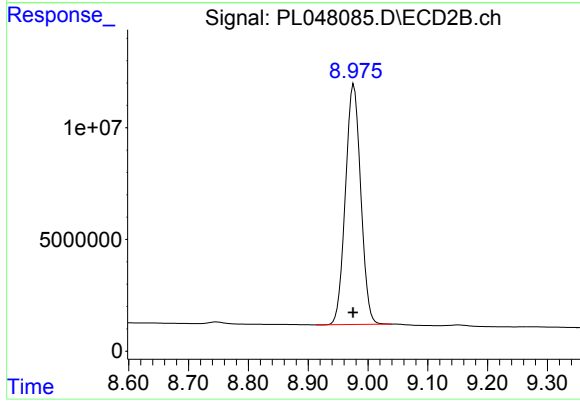

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.001 min
Response: 191133901
Conc: 71.45 ng/ml