

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050119\
 Data File : PL048084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2019 19:17
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 09:29:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:29:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	1074.4E6	256.8E6	98.461	98.847
28)	SA Decachlor...	7.996	8.974	984.6E6	251.3E6	95.496	93.952
Target Compounds							
23)	Chlordane-1	4.169	4.927	482.4E6	128.1E6	1008.552	1017.847
24)	Chlordane-2	4.659	5.394	510.9E6	125.6E6	967.762	950.796
25)	Chlordane-3	5.215	6.038	1657.0E6	454.9E6	985.137	1015.740
26)	Chlordane-4	5.270	6.111	1534.6E6	534.3E6	1006.157	1006.308
27)	Chlordane-5	6.093	6.913	495.9E6	103.5E6	1028.464	992.832



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050119\
Data File : PL048084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2019 19:17
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 09:29:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:29:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

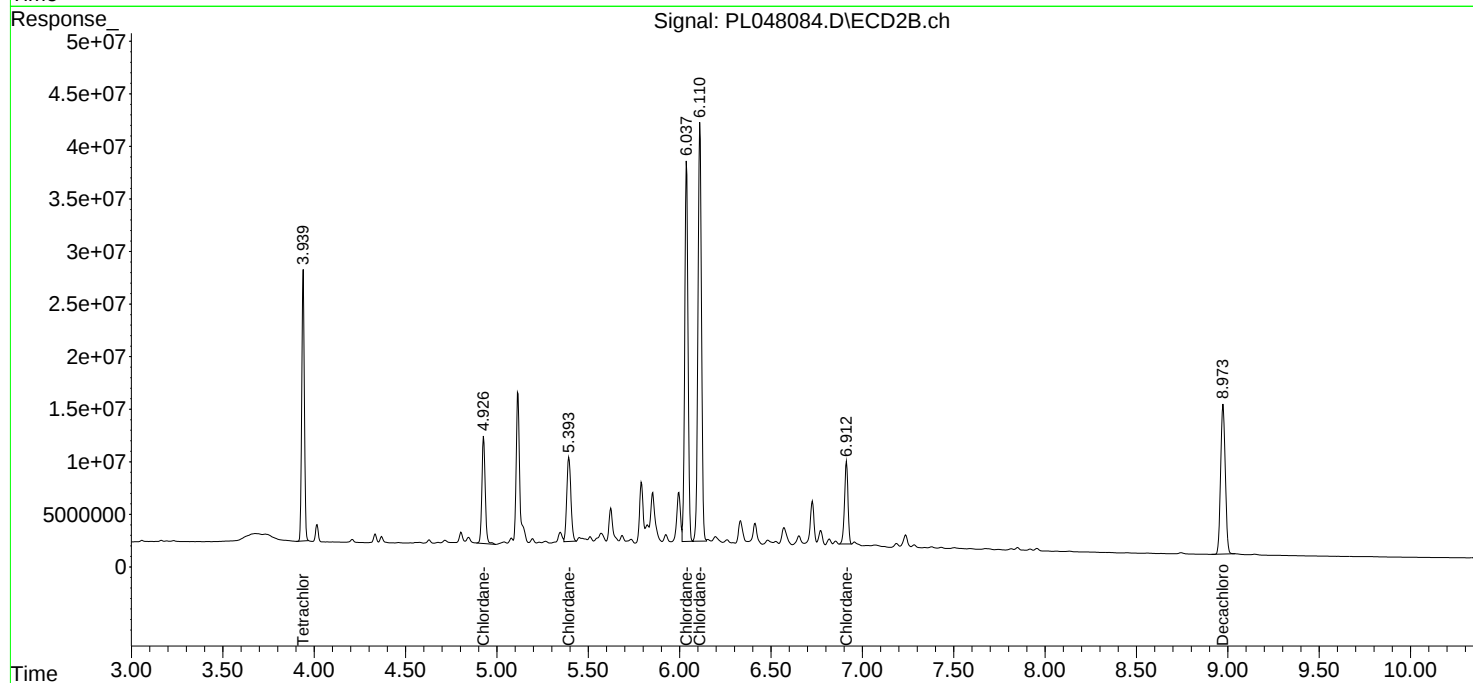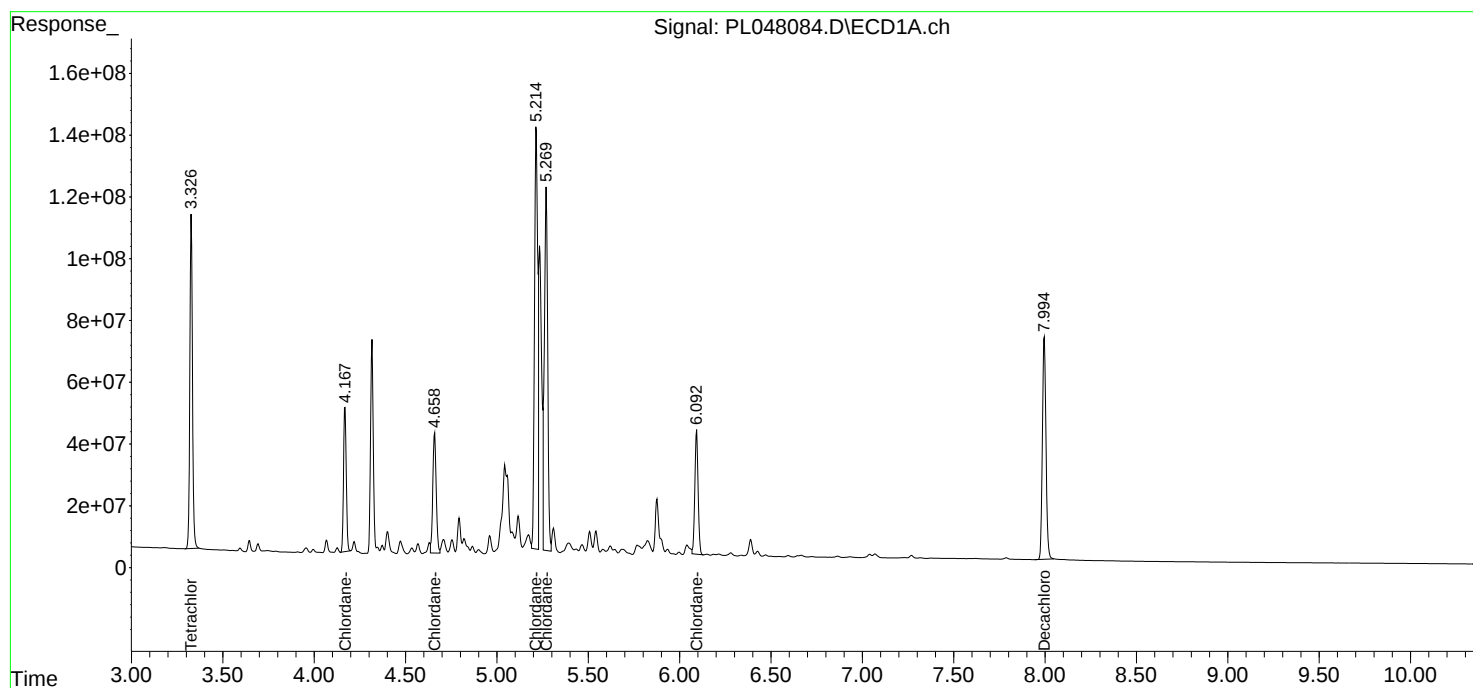


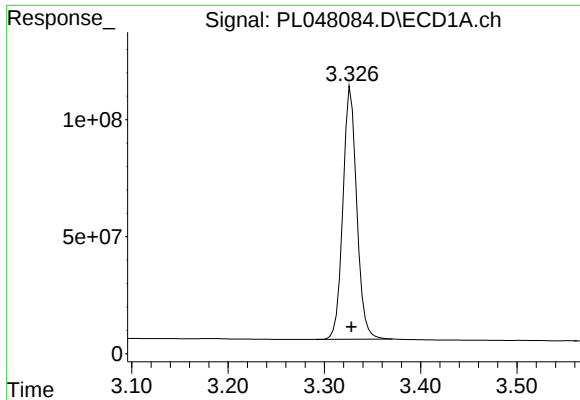

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 1074379169
Conc: 98.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

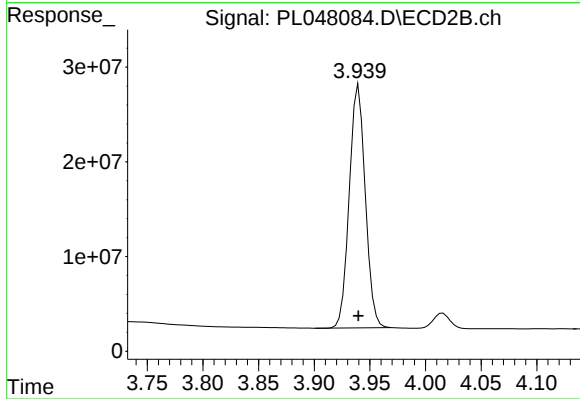


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 256771628
Conc: 98.85 ng/ml

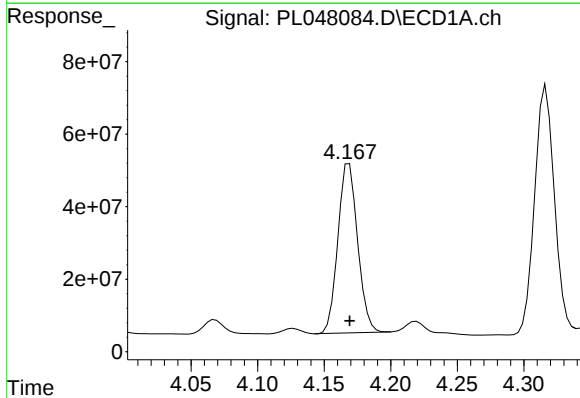


#23 Chlordane-1

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 482418706
Conc: 1008.55 ng/ml

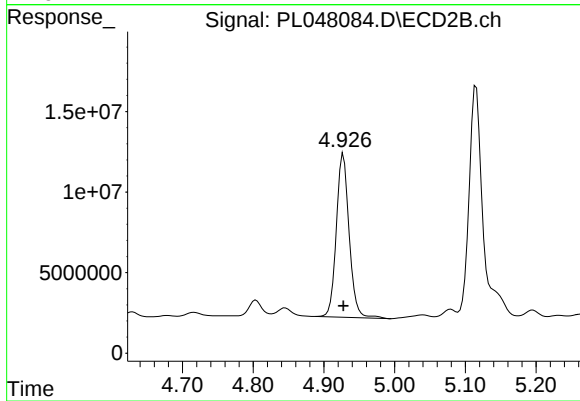

#23 Chlordane-1


R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 128146070
Conc: 1017.85 ng/ml

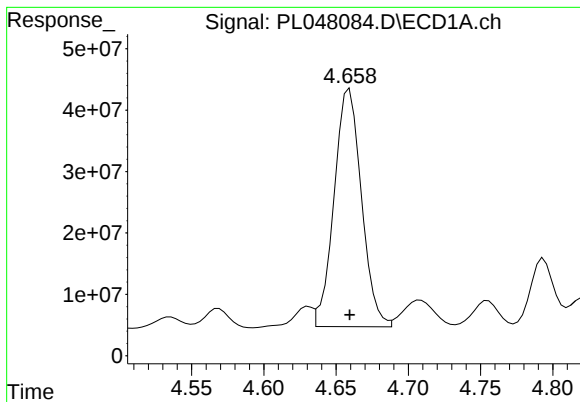

#24 Chlordane-2


R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 510915033
Conc: 967.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

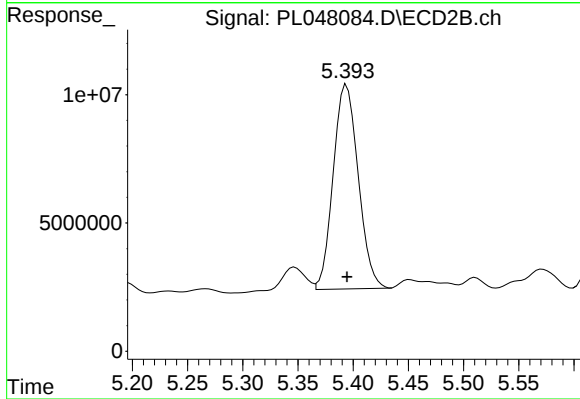


#24 Chlordane-2

R.T.: 5.394 min
Delta R.T.: 0.000 min
Response: 125643653
Conc: 950.80 ng/ml

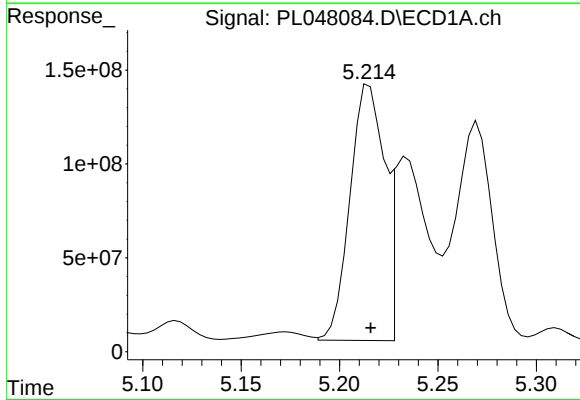


#25 Chlordane-3

R.T.: 5.215 min
Delta R.T.: 0.000 min
Response: 1656952415
Conc: 985.14 ng/ml

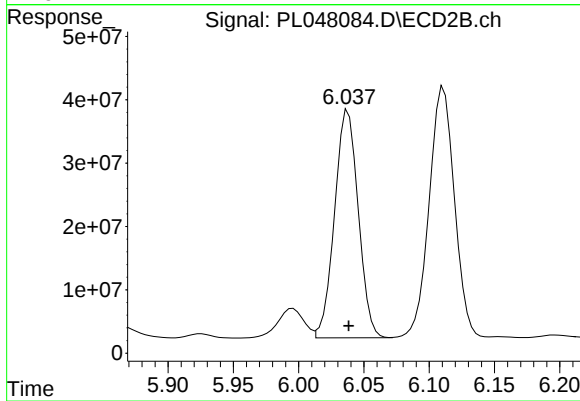

#25 Chlordane-3


R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 454924778
Conc: 1015.74 ng/ml

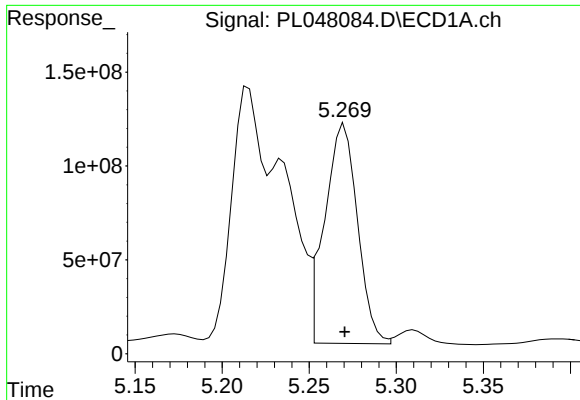

#26 Chlordane-4


R.T.: 5.270 min
Delta R.T.: 0.000 min
Response: 1534592238
Conc: 1006.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

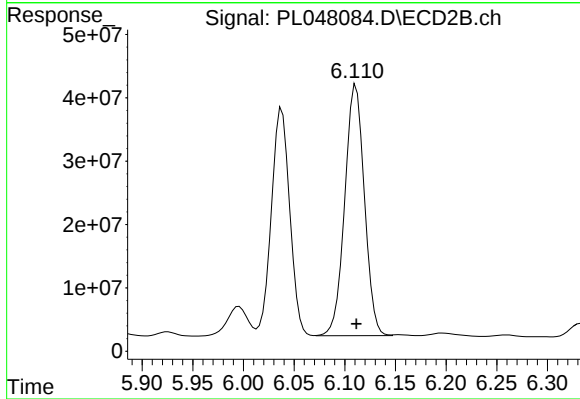


#26 Chlordane-4

R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 534296021
Conc: 1006.31 ng/ml

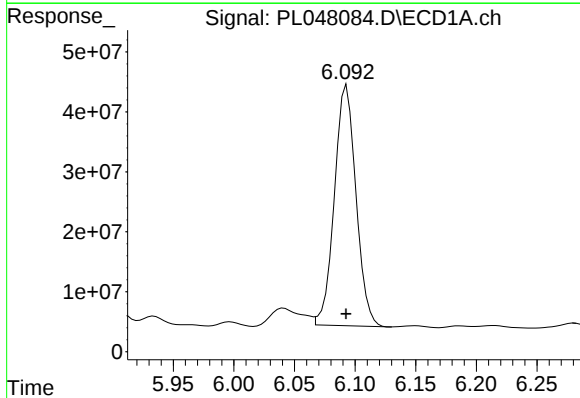


#27 Chlordane-5

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 495899306
Conc: 1028.46 ng/ml

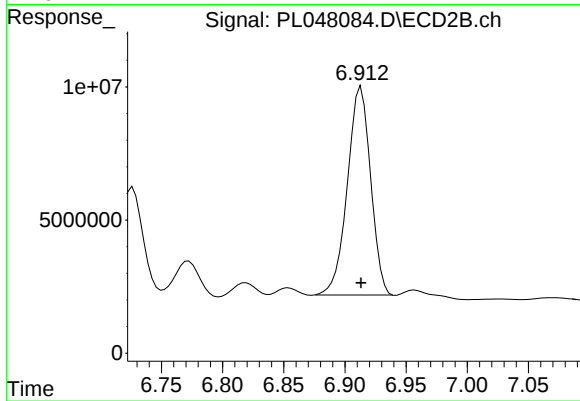

#27 Chlordane-5


R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 103515299
Conc: 992.83 ng/ml

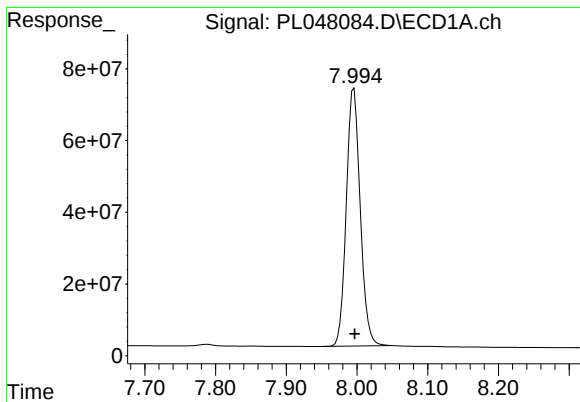

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: -0.001 min
Response: 984618449
Conc: 95.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

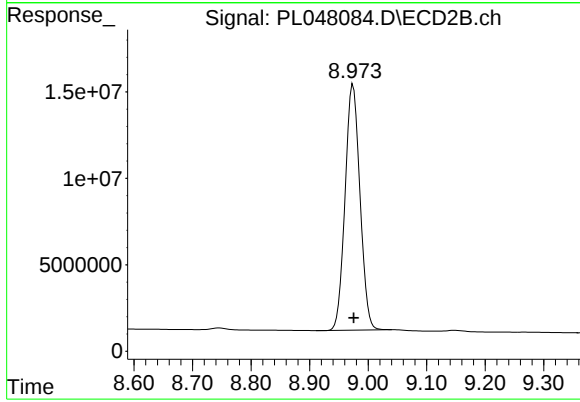

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.001 min
Response: 251341055
Conc: 93.95 ng/ml