

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050119\
 Data File : PL048086.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2019 19:47
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 09:30:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:29:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	545.6E6	129.9E6	50.000	50.000
28)	SA Decachlor...	7.997	8.975	515.5E6	133.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.169	4.927	239.2E6	62949549	500.000	500.000
24)	Chlordane-2	4.659	5.394	264.0E6	66072895	500.000	500.000
25)	Chlordane-3	5.216	6.038	841.0E6	223.9E6	500.000	500.000
26)	Chlordane-4	5.270	6.111	762.6E6	265.5E6	500.000	500.000
27)	Chlordane-5	6.093	6.913	241.1E6	52131315	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050119\
Data File : PL048086.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2019 19:47
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 09:30:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:29:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

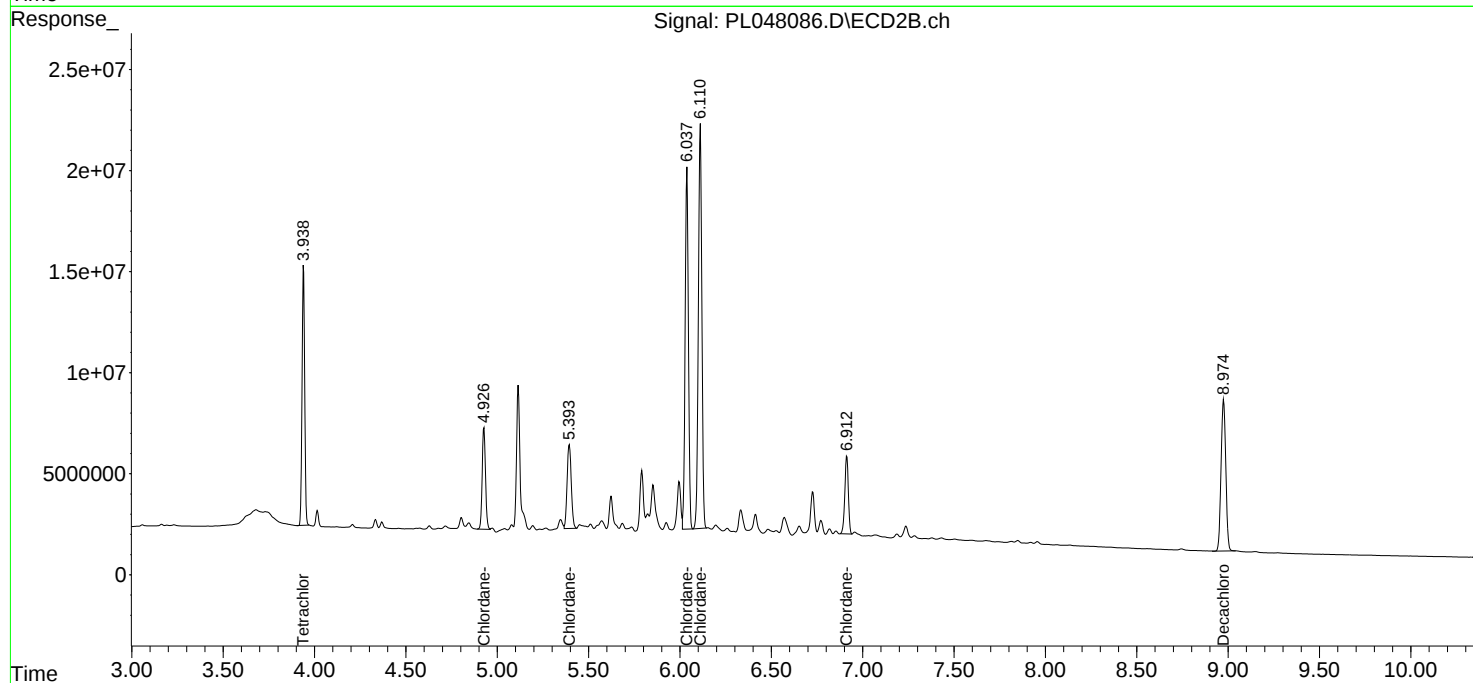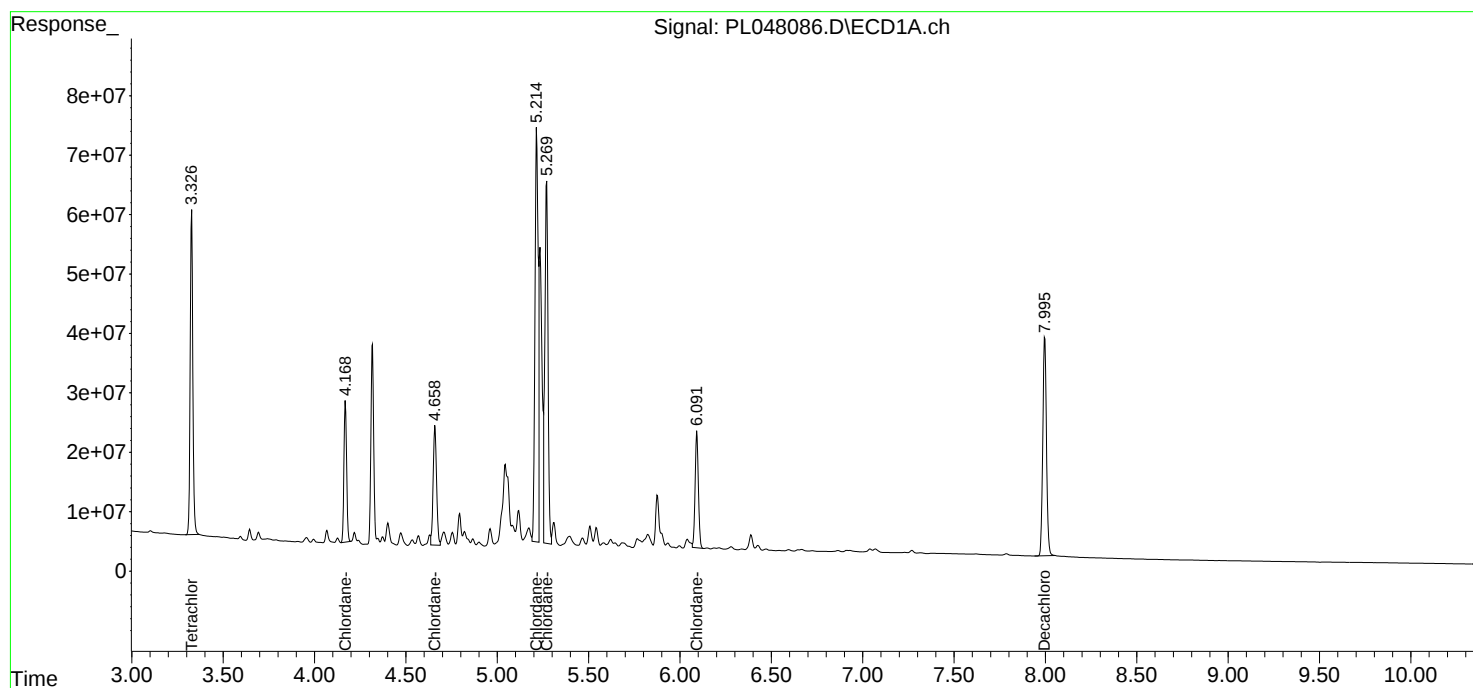


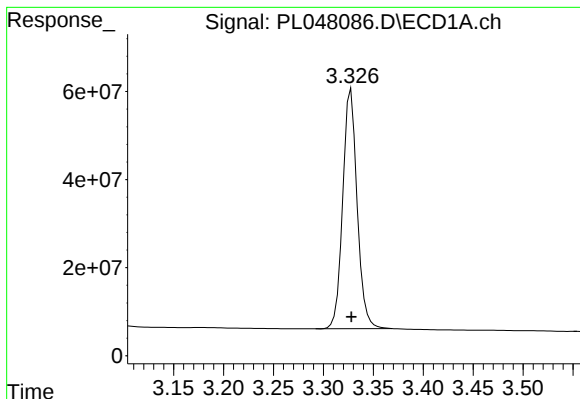

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 545585630
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

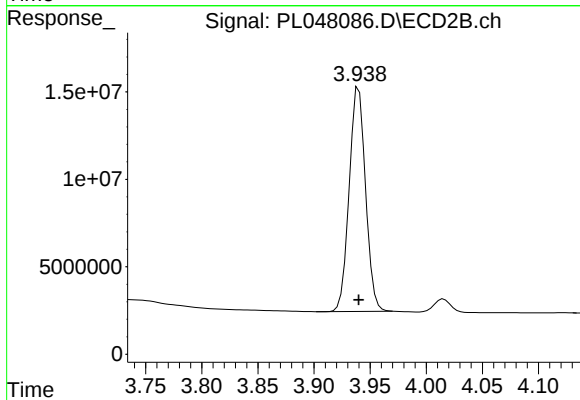


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 129883368
Conc: 50.00 ng/ml

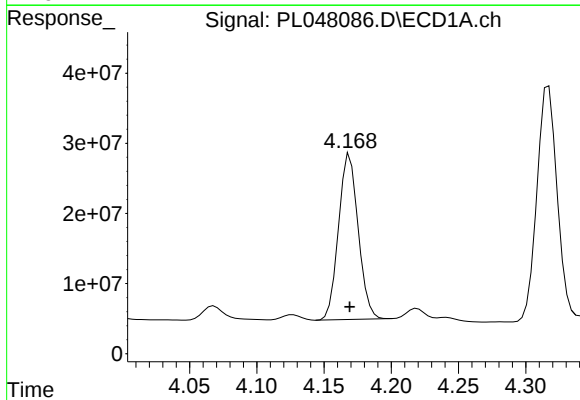


#23 Chlordane-1

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 239164108
Conc: 500.00 ng/ml

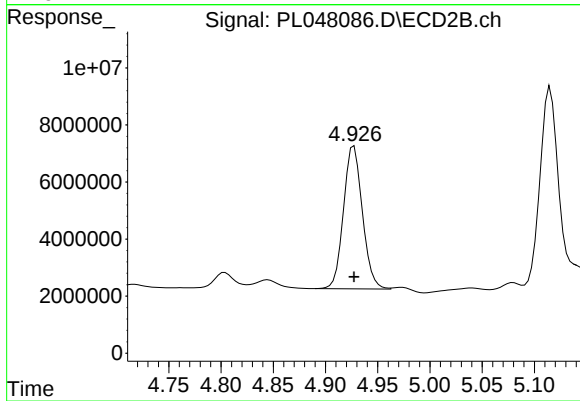

#23 Chlordane-1


R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 62949549
Conc: 500.00 ng/ml

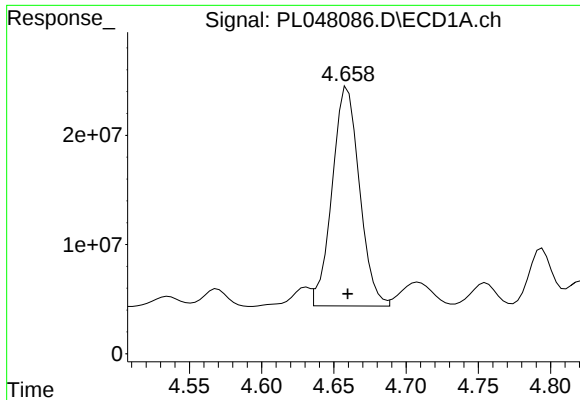

#24 Chlordane-2


R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 263967308
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

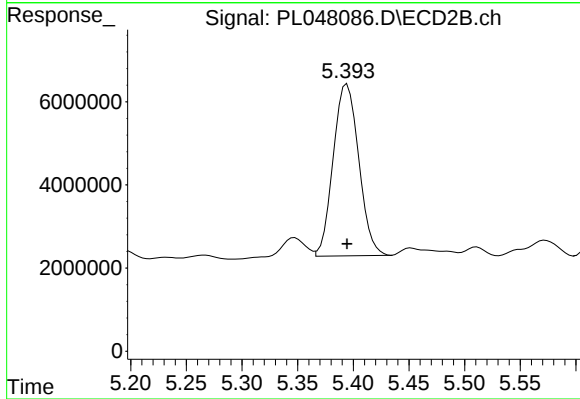


#24 Chlordane-2

R.T.: 5.394 min
Delta R.T.: 0.000 min
Response: 66072895
Conc: 500.00 ng/ml

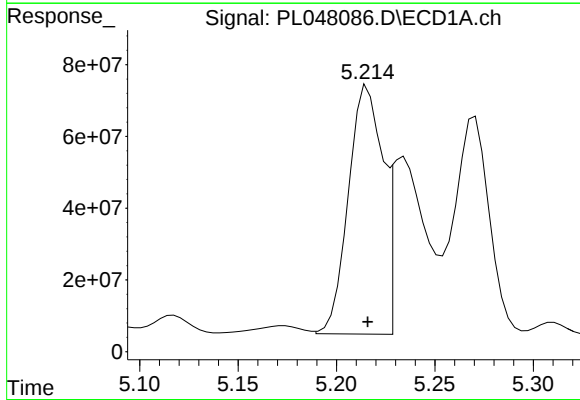


#25 Chlordane-3

R.T.: 5.216 min
Delta R.T.: 0.000 min
Response: 840975525
Conc: 500.00 ng/ml

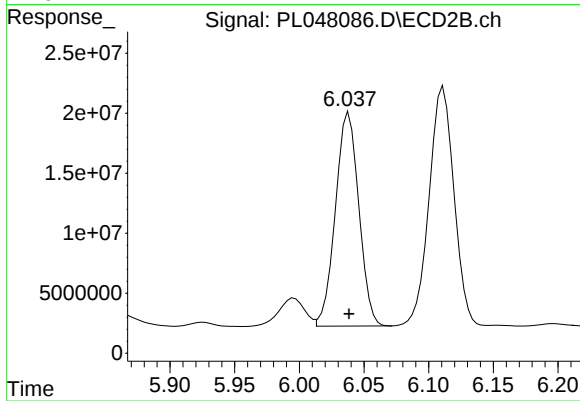

#25 Chlordane-3


R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 223937619
Conc: 500.00 ng/ml

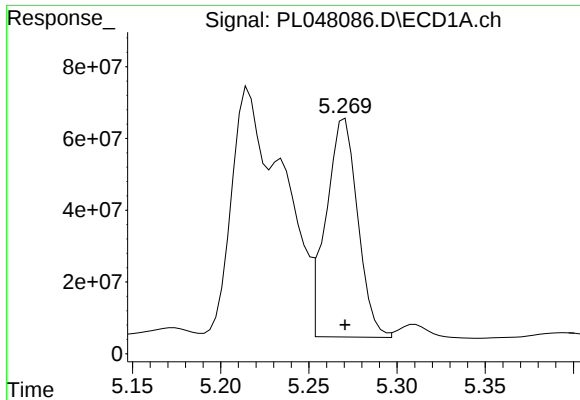

#26 Chlordane-4


R.T.: 5.270 min
Delta R.T.: 0.000 min
Response: 762600838
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

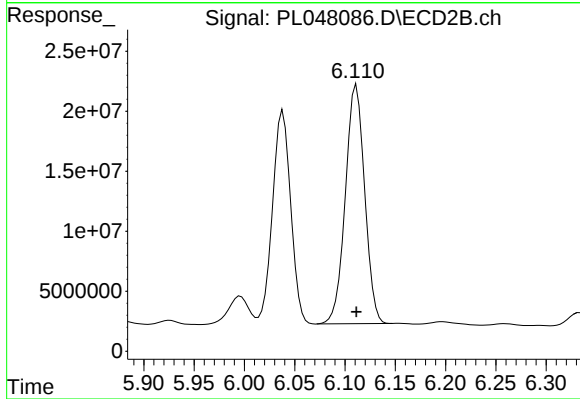


#26 Chlordane-4

R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 265473276
Conc: 500.00 ng/ml

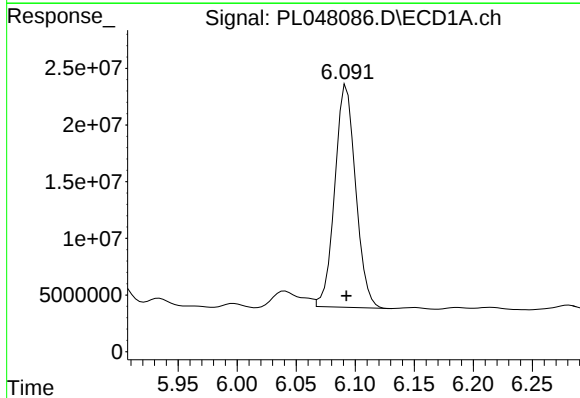


#27 Chlordane-5

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 241087230
Conc: 500.00 ng/ml

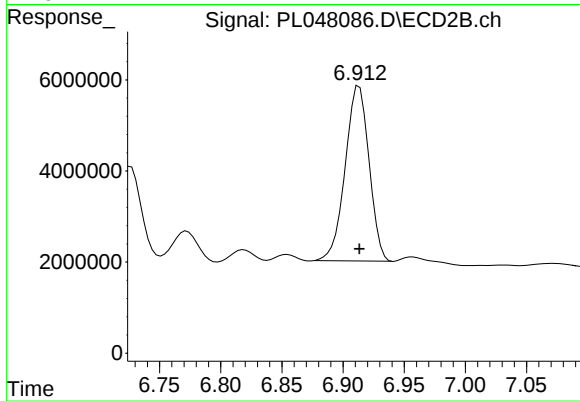

#27 Chlordane-5


R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 52131315
Conc: 500.00 ng/ml

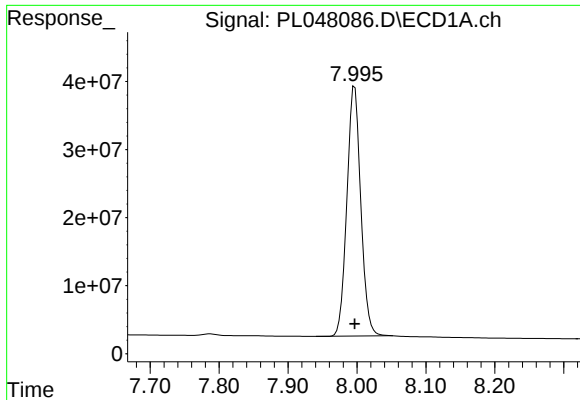

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: 0.000 min
Response: 515529071
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

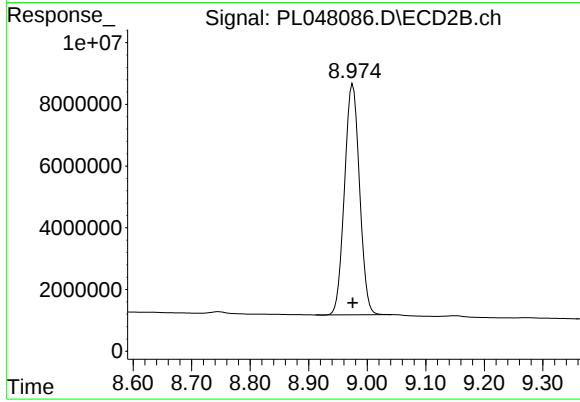

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 133759748
Conc: 50.00 ng/ml