

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050119\
 Data File : PL048087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2019 20:02
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 09:30:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:29:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	260.4E6	62342174	23.866	23.999
28)	SA Decachlor...	7.996	8.976	261.9E6	69611718	25.400	26.021
Target Compounds							
23)	Chlordane-1	4.169	4.928	111.7E6	30359473	233.567	241.141
24)	Chlordane-2	4.660	5.395	135.4E6	33400960	256.477	252.758
25)	Chlordane-3	5.216	6.039	388.3E6	107.0E6	230.848	238.891
26)	Chlordane-4	5.271	6.112	363.0E6	129.7E6	237.995	244.314
27)	Chlordane-5	6.093	6.914	111.2E6	25687920	230.691	246.377



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050119\
Data File : PL048087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2019 20:02
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 09:30:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:29:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

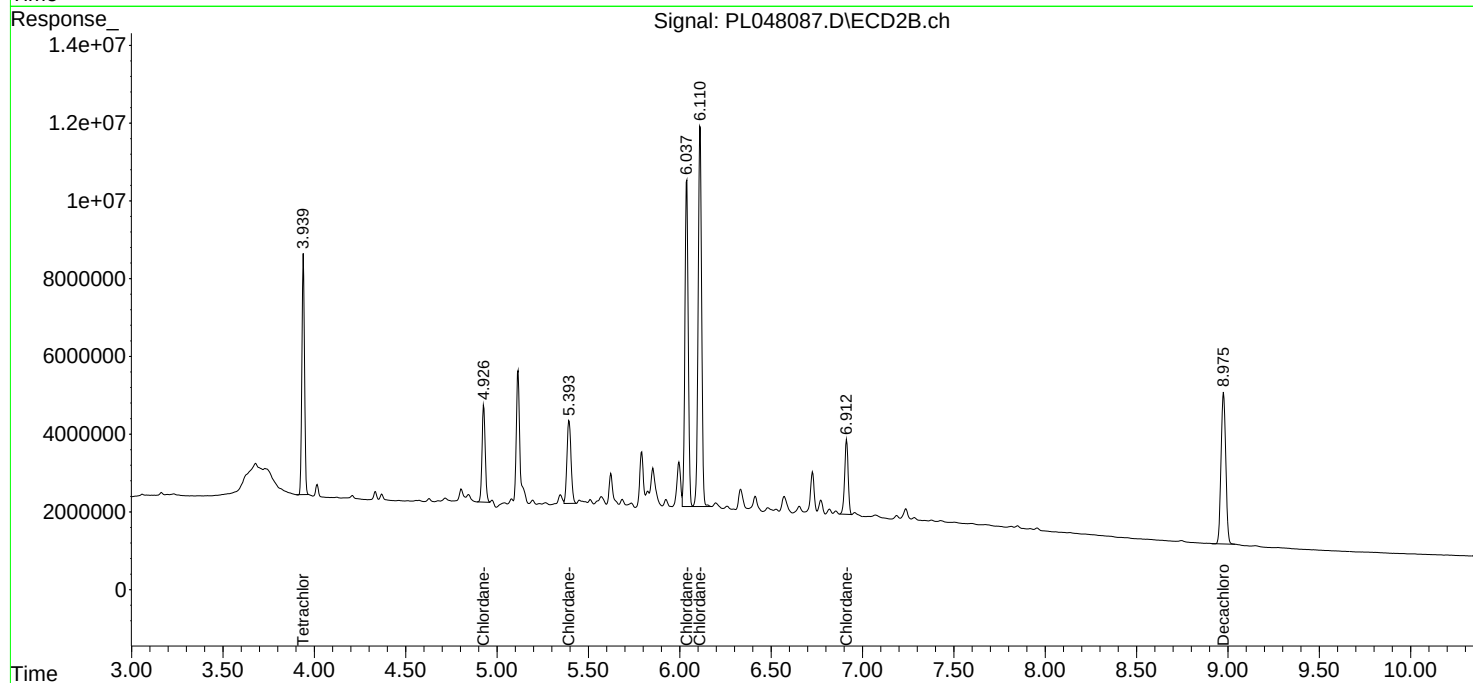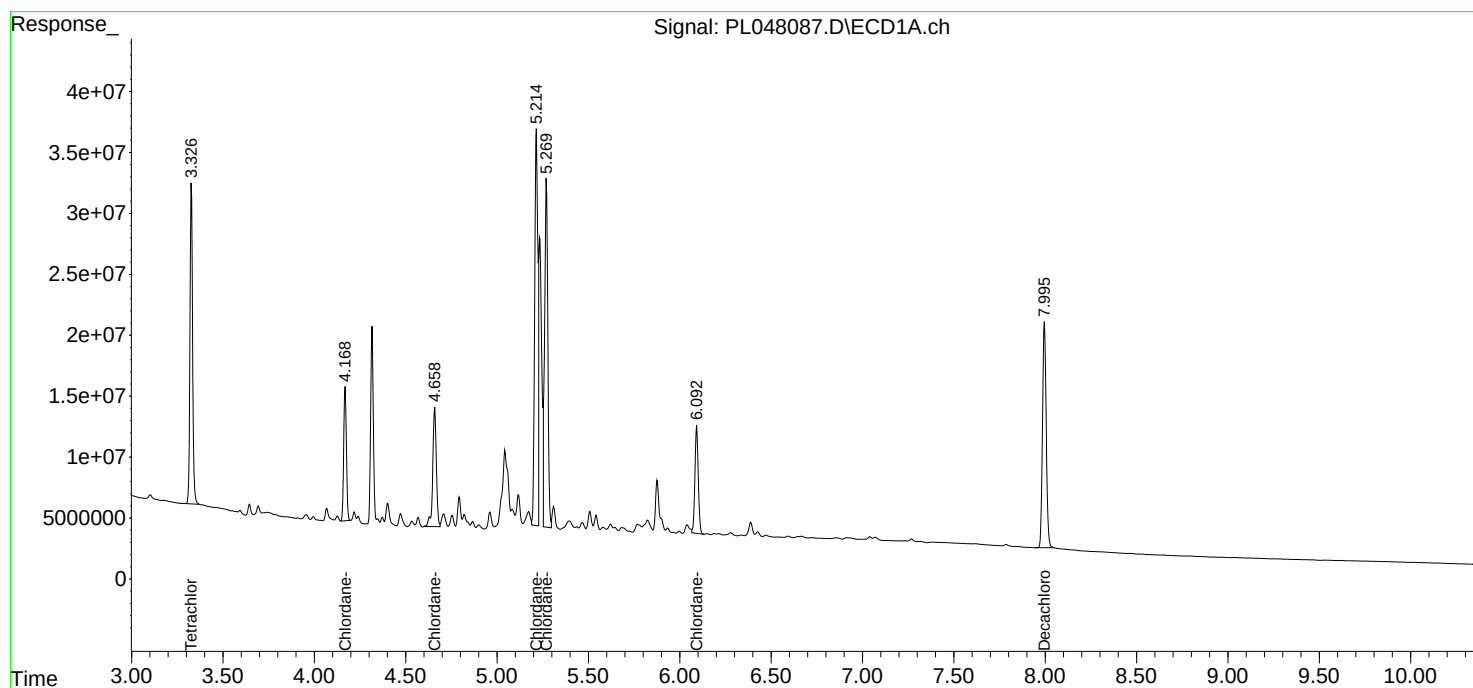


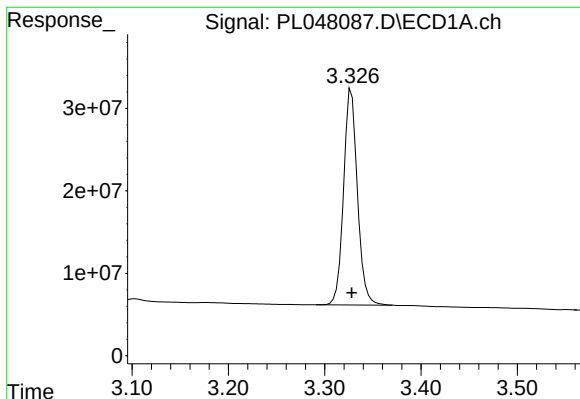

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 260421391
Conc: 23.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

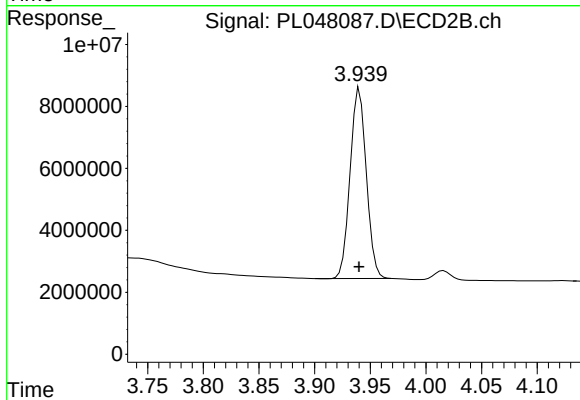


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 62342174
Conc: 24.00 ng/ml

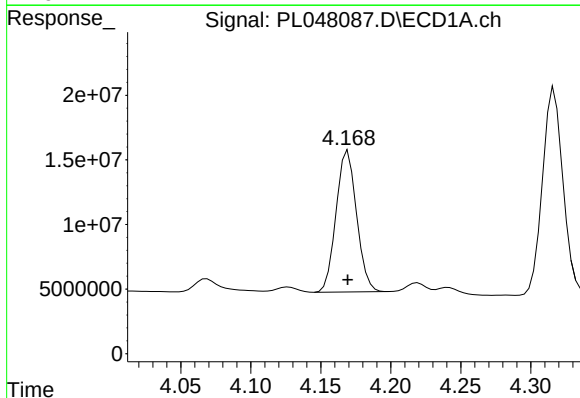


#23 Chlordane-1

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 111721592
Conc: 233.57 ng/ml

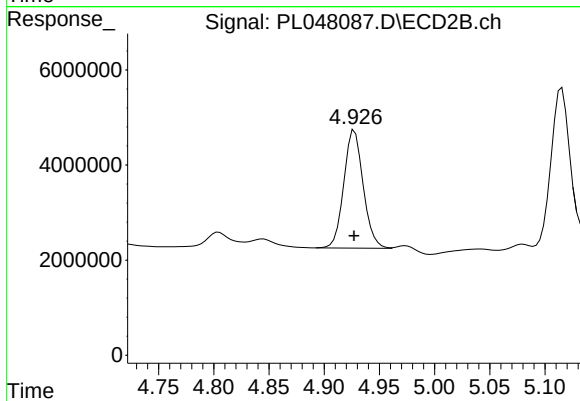

#23 Chlordane-1


R.T.: 4.928 min
Delta R.T.: 0.000 min
Response: 30359473
Conc: 241.14 ng/ml

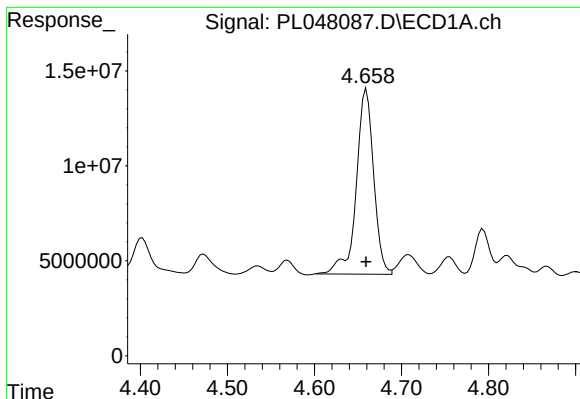

#24 Chlordane-2


R.T.: 4.660 min
Delta R.T.: 0.000 min
Response: 135403088
Conc: 256.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

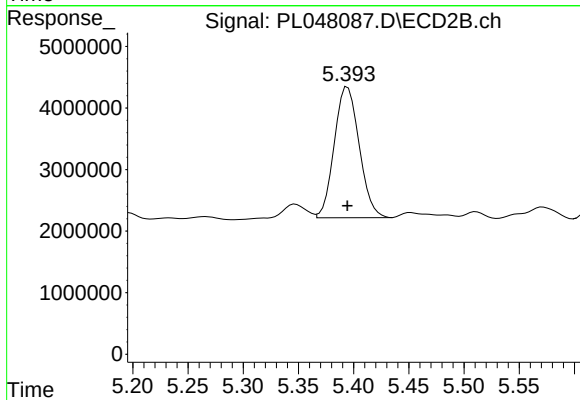


#24 Chlordane-2

R.T.: 5.395 min
Delta R.T.: 0.000 min
Response: 33400960
Conc: 252.76 ng/ml

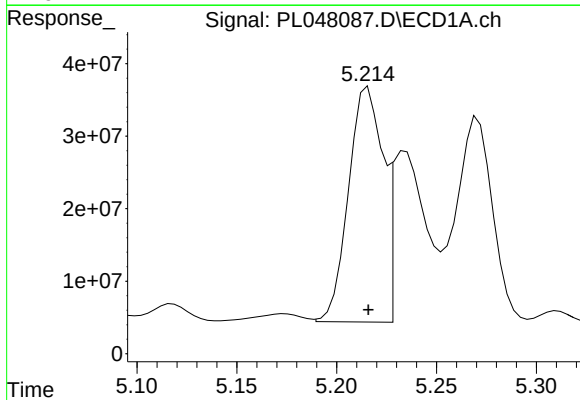


#25 Chlordane-3

R.T.: 5.216 min
Delta R.T.: 0.000 min
Response: 388274331
Conc: 230.85 ng/ml

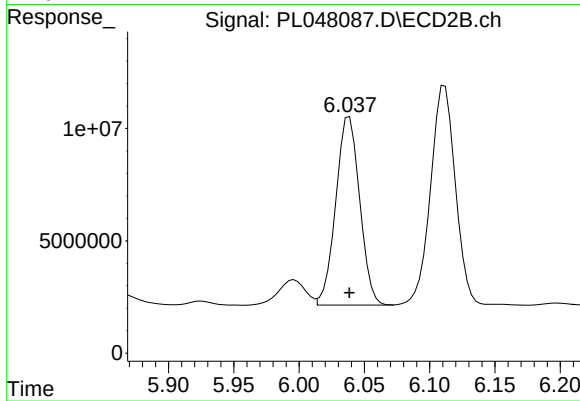

#25 Chlordane-3


R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 106993489
Conc: 238.89 ng/ml

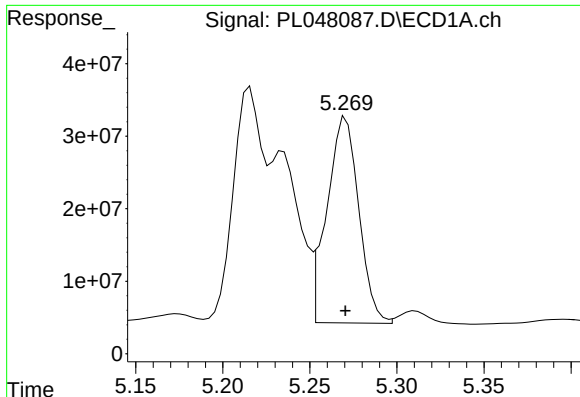

#26 Chlordane-4


R.T.: 5.271 min
Delta R.T.: 0.000 min
Response: 362990391
Conc: 238.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

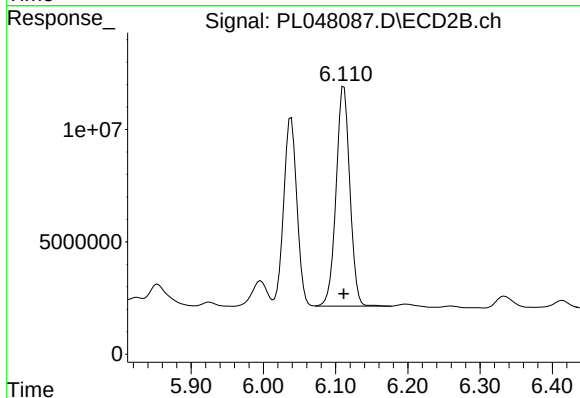


#26 Chlordane-4

R.T.: 6.112 min
Delta R.T.: 0.000 min
Response: 129717604
Conc: 244.31 ng/ml

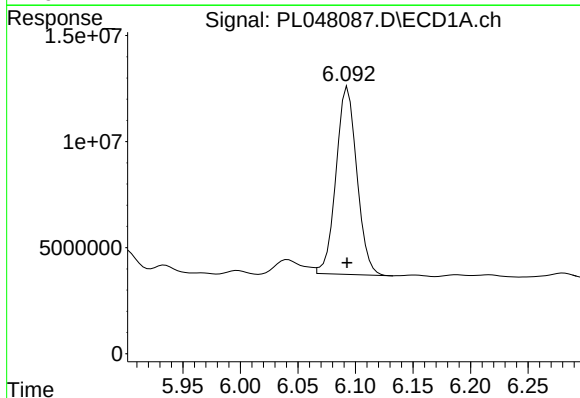


#27 Chlordane-5

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 111233537
Conc: 230.69 ng/ml

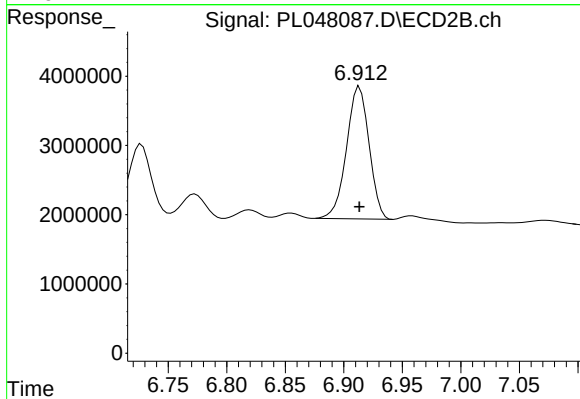

#27 Chlordane-5


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 25687920
Conc: 246.38 ng/ml

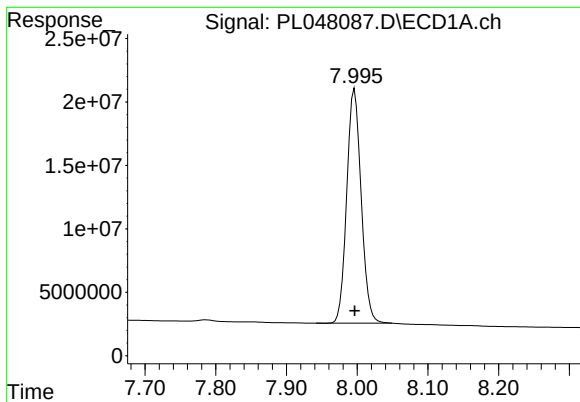

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 261892276
Conc: 25.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

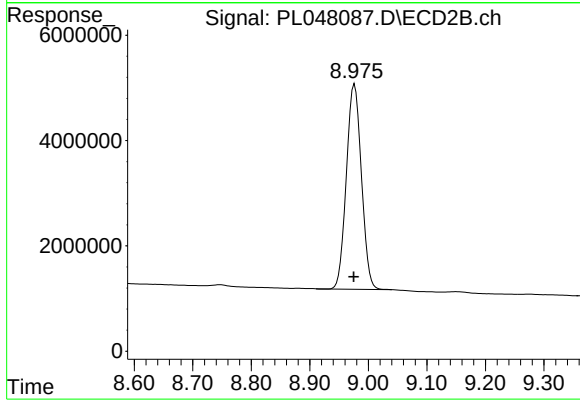

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.001 min
Response: 69611718
Conc: 26.02 ng/ml