

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050119\
 Data File : PL048095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2019 22:02
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL050119CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 09:37:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	525.3E6	126.8E6	54.232	50.892
28)	SA Decachlor...	7.997	8.977	508.0E6	131.4E6	50.523	49.497
Target Compounds							
23)	Chlordane-1	4.170	4.928	227.2E6	60964886	506.226	499.110
24)	Chlordane-2	4.660	5.395	251.6E6	63674008	486.389	492.304
25)	Chlordane-3	5.216	6.039	798.2E6	215.7E6	506.939	492.136
26)	Chlordane-4	5.271	6.112	727.5E6	254.6E6	501.087	485.381
27)	Chlordane-5	6.093	6.914	224.2E6	49842176	477.409	490.230



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050119\
Data File : PL048095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2019 22:02
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL050119CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 09:37:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

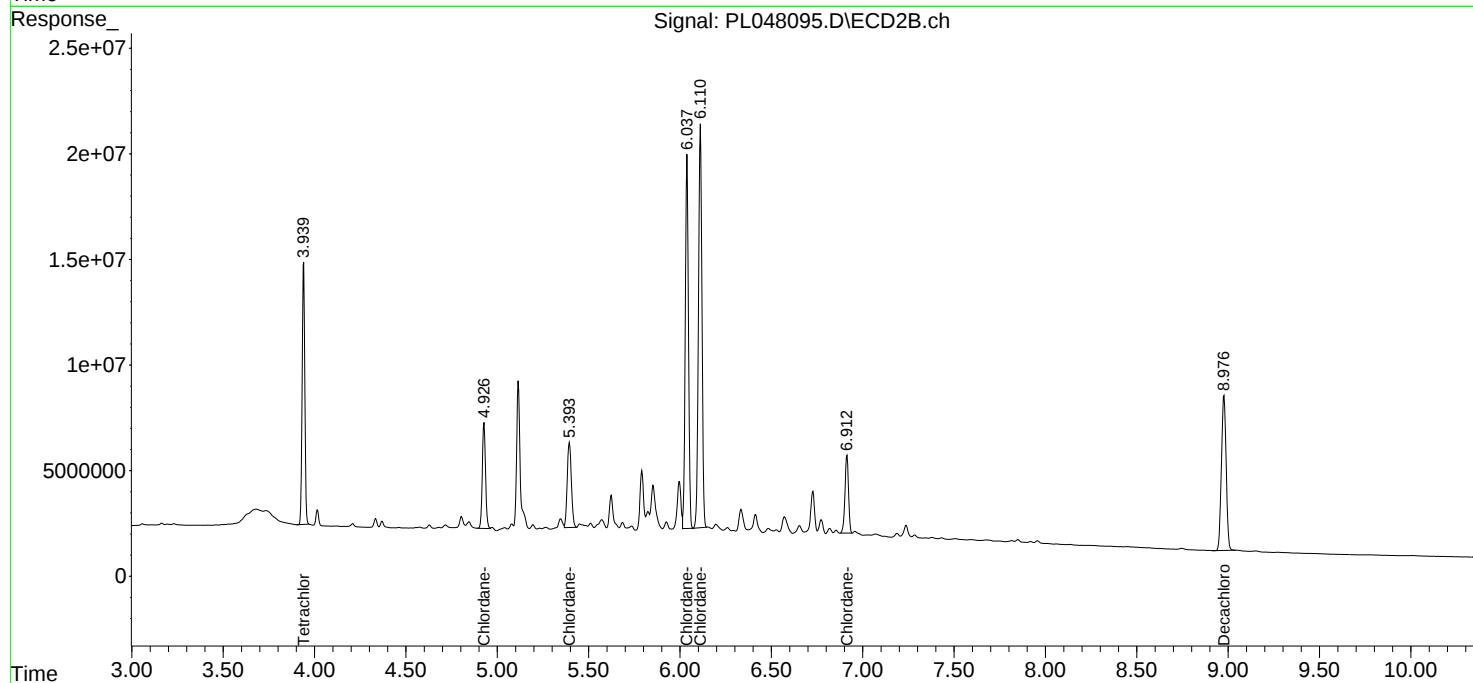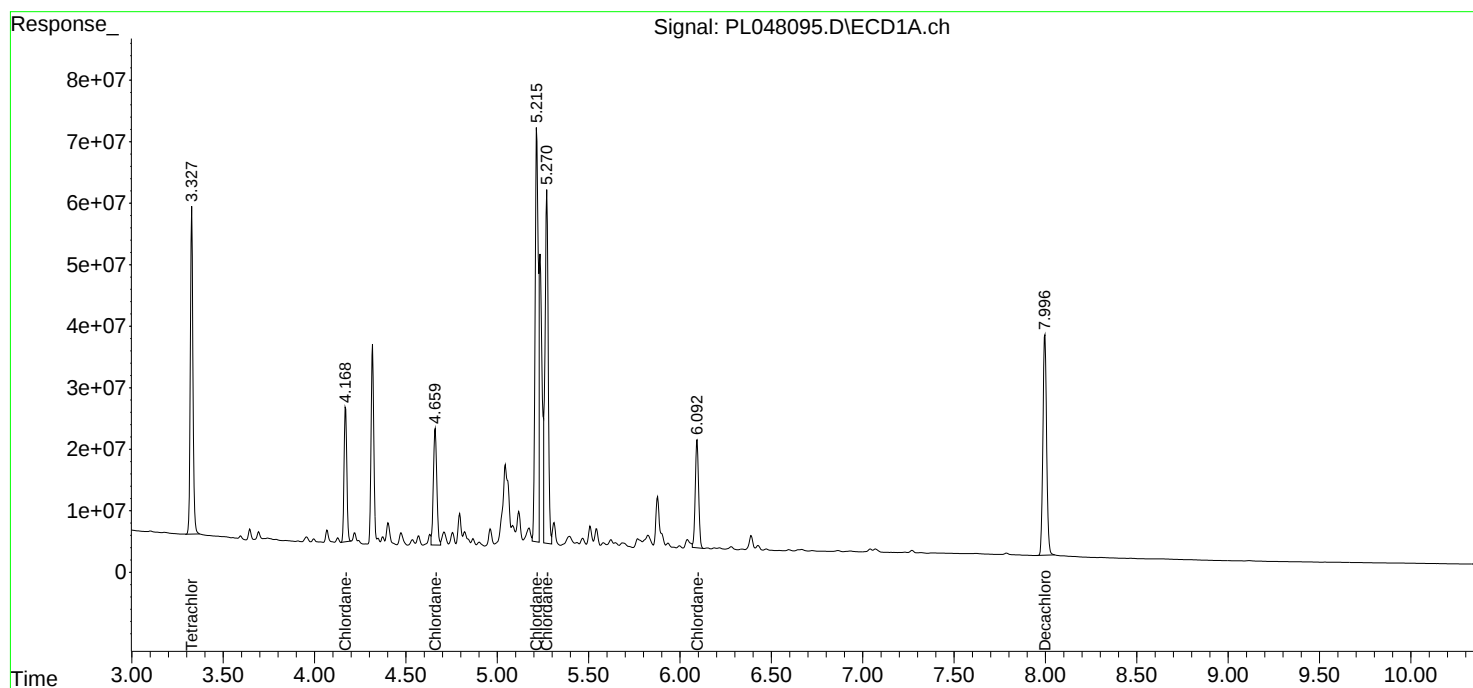


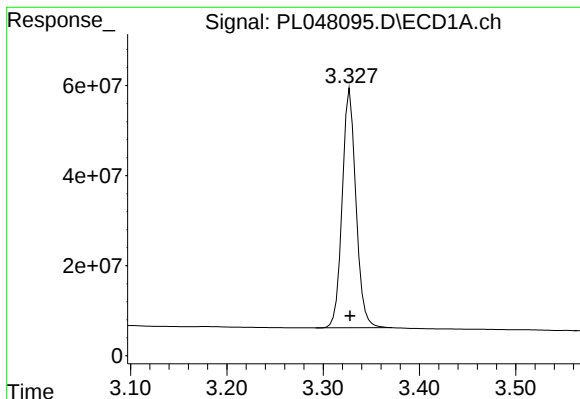

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 525339434
Conc: 54.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL050119CHLOR

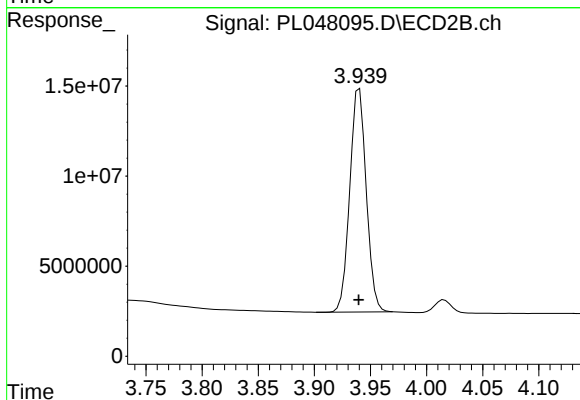


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 126766722
Conc: 50.89 ng/ml

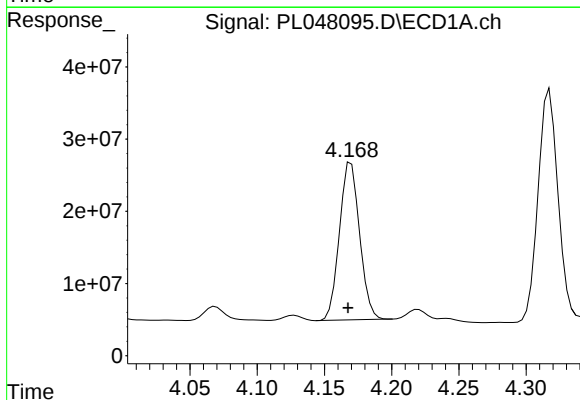


#23 Chlordane-1

R.T.: 4.170 min
Delta R.T.: 0.002 min
Response: 227248412
Conc: 506.23 ng/ml

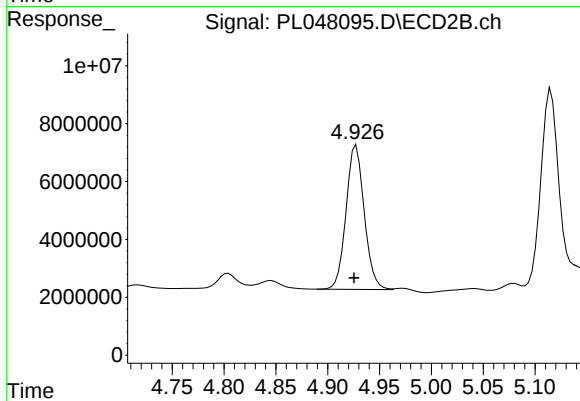

#23 Chlordane-1


R.T.: 4.928 min
Delta R.T.: 0.002 min
Response: 60964886
Conc: 499.11 ng/ml

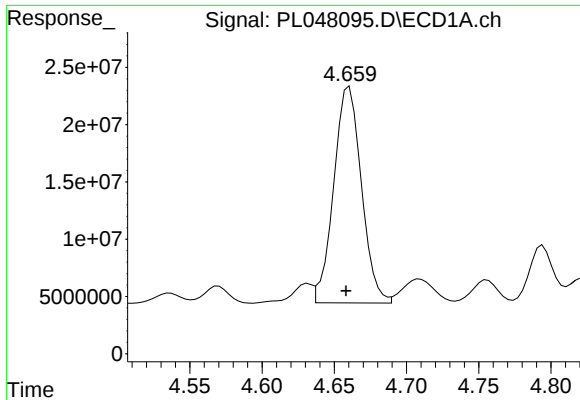

#24 Chlordane-2


R.T.: 4.660 min
Delta R.T.: 0.002 min
Response: 251614969
Conc: 486.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL050119CHLOR

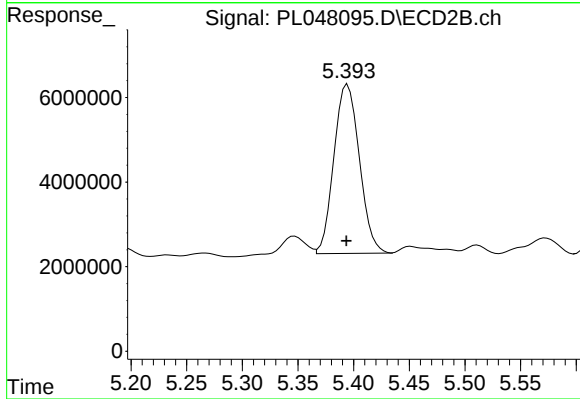


#24 Chlordane-2

R.T.: 5.395 min
Delta R.T.: 0.001 min
Response: 63674008
Conc: 492.30 ng/ml

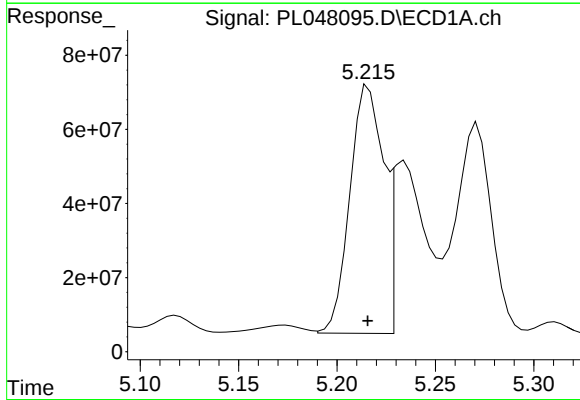


#25 Chlordane-3

R.T.: 5.216 min
Delta R.T.: 0.000 min
Response: 798204884
Conc: 506.94 ng/ml

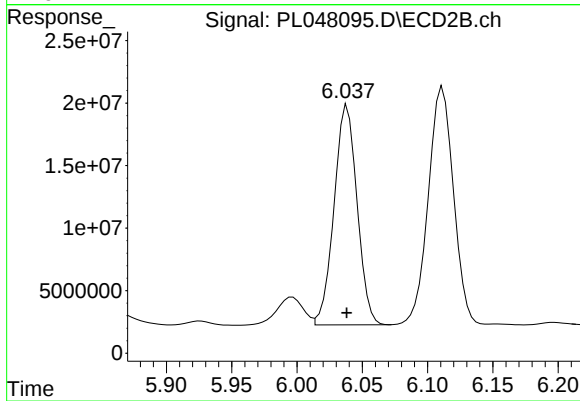

#25 Chlordane-3


R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 215668993
Conc: 492.14 ng/ml

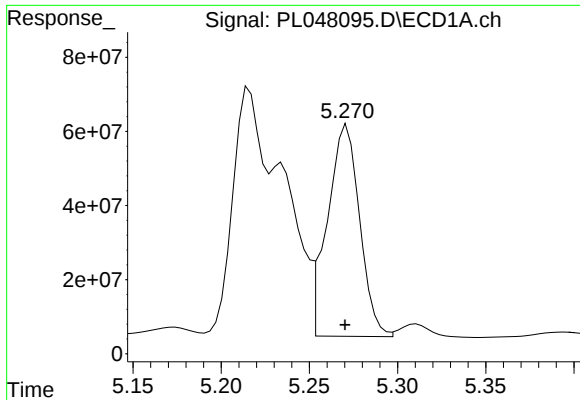

#26 Chlordane-4


R.T.: 5.271 min
Delta R.T.: 0.000 min
Response: 727489030
Conc: 501.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL050119CHLOR

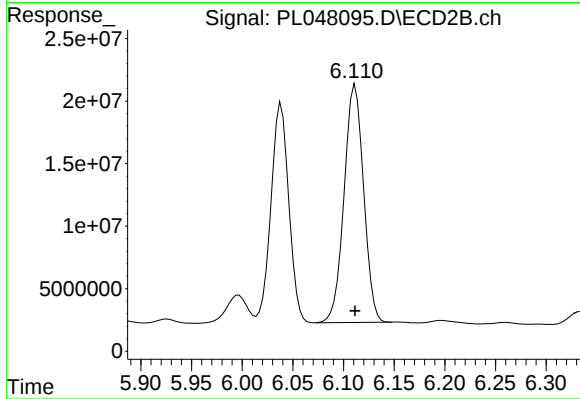


#26 Chlordane-4

R.T.: 6.112 min
Delta R.T.: 0.000 min
Response: 254630938
Conc: 485.38 ng/ml

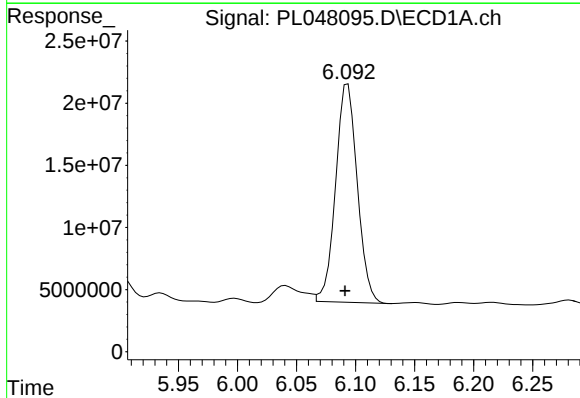


#27 Chlordane-5

R.T.: 6.093 min
Delta R.T.: 0.002 min
Response: 224170543
Conc: 477.41 ng/ml

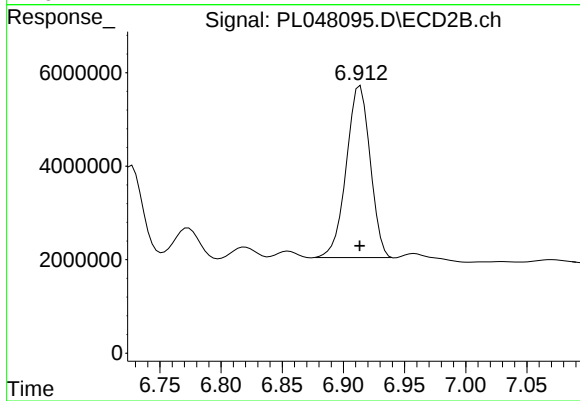

#27 Chlordane-5


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 49842176
Conc: 490.23 ng/ml

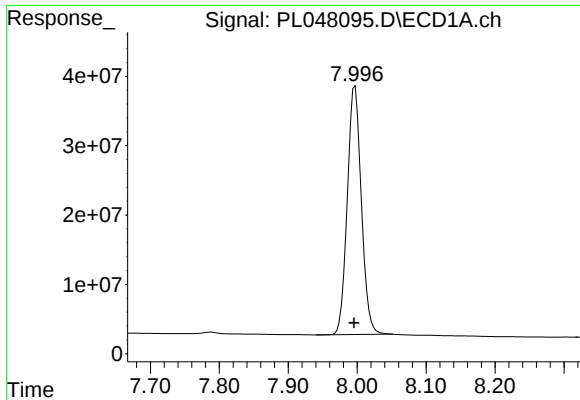

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: 0.001 min
Response: 507971304
Conc: 50.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL050119CHLOR

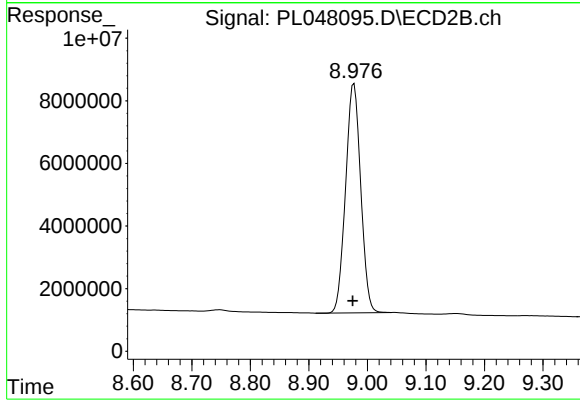

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.002 min
Response: 131380123
Conc: 49.50 ng/ml