

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050120\
 Data File : PL058498.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2020 18:29
 Operator : AJ\MA
 Sample : L2463-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AOC14-CARWASH

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 00:44:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 29 00:55:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.955	211.2E6	47540784	19.847	21.995
28)	SA Decachlor...	8.201	8.976	228.3E6	50433914	21.112	22.730
Target Compounds							
3)	MA gamma-BHC...	4.197f	0.000	1534283	0	0.089	N.D. #
4)	MA Heptachlor	0.000	5.135	0	761428	N.D.	0.220 #
5)	MB Aldrin	4.715	0.000	1314769	0	0.079	N.D. #
7)	B delta-BHC	0.000	4.987f	0	2644505	N.D.	1.052 #
10)	B gamma-Chl...	0.000	6.043	0	2248310	N.D.	0.666 #
11)	B alpha-Chl...	0.000	6.142f	0	142462	N.D.	0.042 #
15)	B Endosulfa...	0.000	6.869f	0	1301302	N.D.	0.488 #
23)	Chlordane-1	4.297f	0.000	8136172	0	18.928	N.D. #
24)	Chlordane-2	4.813	0.000	1956935	0	4.712	N.D. #
25)	Chlordane-3	0.000	6.043	0	2248310	N.D.	5.621 #
26)	Chlordane-4	0.000	6.142f	0	142462	N.D.	0.293 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050120\
Data File : PL058498.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2020 18:29
Operator : AJ\MA
Sample : L2463-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AOC14-CARWASH

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 00:44:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
Quant Title : GC Extractables
QLast Update : Wed Apr 29 00:55:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

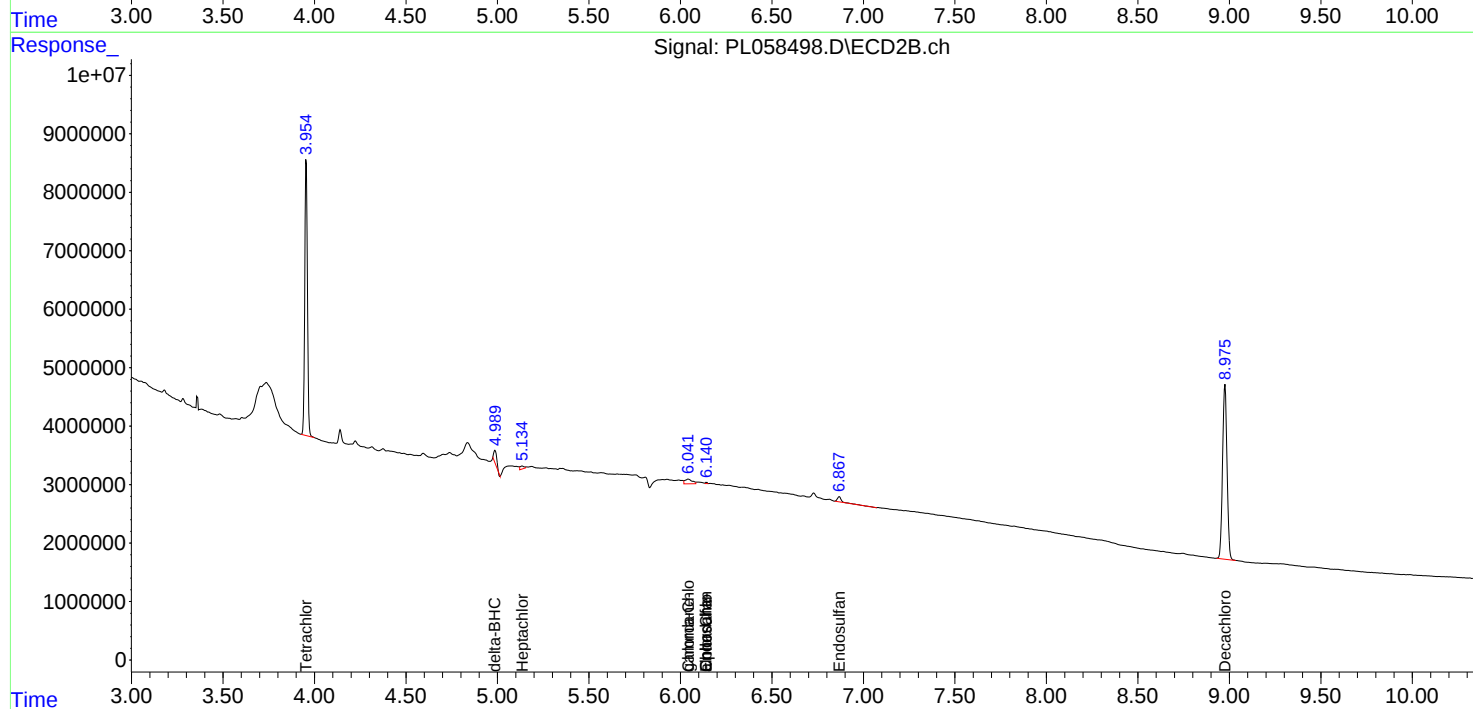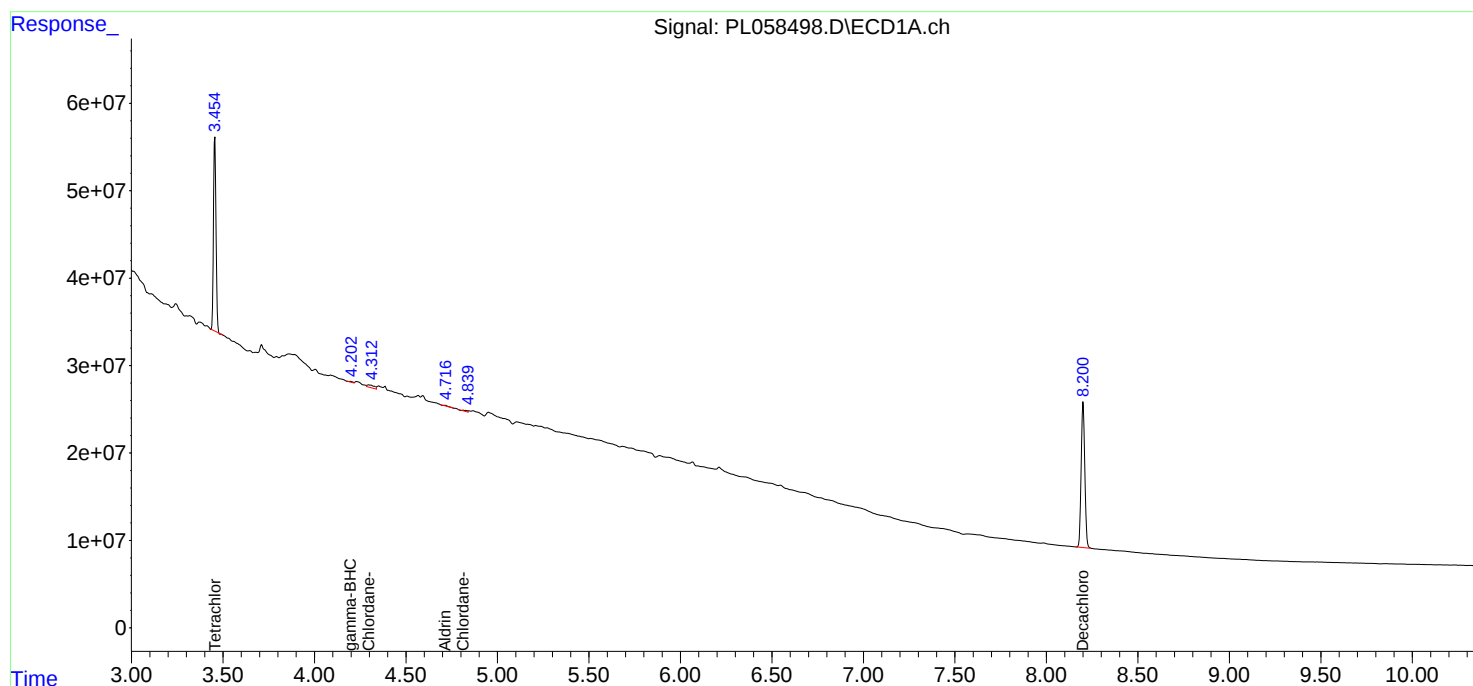


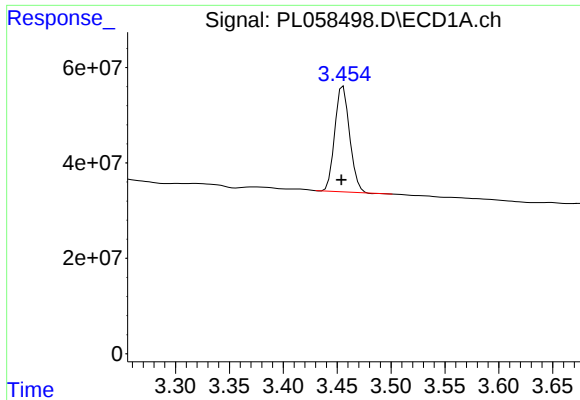

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: 0.002 min
Response: 211210306
Conc: 19.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
AOC14-CARWASH

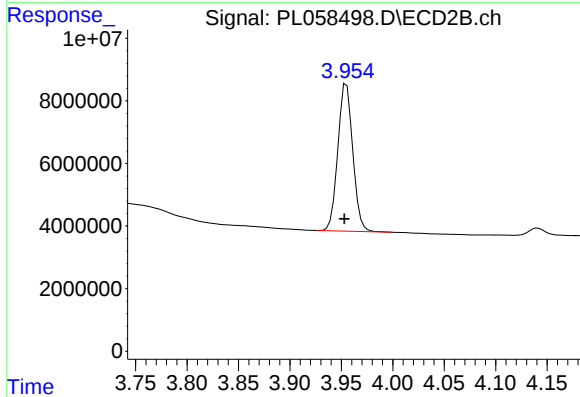


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: 0.002 min
Response: 47540784
Conc: 22.00 ng/ml

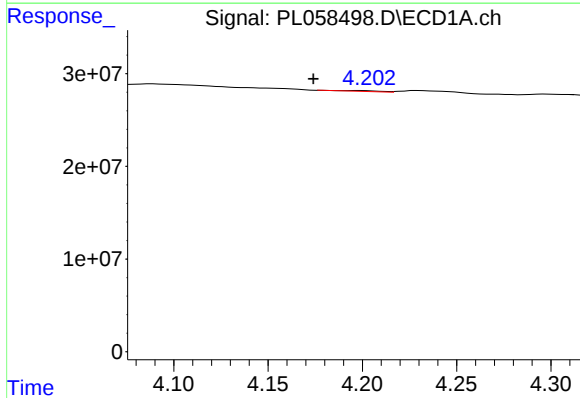


#3 gamma-BHC (Lindane)

R.T.: 4.197 min
Delta R.T.: 0.023 min
Response: 1534283
Conc: 0.09 ng/ml

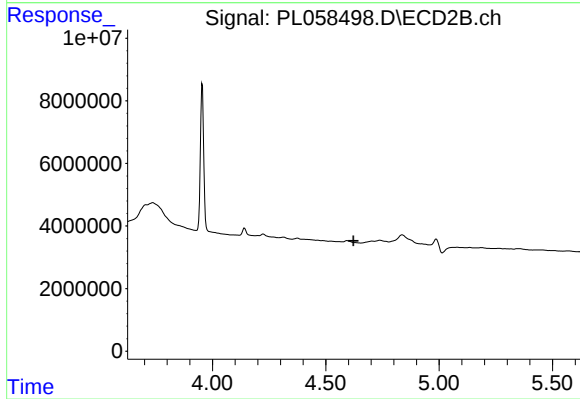

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.622 min
Response: 0
Conc: N.D.

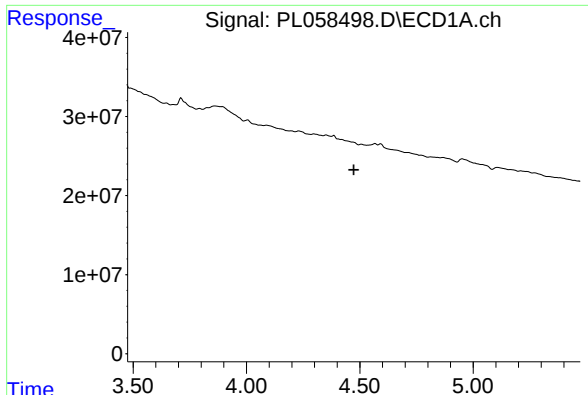

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AOC14-CARWASH

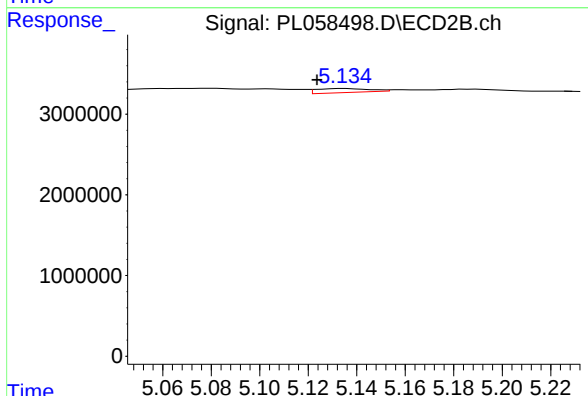


#4 Heptachlor

R.T.: 5.135 min
Delta R.T.: 0.012 min
Response: 761428
Conc: 0.22 ng/ml

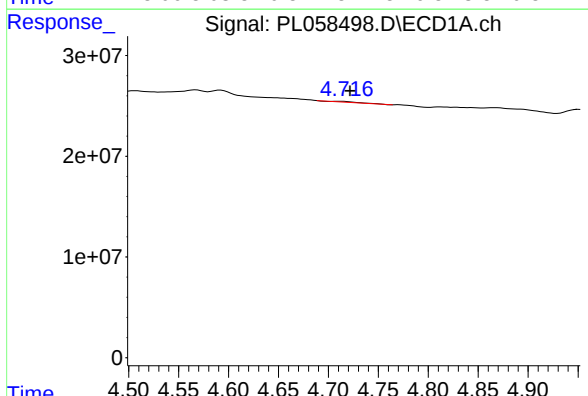


#5 Aldrin

R.T.: 4.715 min
Delta R.T.: -0.007 min
Response: 1314769
Conc: 0.08 ng/ml

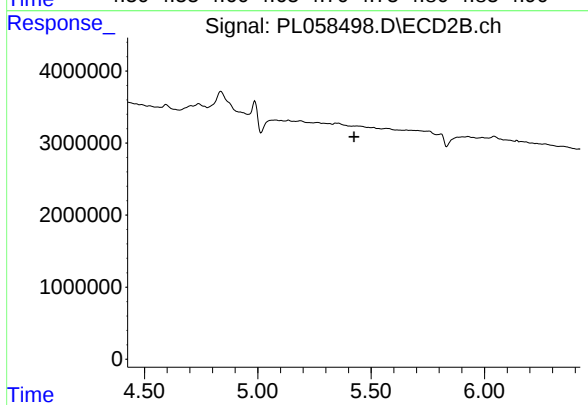

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.425 min
Response: 0
Conc: N.D.

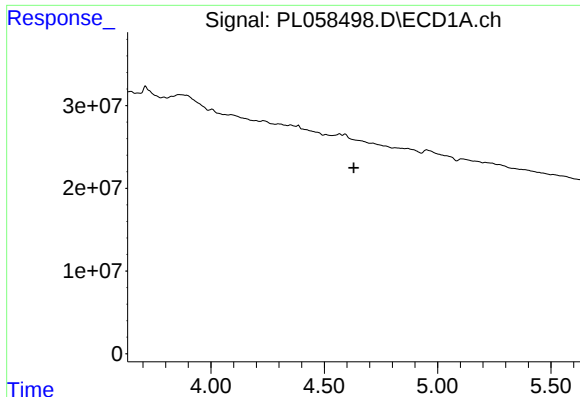

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.630 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AOC14-CARWASH

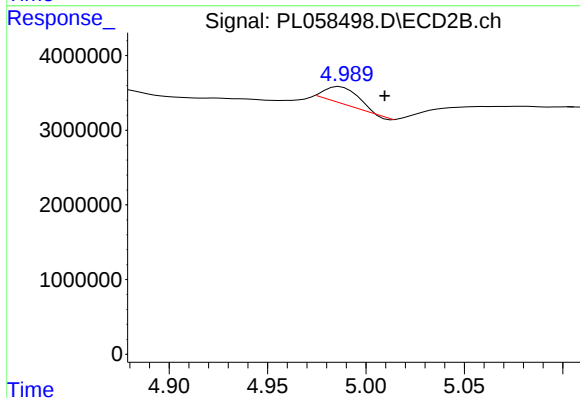


#7 delta-BHC

R.T.: 4.987 min
Delta R.T.: -0.023 min
Response: 2644505
Conc: 1.05 ng/ml

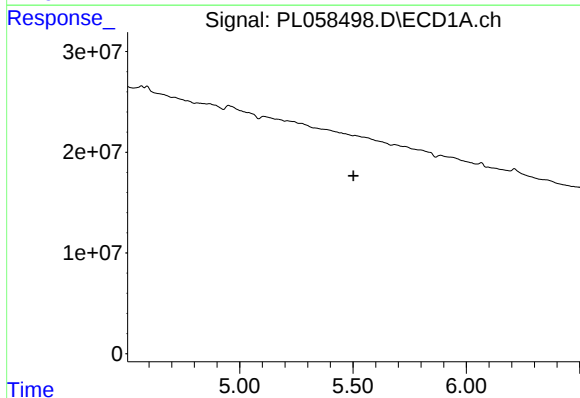


#9 Endosulfan I

R.T.: 5.509 min
Delta R.T.: 0.006 min
Response: -2224337
Conc: N.D.

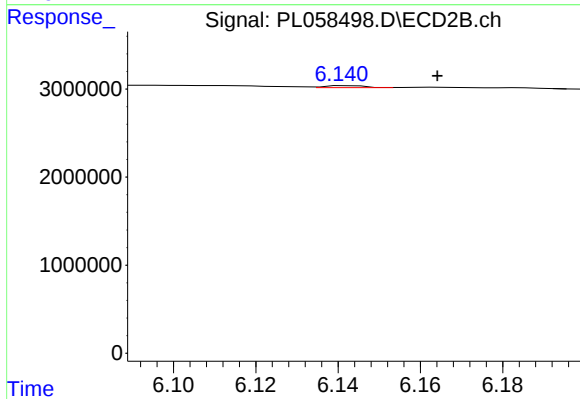

#9 Endosulfan I


R.T.: 6.142 min
Delta R.T.: -0.022 min
Response: 142462
Conc: 0.05 ng/ml

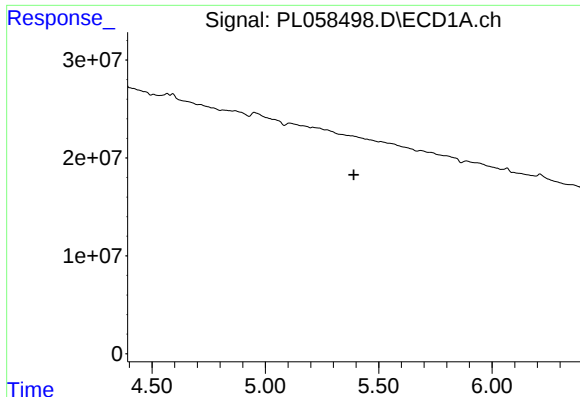

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AOC14-CARWASH

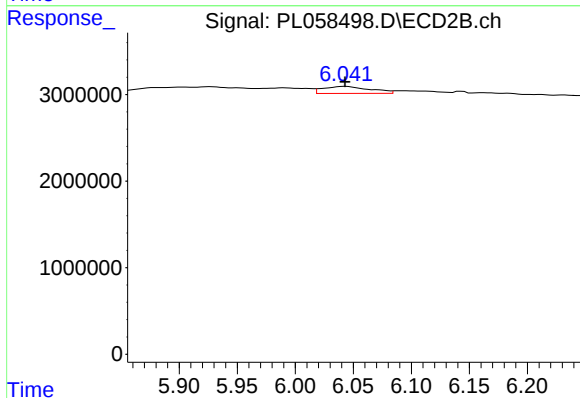


#10 gamma-Chlordane

R.T.: 6.043 min
Delta R.T.: 0.000 min
Response: 2248310
Conc: 0.67 ng/ml

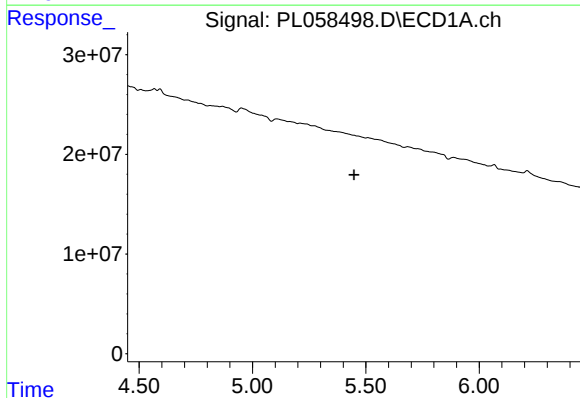


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.449 min
Response: 0
Conc: N.D.

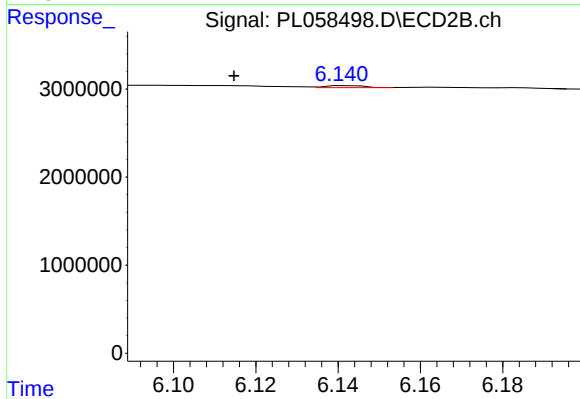

#11 alpha-Chlordane


R.T.: 6.142 min
Delta R.T.: 0.027 min
Response: 142462
Conc: 0.04 ng/ml

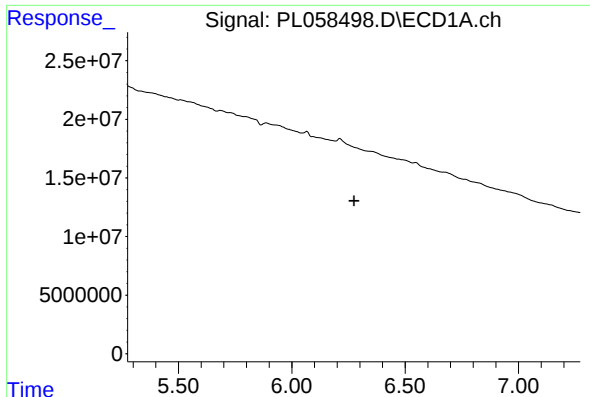

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AOC14-CARWASH

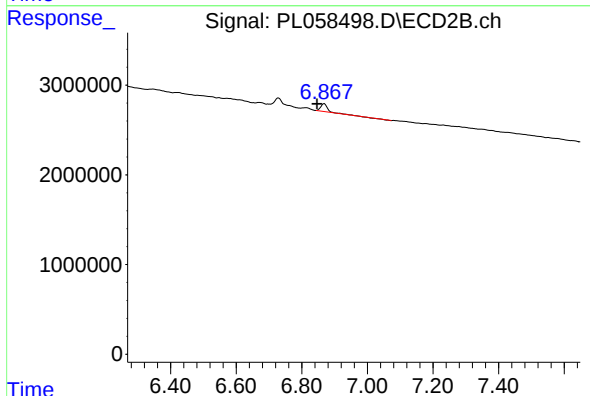


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.022 min
Response: 1301302
Conc: 0.49 ng/ml

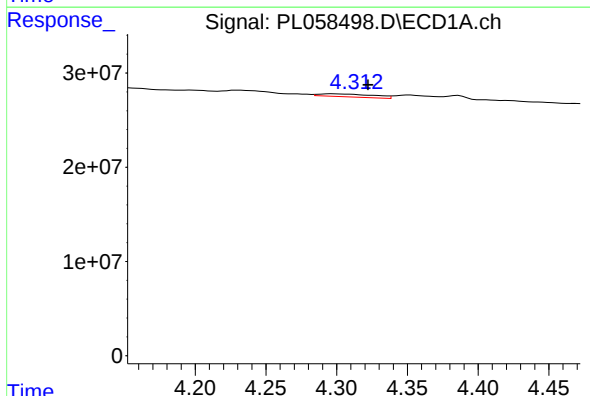


#23 Chlordane-1

R.T.: 4.297 min
Delta R.T.: -0.026 min
Response: 8136172
Conc: 18.93 ng/ml

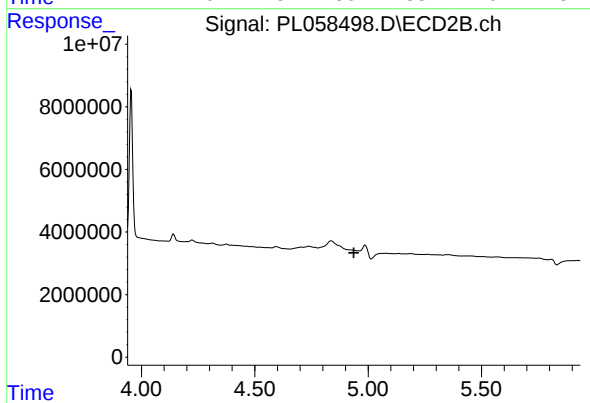

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.936 min
Response: 0
Conc: N.D.

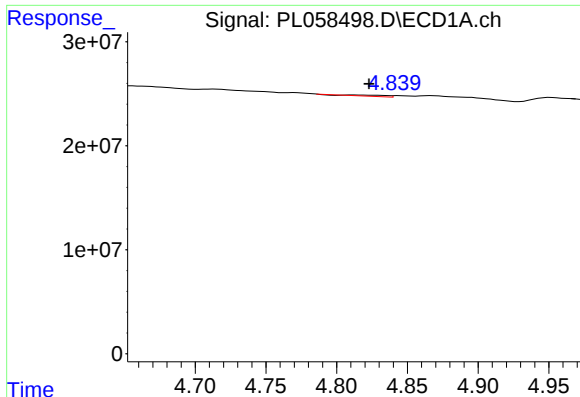

#24 Chlordane-2


R.T.: 4.813 min
Delta R.T.: -0.010 min
Response: 1956935
Conc: 4.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
AOC14-CARWASH

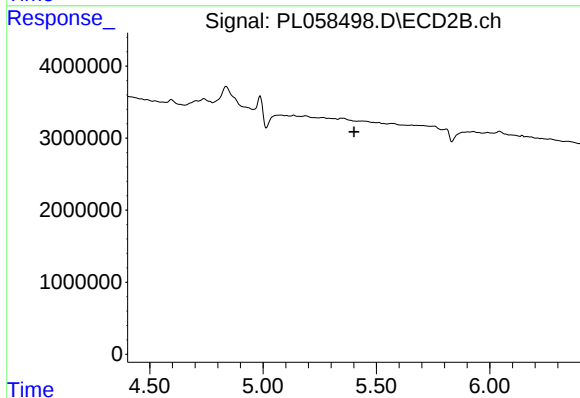


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

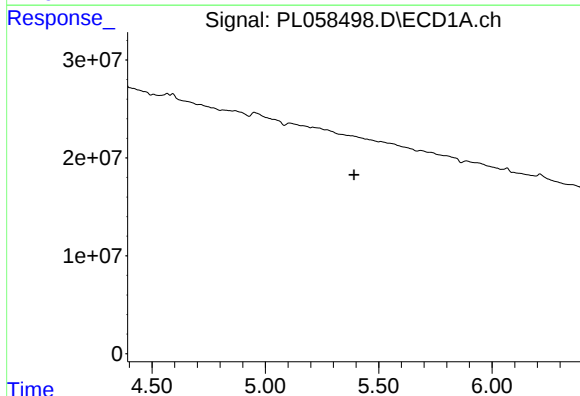


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.392 min
Response: 0
Conc: N.D.

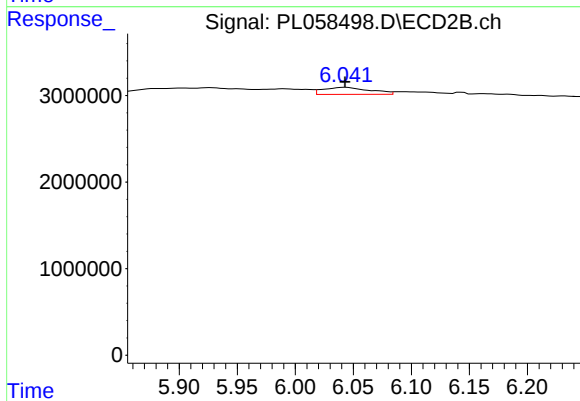

#25 Chlordane-3


R.T.: 6.043 min
Delta R.T.: 0.000 min
Response: 2248310
Conc: 5.62 ng/ml

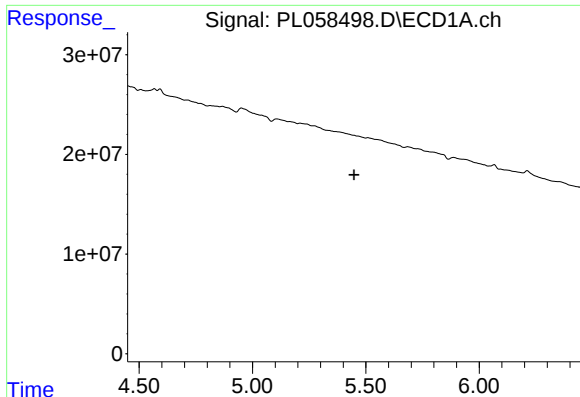

#26 Chlorine-4


R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AOC14-CARWASH

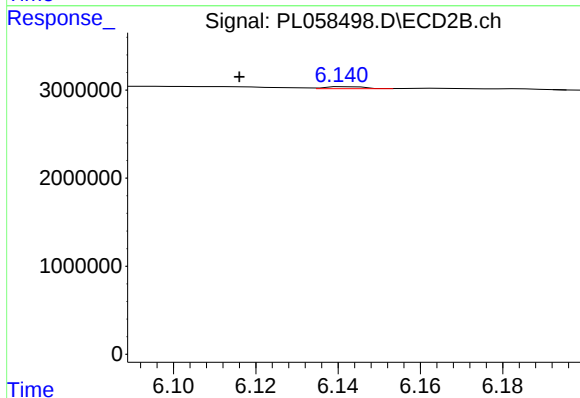


#26 Chlorine-4

R.T.: 6.142 min
Delta R.T.: 0.026 min
Response: 142462
Conc: 0.29 ng/ml

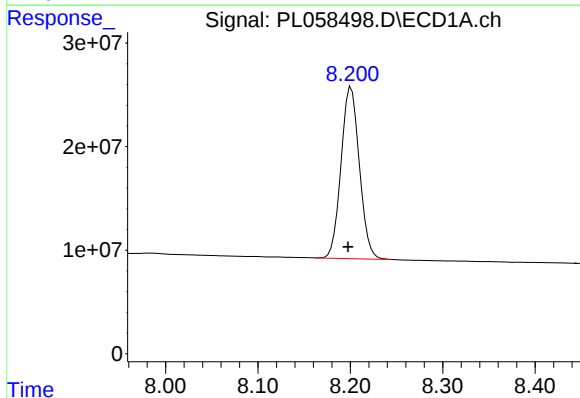

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.004 min
Response: 228321129
Conc: 21.11 ng/ml

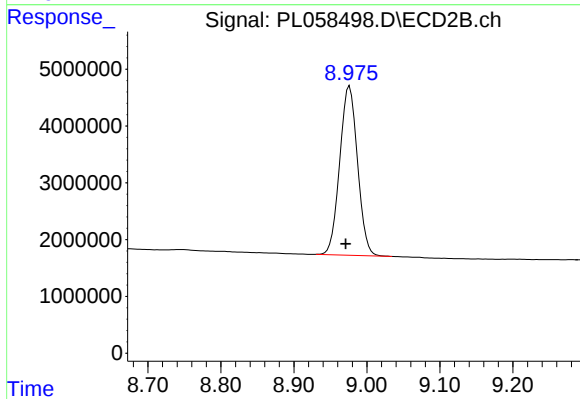

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.005 min
Response: 50433914
Conc: 22.73 ng/ml