

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050120\
 Data File : PL058496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2020 18:00
 Operator : AJ\MA
 Sample : L2452-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 227

Manual Integrations
 APPROVED

mohammad
 5/4/2020 12:33:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 00:43:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 29 00:55:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.454	3.955	210.8E6	47311647	19.811m	21.889
28)	SA Decachlor...	8.201	8.976	209.7E6	46365231	19.390	20.896

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050120\
Data File : PL058496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2020 18:00
Operator : AJ\MA
Sample : L2452-06
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
227


Manual Integrations
APPROVED

mohammad
5/4/2020 12:33:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 00:43:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
Quant Title : GC Extractables
QLast Update : Wed Apr 29 00:55:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

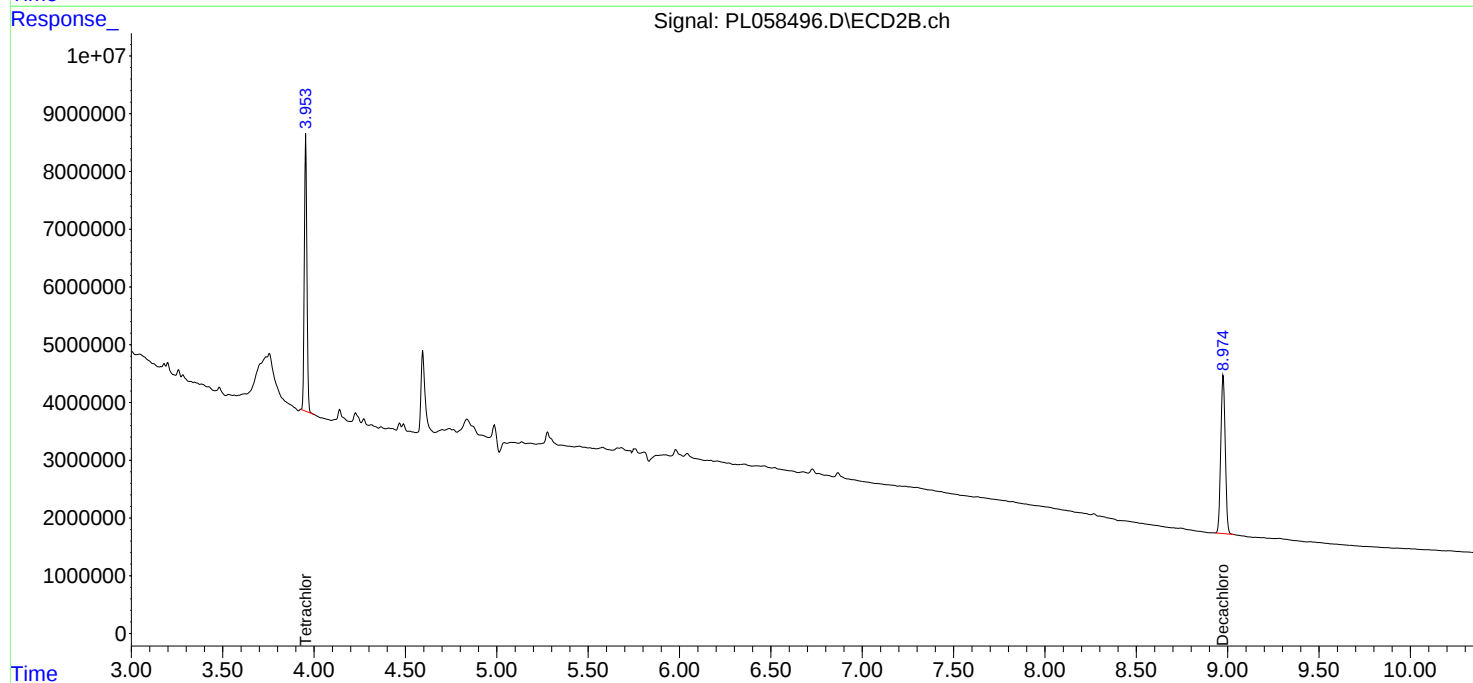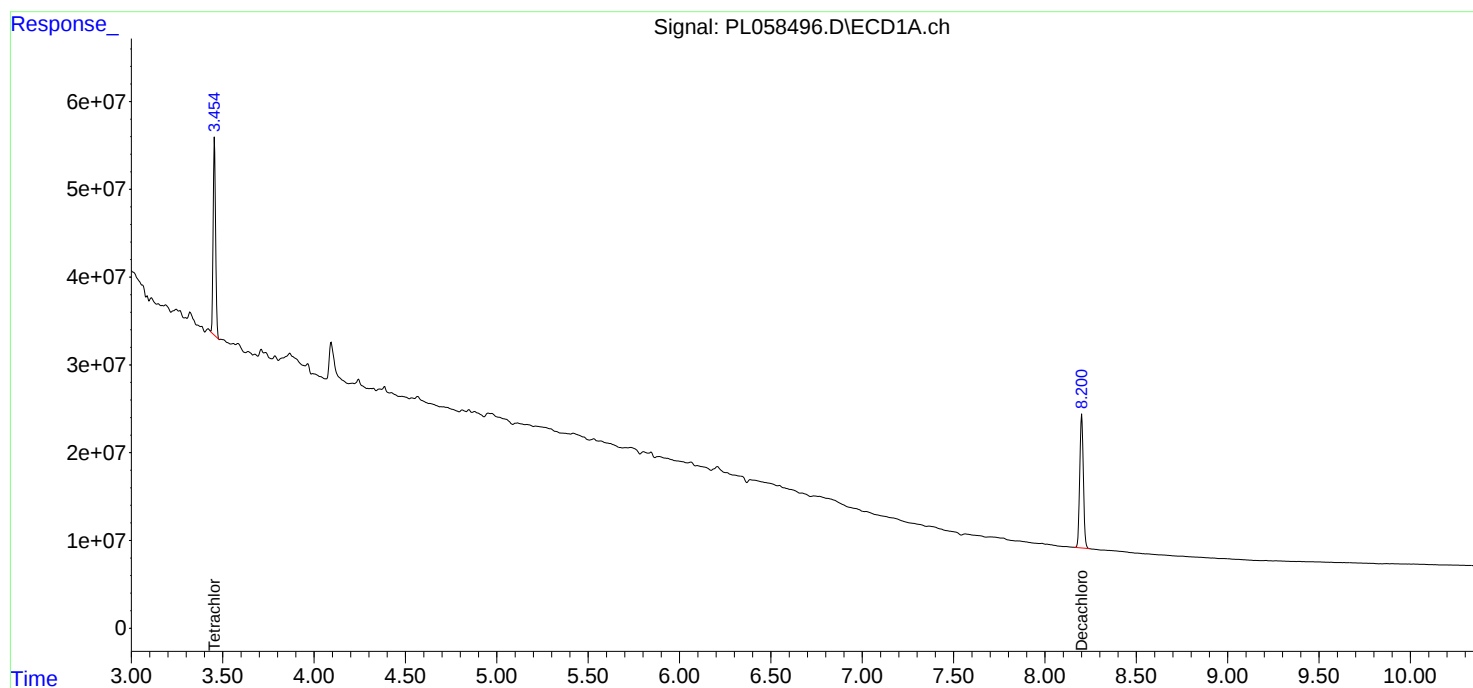

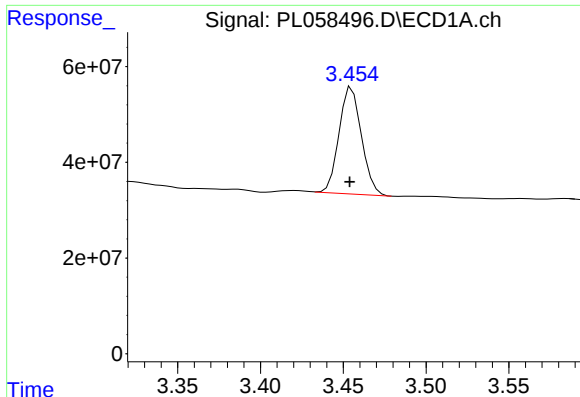


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: 0.000 min
Response: 210824885
Conc: 19.81 ng/ml m

Instrument :
ECD_L
ClientSampleId :
227


Manual Integrations
APPROVED

mohammad
5/4/2020 12:33:06 PM

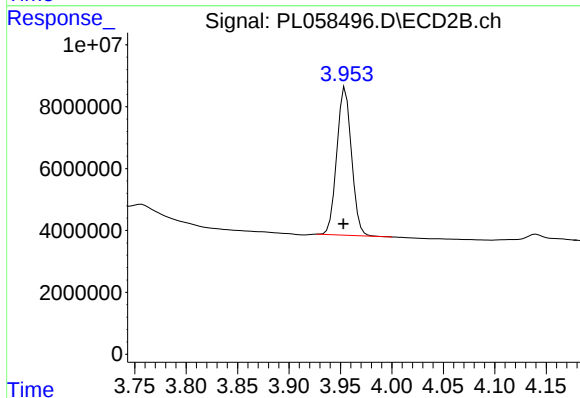


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: 0.002 min
Response: 47311647
Conc: 21.89 ng/ml

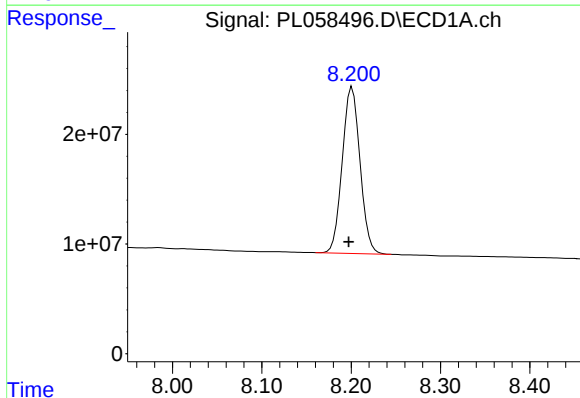

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.004 min
Response: 209694359
Conc: 19.39 ng/ml

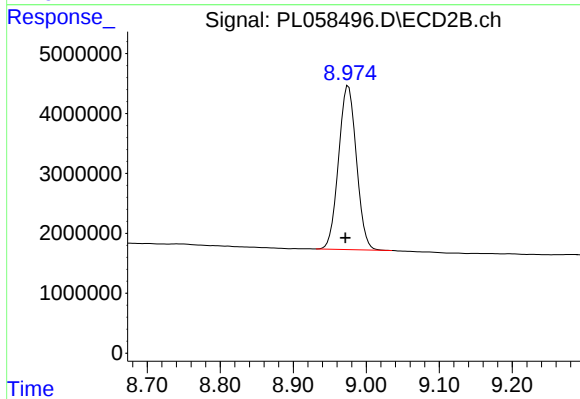

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.004 min
Response: 46365231
Conc: 20.90 ng/ml