

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050123\
 Data File : PL082403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 11:27
 Operator : AR\AJ
 Sample : 02503-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-305A-COMP-02

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/02/2023
 Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 13:51:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.325	2.646	34222295	28003980	12.812	12.088
28) SA Decachlor...	8.752	7.762	28517773	30919476	14.938m	13.546

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050123\
Data File : PL082403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 11:27
Operator : AR\AJ
Sample : 02503-08
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-305A-COMP-02


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/02/2023
Supervised By : Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 13:51:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

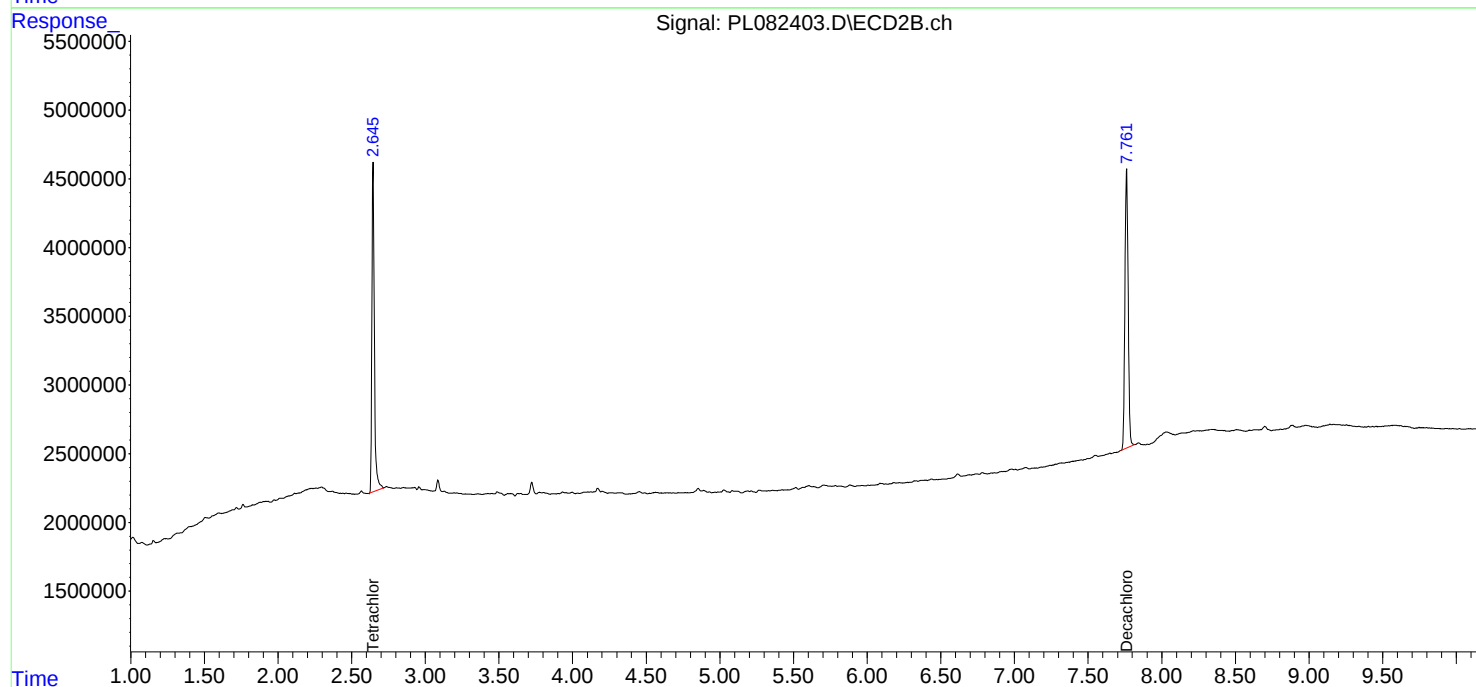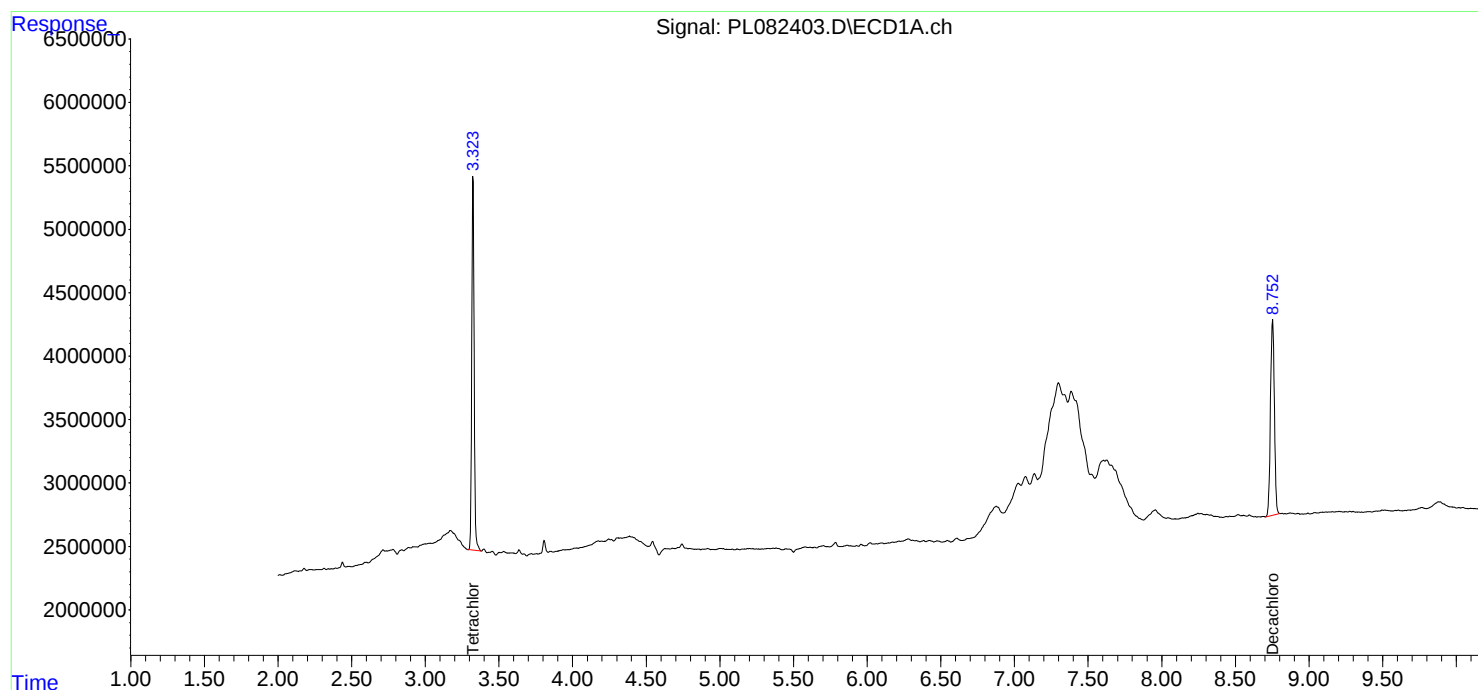

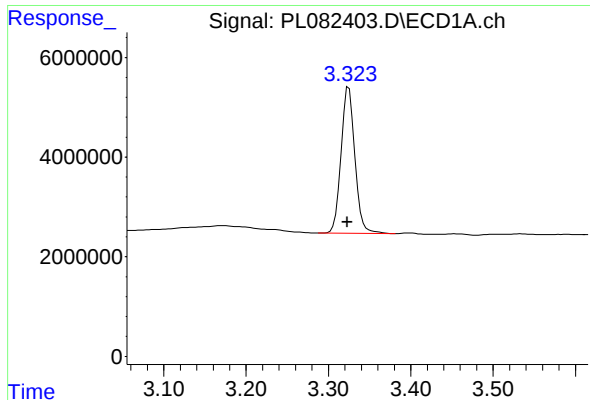


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: 0.002 min
Response: 34222295
Conc: 12.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-305A-COMP-02


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

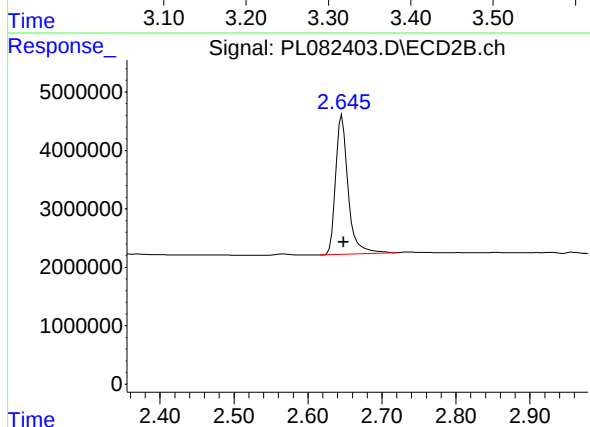


#1 Tetrachloro-m-xylene

R.T.: 2.646 min
Delta R.T.: -0.002 min
Response: 28003980
Conc: 12.09 ng/ml

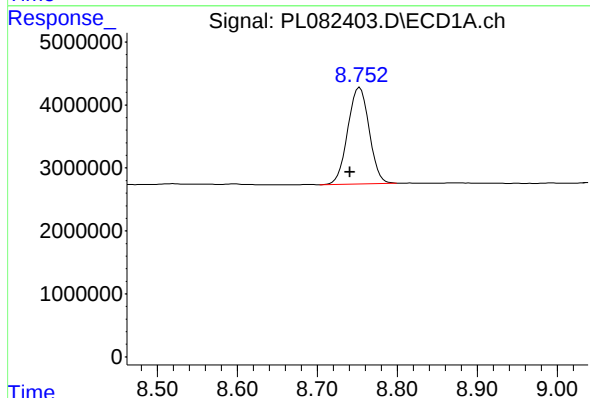

#28 Decachlorobiphenyl

R.T.: 8.752 min
Delta R.T.: 0.011 min
Response: 28517773
Conc: 14.94 ng/ml m

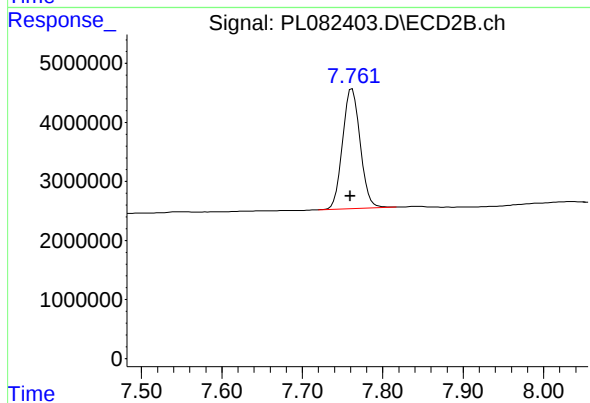

#28 Decachlorobiphenyl

R.T.: 7.762 min
Delta R.T.: 0.002 min
Response: 30919476
Conc: 13.55 ng/ml