

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050123\
 Data File : PL082409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 14:40
 Operator : AR\AJ
 Sample : 02555-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OE-1-042823

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 21:25:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.324	2.645	27984835	23578686	10.476	10.178
28) SA Decachlor...	8.748	7.759	23946623	24545839	12.544	10.754
Target Compounds						
12) B 4,4'-DDE	5.957	5.083	1425782	1114291	0.561	0.485



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050123\
Data File : PL082409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 14:40
Operator : AR\AJ
Sample : 02555-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OE-1-042823

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 21:25:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

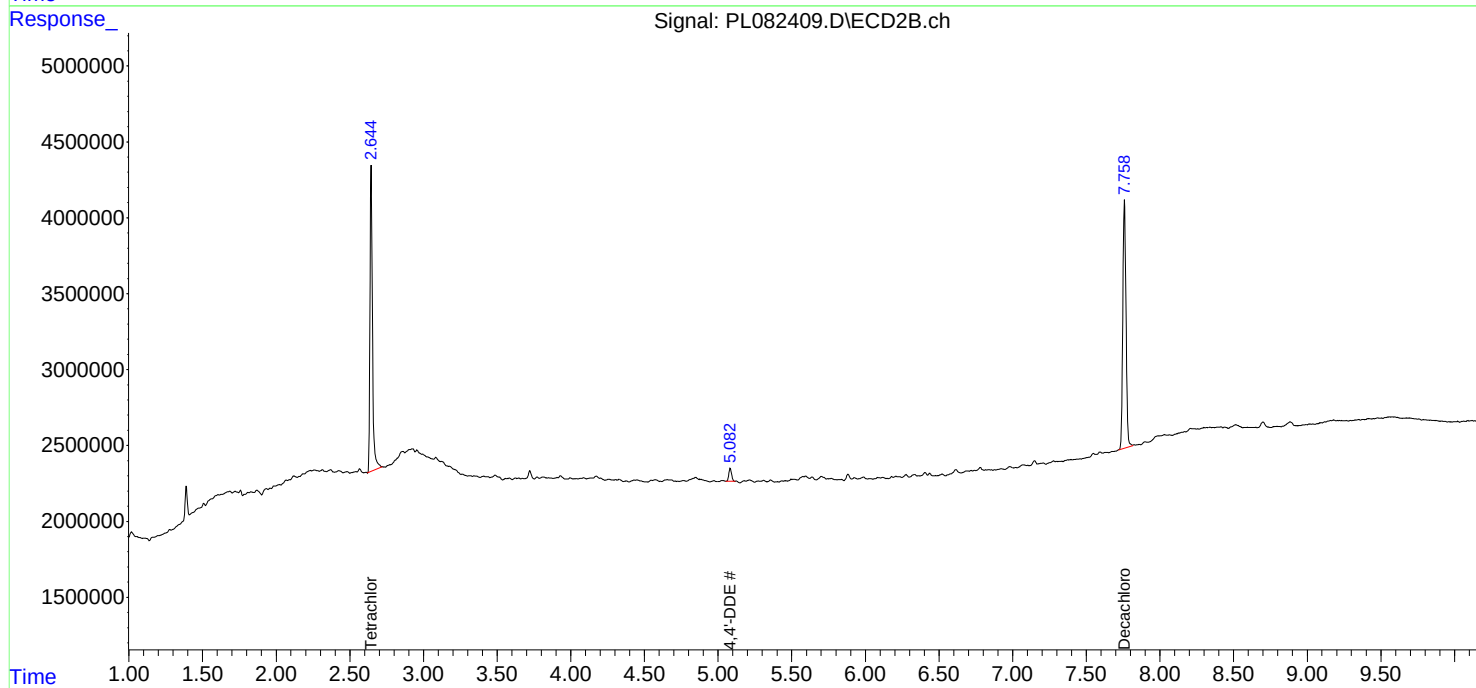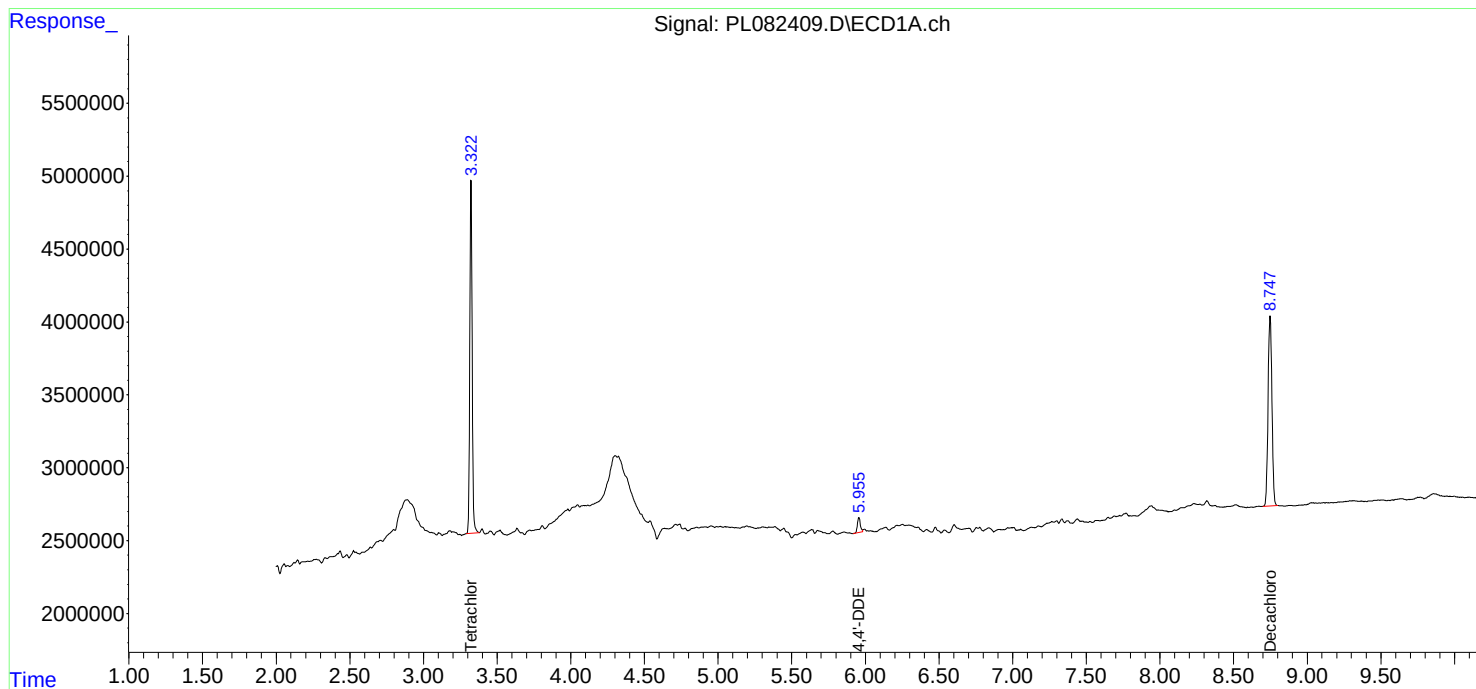


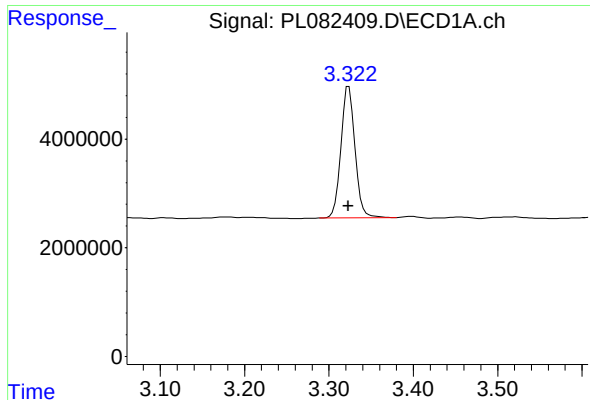

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 27984835
Conc: 10.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
OE-1-042823

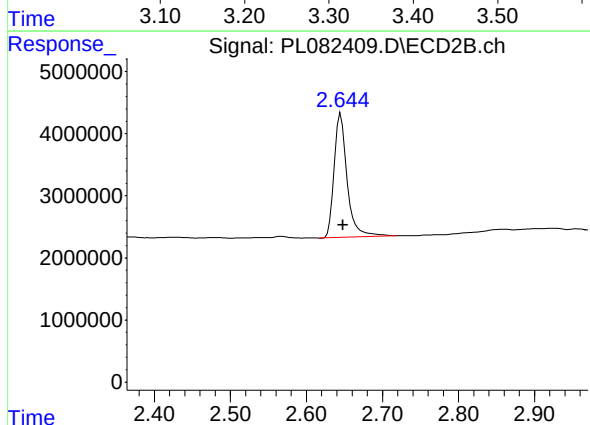


#1 Tetrachloro-m-xylene

R.T.: 2.645 min
Delta R.T.: -0.003 min
Response: 23578686
Conc: 10.18 ng/ml

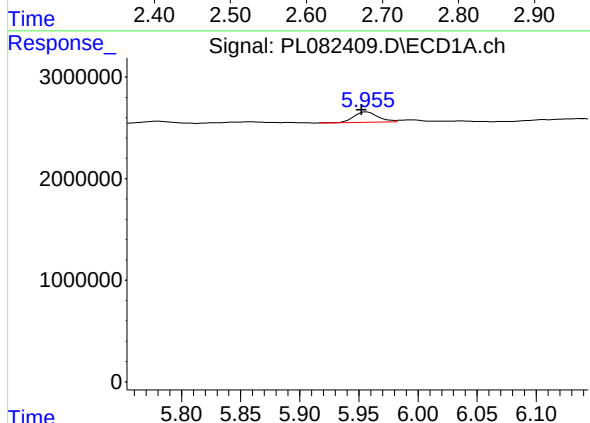


#12 4,4'-DDE

R.T.: 5.957 min
Delta R.T.: 0.004 min
Response: 1425782
Conc: 0.56 ng/ml

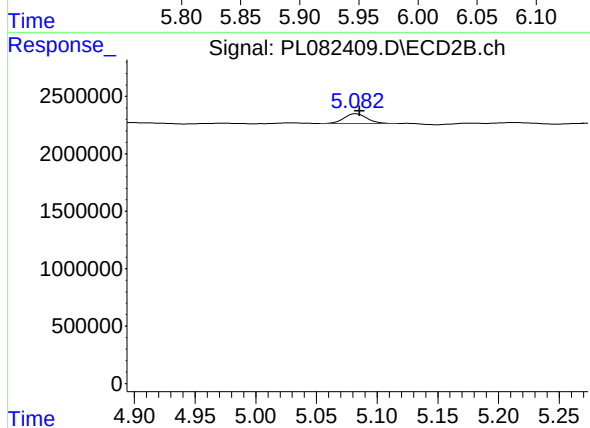

#12 4,4'-DDE


R.T.: 5.083 min
Delta R.T.: -0.002 min
Response: 1114291
Conc: 0.48 ng/ml

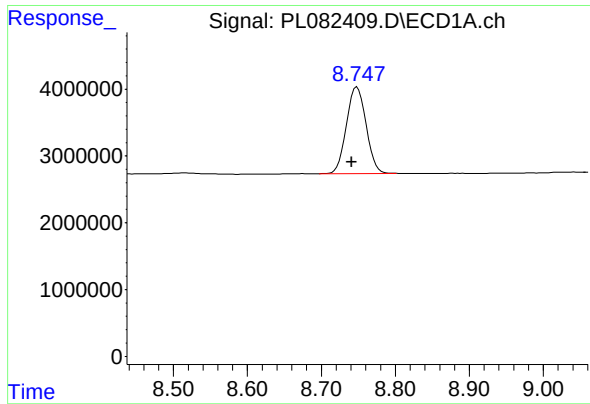

#28 Decachlorobiphenyl

R.T.: 8.748 min
Delta R.T.: 0.007 min
Response: 23946623
Conc: 12.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
OE-1-042823

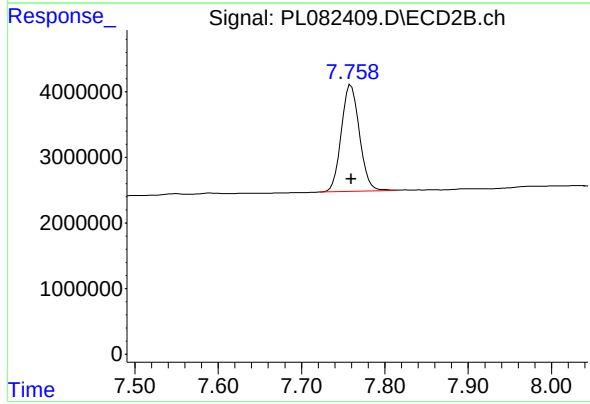

#28 Decachlorobiphenyl

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 24545839
Conc: 10.75 ng/ml