

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050123\
 Data File : PL082412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 15:22
 Operator : AR\AJ
 Sample : 02558-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P001-SS011-0006-02

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/02/2023
 Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 21:27:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.321	2.646	17183725	18408035	6.433m	7.946
28) SA Decachlor...	8.745	7.759	21377027	20503196	11.198	8.983

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050123\
Data File : PL082412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 15:22
Operator : AR\AJ
Sample : 02558-04
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
P001-SS011-0006-02


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/02/2023
Supervised By : Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 21:27:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

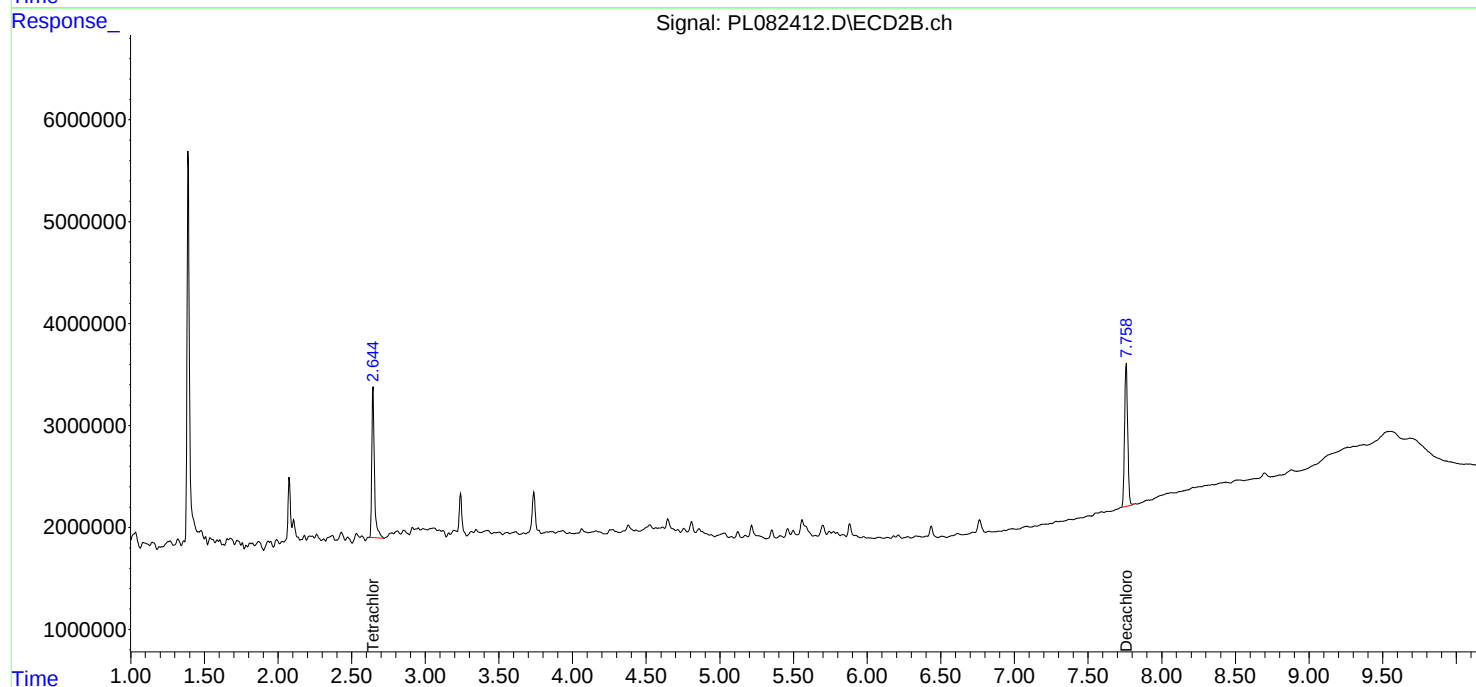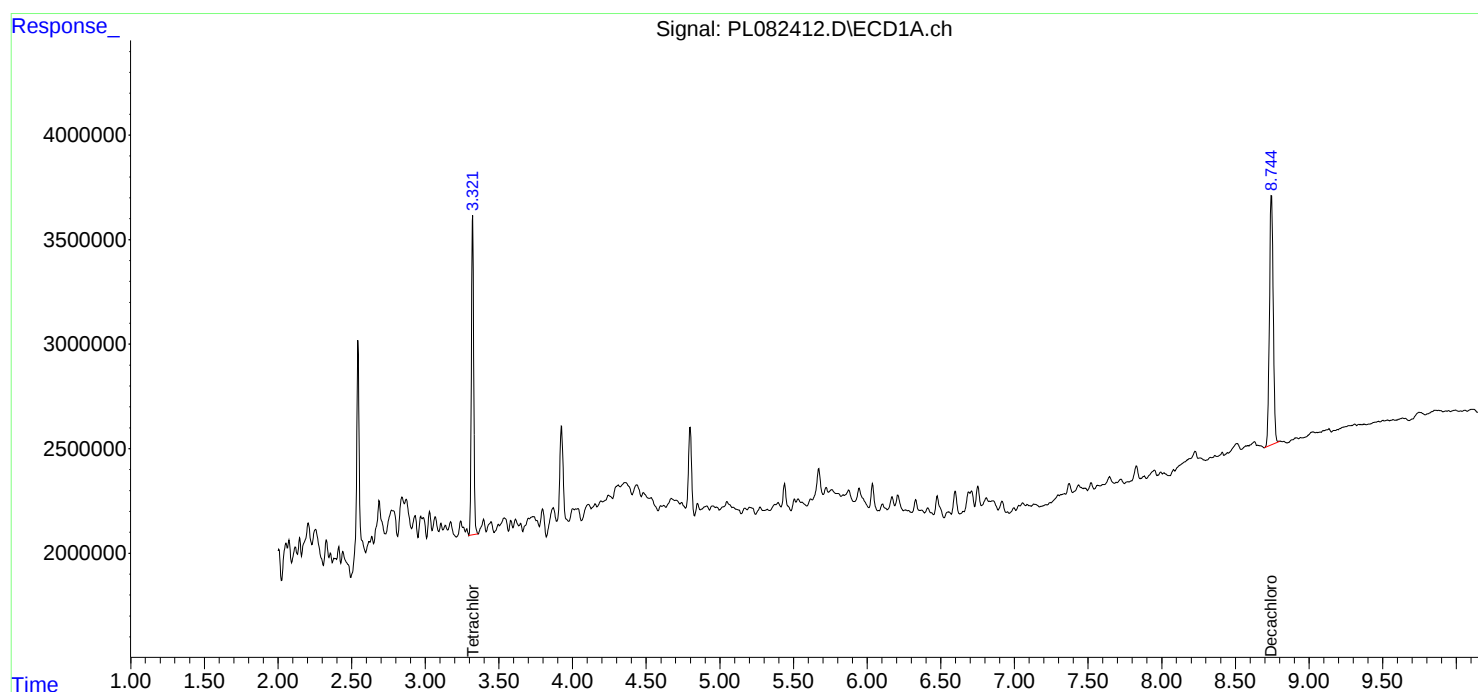

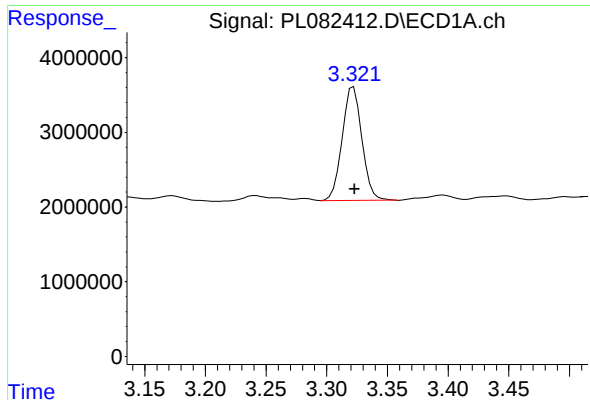


#1 Tetrachloro-m-xylene

R.T.: 3.321 min
Delta R.T.: -0.002 min
Response: 17183725
Conc: 6.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
P001-SS011-0006-02


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

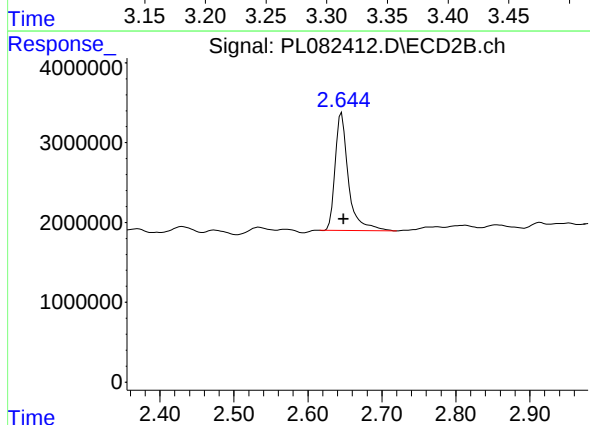


#1 Tetrachloro-m-xylene

R.T.: 2.646 min
Delta R.T.: -0.003 min
Response: 18408035
Conc: 7.95 ng/ml

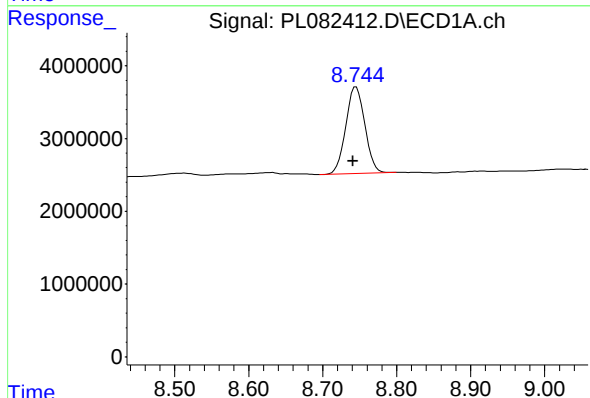

#28 Decachlorobiphenyl

R.T.: 8.745 min
Delta R.T.: 0.004 min
Response: 21377027
Conc: 11.20 ng/ml

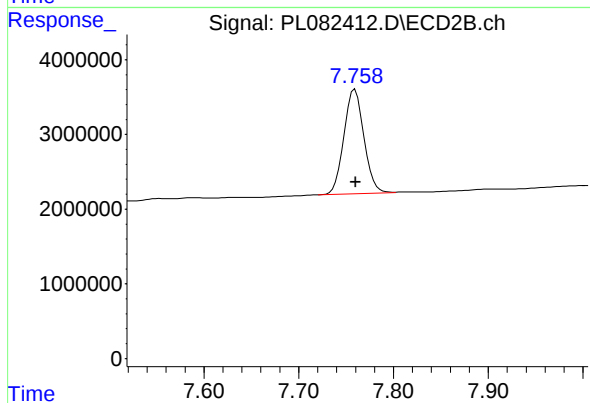

#28 Decachlorobiphenyl

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 20503196
Conc: 8.98 ng/ml