

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050123\
 Data File : PL082416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 16:18
 Operator : AR\AJ
 Sample : 02558-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P001-SS013-1218-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 21:30:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	2.646	50961225	43702634	19.078	18.864
28) SA Decachlor...	8.745	7.758	32450637	35188821	16.998	15.417

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050123\
Data File : PL082416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 16:18
Operator : AR\AJ
Sample : 02558-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
P001-SS013-1218-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 21:30:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

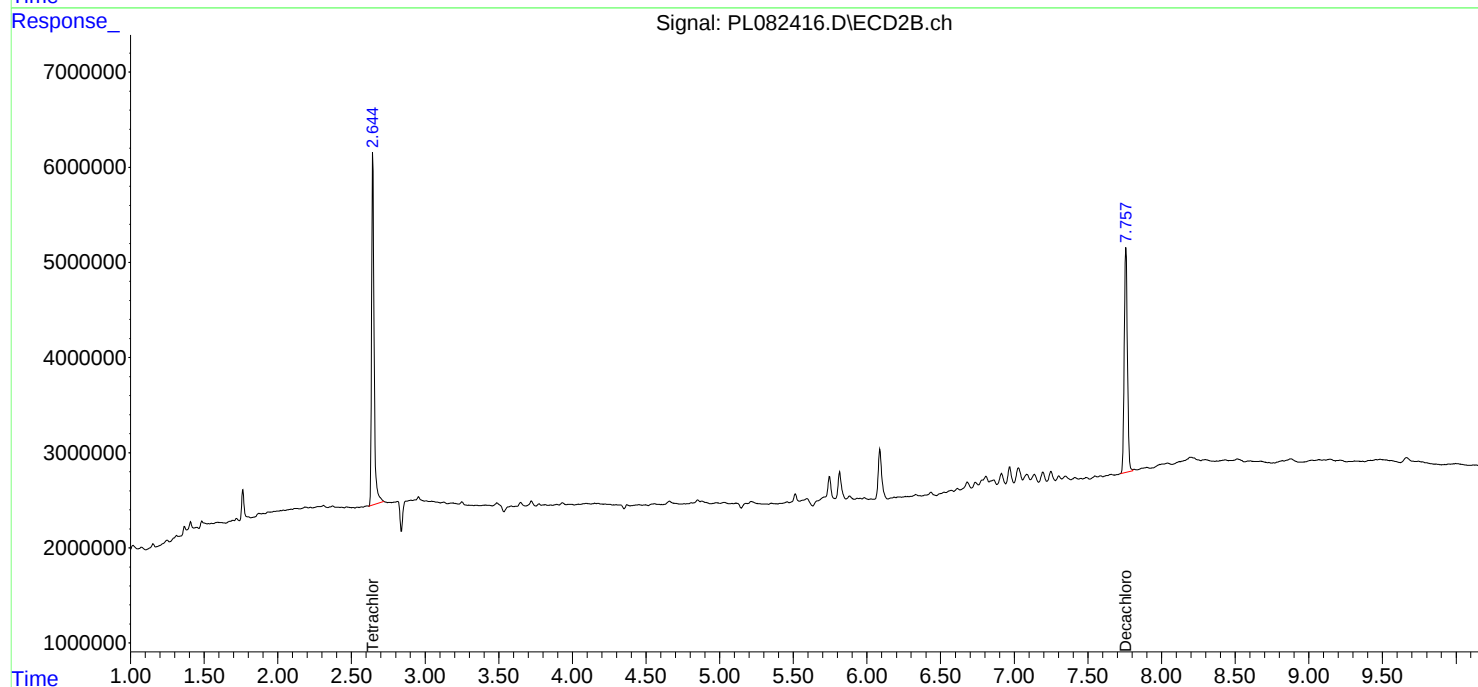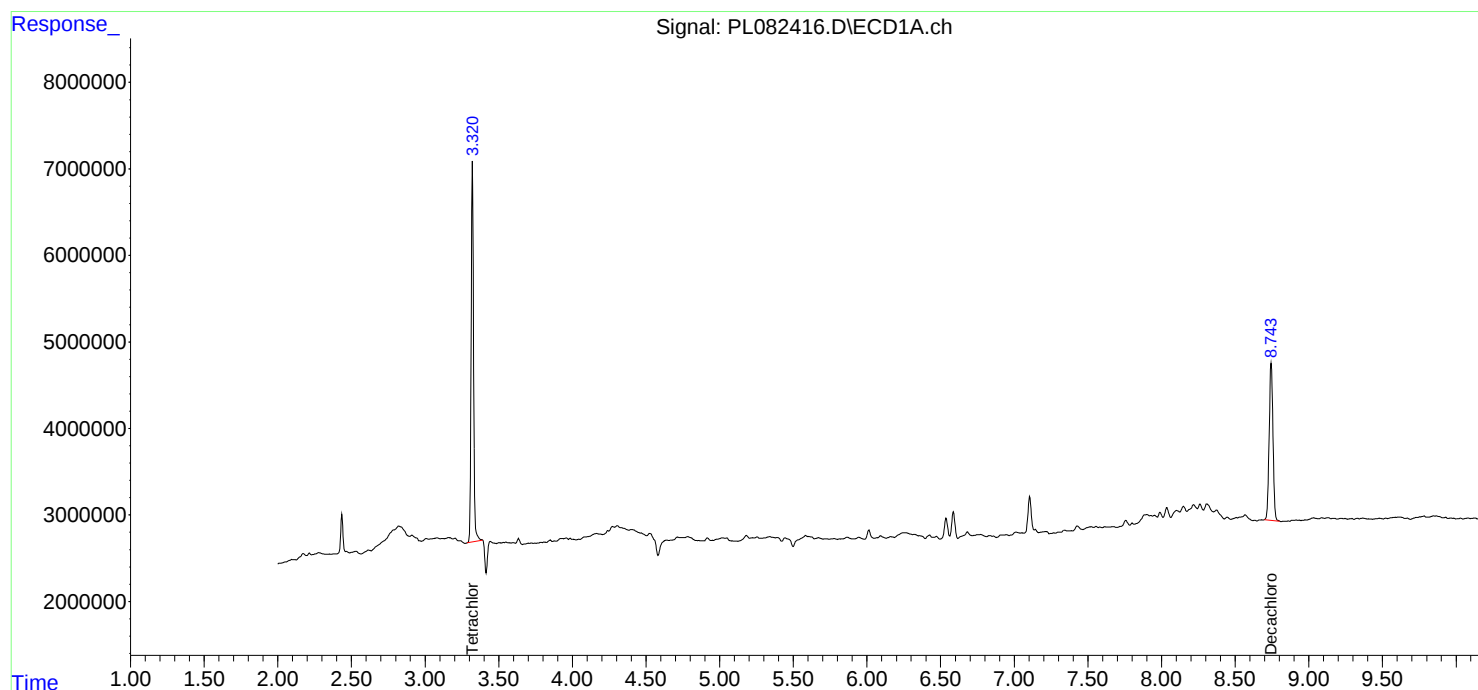


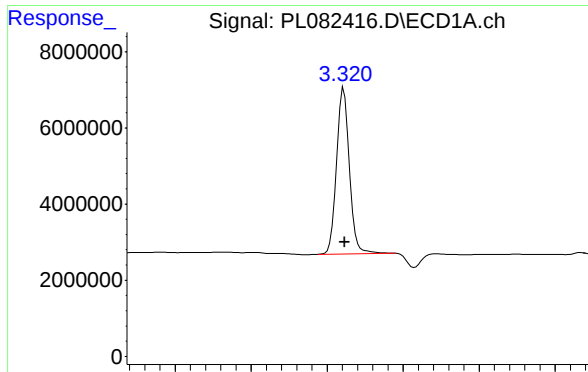

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.001 min
Response: 50961225
Conc: 19.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
P001-SS013-1218-01

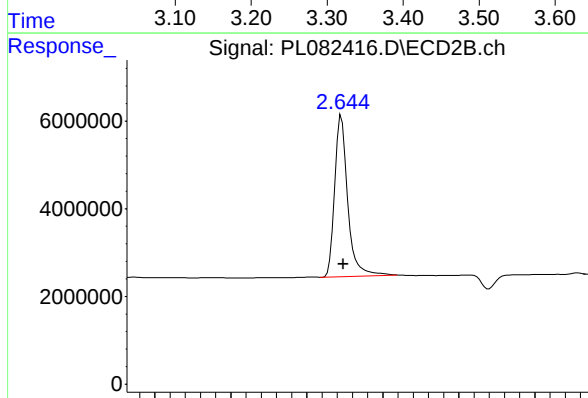


#1 Tetrachloro-m-xylene

R.T.: 2.646 min
Delta R.T.: -0.003 min
Response: 43702634
Conc: 18.86 ng/ml

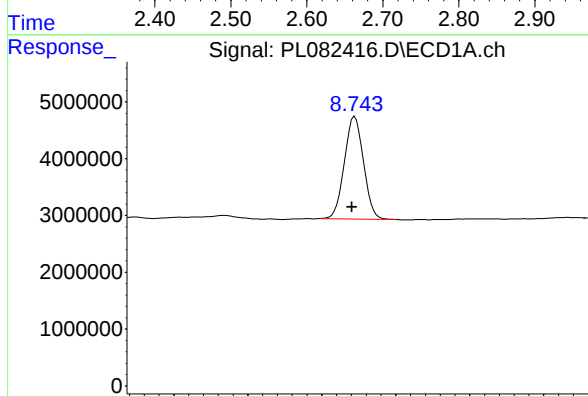

#28 Decachlorobiphenyl

R.T.: 8.745 min
Delta R.T.: 0.004 min
Response: 32450637
Conc: 17.00 ng/ml

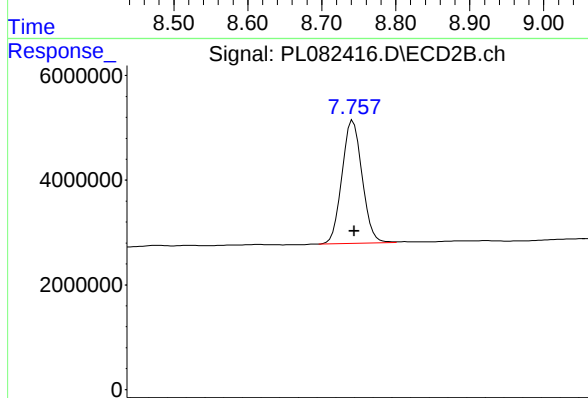

#28 Decachlorobiphenyl

R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 35188821
Conc: 15.42 ng/ml