

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050123\
 Data File : PL082420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 17:42
 Operator : AR\AJ
 Sample : 02558-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P001-SS011-0006-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/02/2023
 Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 21:34:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.319	2.644	2507226	3253755	0.939m	1.404m#
28) SA Decachlor...	8.743	7.758	3025650	2599301	1.585m	1.139 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050123\
Data File : PL082420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 17:42
Operator : AR\AJ
Sample : 02558-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
P001-SS011-0006-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/02/2023
Supervised By : Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 21:34:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

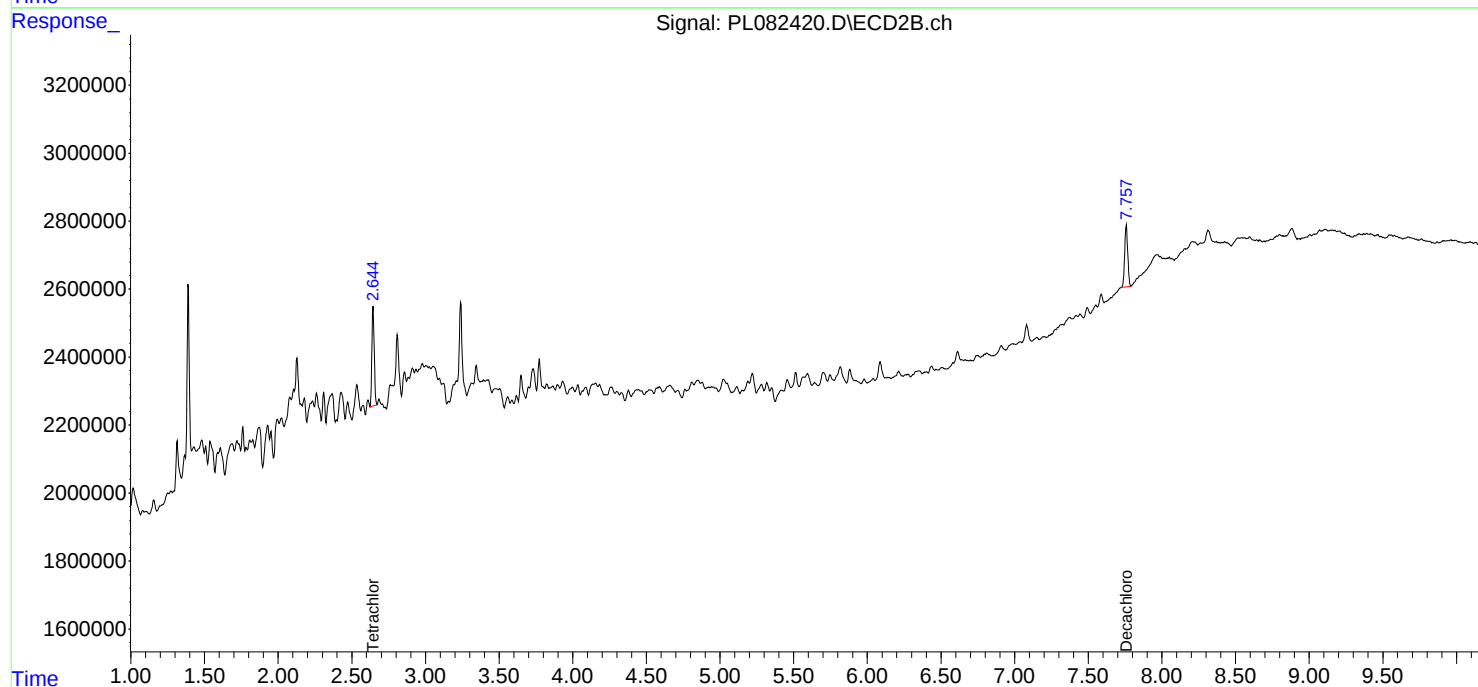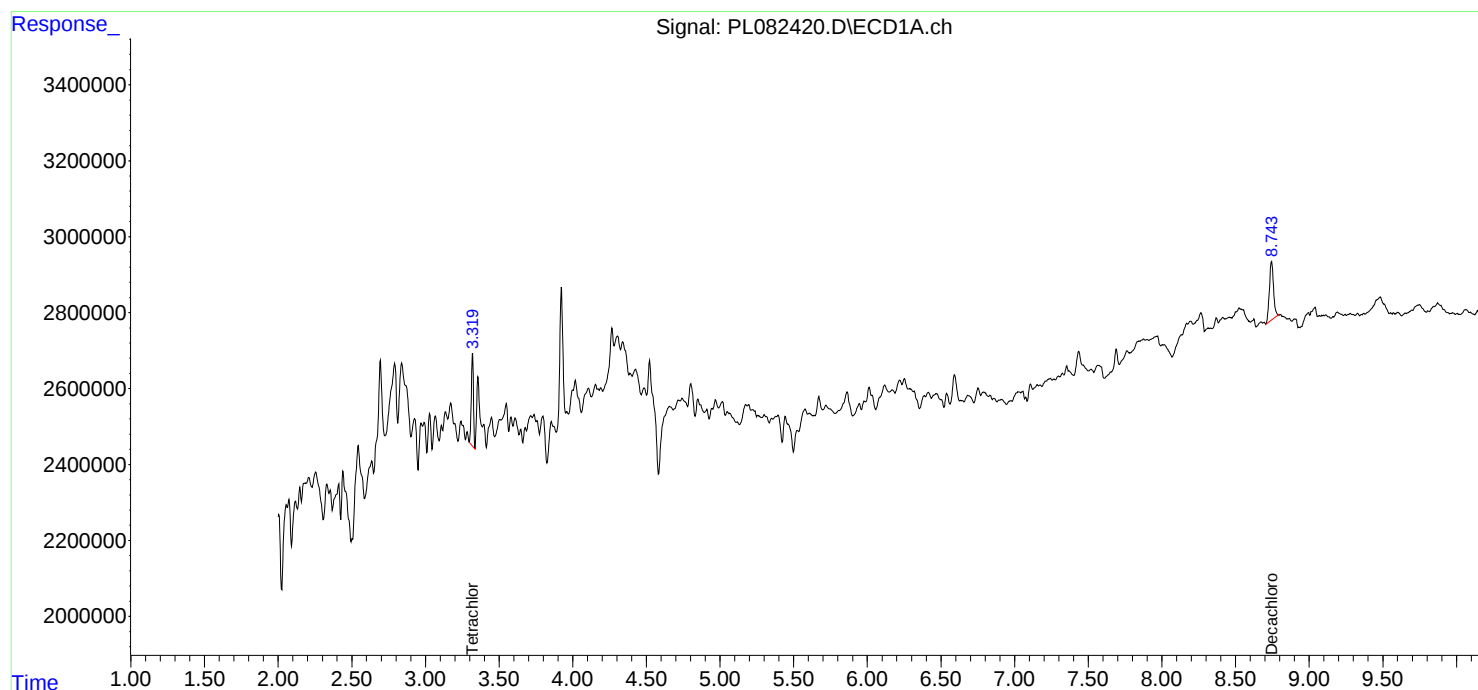

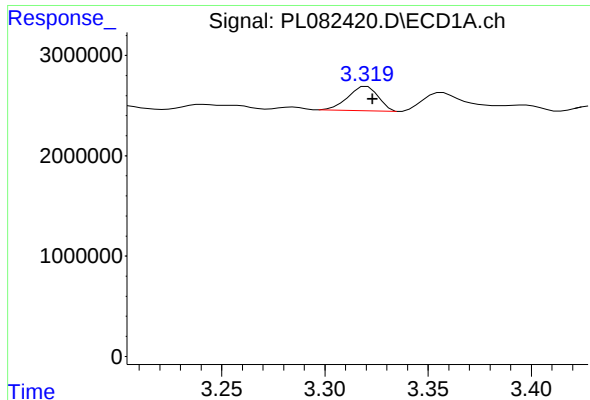


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: -0.004 min
Response: 2507226
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
P001-SS011-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

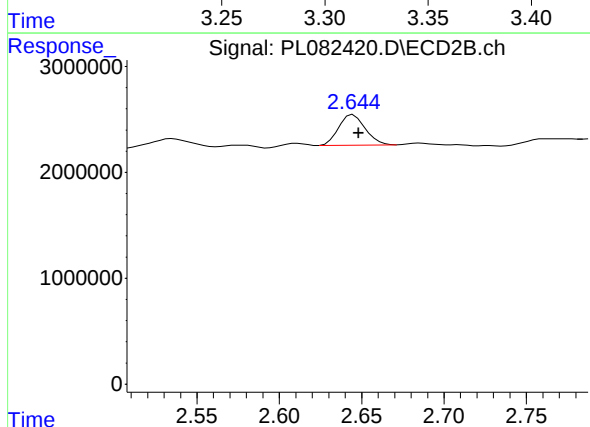


#1 Tetrachloro-m-xylene

R.T.: 2.644 min
Delta R.T.: -0.005 min
Response: 3253755
Conc: 1.40 ng/ml m

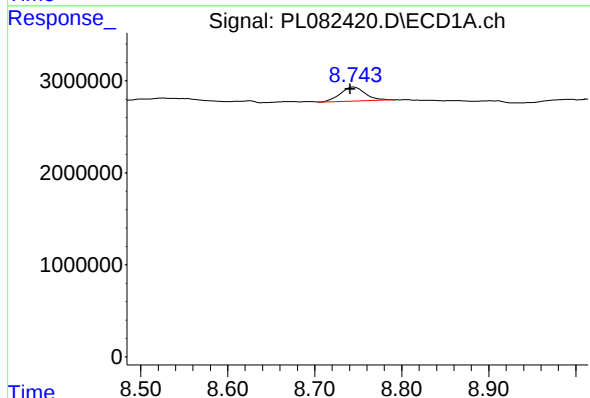

#28 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.002 min
Response: 3025650
Conc: 1.58 ng/ml m

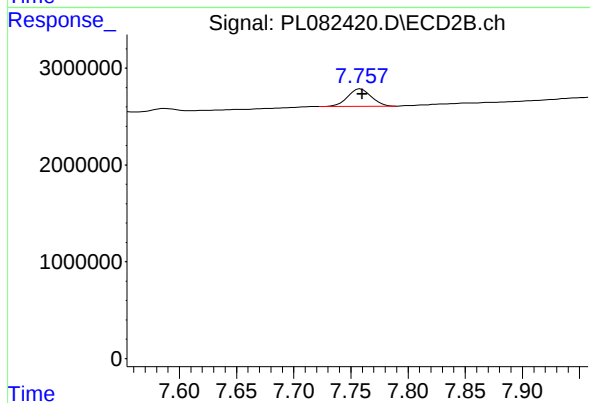

#28 Decachlorobiphenyl

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 2599301
Conc: 1.14 ng/ml