

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050219\
 Data File : PL048145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2019 17:48
 Operator : AJ\SJ
 Sample : K2653-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MR-SUMP-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 01:01:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	172.5E6	46456327	17.807	18.651
28)	SA Decachlor...	7.997	8.977	124.4E6	33207728	12.376	12.511
Target Compounds							
3)	MA gamma-BHC...	4.039	0.000	47037628	0	3.310	N.D. #
7)	B delta-BHC	0.000	4.975f	0	7505428	N.D.	2.654 #
9)	A Endosulfan I	5.342f	0.000	2334022	0	0.194	N.D. #
11)	B alpha-Chl...	5.281	0.000	4197641	0	0.321	N.D. #
13)	MA Dieldrin	5.550	0.000	5110106	0	0.392	N.D. #
19)	B Endosulfa...	0.000	7.161f	0	9239131	N.D.	3.570 #
20)	A Methoxychlor	6.703f	0.000	7494141	0	1.376	N.D. #
26)	Chlordane-4	5.281	0.000	4197641	0	2.891	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050219\
Data File : PL048145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2019 17:48
Operator : AJ\SJ
Sample : K2653-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MR-SUMP-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 01:01:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

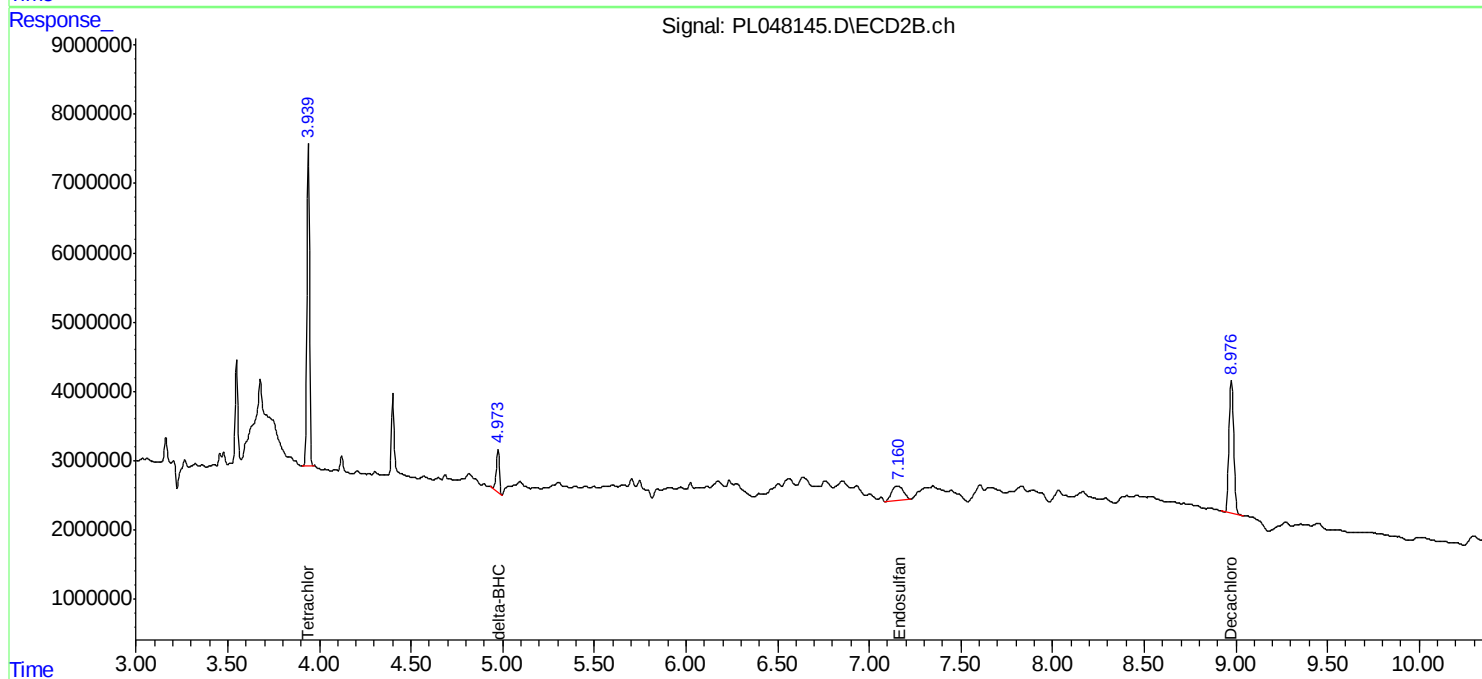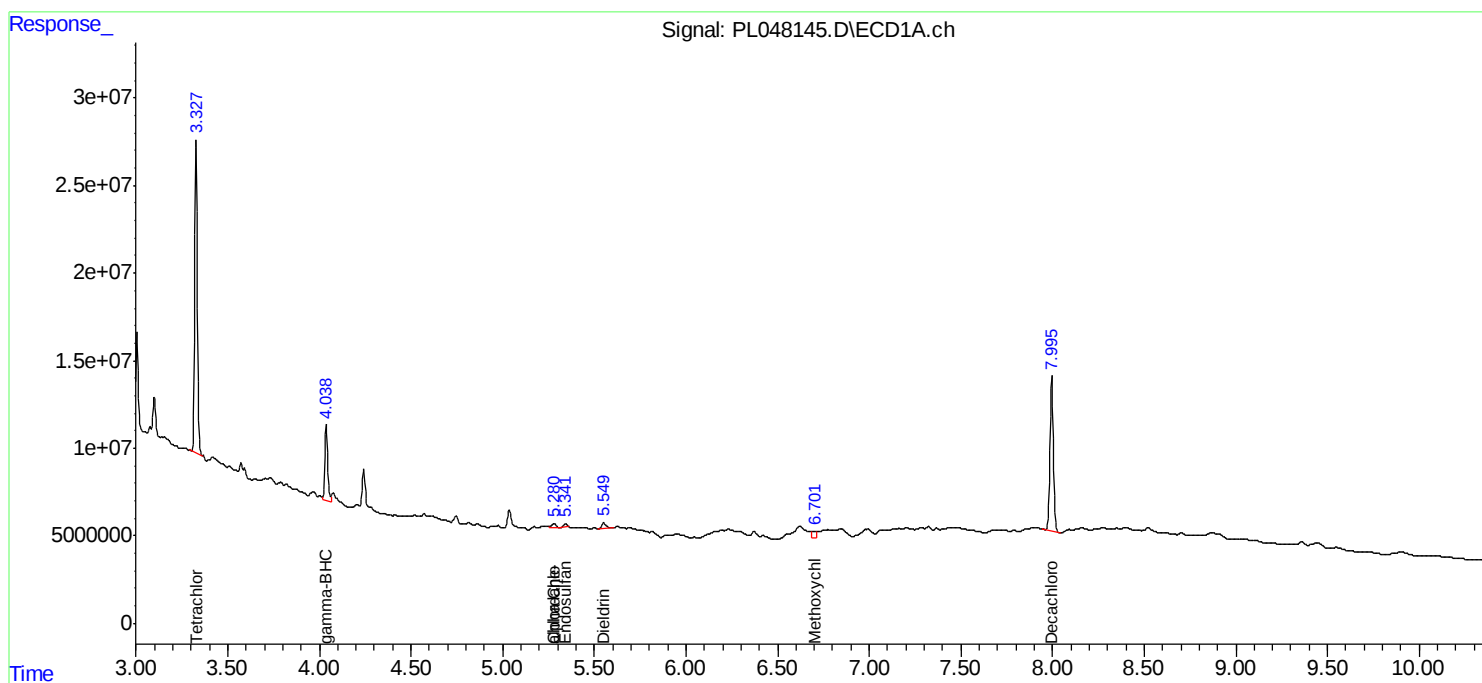


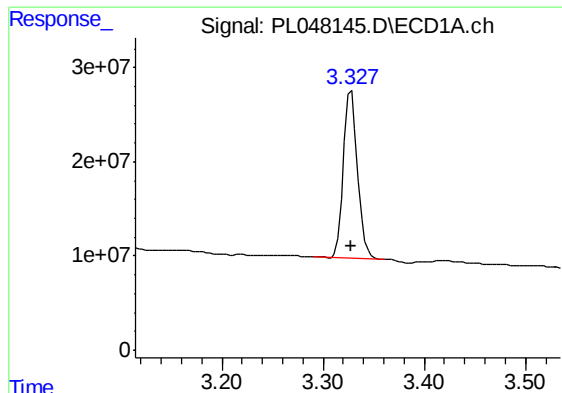

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 172492218
Conc: 17.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
MR-SUMP-PIT

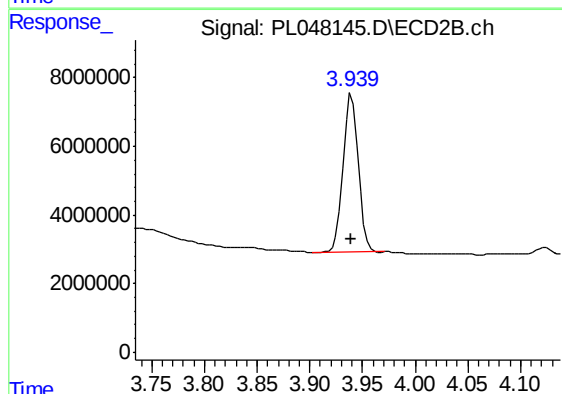


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 46456327
Conc: 18.65 ng/ml

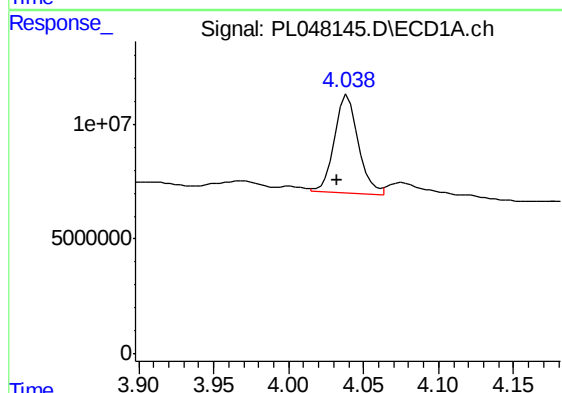


#3 gamma-BHC (Lindane)

R.T.: 4.039 min
Delta R.T.: 0.007 min
Response: 47037628
Conc: 3.31 ng/ml

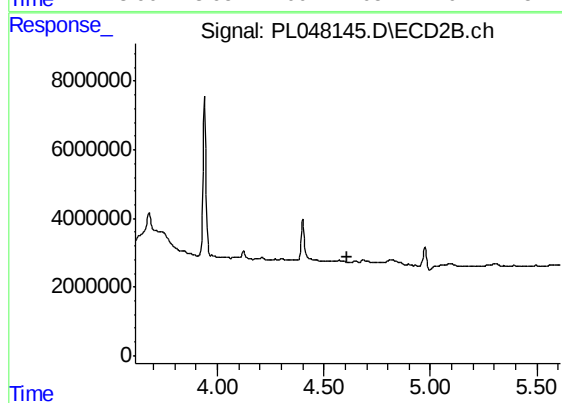

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

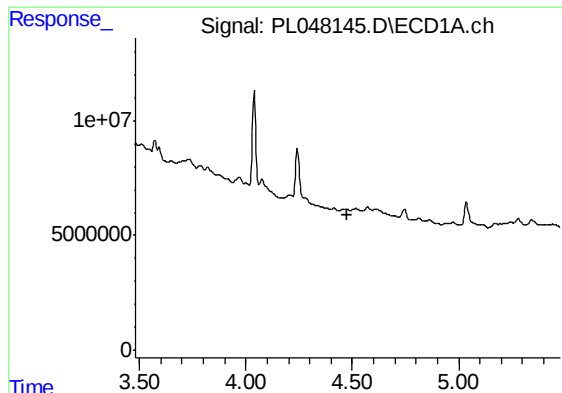

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MR-SUMP-PIT

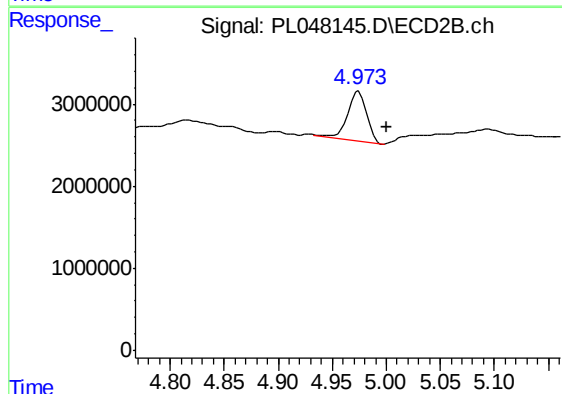


#7 delta-BHC

R.T.: 4.975 min
Delta R.T.: -0.025 min
Response: 7505428
Conc: 2.65 ng/ml

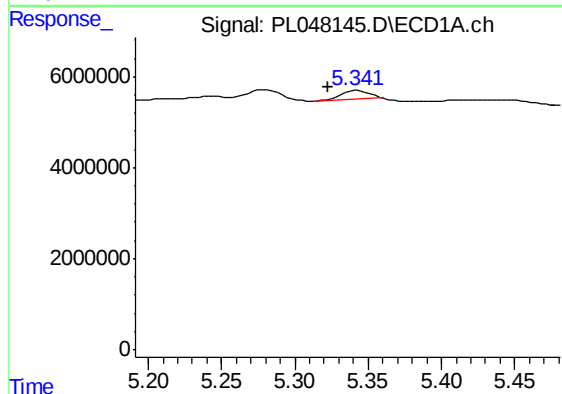


#9 Endosulfan I

R.T.: 5.342 min
Delta R.T.: 0.020 min
Response: 2334022
Conc: 0.19 ng/ml

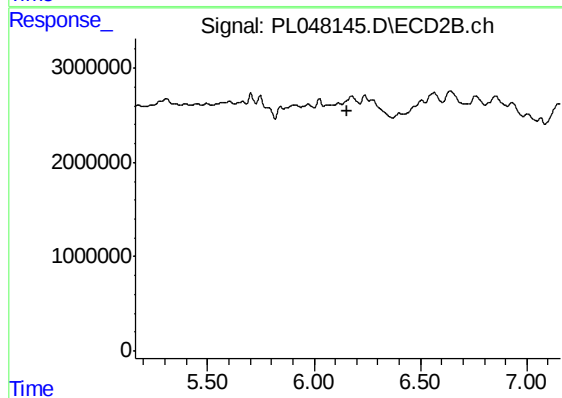

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.159 min
Response: 0
Conc: N.D.

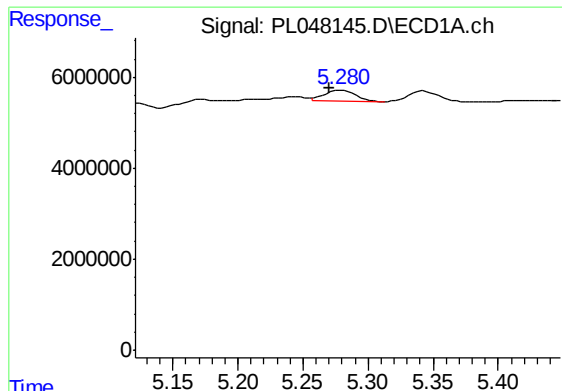

#11 alpha-Chlordane


R.T.: 5.281 min
Delta R.T.: 0.010 min
Response: 4197641
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
MR-SUMP-PIT

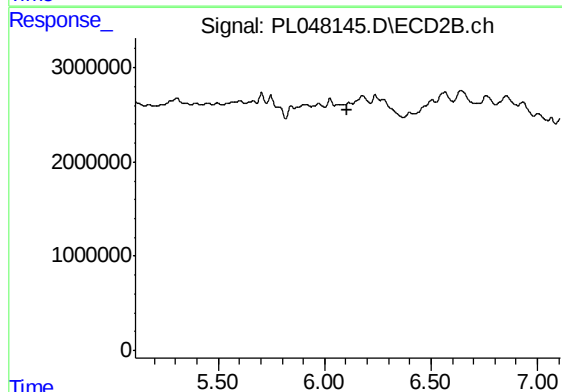


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

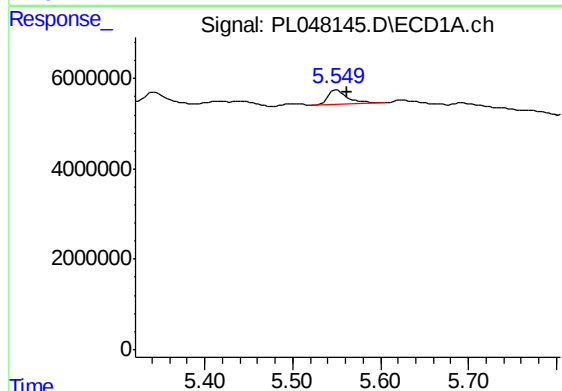


#13 Dieldrin

R.T.: 5.550 min
Delta R.T.: -0.012 min
Response: 5110106
Conc: 0.39 ng/ml

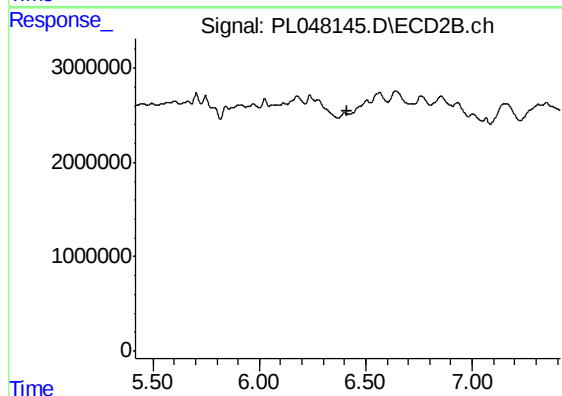

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

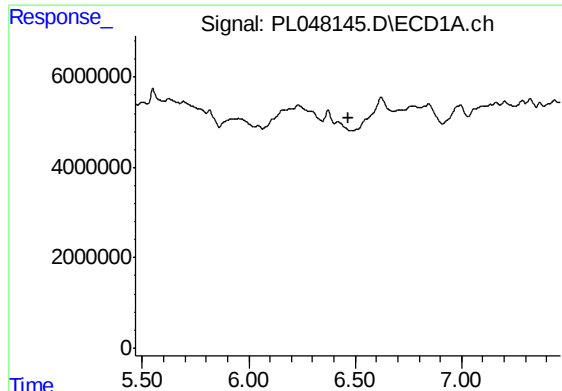

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.468 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MR-SUMP-PIT

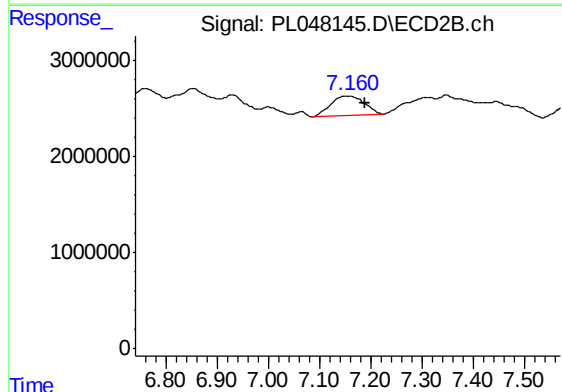


#19 Endosulfan Sulfate

R.T.: 7.161 min
Delta R.T.: -0.029 min
Response: 9239131
Conc: 3.57 ng/ml

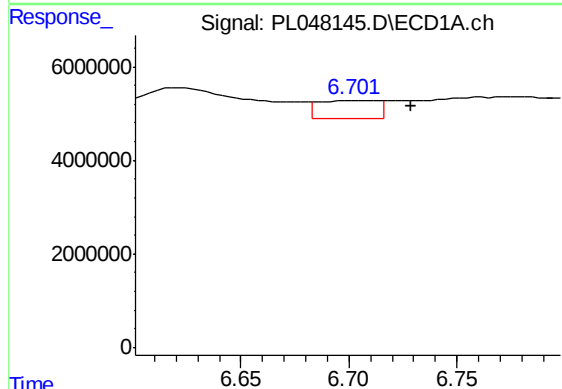


#20 Methoxychlor

R.T.: 6.703 min
Delta R.T.: -0.026 min
Response: 7494141
Conc: 1.38 ng/ml

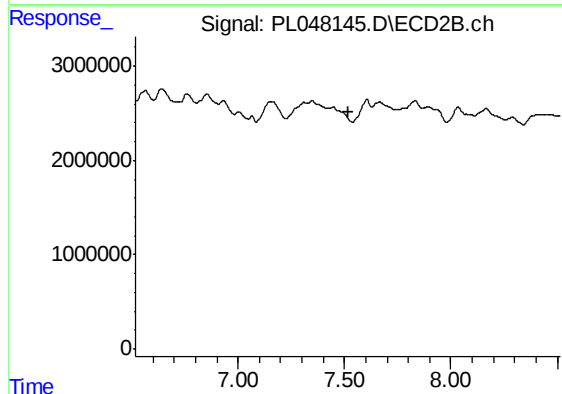

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.

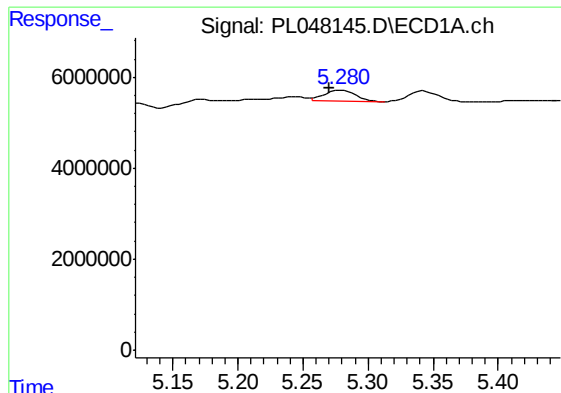

#26 Chlordane-4


R.T.: 5.281 min
Delta R.T.: 0.010 min
Response: 4197641
Conc: 2.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
MR-SUMP-PIT

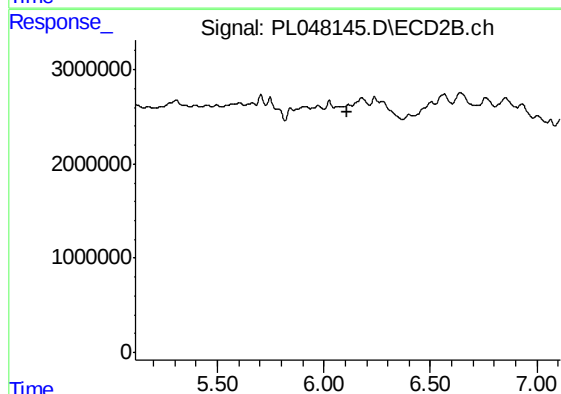


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

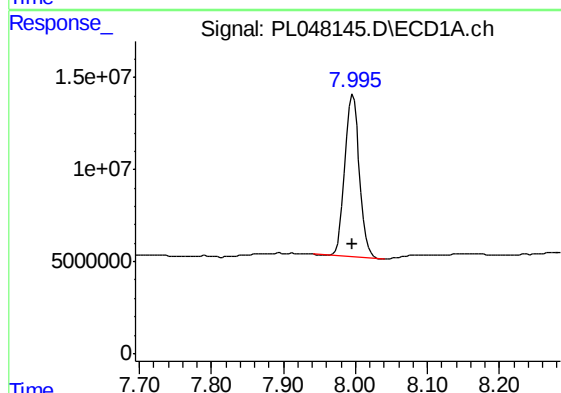

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: 0.000 min
Response: 124431175
Conc: 12.38 ng/ml

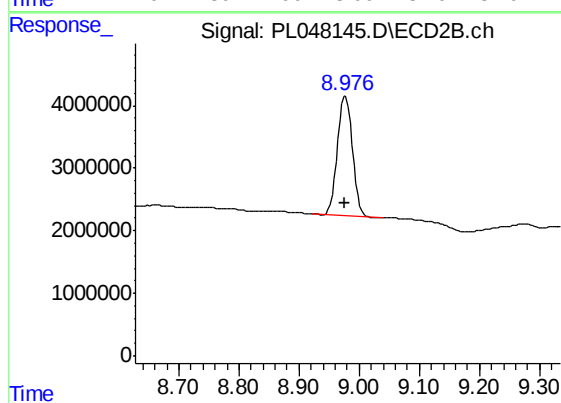

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.002 min
Response: 33207728
Conc: 12.51 ng/ml