

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050219\
 Data File : PL048144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2019 17:33
 Operator : AJ\SJ
 Sample : K2650-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 GROUND-WATER

Manual Integrations
 APPROVED

Ankita
 5/3/2019 10:22:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 01:00:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.326	3.930	39645170	47588631	4.093m	19.105m#
28) SA Decachlor...	7.997	8.976	24904086	7206651	2.477	2.715m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050219\
Data File : PL048144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2019 17:33
Operator : AJ\SJ
Sample : K2650-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
GROUND-WATER


Manual Integrations
APPROVED

Ankita
5/3/2019 10:22:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 01:00:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

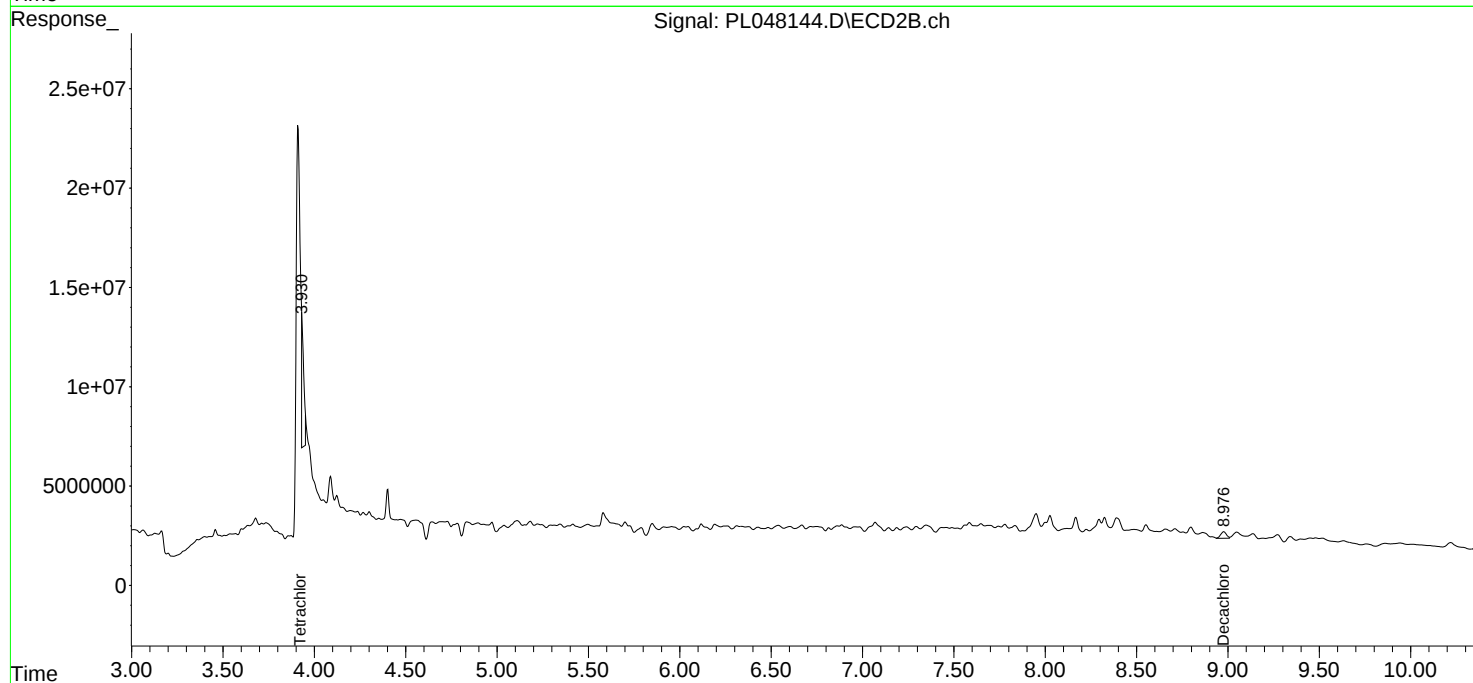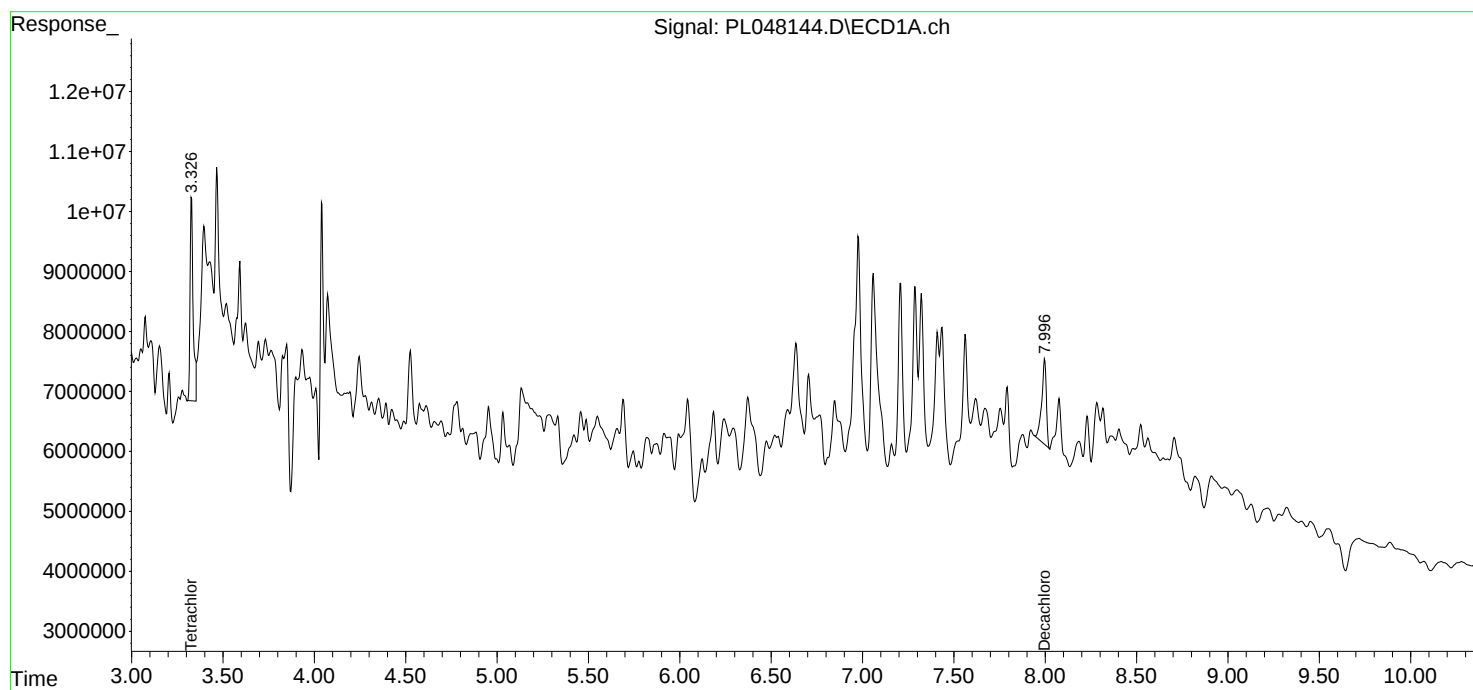

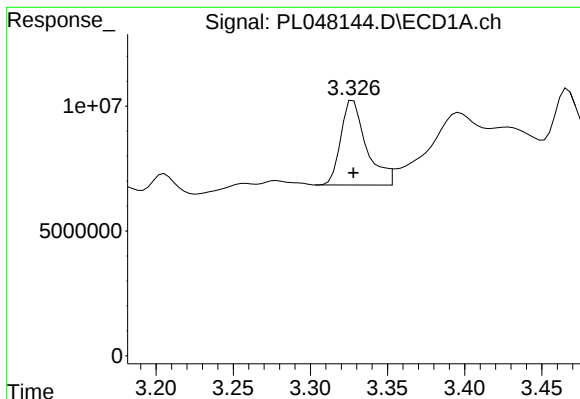


#1 Tetrachloro-m-xylene

R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 39645170
Conc: 4.09 ng/ml m

Instrument :
ECD_L
ClientSampleId :
GROUND-WATER


Manual Integrations
APPROVED

Ankita
5/3/2019 10:22:50 AM

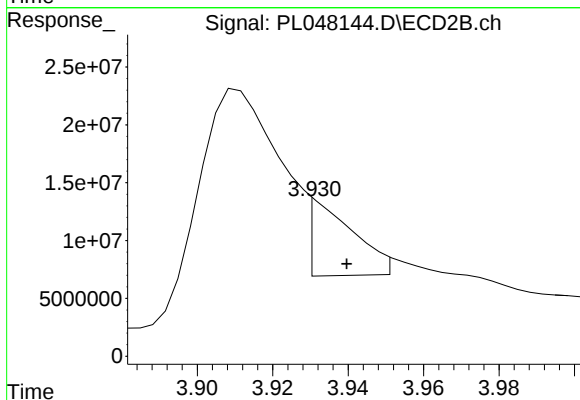


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.009 min
Response: 47588631
Conc: 19.11 ng/ml m

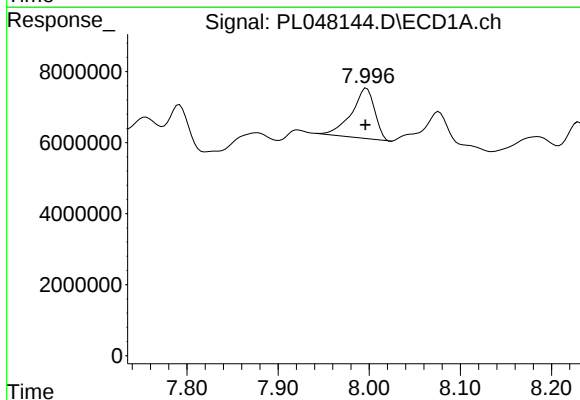

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: 0.001 min
Response: 24904086
Conc: 2.48 ng/ml

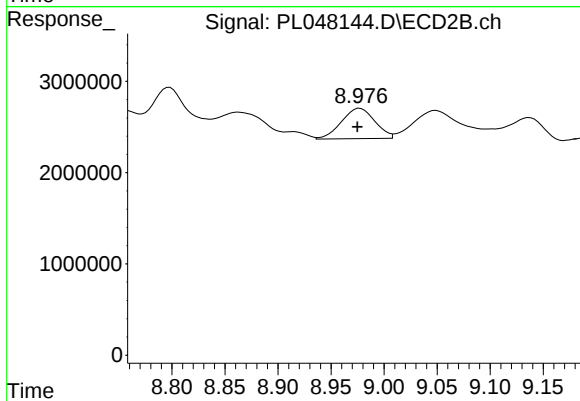

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.000 min
Response: 7206651
Conc: 2.72 ng/ml m