

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050224\
 Data File : PL089320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2024 14:59
 Operator : AR\AJ
 Sample : P2332-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAT-DIS-02-05012024

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/03/2024
 Supervised By :Ankita Jodhani 05/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 23:02:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 26 19:27:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.797	22112614	14440911	10.981	11.255
2) SA Decachlor...	9.066	7.949	18077521	14648633	12.922	10.890
Target Compounds						
17) MA 4,4'-DDT	7.029	6.063	1005924	1055716	0.547m	0.780m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050224\
Data File : PL089320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2024 14:59
Operator : AR\AJ
Sample : P2332-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PAT-DIS-02-05012024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/03/2024
Supervised By : Ankita Jodhani 05/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 23:02:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
Quant Title : GC Extractables
QLast Update : Fri Apr 26 19:27:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

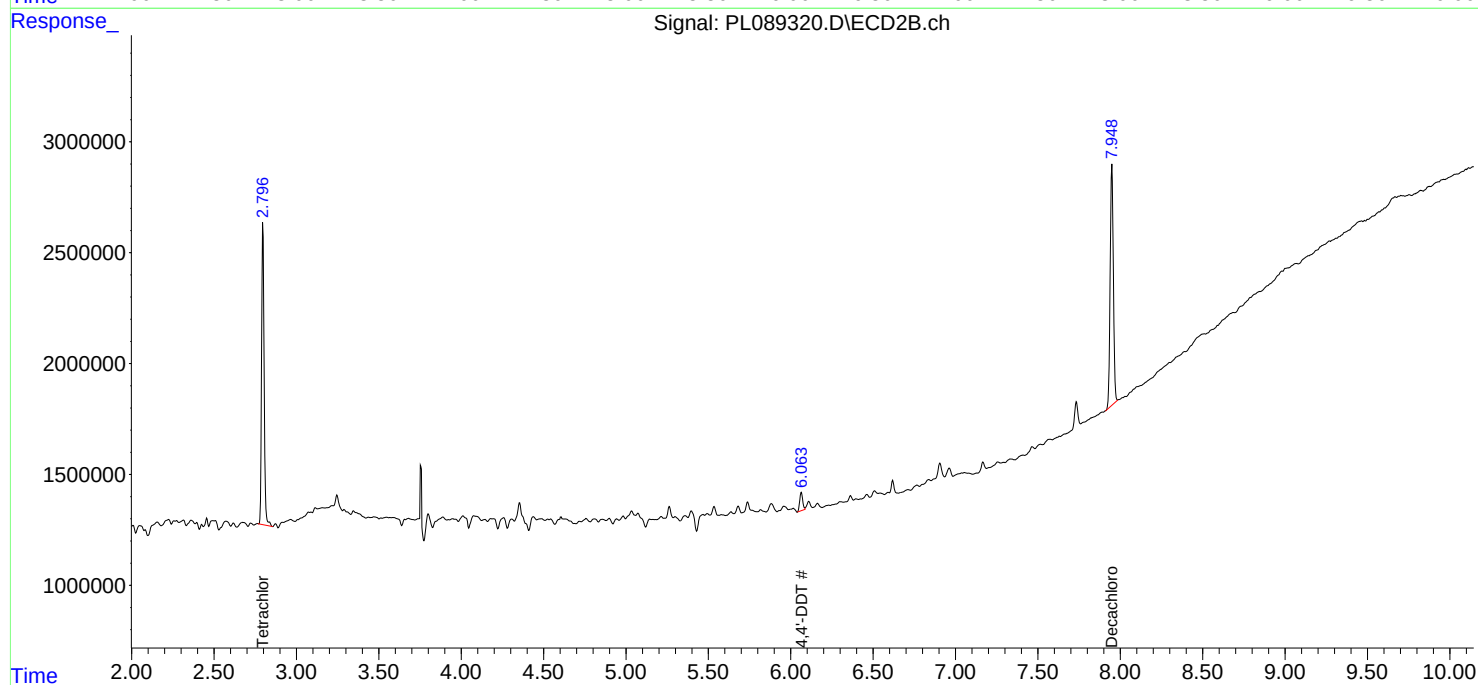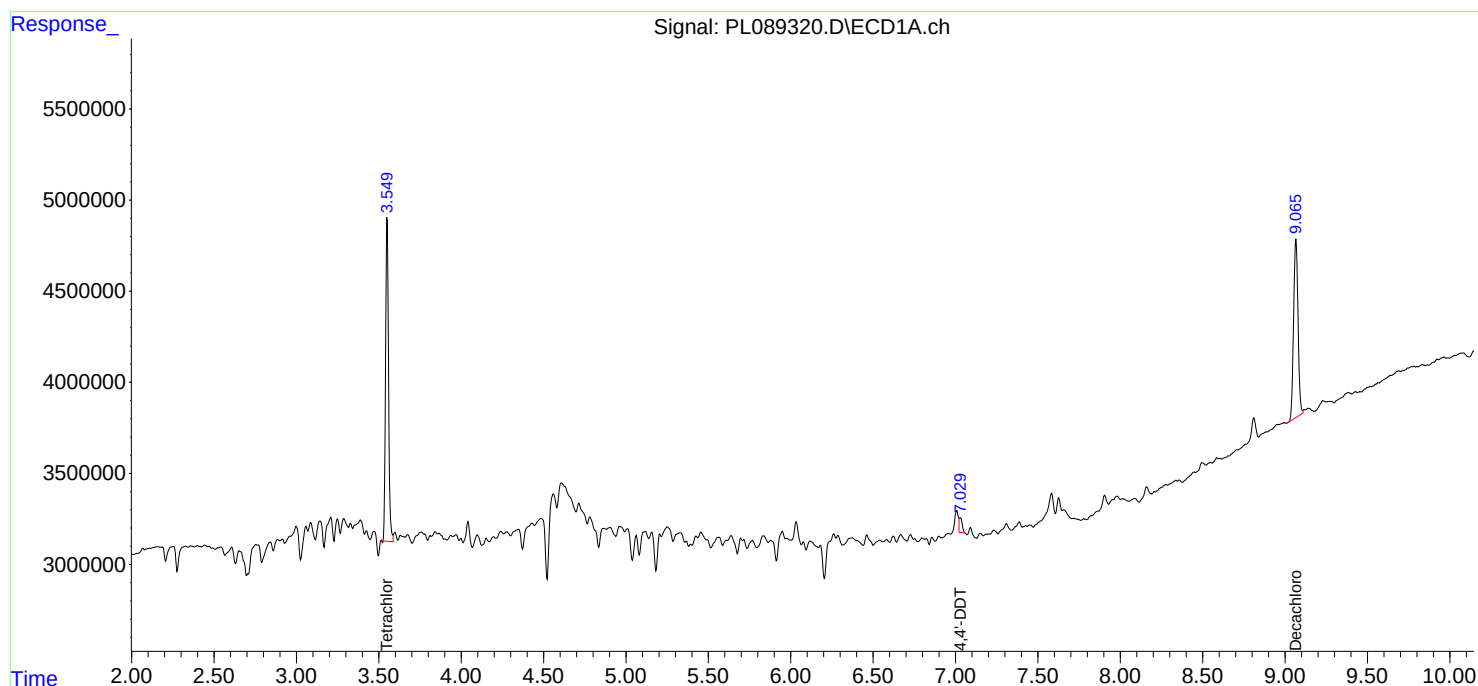

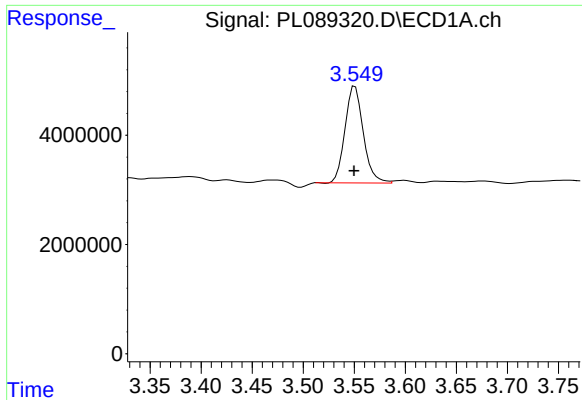


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 22112614
Conc: 10.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAT-DIS-02-05012024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/03/2024
Supervised By :Ankita Jodhani 05/06/2024

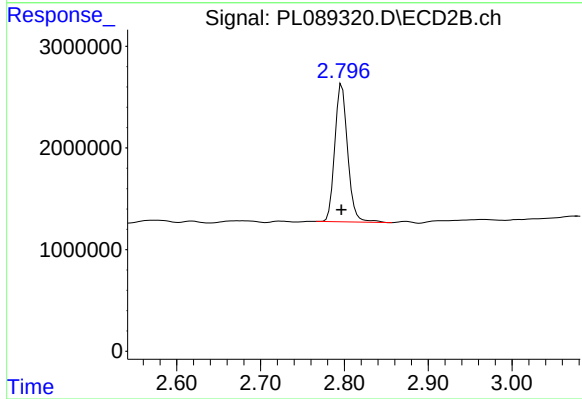


#1 Tetrachloro-m-xylene

R.T.: 2.797 min
Delta R.T.: 0.000 min
Response: 14440911
Conc: 11.26 ng/ml

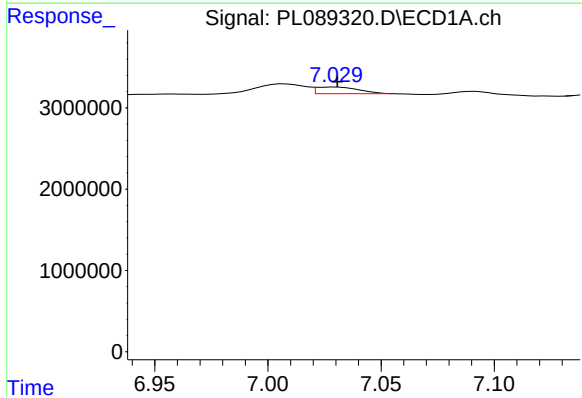


#17 4,4'-DDT

R.T.: 7.029 min
Delta R.T.: -0.002 min
Response: 1005924
Conc: 0.55 ng/ml m

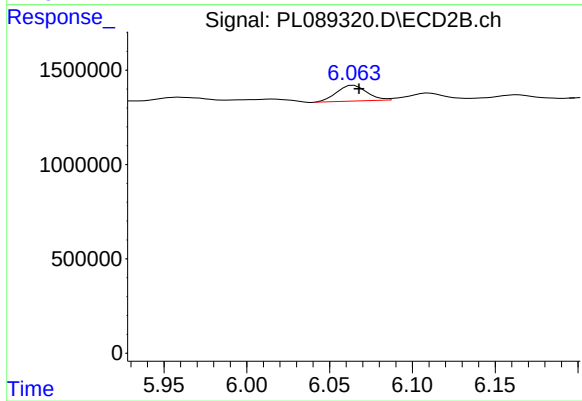

#17 4,4'-DDT

R.T.: 6.063 min
Delta R.T.: -0.005 min
Response: 1055716
Conc: 0.78 ng/ml m

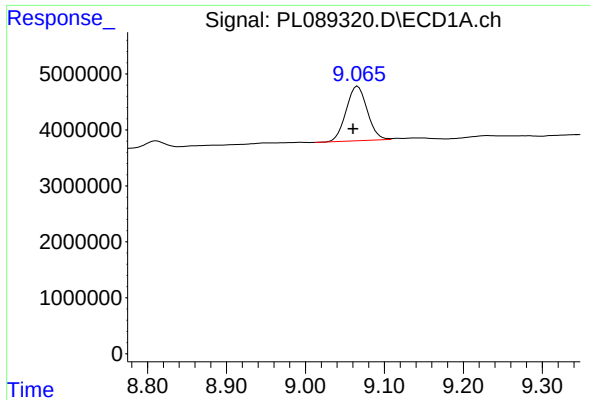


#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.006 min
Response: 18077521
Conc: 12.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAT-DIS-02-05012024

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/03/2024
Supervised By :Ankita Jodhani 05/06/2024

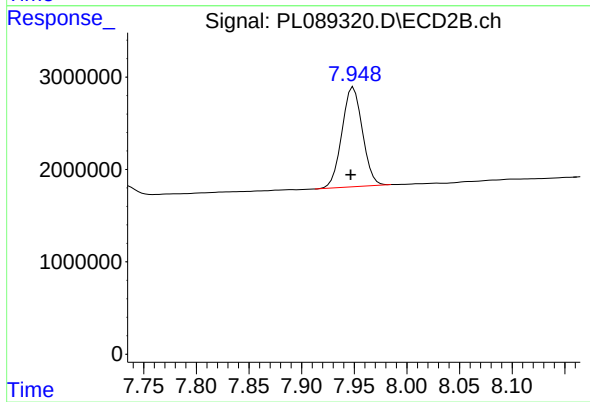

#28 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.003 min
Response: 14648633
Conc: 10.89 ng/ml