

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050225\
 Data File : PL095477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2025 14:27
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 00:56:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.599	2.905	169.7E6	161.0E6	51.988	50.643
28)	SA Decachlor...	9.125	8.085	152.8E6	163.2E6	55.160	55.141
Target Compounds							
10)	B gamma-Chl...	0.000	5.164f	0	13781684	N.D.	3.401 #
14)	MA Endrin	6.599f	0.000	17973972	0	5.644	N.D. #
15)	B Endosulfa...	6.857f	6.093	13866313	10038817	4.344	2.795 #
16)	A 4,4'-DDD	0.000	5.968f	0	5907156	N.D.	1.808 #
17)	MA 4,4'-DDT	0.000	6.209	0	7294895	N.D.	2.123 #
18)	B Endrin al...	0.000	6.286	0	10461917	N.D.	4.004 #
19)	B Endosulfa...	7.198	0.000	34567342	0	12.338	N.D. #
20)	A Methoxychlor	0.000	6.769	0	46079919	N.D.	24.158 #
22)	Mirex	0.000	7.209	0	35294575	N.D.	12.245 #
25)	Chlordane-3	0.000	5.164	0	13781684	N.D.	26.677 #
27)	Chlordane-5	6.904	6.093	25034527	10038817	165.150	54.341 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050225\
Data File : PL095477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2025 14:27
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 00:56:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

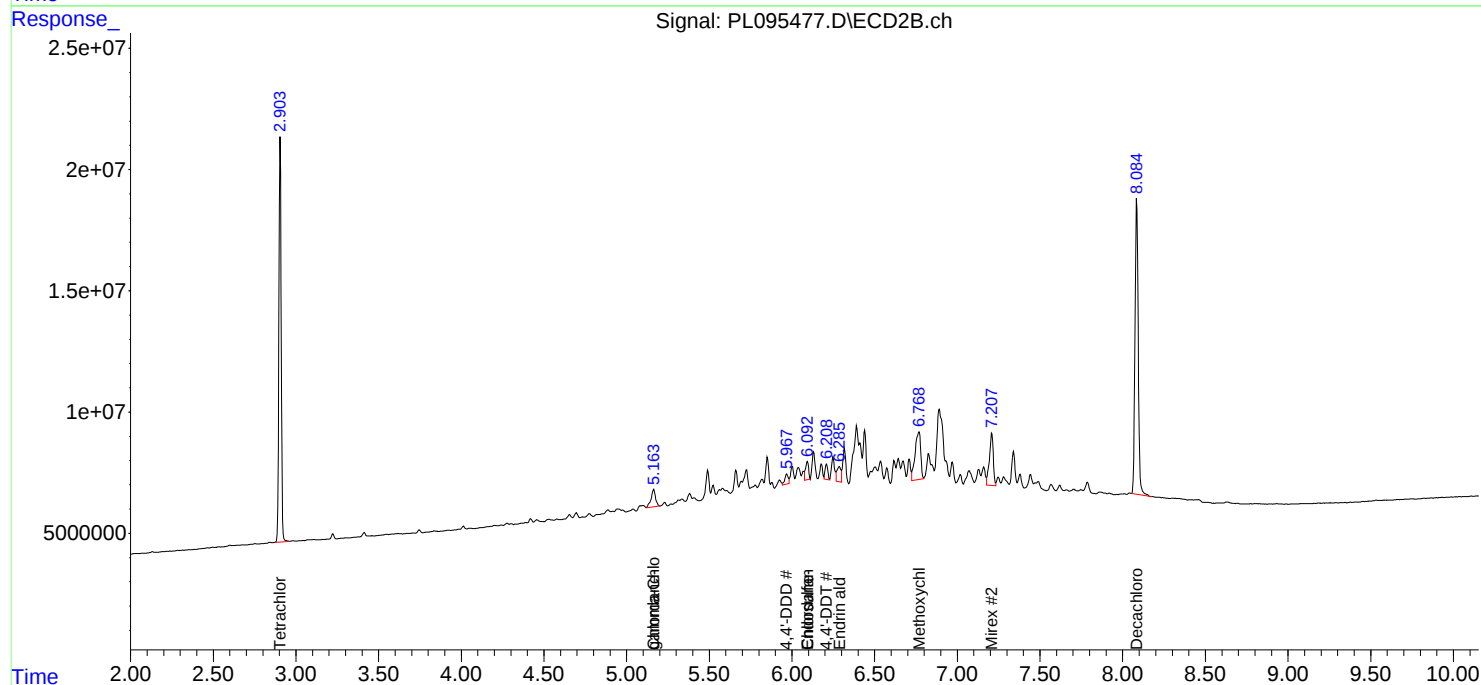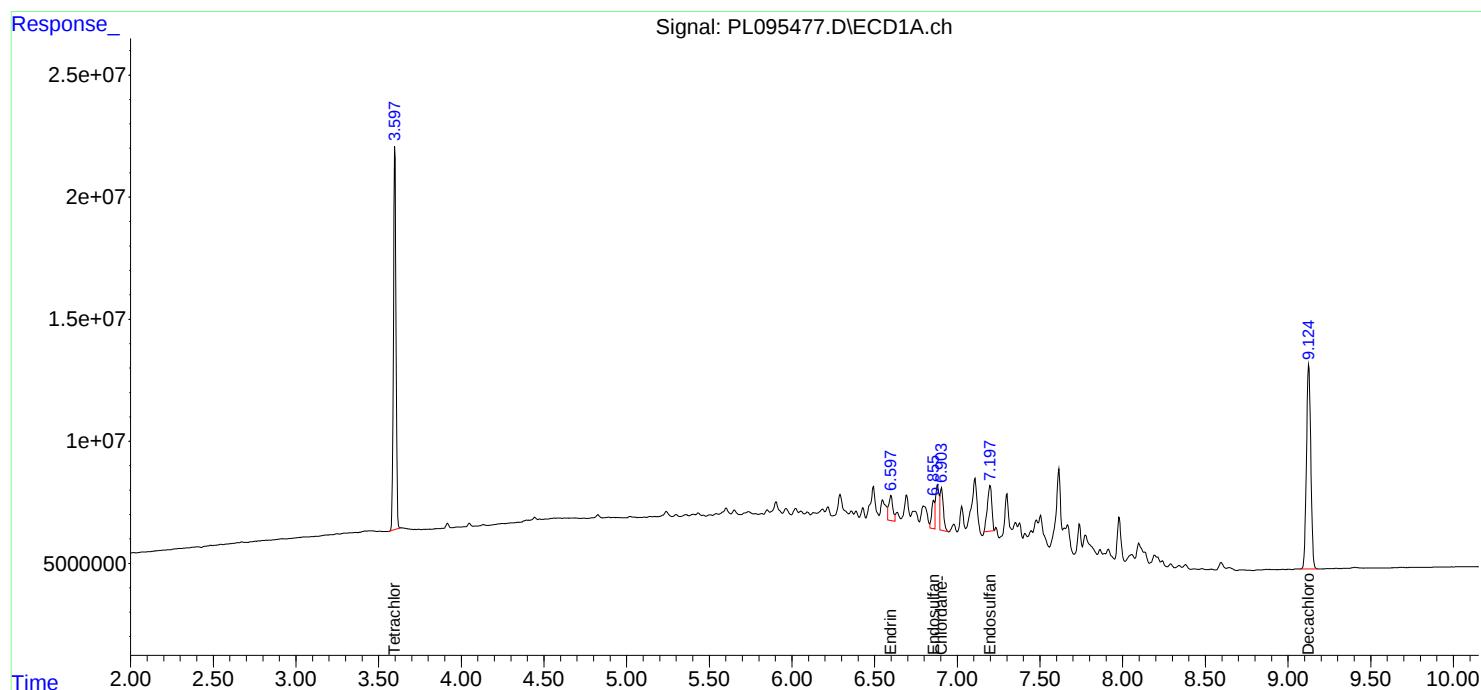


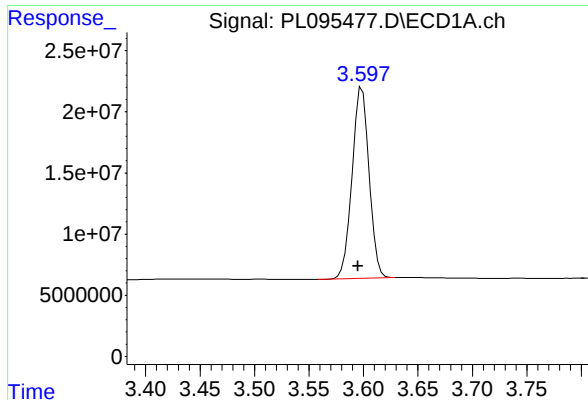

#1 Tetrachloro-m-xylene


R.T.: 3.599 min
Delta R.T.: 0.004 min
Response: 169723255
Conc: 51.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

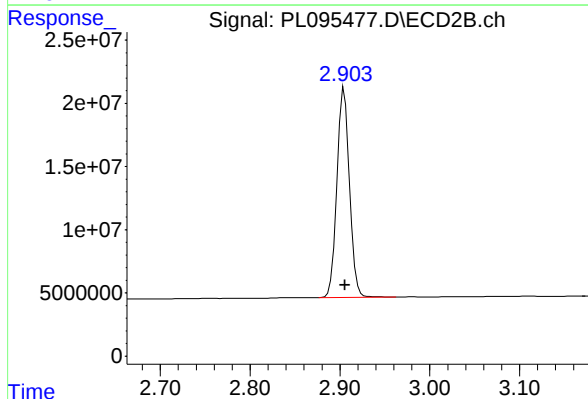


#1 Tetrachloro-m-xylene

R.T.: 2.905 min
Delta R.T.: 0.000 min
Response: 161033374
Conc: 50.64 ng/ml

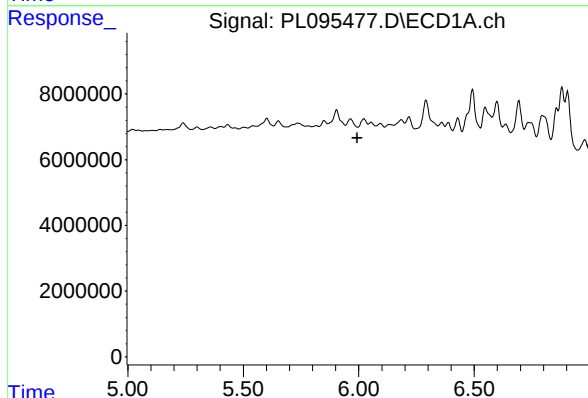


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.994 min
Response: 0
Conc: N.D.

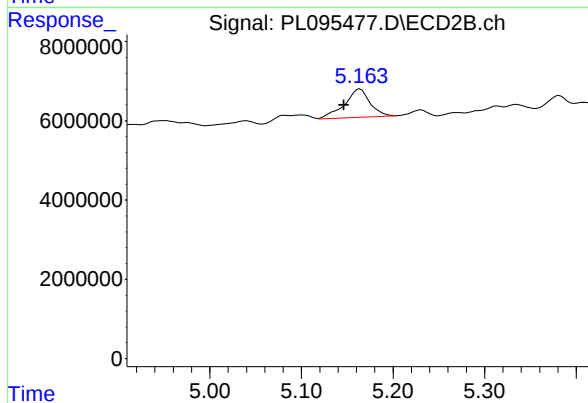

#10 gamma-Chlordane


R.T.: 5.164 min
Delta R.T.: 0.017 min
Response: 13781684
Conc: 3.40 ng/ml

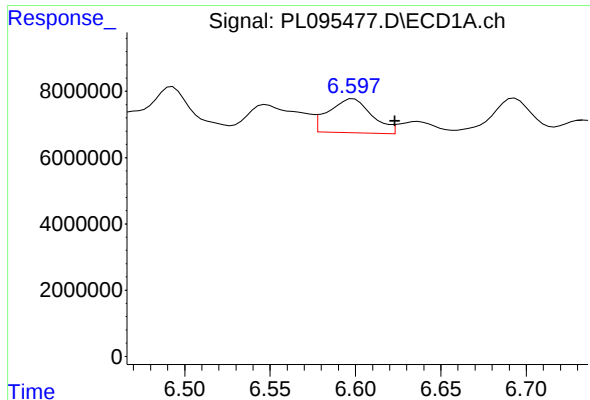

#14 Endrin


R.T.: 6.599 min
Delta R.T.: -0.024 min
Response: 17973972
Conc: 5.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

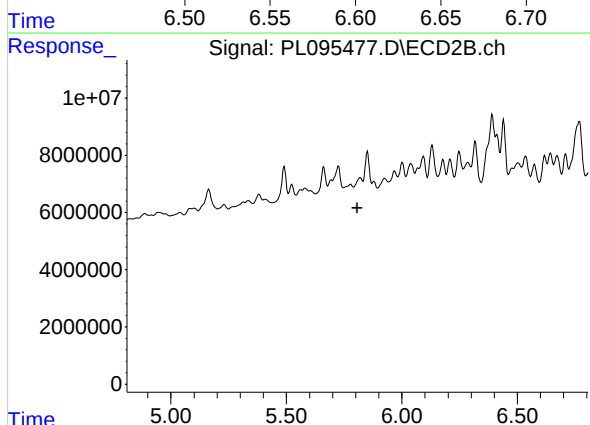


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.807 min
Response: 0
Conc: N.D.

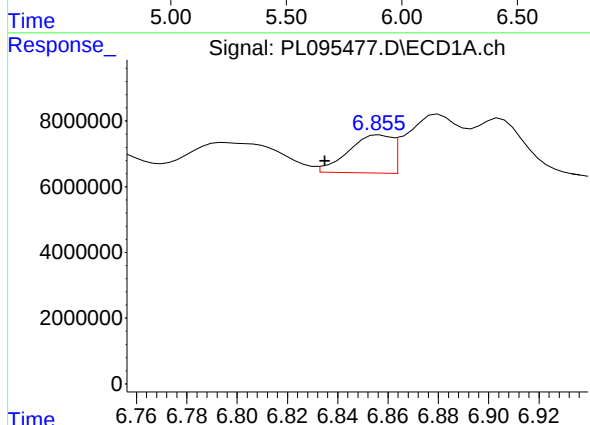


#15 Endosulfan II

R.T.: 6.857 min
Delta R.T.: 0.022 min
Response: 13866313
Conc: 4.34 ng/ml

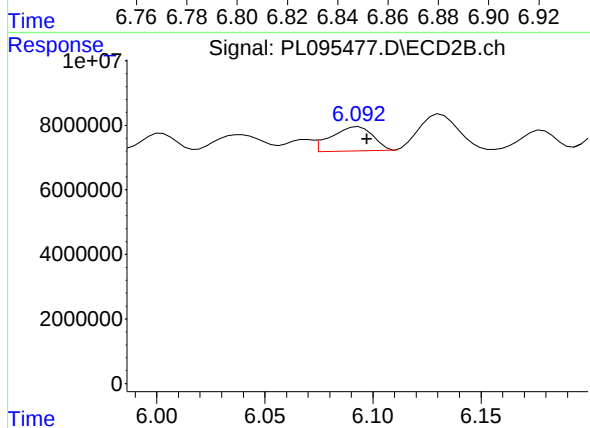

#15 Endosulfan II


R.T.: 6.093 min
Delta R.T.: -0.004 min
Response: 10038817
Conc: 2.80 ng/ml

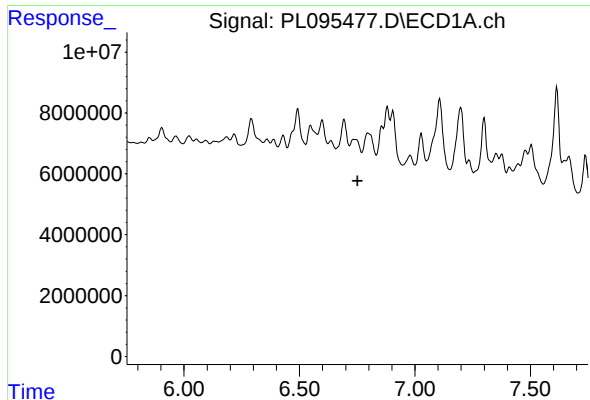

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.753 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

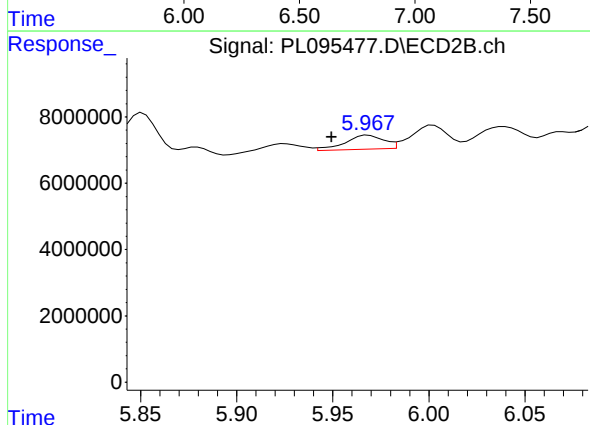


#16 4,4'-DDD

R.T.: 5.968 min
Delta R.T.: 0.019 min
Response: 5907156
Conc: 1.81 ng/ml

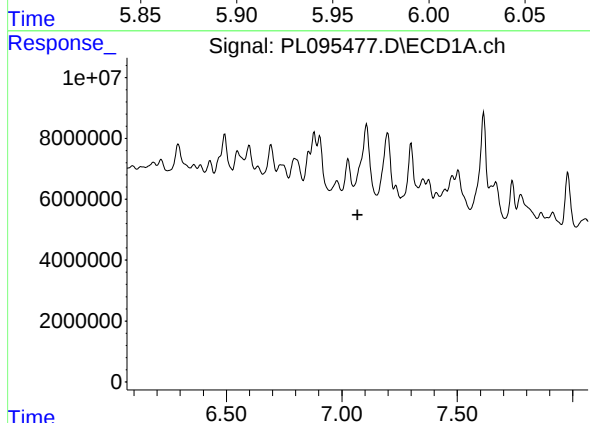


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 7.069 min
Response: 0
Conc: N.D.

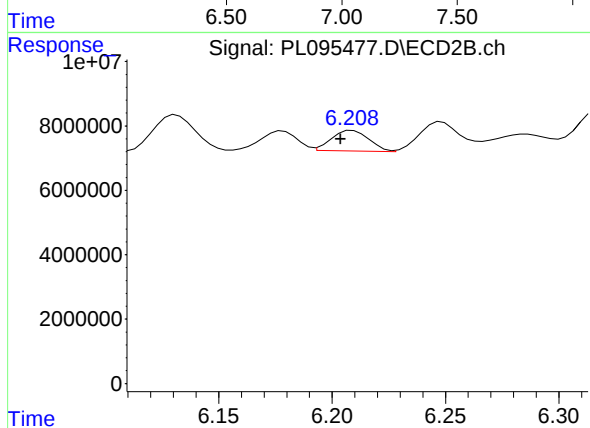

#17 4,4'-DDT


R.T.: 6.209 min
Delta R.T.: 0.005 min
Response: 7294895
Conc: 2.12 ng/ml

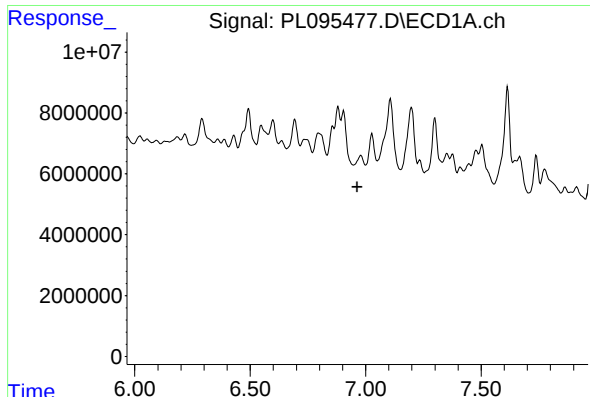

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.964 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

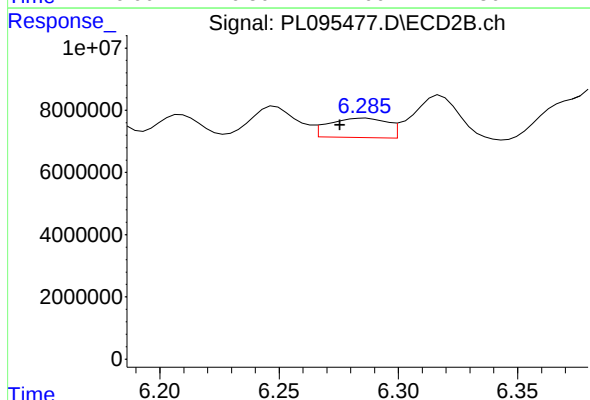


#18 Endrin aldehyde

R.T.: 6.286 min
Delta R.T.: 0.010 min
Response: 10461917
Conc: 4.00 ng/ml

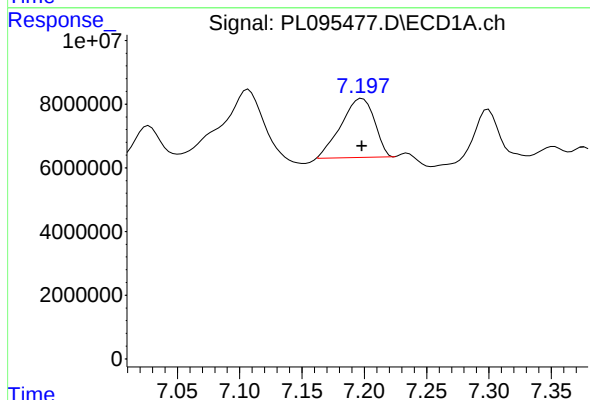


#19 Endosulfan Sulfate

R.T.: 7.198 min
Delta R.T.: 0.000 min
Response: 34567342
Conc: 12.34 ng/ml

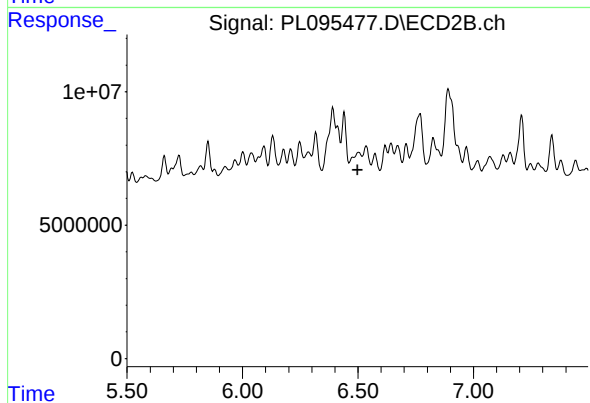

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.498 min
Response: 0
Conc: N.D.

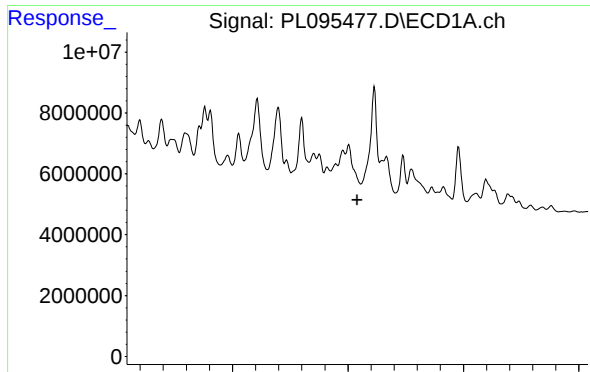

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.540 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

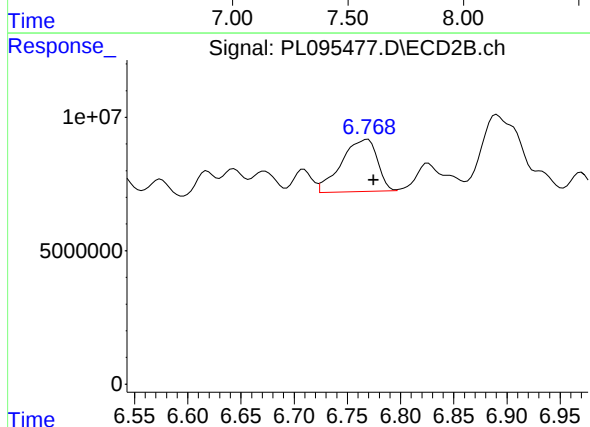


#20 Methoxychlor

R.T.: 6.769 min
Delta R.T.: -0.006 min
Response: 46079919
Conc: 24.16 ng/ml

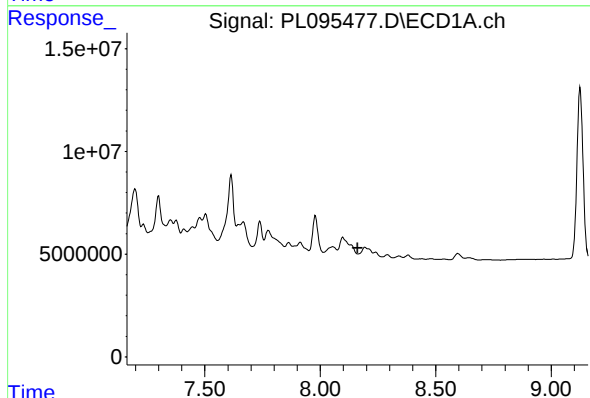


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.161 min
Response: 0
Conc: N.D.

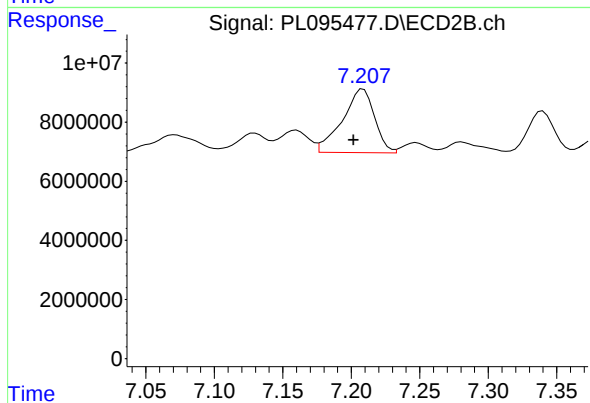

#22 Mirex


R.T.: 7.209 min
Delta R.T.: 0.007 min
Response: 35294575
Conc: 12.24 ng/ml

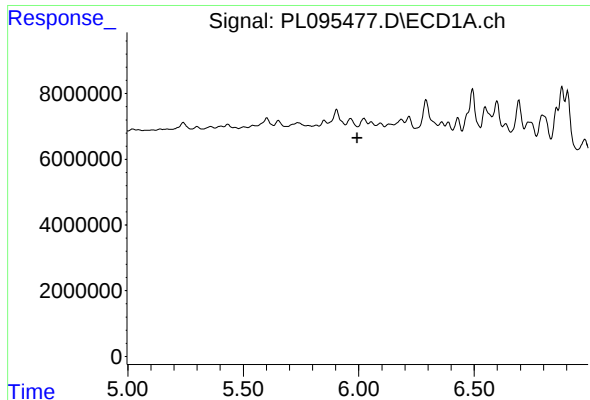

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.994 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

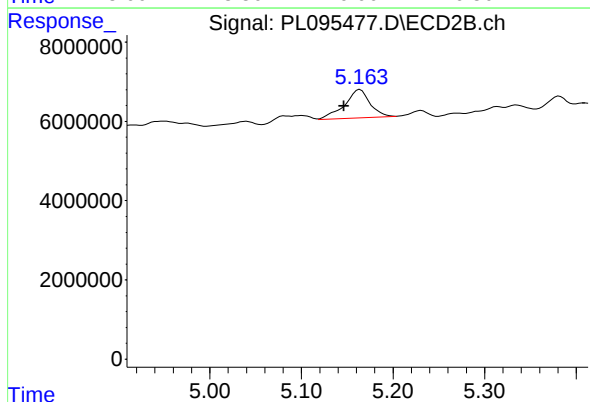


#25 Chlordane-3

R.T.: 5.164 min
Delta R.T.: 0.017 min
Response: 13781684
Conc: 26.68 ng/ml

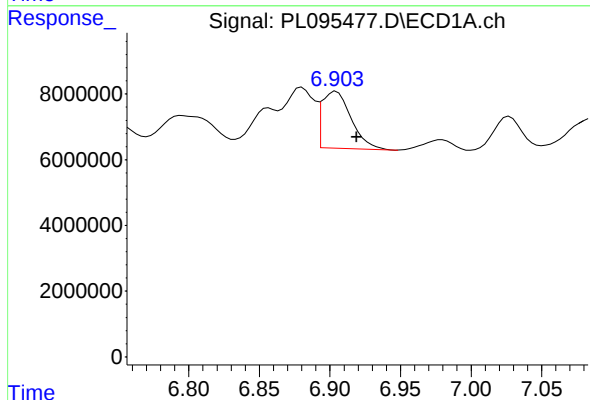


#27 Chlordane-5

R.T.: 6.904 min
Delta R.T.: -0.014 min
Response: 25034527
Conc: 165.15 ng/ml

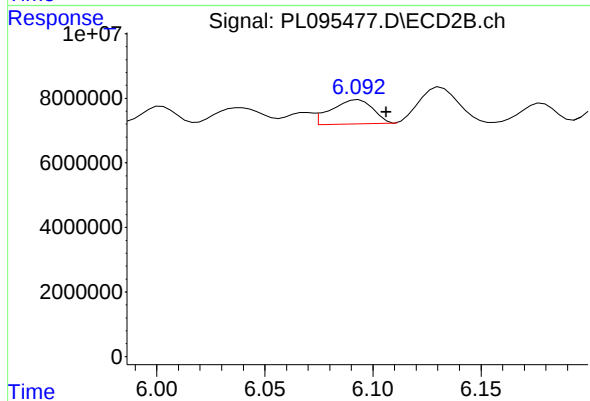

#27 Chlordane-5


R.T.: 6.093 min
Delta R.T.: -0.013 min
Response: 10038817
Conc: 54.34 ng/ml

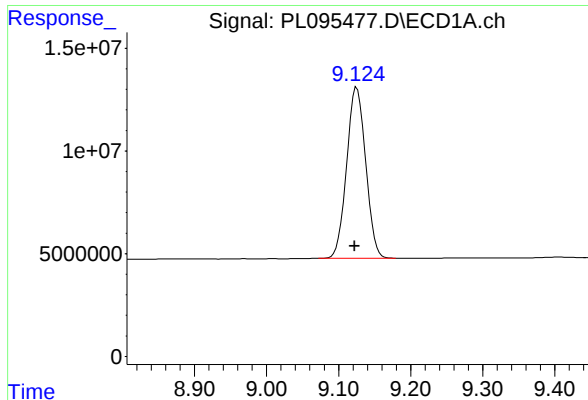

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.003 min
Response: 152837315
Conc: 55.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

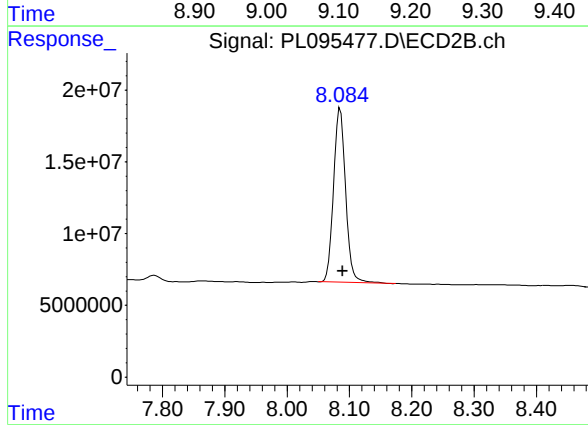

#28 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: -0.004 min
Response: 163178234
Conc: 55.14 ng/ml