

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050225\
 Data File : PL095480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2025 15:23
 Operator : AR\AJ
 Sample : PB167766BS
 Misc : BS CHLOR
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB167766BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 00:56:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.595	2.907	60804190	70190392	18.625	22.074
28) SA Decachlor...	9.121	8.084	60036723	62779921	21.668	21.215
Target Compounds						
23) Chlordane-1	4.760	3.926	36595296	30029394	187.182	194.192
24) Chlordane-2	5.286	4.506	41718379	35256597	197.049	191.582
25) Chlordane-3	5.993	5.143	157.2E6	97807771	201.756	189.322
26) Chlordane-4	6.078	5.207	192.6E6	83142131	204.289	191.302
27) Chlordane-5	6.918	6.103	29514365	32512801	194.703	175.993



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050225\
Data File : PL095480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2025 15:23
Operator : AR\AJ
Sample : PB167766BS
Misc : BS CHLOR
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB167766BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 00:56:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

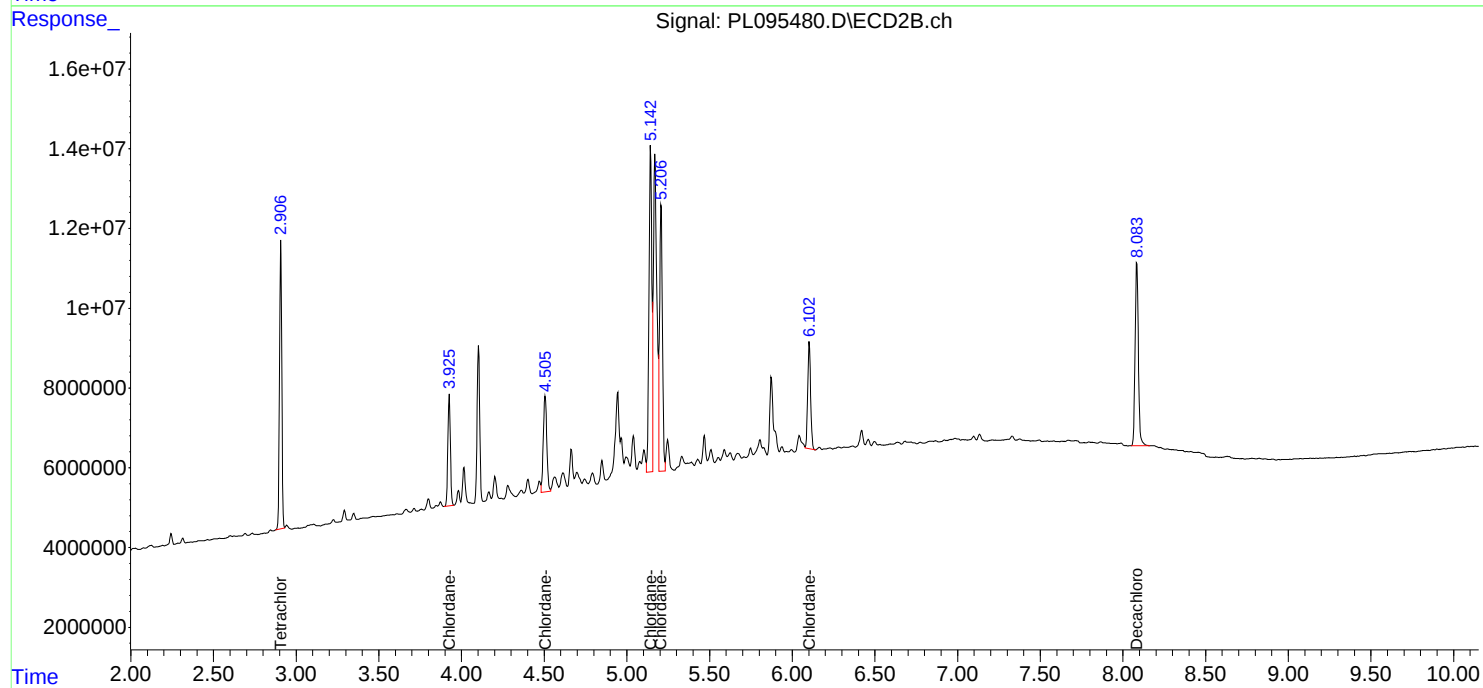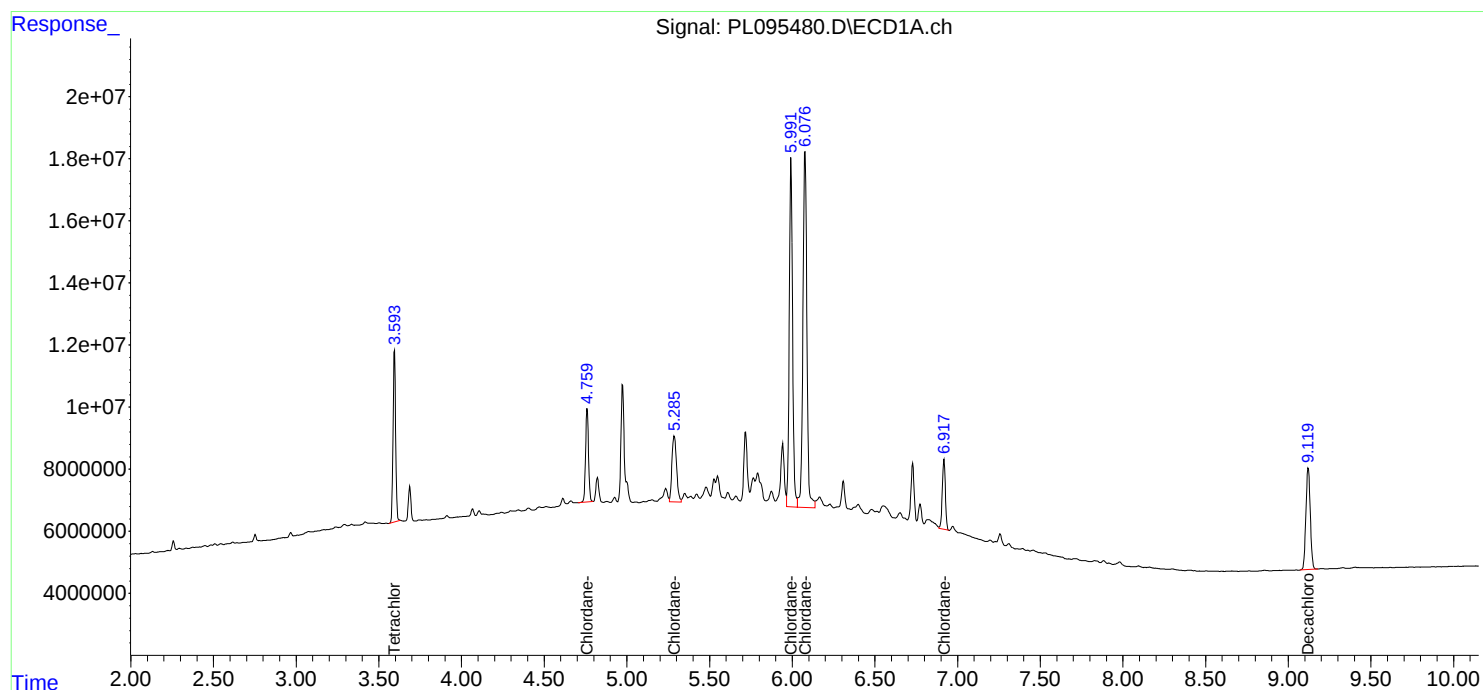


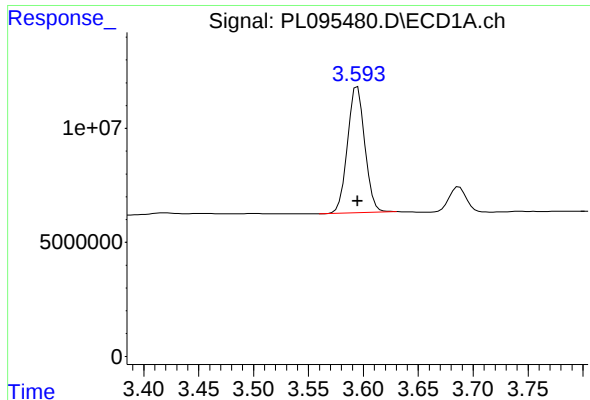

#1 Tetrachloro-m-xylene


R.T.: 3.595 min
Delta R.T.: 0.000 min
Response: 60804190
Conc: 18.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167766BS

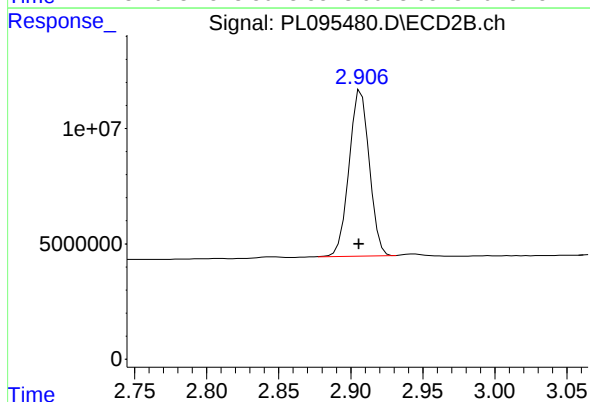


#1 Tetrachloro-m-xylene

R.T.: 2.907 min
Delta R.T.: 0.001 min
Response: 70190392
Conc: 22.07 ng/ml

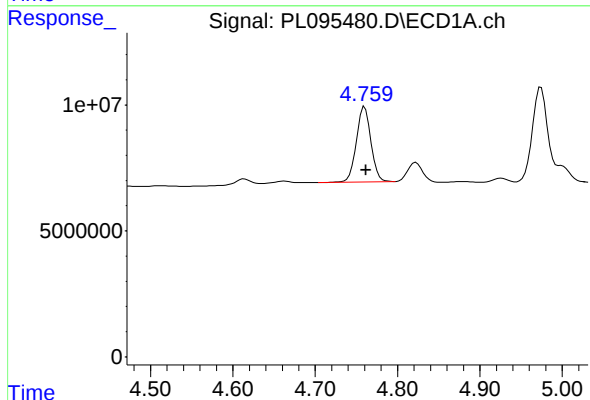


#23 Chlordane-1

R.T.: 4.760 min
Delta R.T.: -0.002 min
Response: 36595296
Conc: 187.18 ng/ml

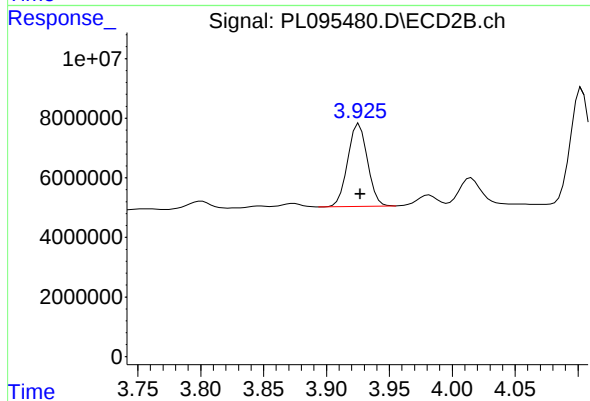

#23 Chlordane-1


R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 30029394
Conc: 194.19 ng/ml

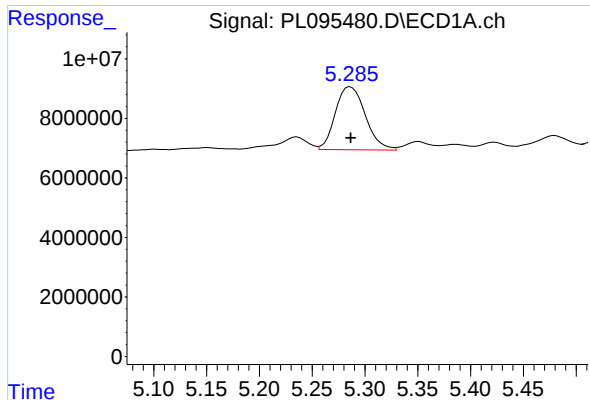

#24 Chlordane-2


R.T.: 5.286 min
Delta R.T.: 0.000 min
Response: 41718379
Conc: 197.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167766BS

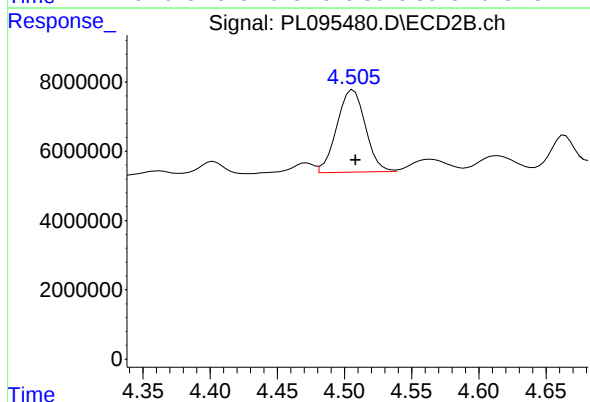


#24 Chlordane-2

R.T.: 4.506 min
Delta R.T.: -0.002 min
Response: 35256597
Conc: 191.58 ng/ml

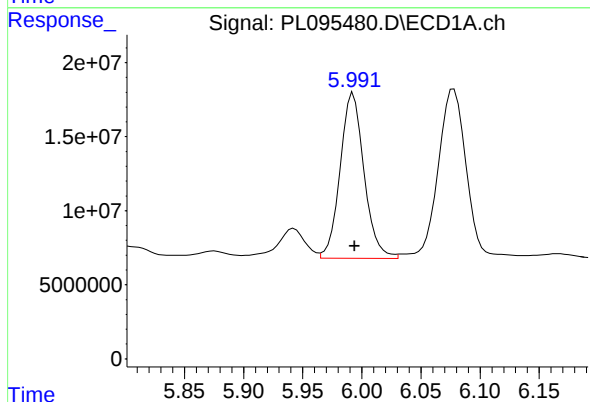


#25 Chlordane-3

R.T.: 5.993 min
Delta R.T.: -0.001 min
Response: 157152790
Conc: 201.76 ng/ml

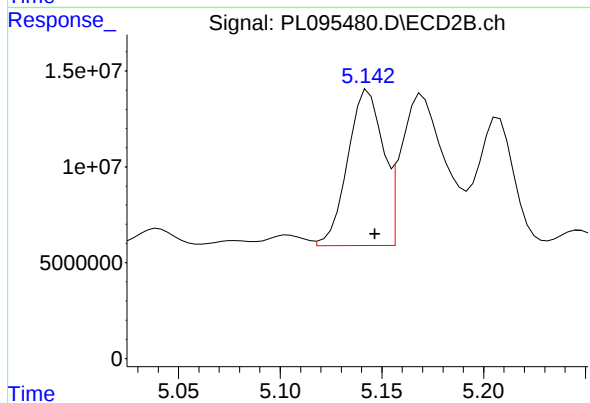

#25 Chlordane-3


R.T.: 5.143 min
Delta R.T.: -0.003 min
Response: 97807771
Conc: 189.32 ng/ml

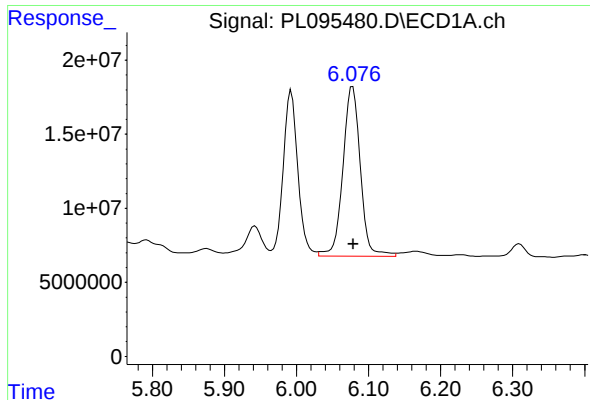

#26 Chlordane-4


R.T.: 6.078 min
Delta R.T.: -0.001 min
Response: 192629899
Conc: 204.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167766BS

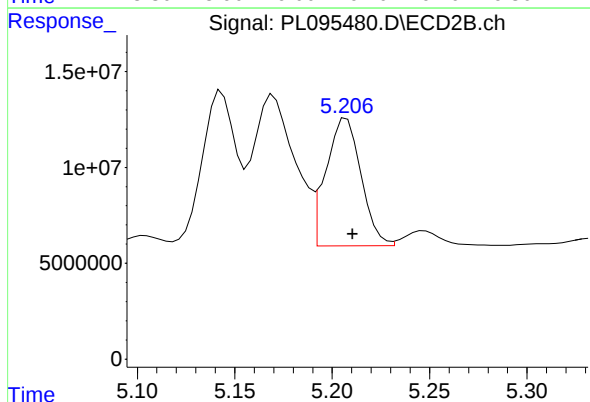


#26 Chlordane-4

R.T.: 5.207 min
Delta R.T.: -0.003 min
Response: 83142131
Conc: 191.30 ng/ml

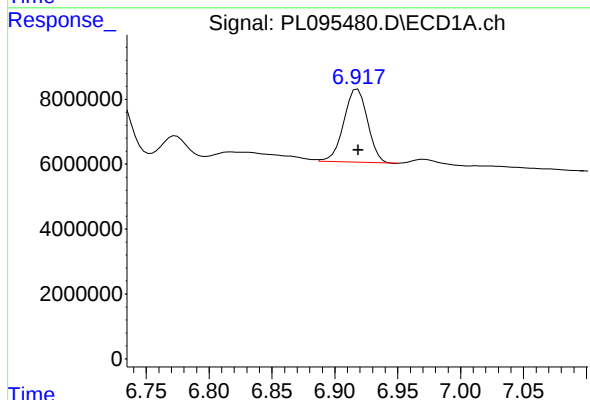


#27 Chlordane-5

R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 29514365
Conc: 194.70 ng/ml

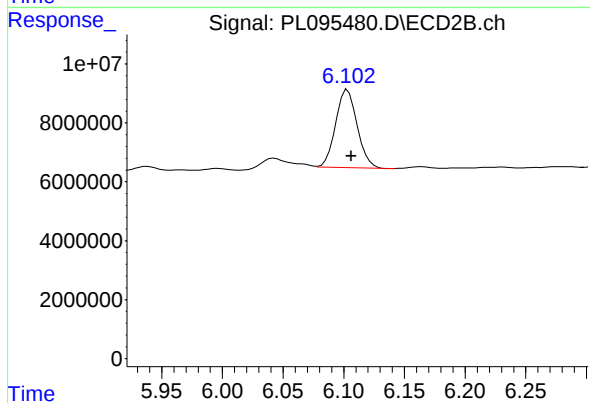

#27 Chlordane-5


R.T.: 6.103 min
Delta R.T.: -0.003 min
Response: 32512801
Conc: 175.99 ng/ml

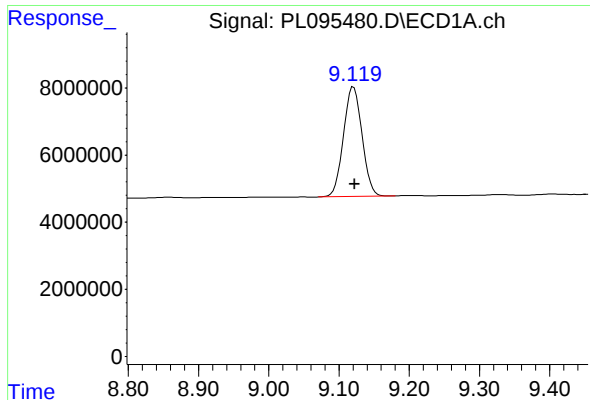

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.002 min
Response: 60036723
Conc: 21.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167766BS

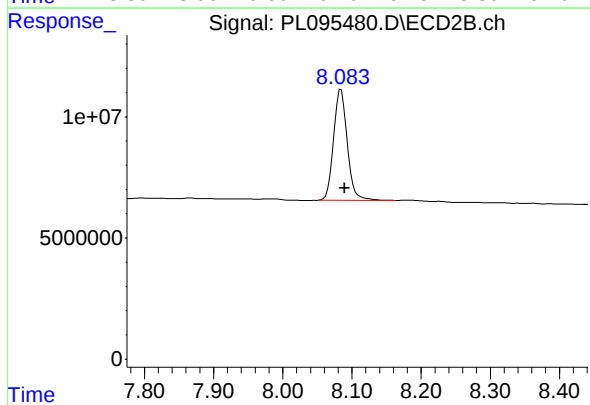

#28 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.005 min
Response: 62779921
Conc: 21.21 ng/ml