

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050319\
 Data File : PL048179.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2019 17:26
 Operator : AJ\SJ
 Sample : K2668-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 23:05:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.941	187.3E6	50288167	19.334	20.189
28)	SA Decachlor...	7.998	8.978	130.6E6	39278475	12.985	14.798
Target Compounds							
4)	MA Heptachlor	0.000	5.129	0	20863743	N.D.	6.027 #
5)	MB Aldrin	4.545	0.000	35070381	0	2.560	N.D. #
10)	B gamma-Chl...	5.214	0.000	19362832	0	1.450	N.D. #
11)	B alpha-Chl...	5.282	0.000	5377445	0	0.411	N.D. #
16)	A 4,4'-DDD	5.953	0.000	2599082	0	0.267	N.D. #
19)	B Endosulfa...	6.494f	0.000	13882311	0	1.293	N.D. #
25)	Chlordane-3	5.214	0.000	19362832	0	12.297	N.D. #
26)	Chlordane-4	5.282	0.000	5377445	0	3.704	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050319\
Data File : PL048179.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2019 17:26
Operator : AJ\SJ
Sample : K2668-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 23:05:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

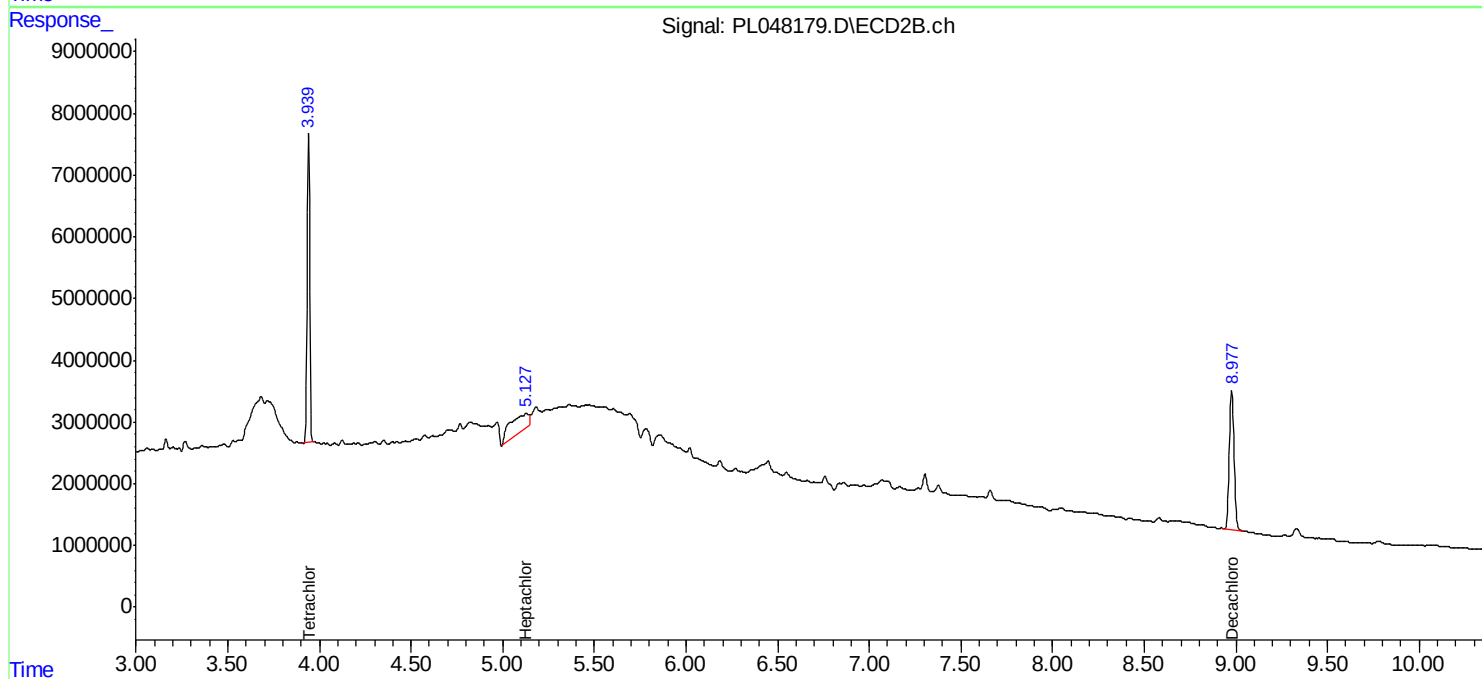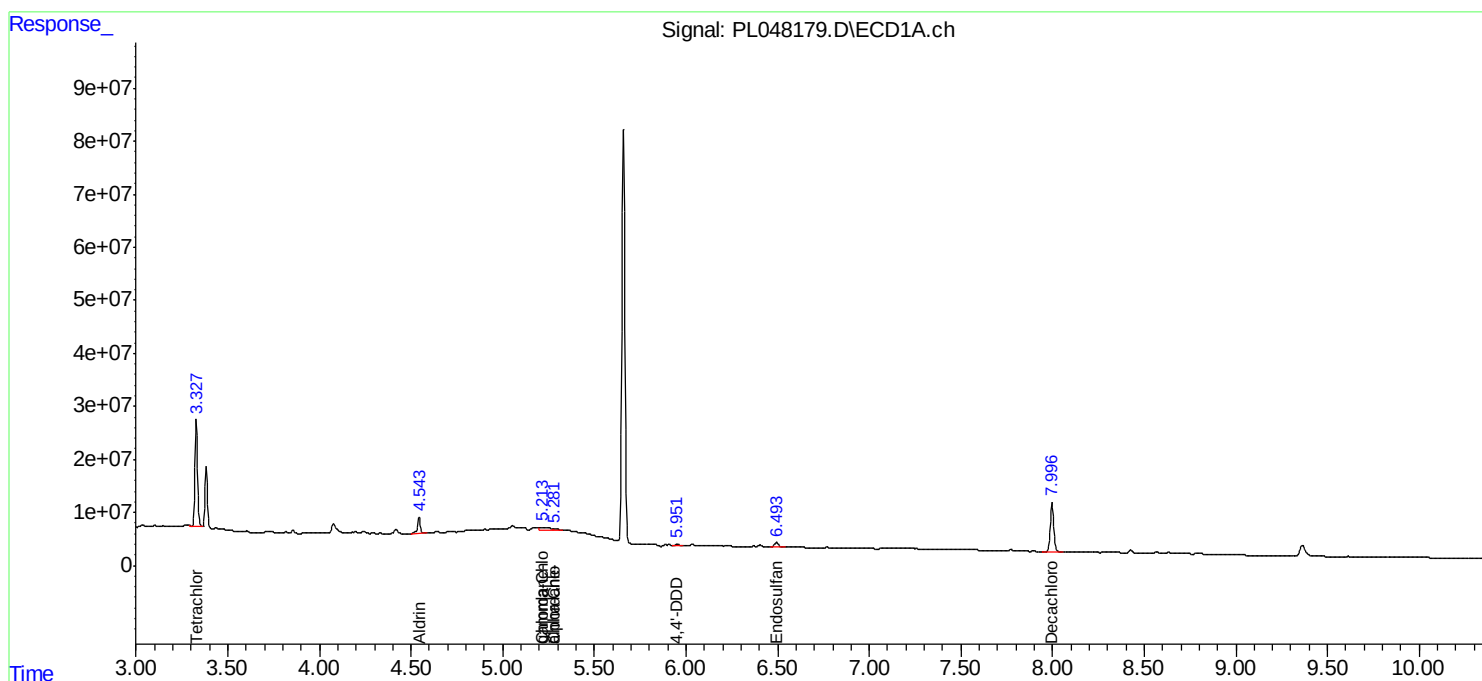


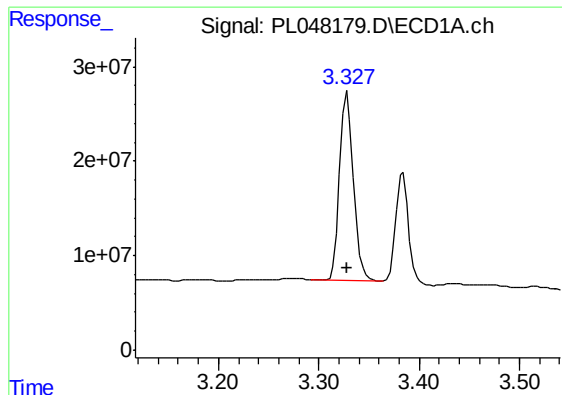

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 187286339
Conc: 19.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

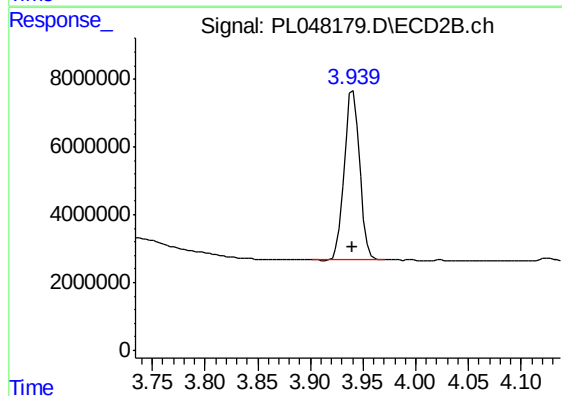


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.001 min
Response: 50288167
Conc: 20.19 ng/ml

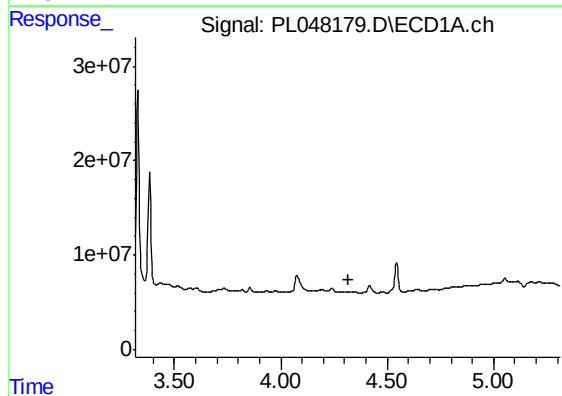


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

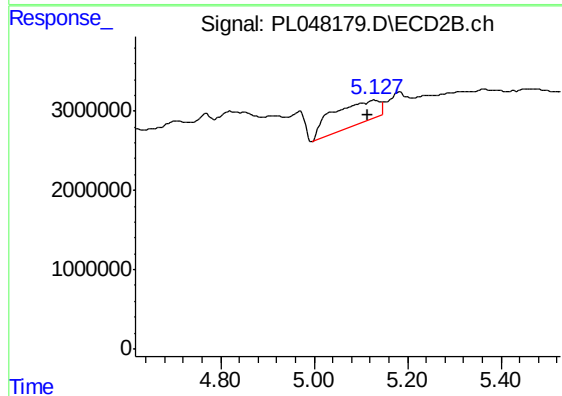

#4 Heptachlor


R.T.: 5.129 min
Delta R.T.: 0.013 min
Response: 20863743
Conc: 6.03 ng/ml

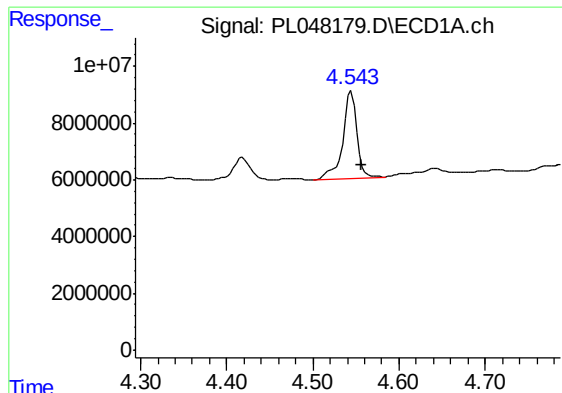

#5 Aldrin


R.T.: 4.545 min
Delta R.T.: -0.011 min
Response: 35070381
Conc: 2.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

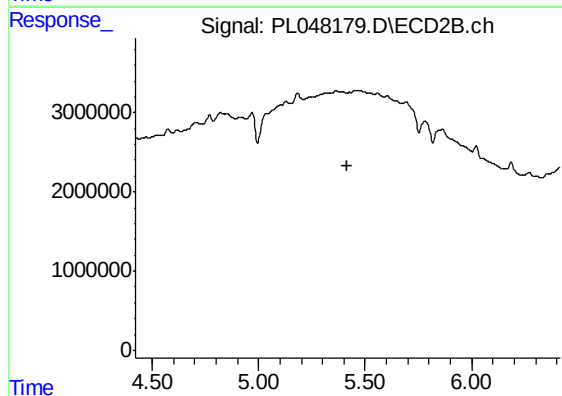


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.418 min
Response: 0
Conc: N.D.

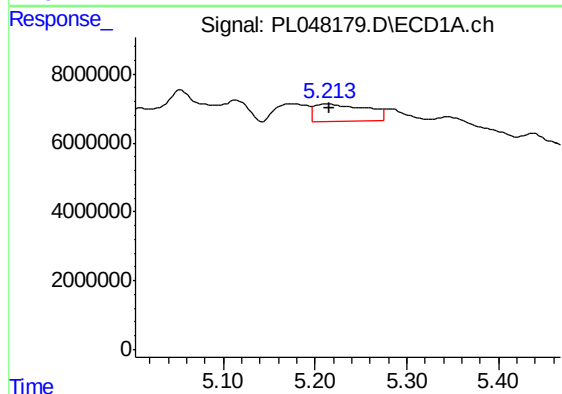


#10 gamma-Chlordane

R.T.: 5.214 min
Delta R.T.: -0.001 min
Response: 19362832
Conc: 1.45 ng/ml

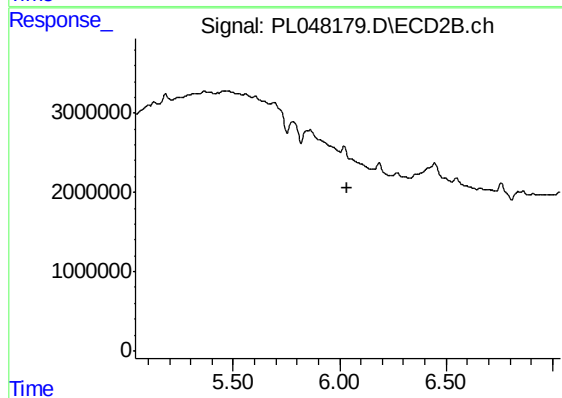

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

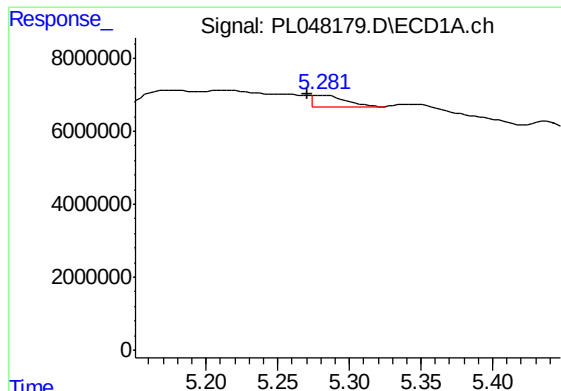

#11 alpha-Chlordane


R.T.: 5.282 min
Delta R.T.: 0.011 min
Response: 5377445
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

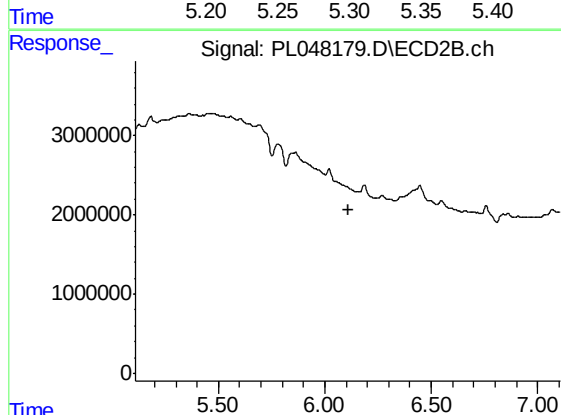


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

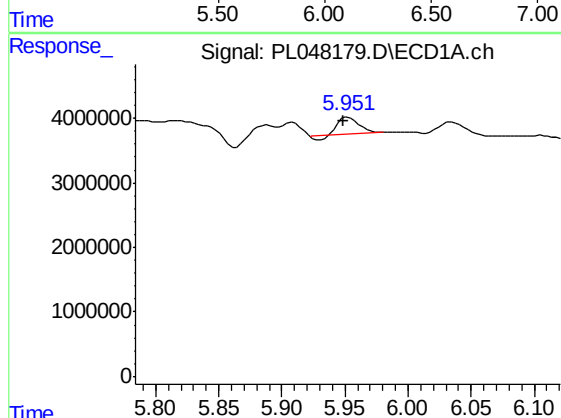


#16 4,4'-DDD

R.T.: 5.953 min
Delta R.T.: 0.003 min
Response: 2599082
Conc: 0.27 ng/ml

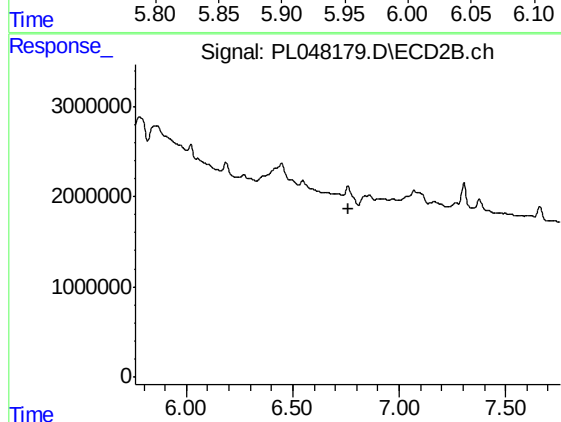

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

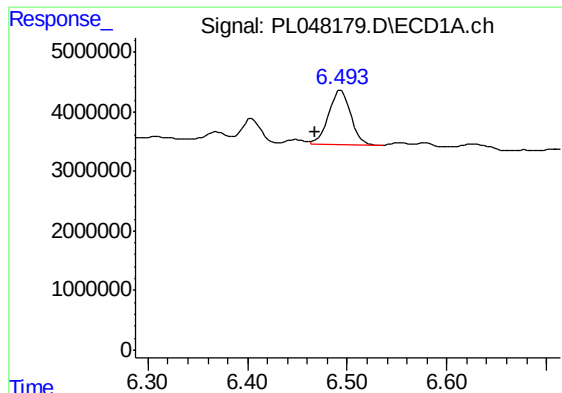

#19 Endosulfan Sulfate


R.T.: 6.494 min
Delta R.T.: 0.026 min
Response: 13882311
Conc: 1.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

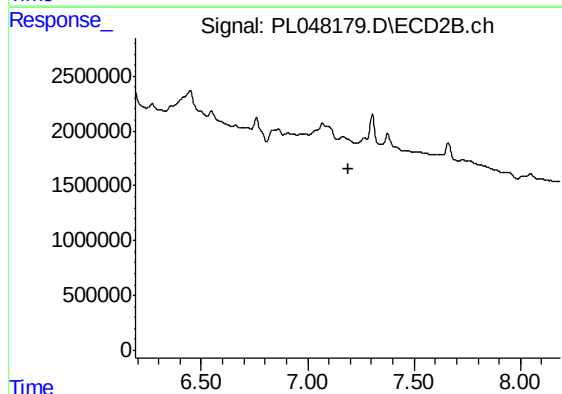


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.190 min
Response: 0
Conc: N.D.

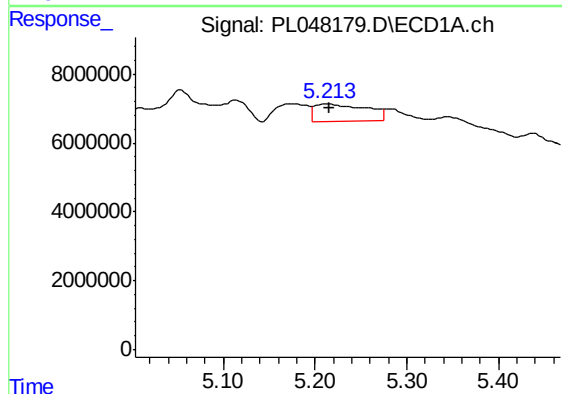


#25 Chlordane-3

R.T.: 5.214 min
Delta R.T.: -0.001 min
Response: 19362832
Conc: 12.30 ng/ml

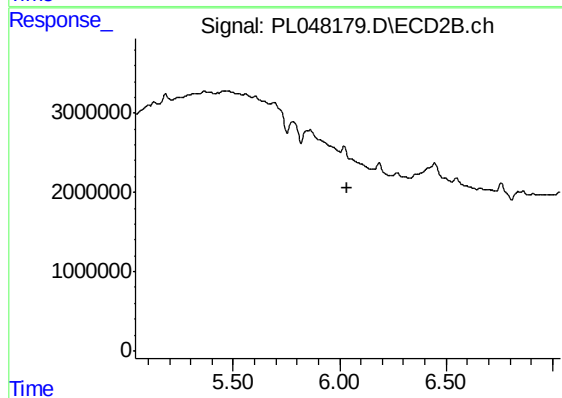

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

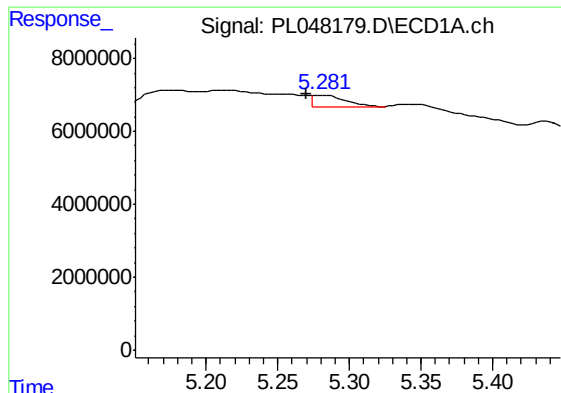

#26 Chlordane-4


R.T.: 5.282 min
Delta R.T.: 0.012 min
Response: 5377445
Conc: 3.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

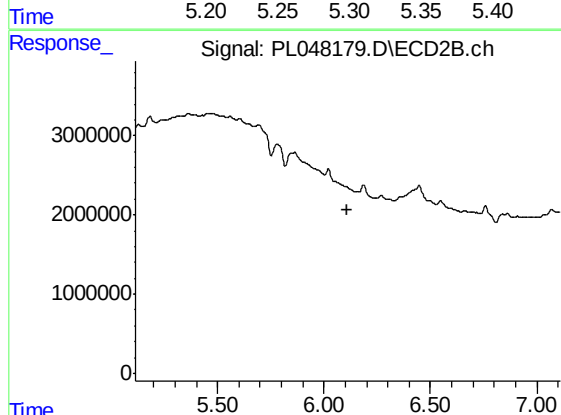


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

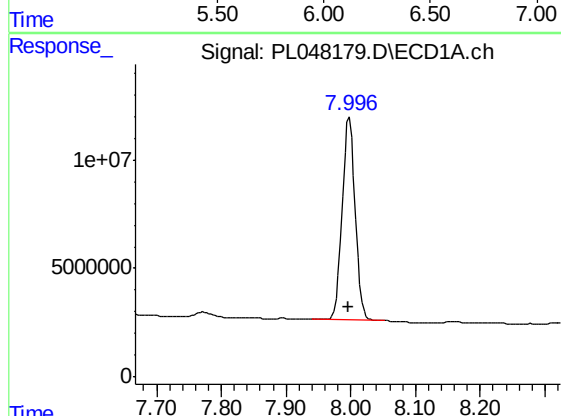

#28 Decachlorobiphenyl

R.T.: 7.998 min
Delta R.T.: 0.002 min
Response: 130557852
Conc: 12.99 ng/ml

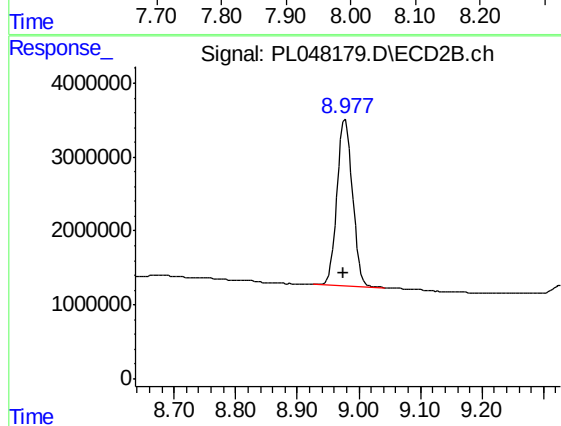

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: 0.003 min
Response: 39278475
Conc: 14.80 ng/ml