

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050319\
 Data File : PL048180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2019 17:41
 Operator : AJ\SJ
 Sample : K2668-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 23:05:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	190.9E6	51503742	19.711	20.677
28)	SA Decachlor...	7.998	8.979	141.0E6	41850304	14.022	15.767
Target Compounds							
5)	MB Aldrin	4.545	0.000	5475496	0	0.400	N.D. #
10)	B gamma-Chl...	5.217	0.000	16785774	0	1.257	N.D. #
11)	B alpha-Chl...	5.280	0.000	5407398	0	0.414	N.D. #
16)	A 4,4'-DDD	5.953	0.000	1556432	0	0.160	N.D. #
17)	MA 4,4'-DDT	0.000	7.073f	0	297173	N.D.	0.127 #
19)	B Endosulfa...	6.488f	0.000	23280057	0	2.169	N.D. #
25)	Chlordane-3	5.217	0.000	16785774	0	10.661	N.D. #
26)	Chlordane-4	5.280	0.000	5407398	0	3.725	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050319\
Data File : PL048180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2019 17:41
Operator : AJ\SJ
Sample : K2668-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 23:05:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

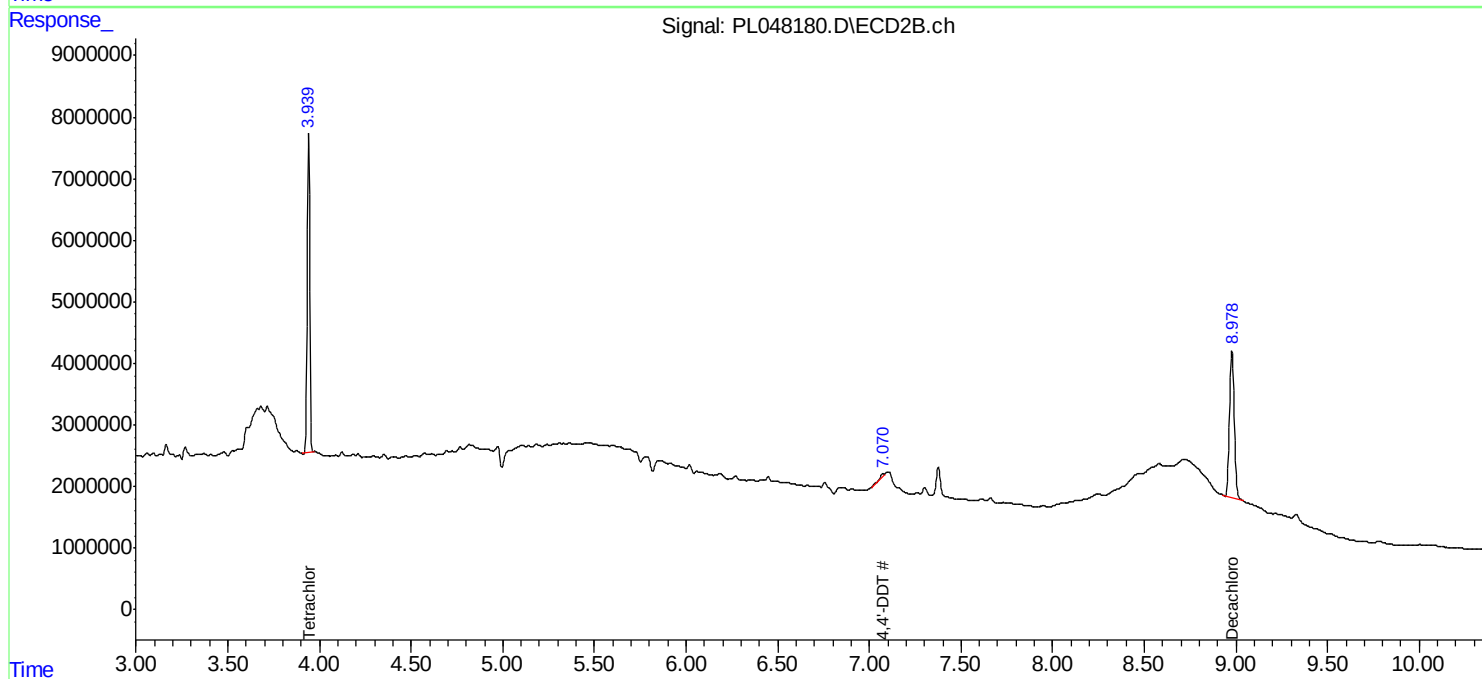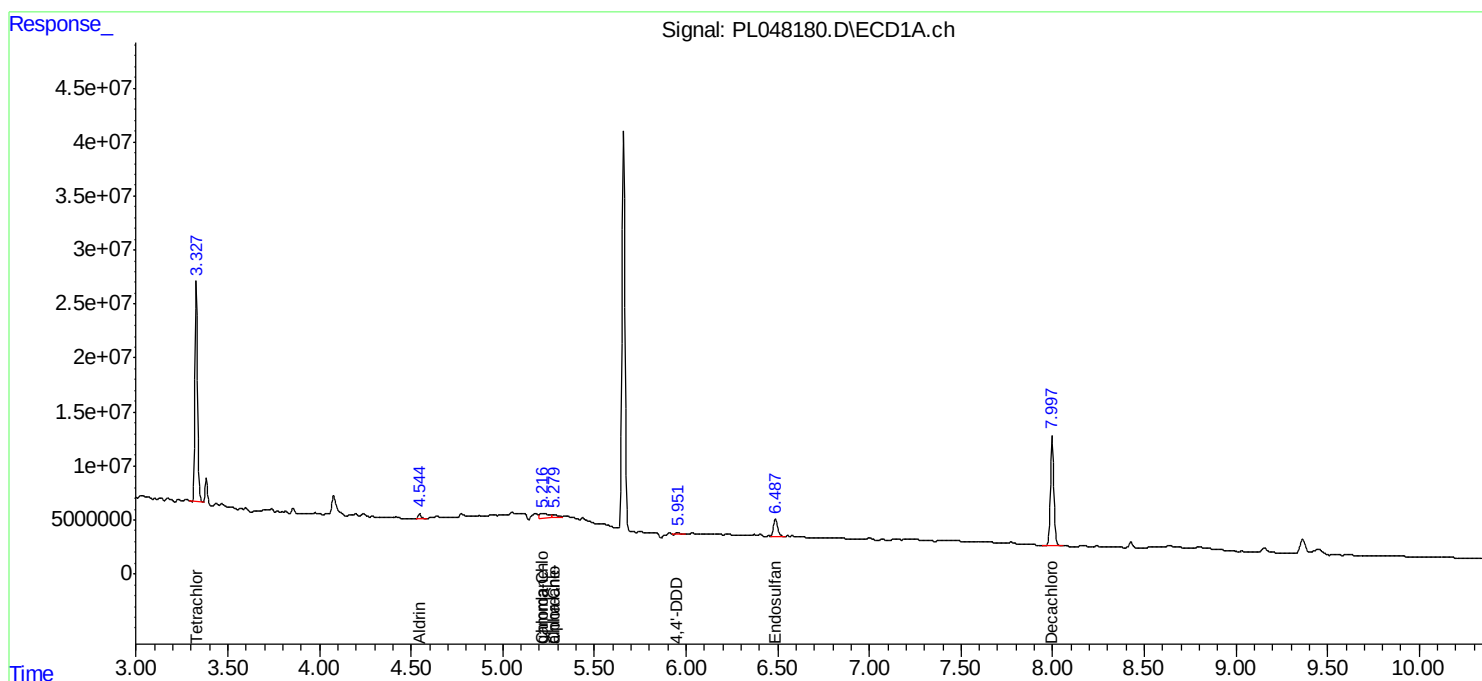


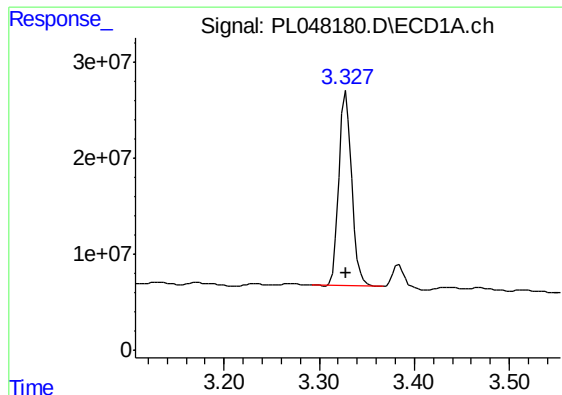

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 190941881
Conc: 19.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

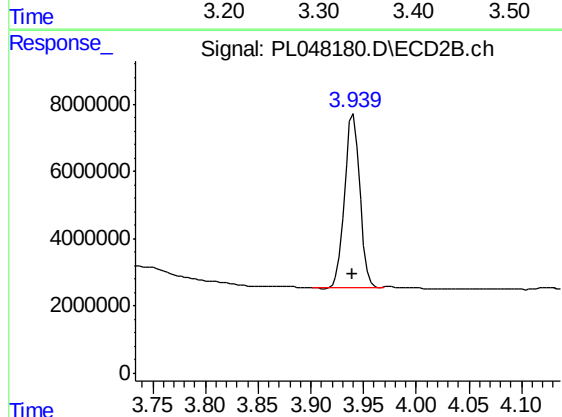


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 51503742
Conc: 20.68 ng/ml

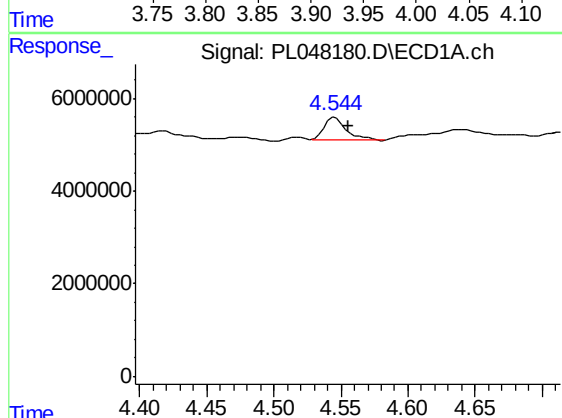


#5 Aldrin

R.T.: 4.545 min
Delta R.T.: -0.010 min
Response: 5475496
Conc: 0.40 ng/ml

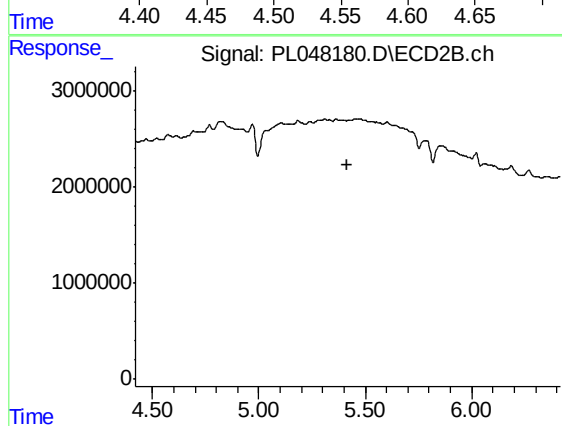

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.418 min
Response: 0
Conc: N.D.

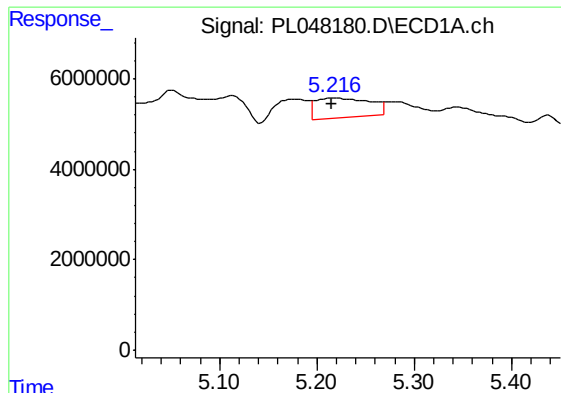

#10 gamma-Chlordane


R.T.: 5.217 min
Delta R.T.: 0.002 min
Response: 16785774
Conc: 1.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

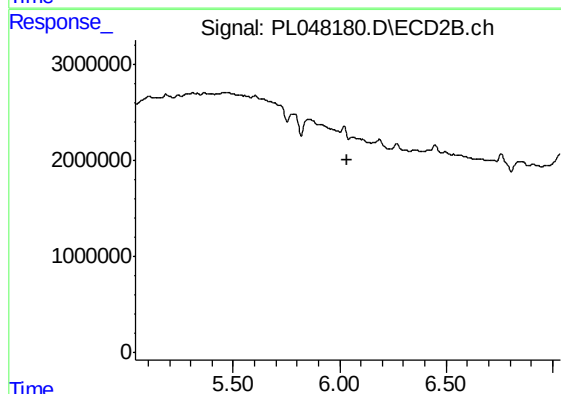


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

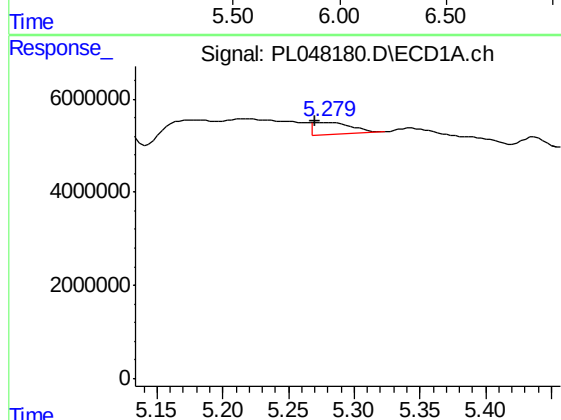


#11 alpha-Chlordane

R.T.: 5.280 min
Delta R.T.: 0.009 min
Response: 5407398
Conc: 0.41 ng/ml

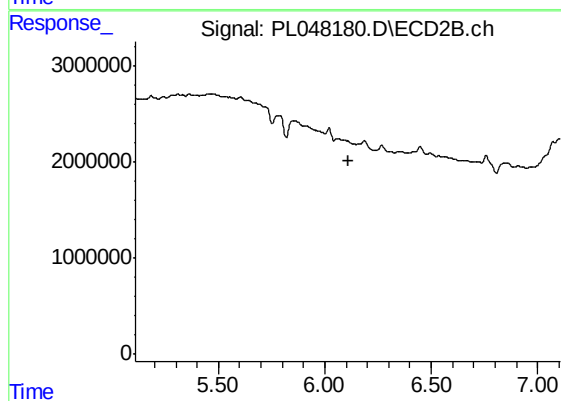

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

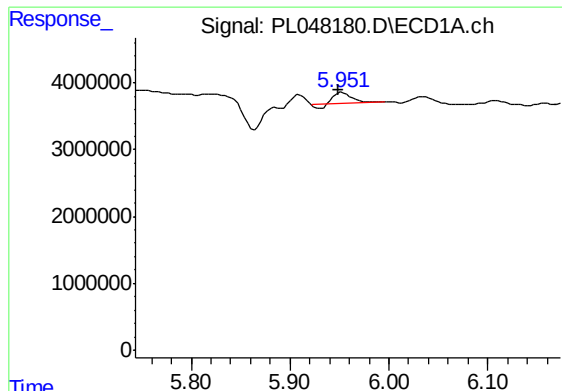

#16 4,4'-DDD


R.T.: 5.953 min
Delta R.T.: 0.004 min
Response: 1556432
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

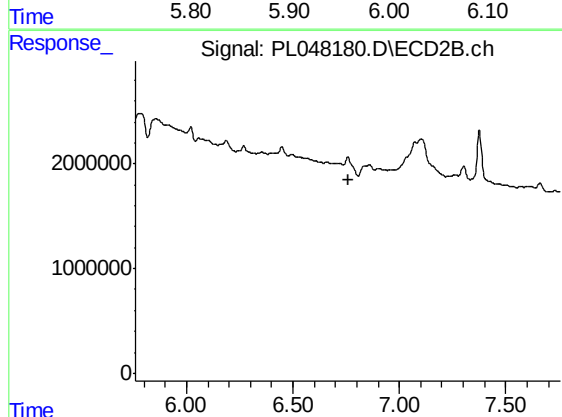


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

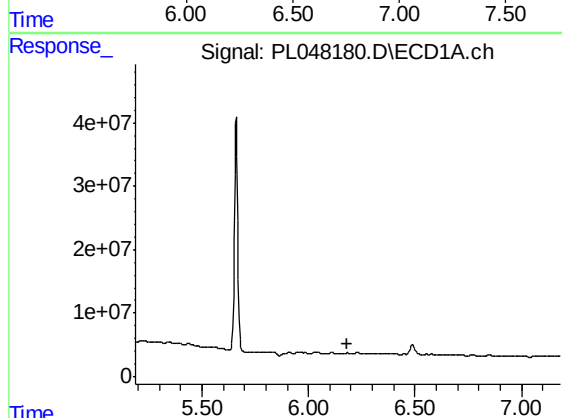


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.184 min
Response: 0
Conc: N.D.

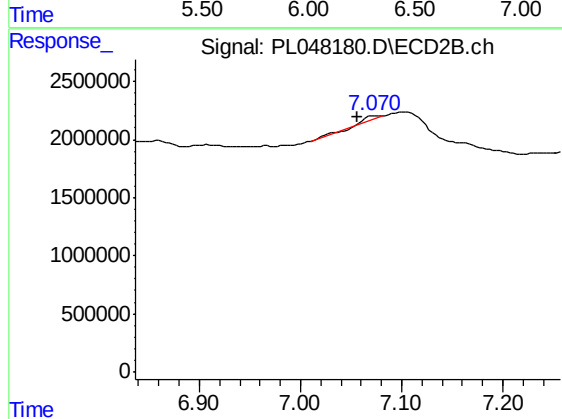

#17 4,4'-DDT


R.T.: 7.073 min
Delta R.T.: 0.017 min
Response: 297173
Conc: 0.13 ng/ml

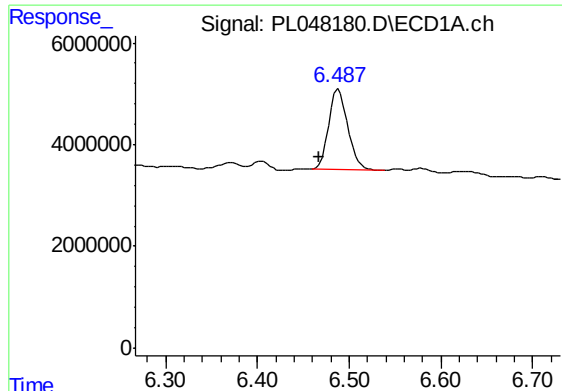

#19 Endosulfan Sulfate


R.T.: 6.488 min
Delta R.T.: 0.021 min
Response: 23280057
Conc: 2.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

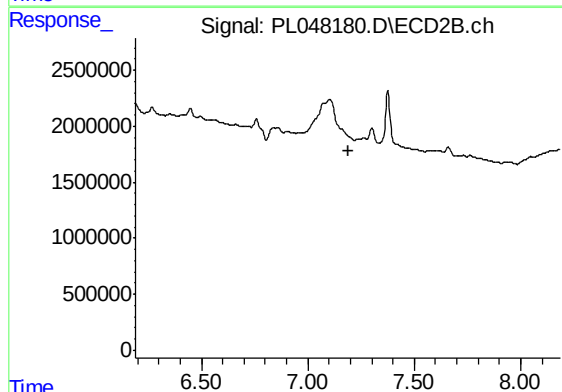


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.190 min
Response: 0
Conc: N.D.

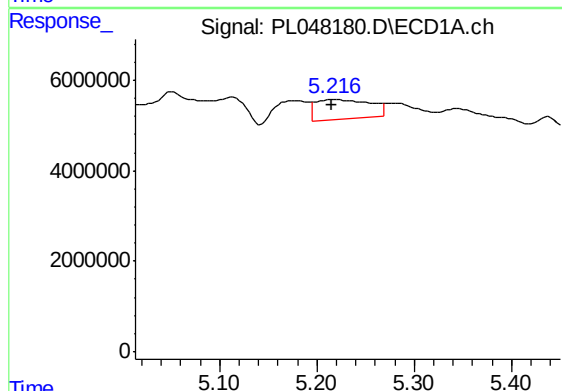


#25 Chlordane-3

R.T.: 5.217 min
Delta R.T.: 0.002 min
Response: 16785774
Conc: 10.66 ng/ml

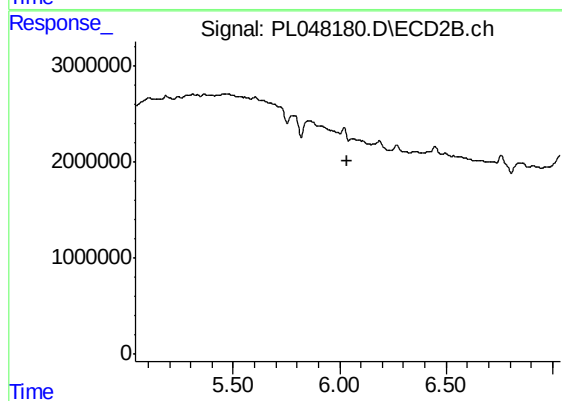

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

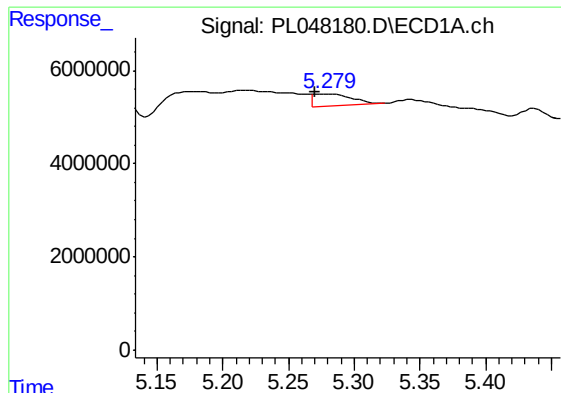

#26 Chlordane-4


R.T.: 5.280 min
Delta R.T.: 0.009 min
Response: 5407398
Conc: 3.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

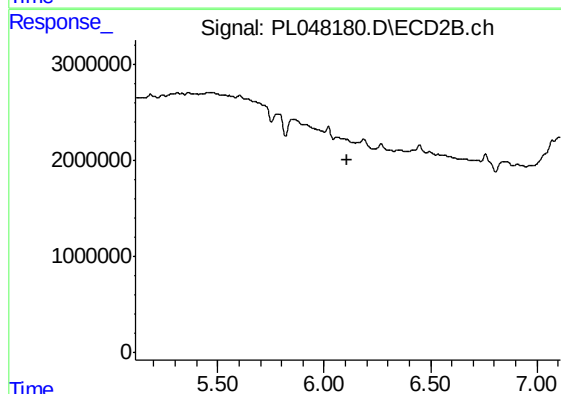


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

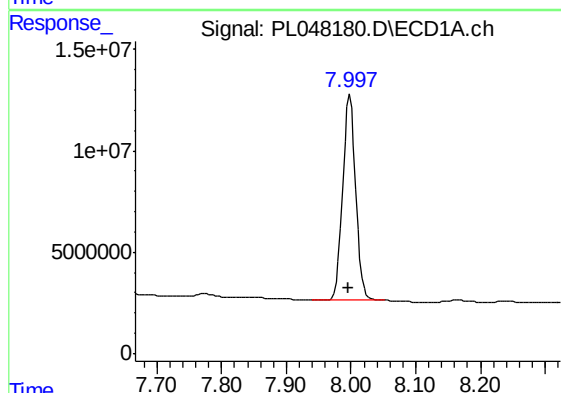

#28 Decachlorobiphenyl

R.T.: 7.998 min
Delta R.T.: 0.002 min
Response: 140976102
Conc: 14.02 ng/ml

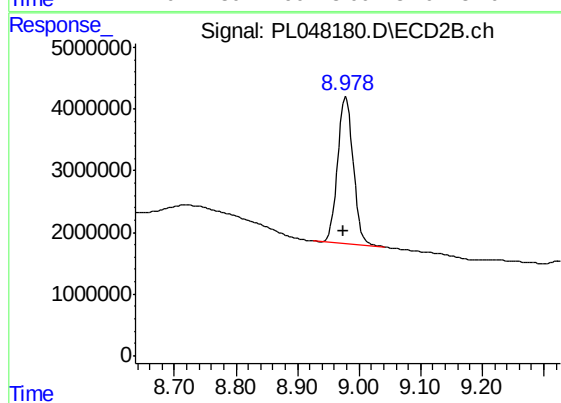

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: 0.004 min
Response: 41850304
Conc: 15.77 ng/ml