

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050319\
 Data File : PL048192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2019 21:12
 Operator : AJ\SJ
 Sample : K2635-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-05-050219-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 23:09:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.941	189.6E6	49630303	19.574	19.925
28)	SA Decachlor...	7.998	8.979	149.5E6	43571884	14.865	16.416
Target Compounds							
4)	MA Heptachlor	4.289f	5.128	5544192	16694102	0.377	4.822 #
5)	MB Aldrin	4.557	0.000	7365319	0	0.538	N.D. #
6)	B beta-BHC	4.289	0.000	5544192	0	0.939	N.D. #
7)	B delta-BHC	4.460f	4.976f	2411296	10414233	0.171	3.683 #
14)	MA Endrin	5.807	0.000	16054930	0	1.319	N.D. #
15)	B Endosulfa...	6.107f	0.000	4689034	0	0.406	N.D. #
19)	B Endosulfa...	6.490f	0.000	7124920	0	0.664	N.D. #
23)	Chlordane-1	4.165	0.000	5874720	0	13.087	N.D. #
27)	Chlordane-5	6.107f	0.000	4689034	0	9.986	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050319\
Data File : PL048192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2019 21:12
Operator : AJ\SJ
Sample : K2635-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 23:09:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

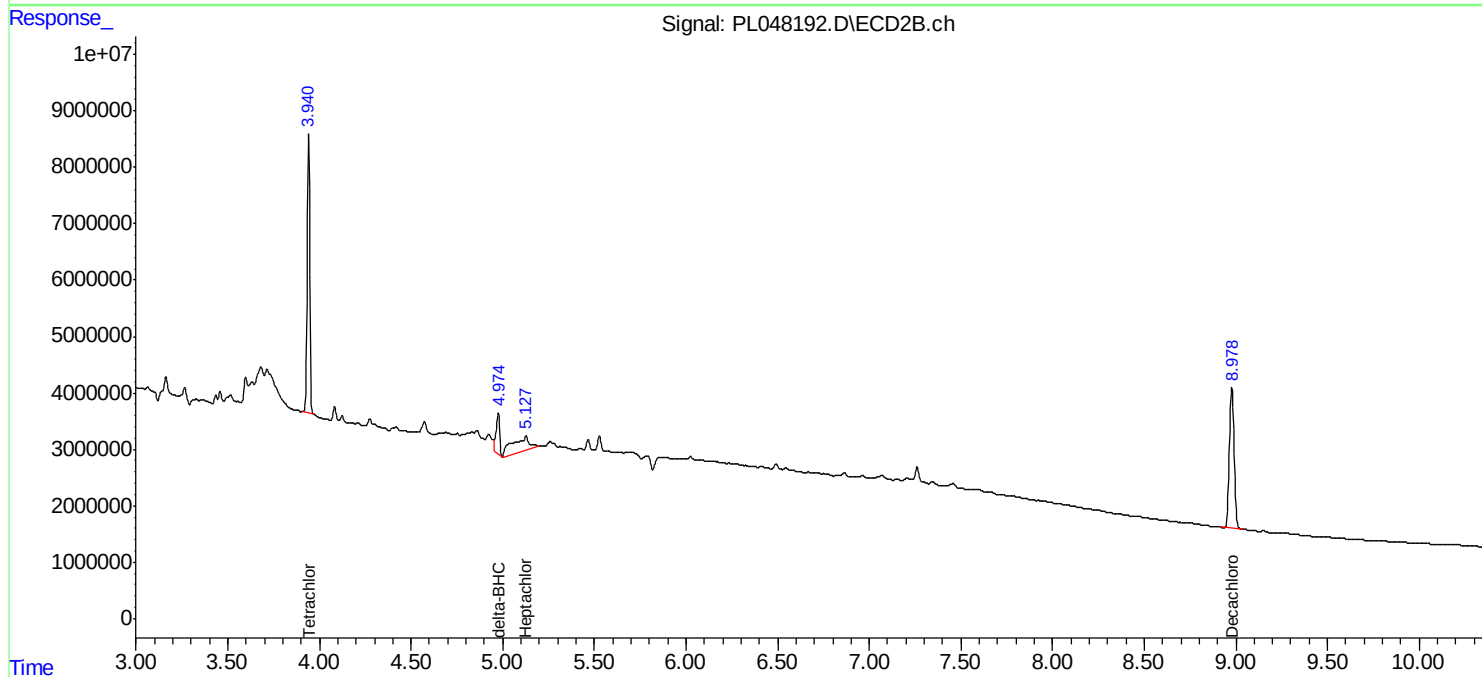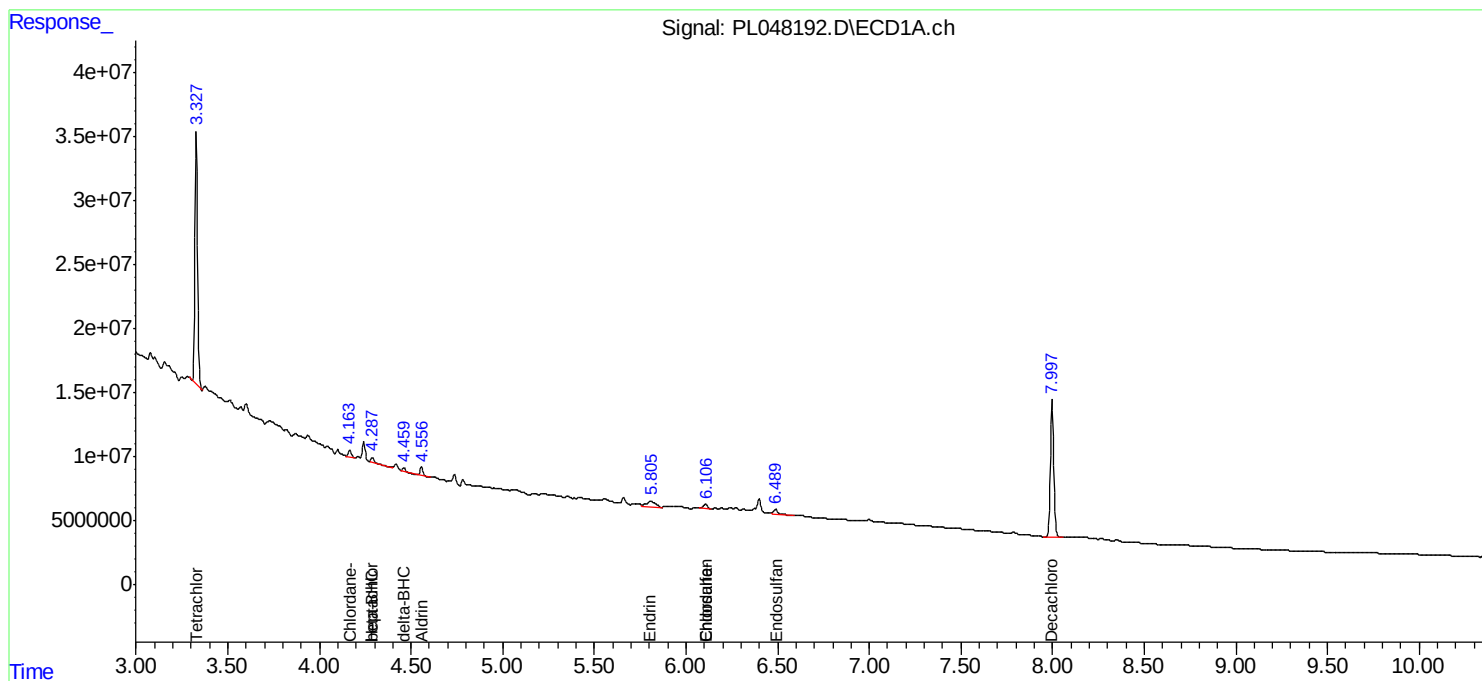


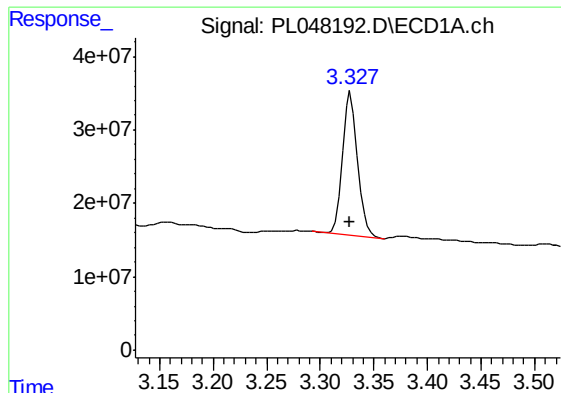

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 189606616
Conc: 19.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-C

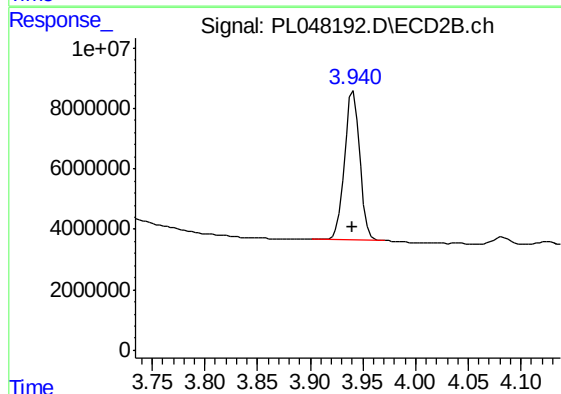


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.001 min
Response: 49630303
Conc: 19.92 ng/ml

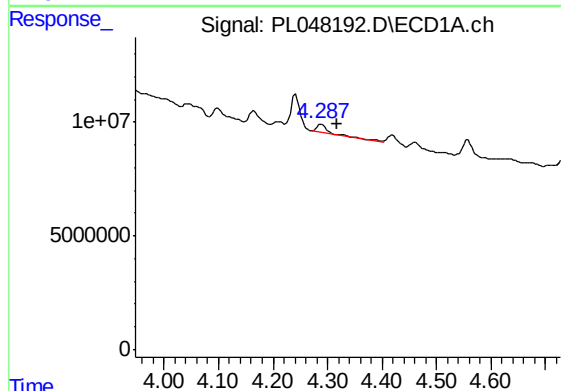


#4 Heptachlor

R.T.: 4.289 min
Delta R.T.: -0.028 min
Response: 5544192
Conc: 0.38 ng/ml

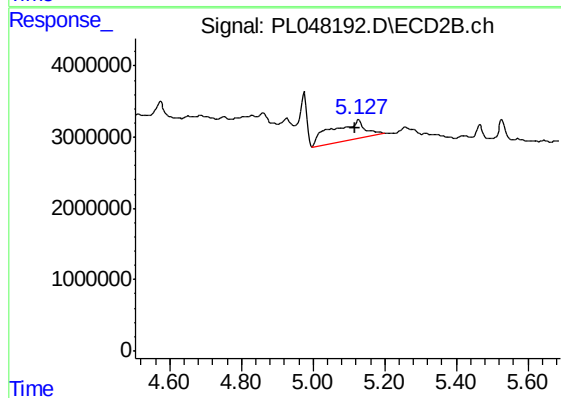

#4 Heptachlor


R.T.: 5.128 min
Delta R.T.: 0.012 min
Response: 16694102
Conc: 4.82 ng/ml

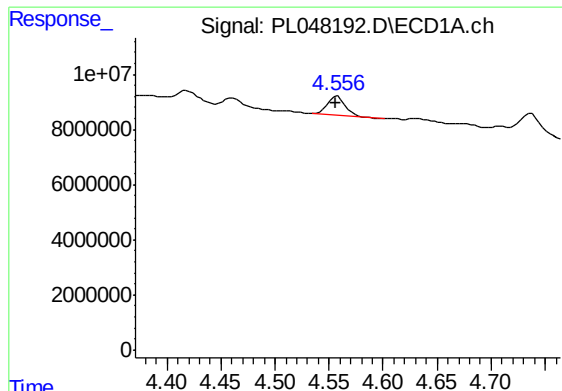

#5 Aldrin


R.T.: 4.557 min
Delta R.T.: 0.002 min
Response: 7365319
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-C

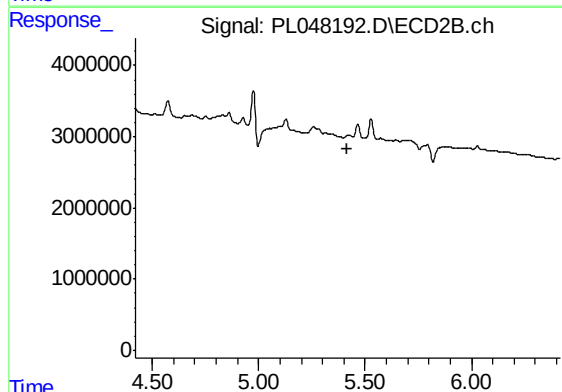


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.418 min
Response: 0
Conc: N.D.

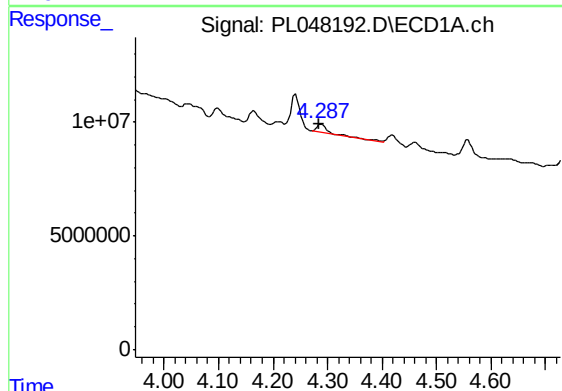


#6 beta-BHC

R.T.: 4.289 min
Delta R.T.: 0.003 min
Response: 5544192
Conc: 0.94 ng/ml

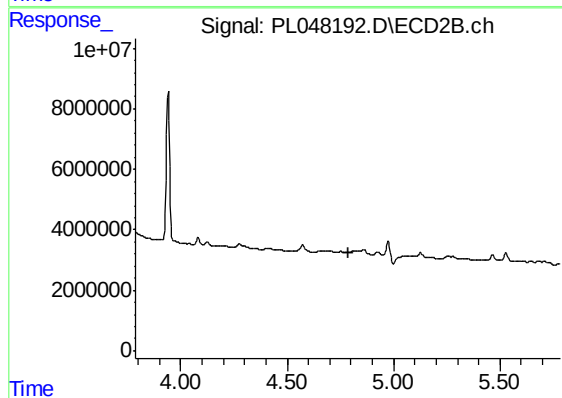

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.786 min
Response: 0
Conc: N.D.

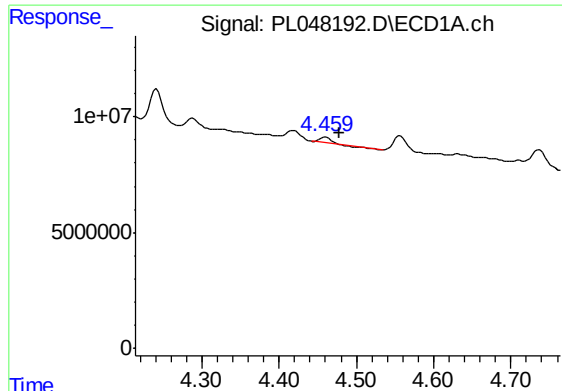

#7 delta-BHC


R.T.: 4.460 min
Delta R.T.: -0.019 min
Response: 2411296
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-C

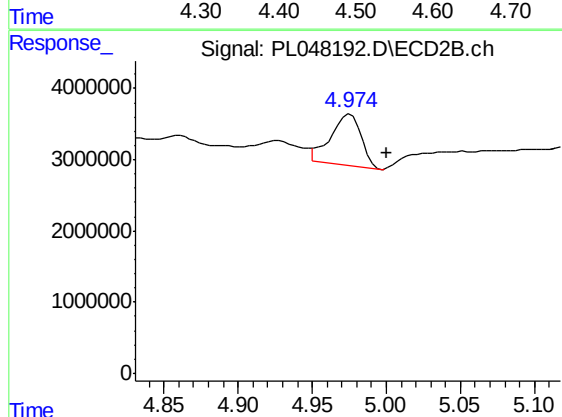


#7 delta-BHC

R.T.: 4.976 min
Delta R.T.: -0.024 min
Response: 10414233
Conc: 3.68 ng/ml

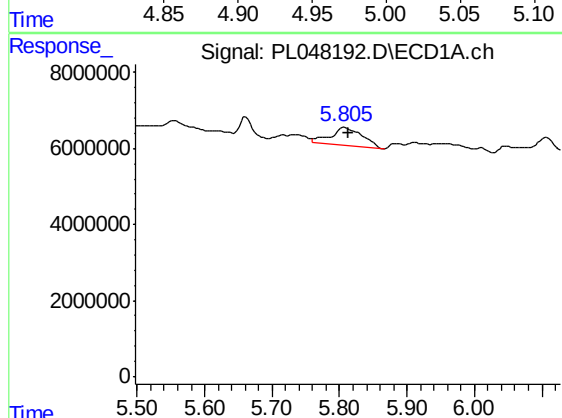


#14 Endrin

R.T.: 5.807 min
Delta R.T.: -0.008 min
Response: 16054930
Conc: 1.32 ng/ml

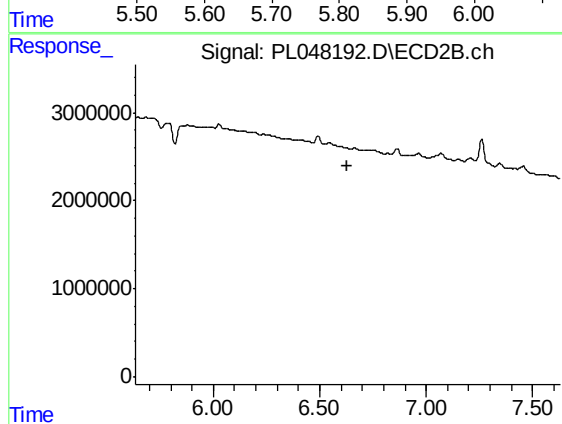

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

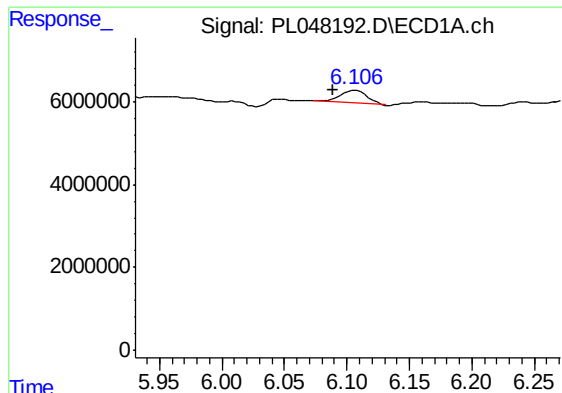

#15 Endosulfan II


R.T.: 6.107 min
Delta R.T.: 0.018 min
Response: 4689034
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-C

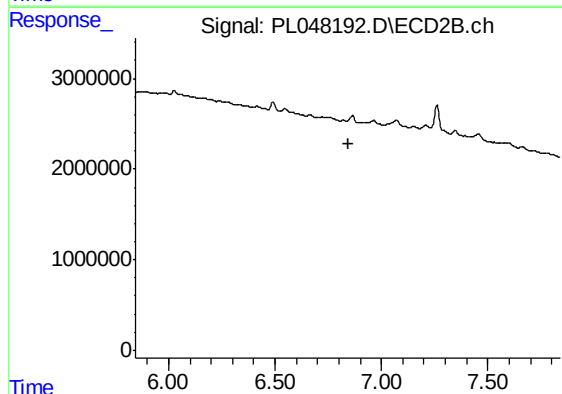


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.

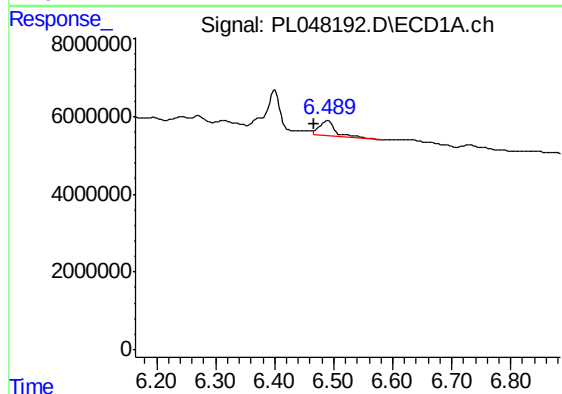


#19 Endosulfan Sulfate

R.T.: 6.490 min
Delta R.T.: 0.023 min
Response: 7124920
Conc: 0.66 ng/ml

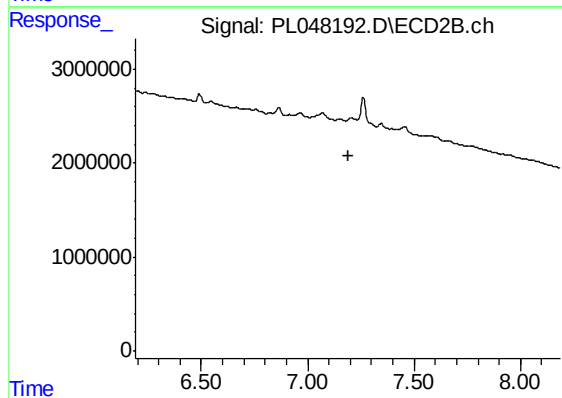

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.190 min
Response: 0
Conc: N.D.

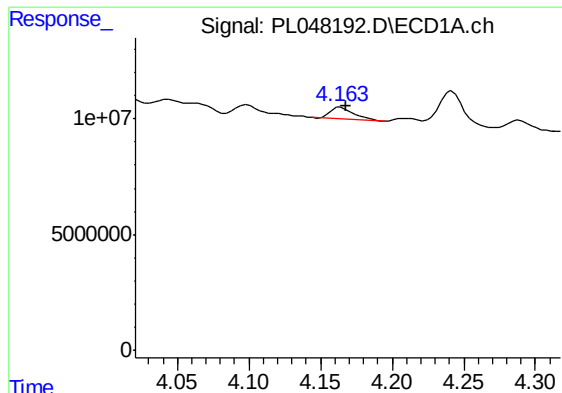

#23 Chlordane-1


R.T.: 4.165 min
Delta R.T.: -0.003 min
Response: 5874720
Conc: 13.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-C

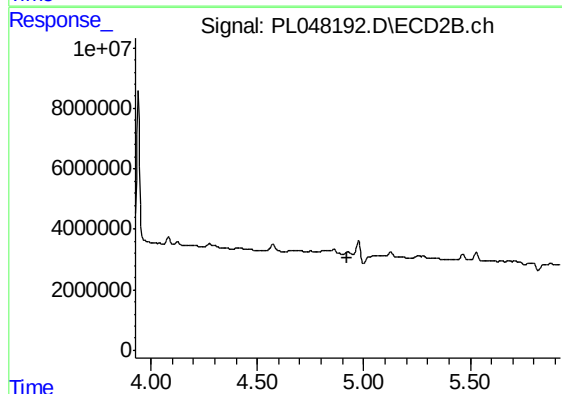


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

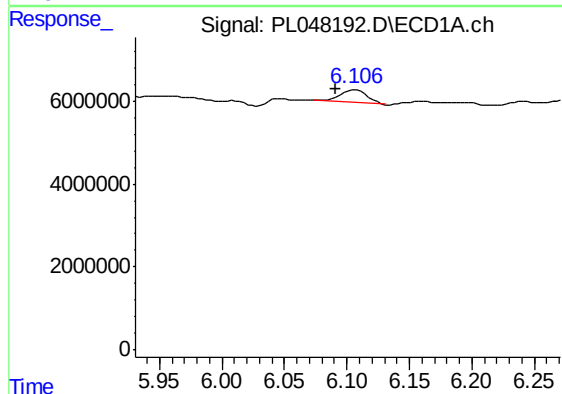


#27 Chlordane-5

R.T.: 6.107 min
Delta R.T.: 0.016 min
Response: 4689034
Conc: 9.99 ng/ml

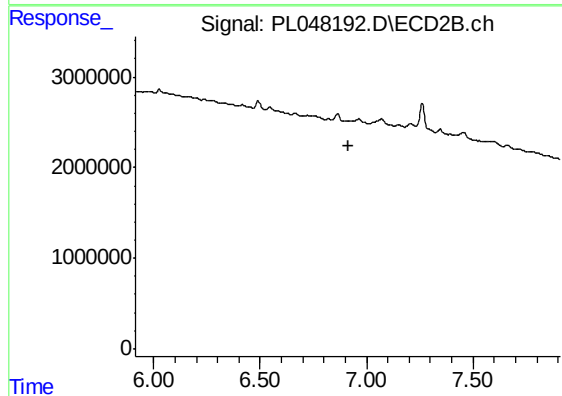

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.913 min
Response: 0
Conc: N.D.

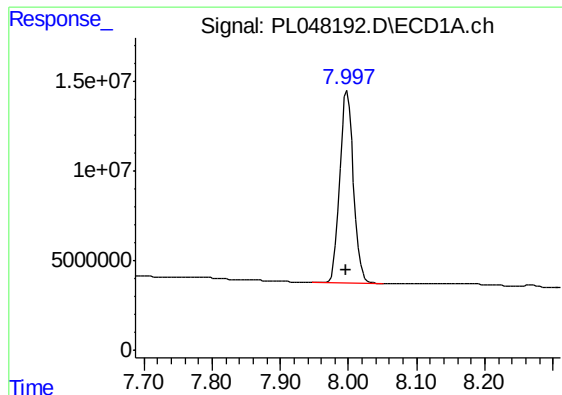

#28 Decachlorobiphenyl

R.T.: 7.998 min
Delta R.T.: 0.002 min
Response: 149455858
Conc: 14.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-C

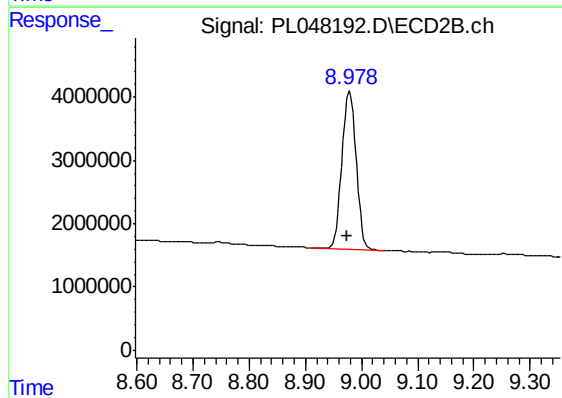

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: 0.004 min
Response: 43571884
Conc: 16.42 ng/ml