

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050319\
 Data File : PL048193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2019 21:27
 Operator : AJ\SJ
 Sample : K2635-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-05-050219-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 23:09:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.941	196.4E6	53195112	20.280	21.356
28)	SA Decachlor...	7.998	8.979	150.4E6	44083444	14.961	16.608
Target Compounds							
3)	MA gamma-BHC...	4.041	0.000	31210146	0	2.196	N.D. #
4)	MA Heptachlor	4.289f	5.125	2729629	12098475	0.186	3.495 #
6)	B beta-BHC	4.289	0.000	2729629	0	0.463	N.D. #
7)	B delta-BHC	0.000	4.974f	0	6997316	N.D.	2.474 #
14)	MA Endrin	5.826	0.000	13566159	0	1.114	N.D. #
15)	B Endosulfa...	6.108f	0.000	3510626	0	0.304	N.D. #
23)	Chlordane-1	4.180	0.000	3762487	0	8.381	N.D. #
27)	Chlordane-5	6.108f	0.000	3510626	0	7.476	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050319\
Data File : PL048193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2019 21:27
Operator : AJ\SJ
Sample : K2635-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
AU-05-050219-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 23:09:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

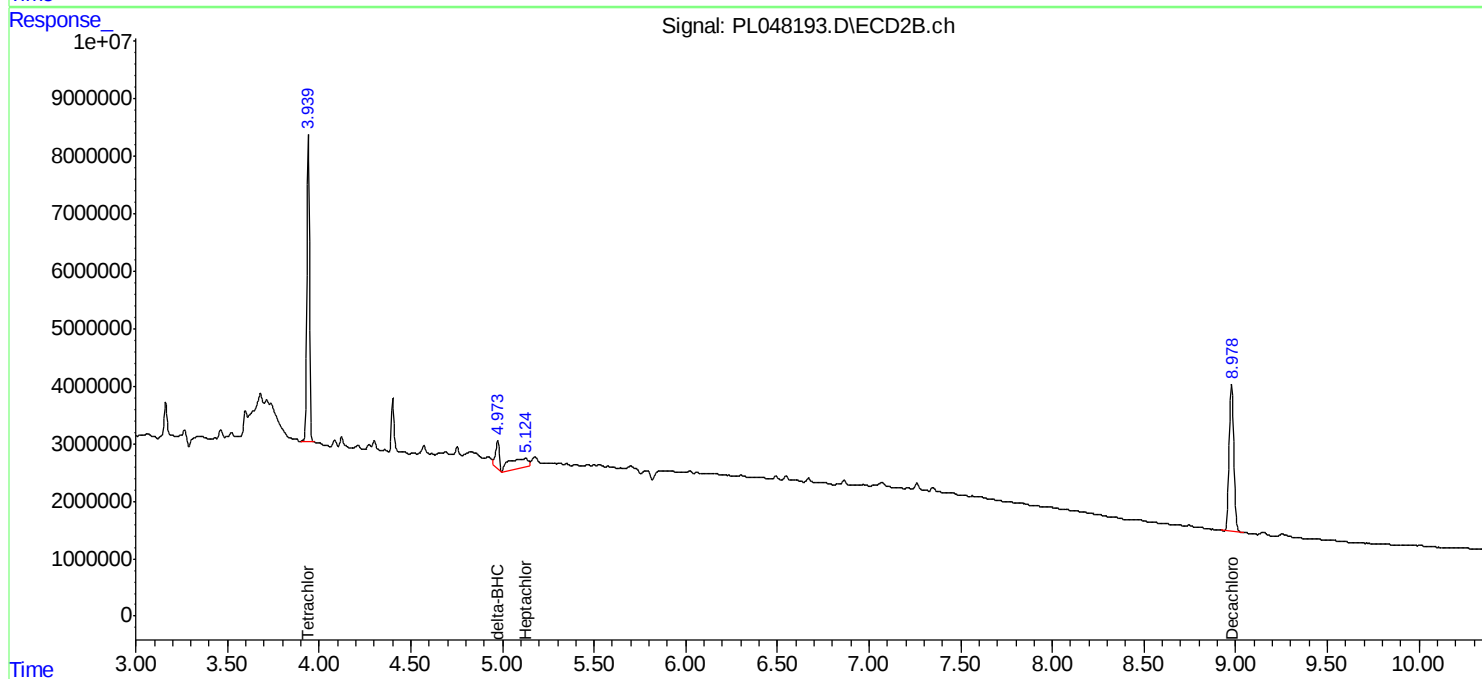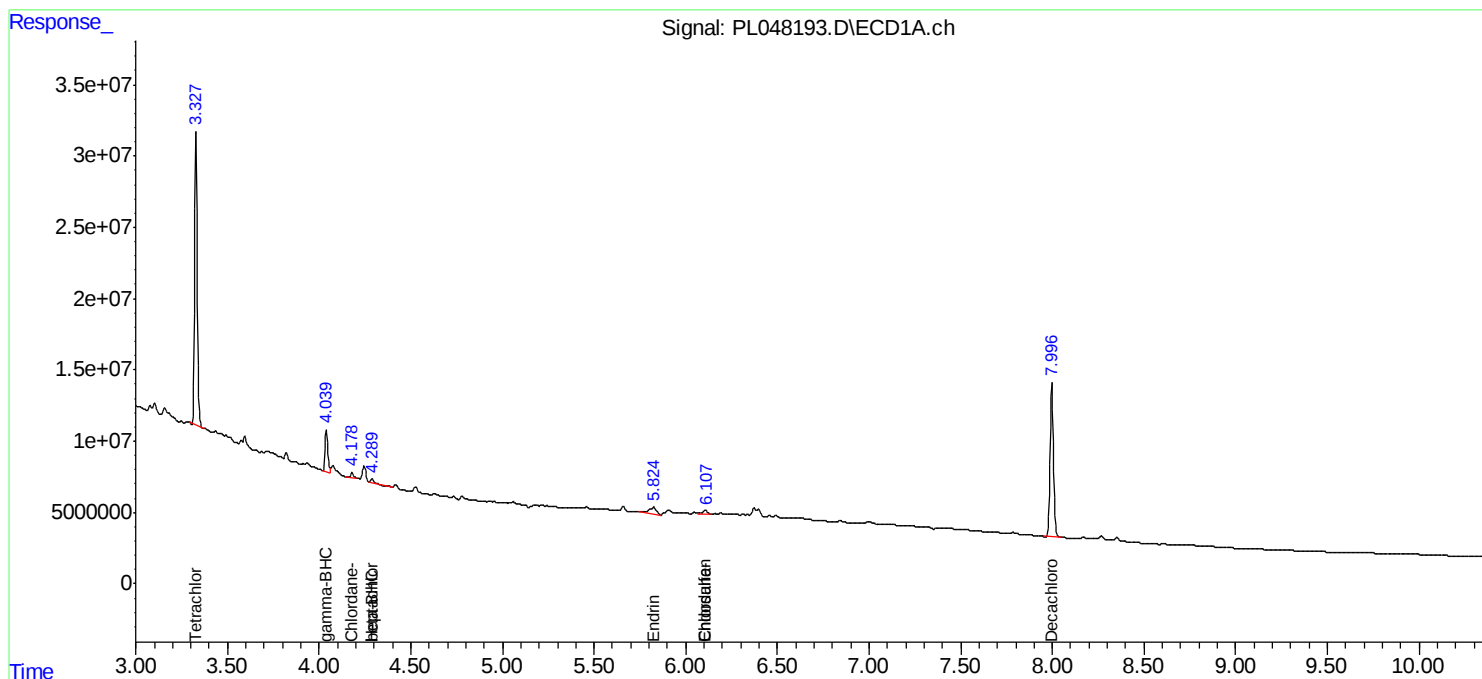


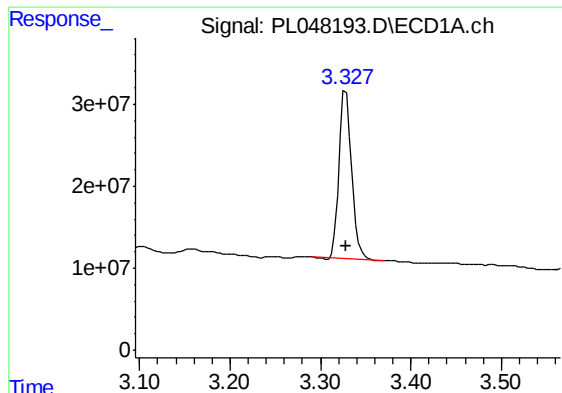

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 196445509
Conc: 20.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-D

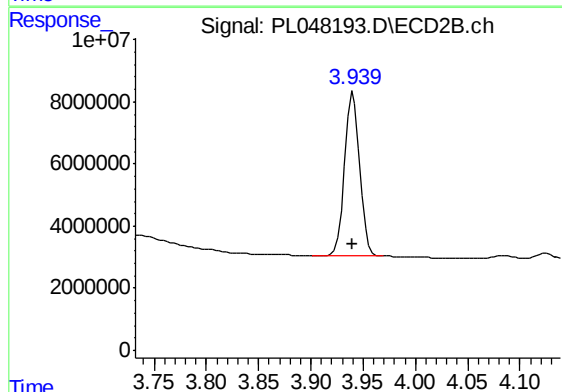


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 53195112
Conc: 21.36 ng/ml

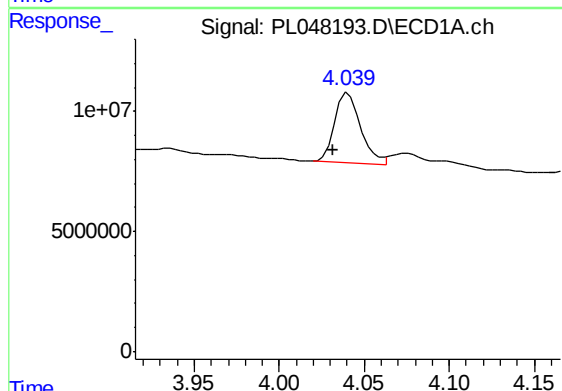


#3 gamma-BHC (Lindane)

R.T.: 4.041 min
Delta R.T.: 0.009 min
Response: 31210146
Conc: 2.20 ng/ml

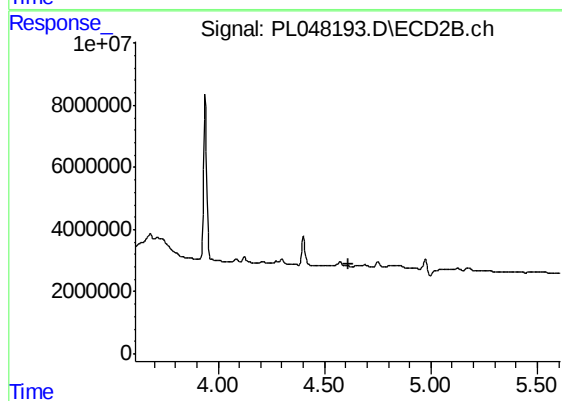

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

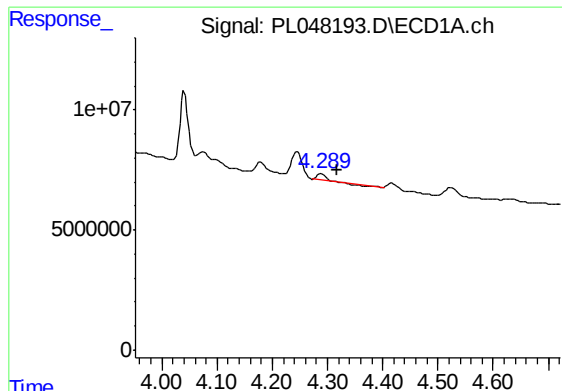

#4 Heptachlor


R.T.: 4.289 min
Delta R.T.: -0.028 min
Response: 2729629
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-D

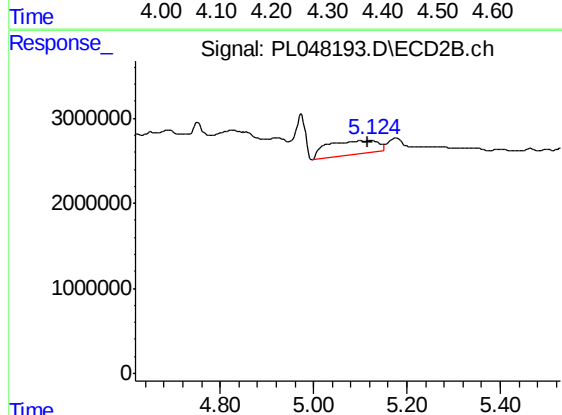


#4 Heptachlor

R.T.: 5.125 min
Delta R.T.: 0.010 min
Response: 12098475
Conc: 3.49 ng/ml

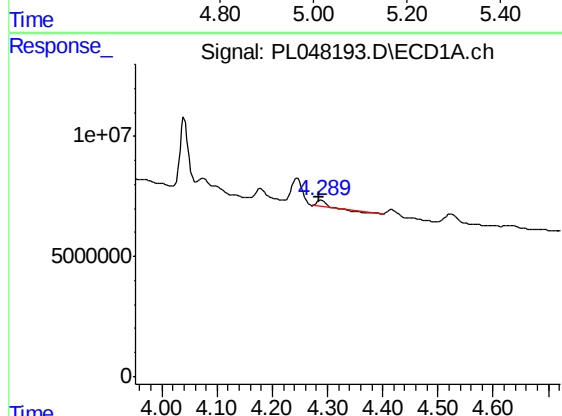


#6 beta-BHC

R.T.: 4.289 min
Delta R.T.: 0.004 min
Response: 2729629
Conc: 0.46 ng/ml

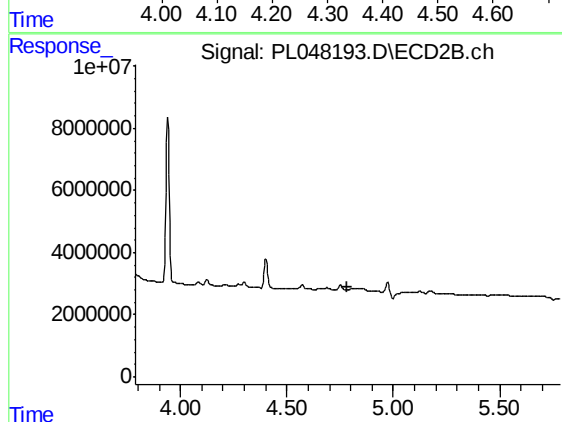

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.786 min
Response: 0
Conc: N.D.

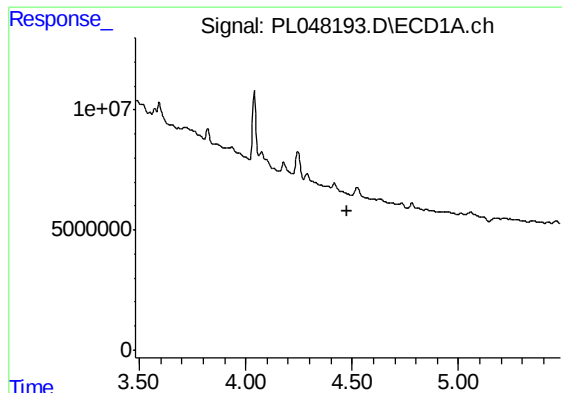

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-D

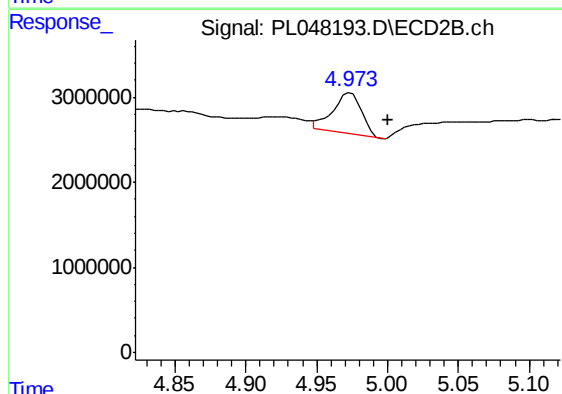


#7 delta-BHC

R.T.: 4.974 min
Delta R.T.: -0.026 min
Response: 6997316
Conc: 2.47 ng/ml

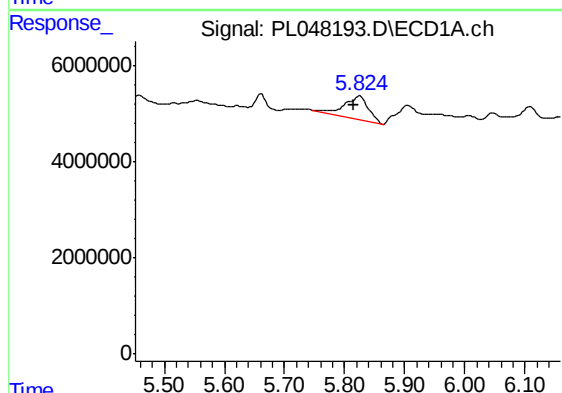


#14 Endrin

R.T.: 5.826 min
Delta R.T.: 0.011 min
Response: 13566159
Conc: 1.11 ng/ml

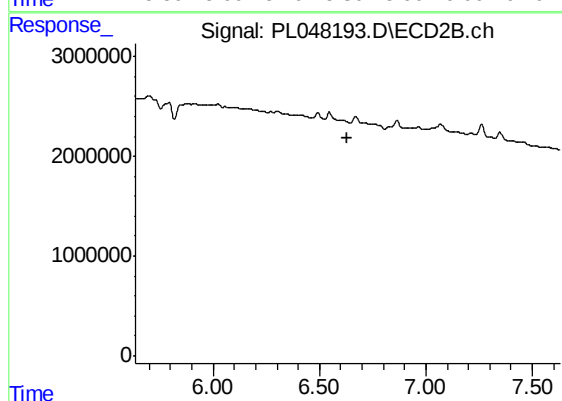

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

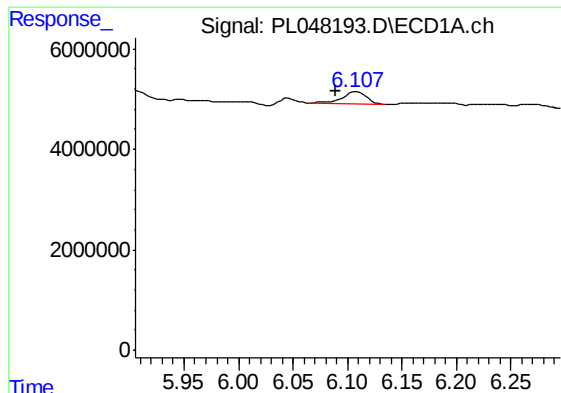

#15 Endosulfan II


R.T.: 6.108 min
Delta R.T.: 0.019 min
Response: 3510626
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-D

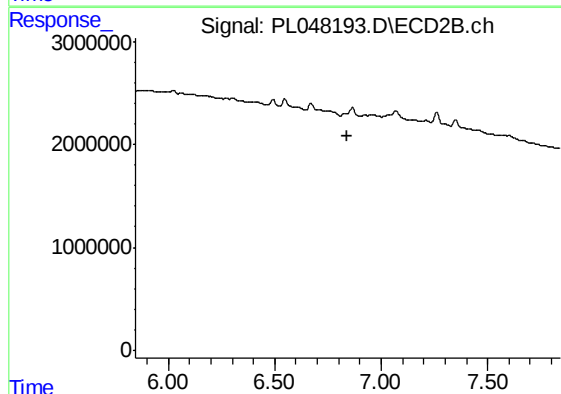


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.

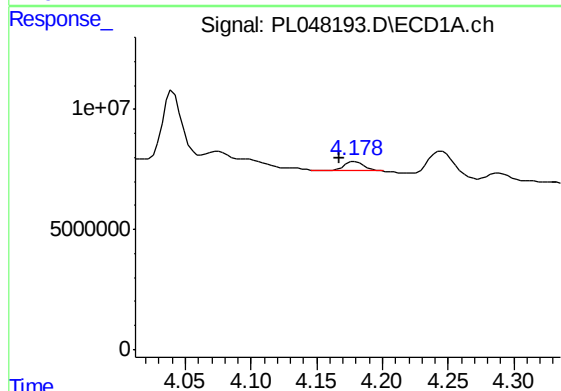


#23 Chlordane-1

R.T.: 4.180 min
Delta R.T.: 0.012 min
Response: 3762487
Conc: 8.38 ng/ml

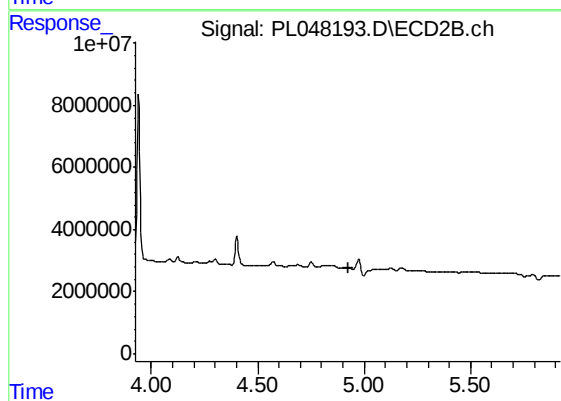

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

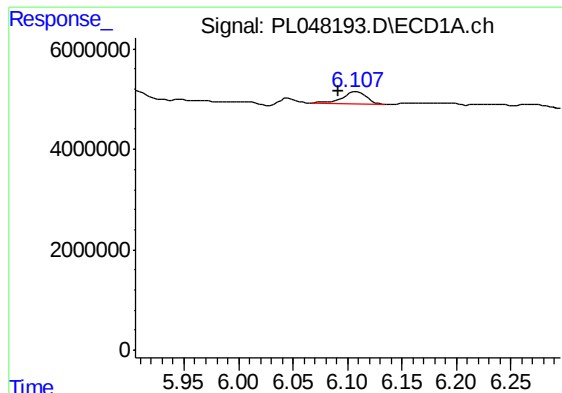

#27 Chlordane-5


R.T.: 6.108 min
Delta R.T.: 0.017 min
Response: 3510626
Conc: 7.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-050219-D

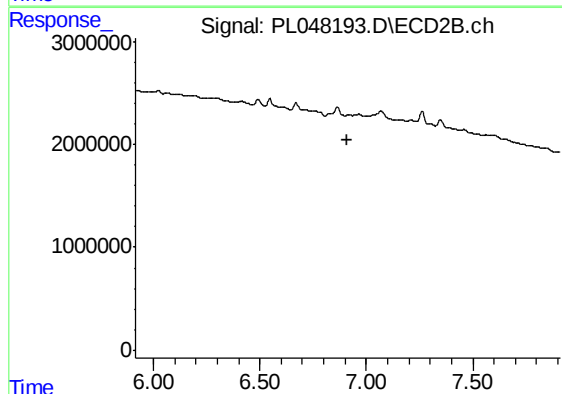


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.913 min
Response: 0
Conc: N.D.

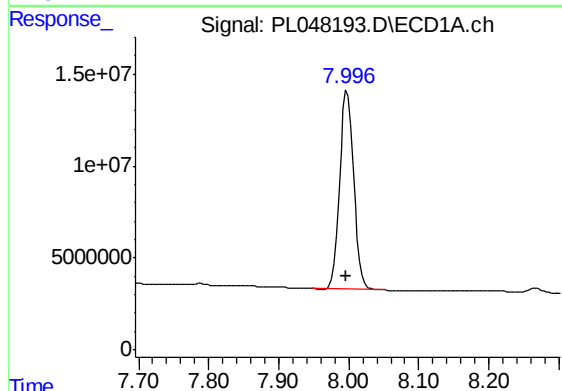

#28 Decachlorobiphenyl

R.T.: 7.998 min
Delta R.T.: 0.002 min
Response: 150423397
Conc: 14.96 ng/ml

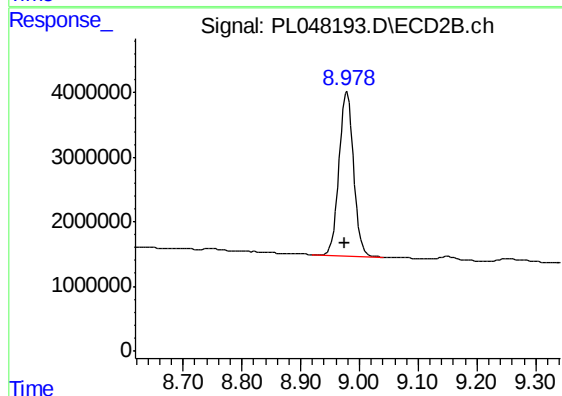

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: 0.004 min
Response: 44083444
Conc: 16.61 ng/ml