

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050321\
 Data File : PL066627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2021 12:11
 Operator : AR\AJ
 Sample : M2229-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

Ankita
 5/4/2021 4:38:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 10:34:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.152	40623102	56317043	10.781	16.035 #
28)	SA Decachlor...	8.171	9.355	42584505	37534195	11.106	12.133
Target Compounds							
12)	B 4,4'-DDE	5.578	6.541	117.2E6	144.6E6	25.681m	38.110 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050321\
Data File : PL066627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2021 12:11
Operator : AR\AJ
Sample : M2229-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-6


Manual Integrations
APPROVED

Ankita
5/4/2021 4:38:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 10:34:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

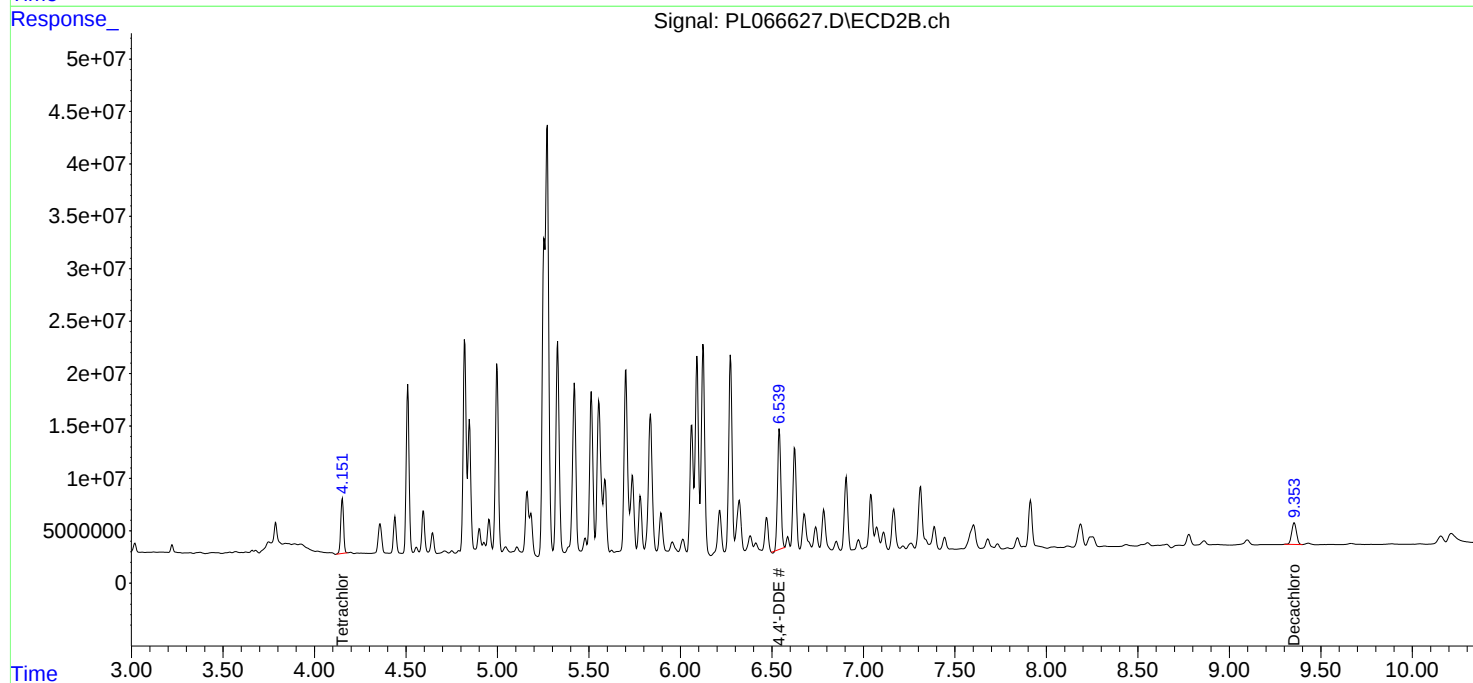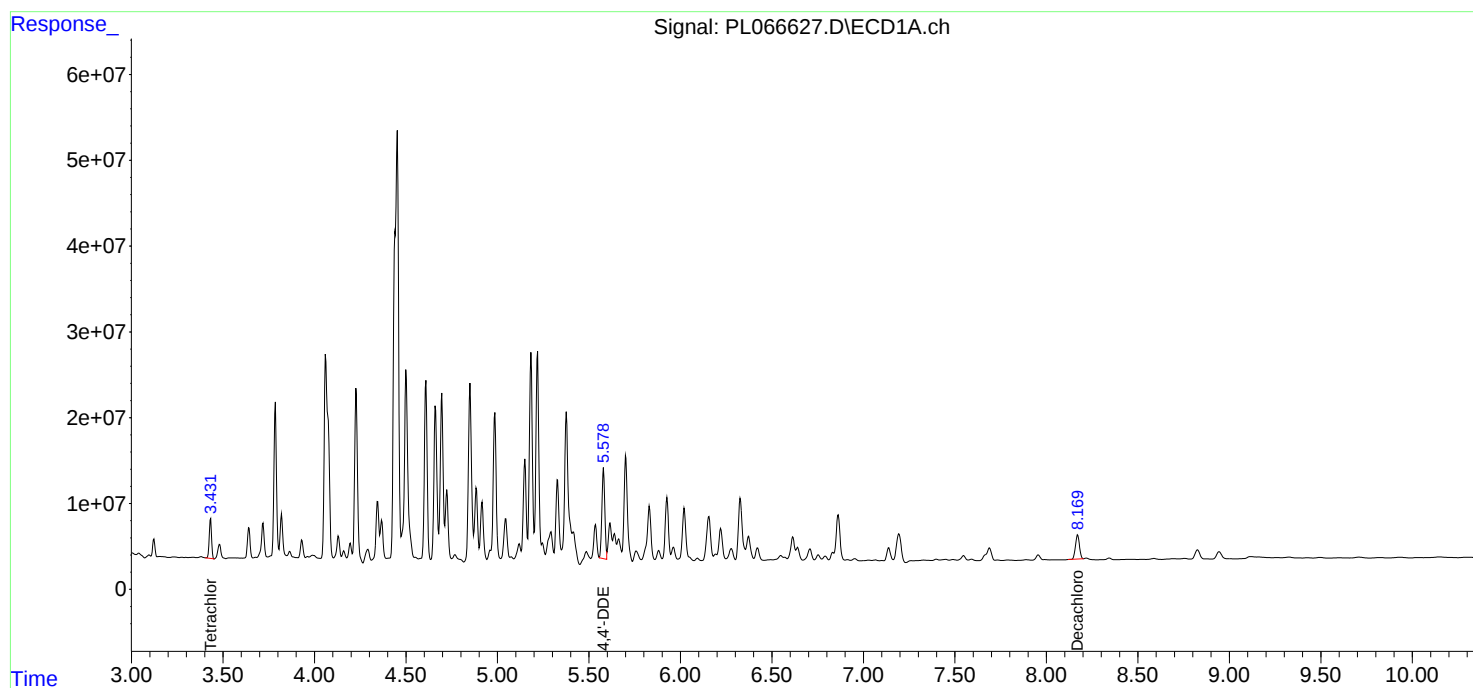

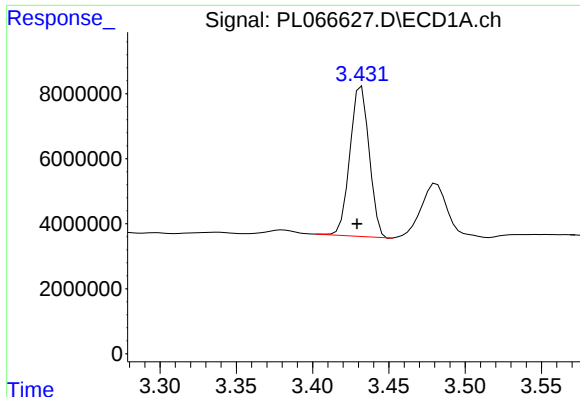


#1 Tetrachloro-m-xylene

R.T.: 3.432 min
Delta R.T.: 0.003 min
Response: 40623102
Conc: 10.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Ankita
5/4/2021 4:38:08 PM

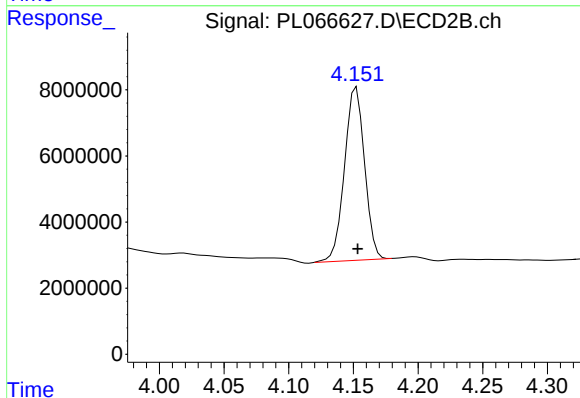


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: 0.000 min
Response: 56317043
Conc: 16.04 ng/ml

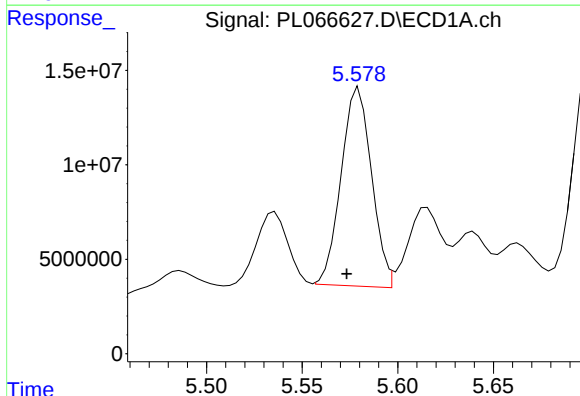


#12 4,4'-DDE

R.T.: 5.578 min
Delta R.T.: 0.005 min
Response: 117181791
Conc: 25.68 ng/ml m

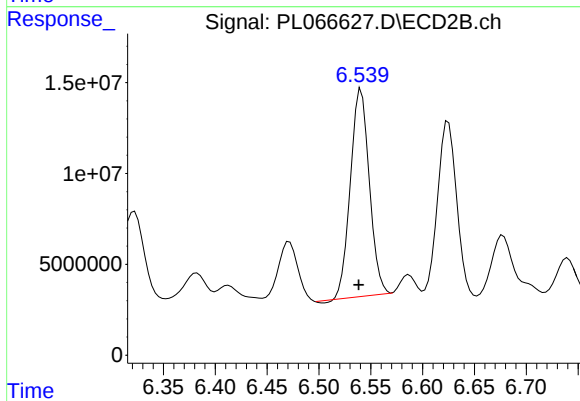

#12 4,4'-DDE

R.T.: 6.541 min
Delta R.T.: 0.002 min
Response: 144597979
Conc: 38.11 ng/ml

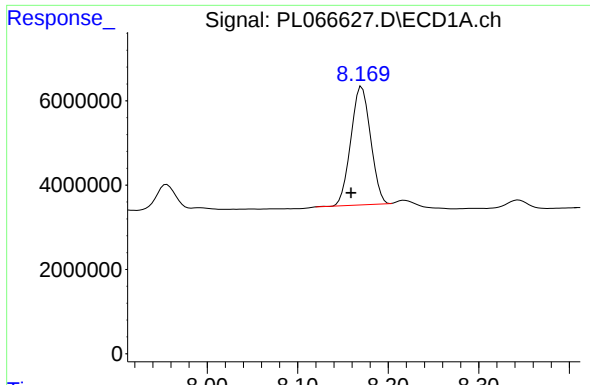


#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.012 min
Response: 42584505
Conc: 11.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

Manual Integrations
APPROVED

Ankita
5/4/2021 4:38:08 PM

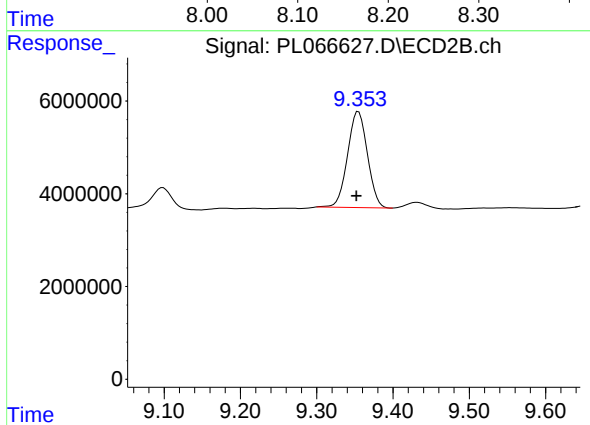

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.003 min
Response: 37534195
Conc: 12.13 ng/ml