

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050321\
 Data File : PL066629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2021 12:39
 Operator : AR\AJ
 Sample : M2224-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-042921

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 05:23:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.427	4.152	46303014	45804367	12.288	13.042
28)	SA Decachlor...	8.161	9.351	47499402	43377292	12.388	14.022
Target Compounds							
17)	MA 4,4'-DDT	6.321	7.338	2356394	1721955	0.604	0.532



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050321\
Data File : PL066629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2021 12:39
Operator : AR\AJ
Sample : M2224-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-01-042921

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 05:23:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

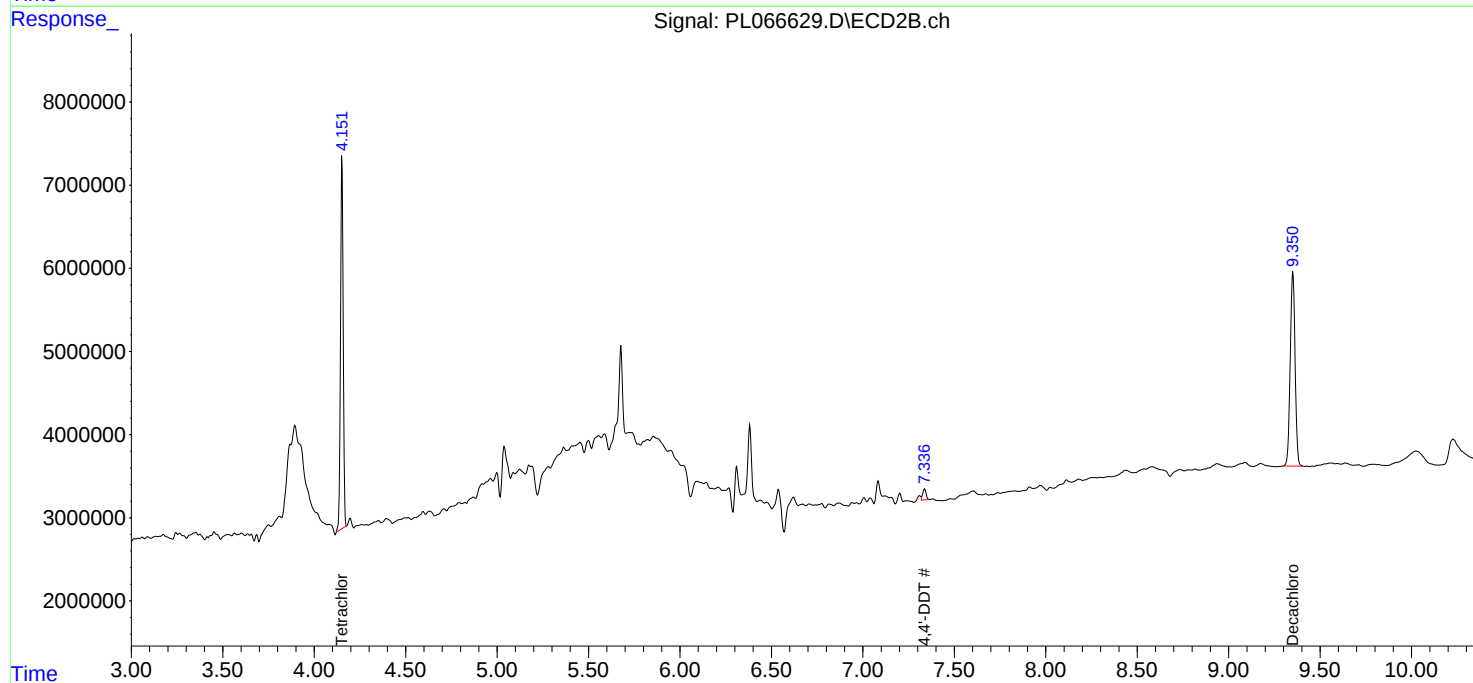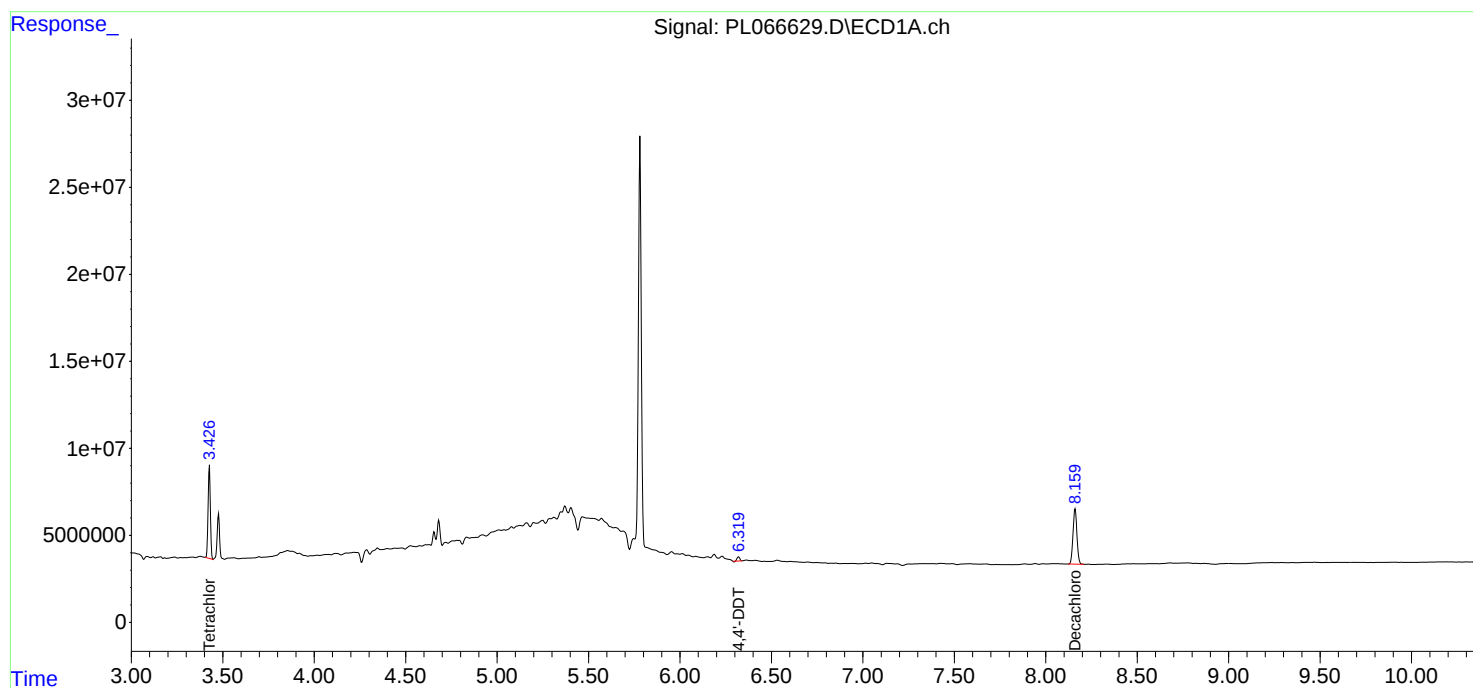


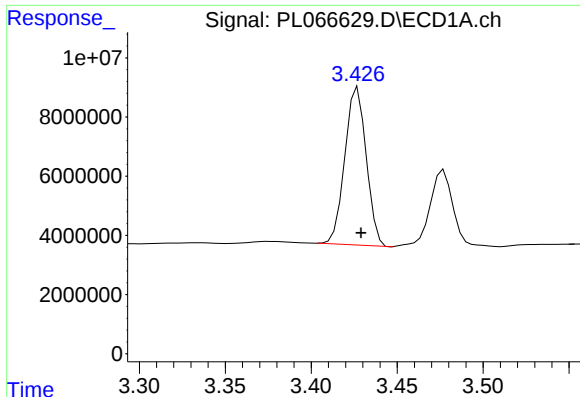

#1 Tetrachloro-m-xylene


R.T.: 3.427 min
Delta R.T.: -0.002 min
Response: 46303014
Conc: 12.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-042921

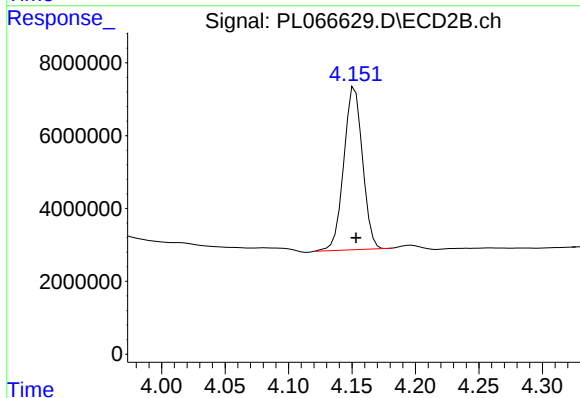


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: 0.000 min
Response: 45804367
Conc: 13.04 ng/ml

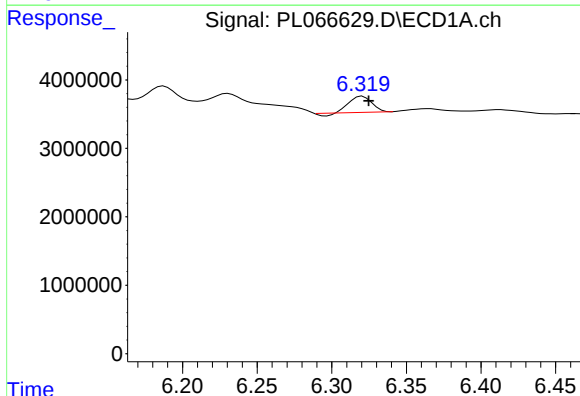


#17 4,4'-DDT

R.T.: 6.321 min
Delta R.T.: -0.004 min
Response: 2356394
Conc: 0.60 ng/ml

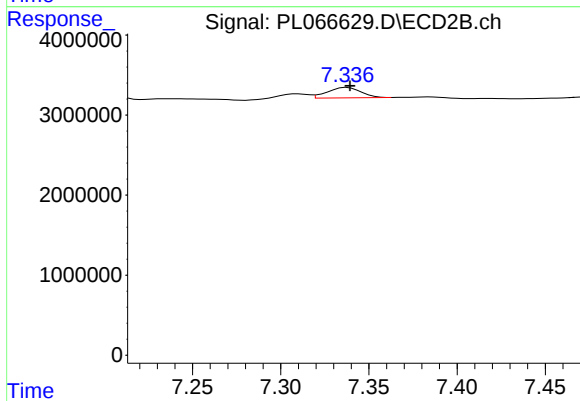

#17 4,4'-DDT


R.T.: 7.338 min
Delta R.T.: -0.002 min
Response: 1721955
Conc: 0.53 ng/ml

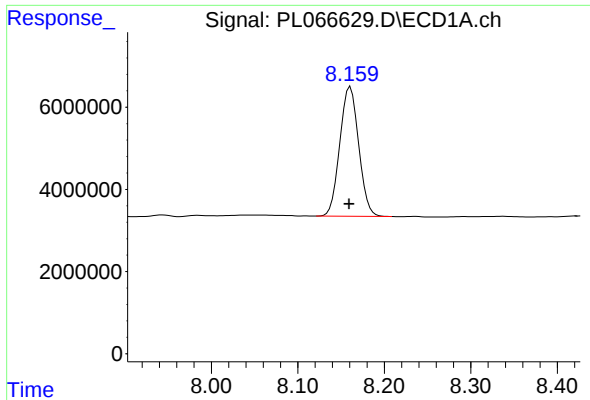

#28 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: 0.002 min
Response: 47499402
Conc: 12.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-042921

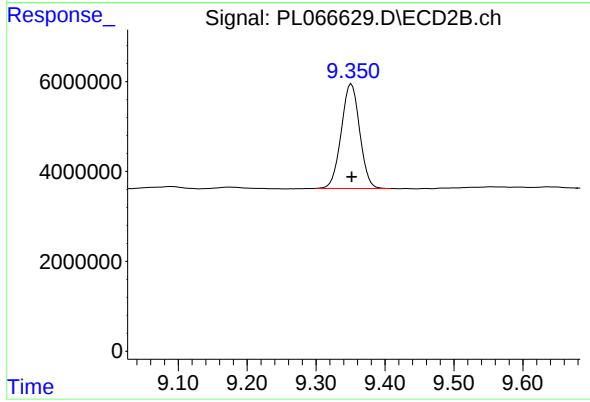

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 43377292
Conc: 14.02 ng/ml