

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050321\
 Data File : PL066634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2021 13:51
 Operator : AR\AJ
 Sample : M2236-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 11991

Manual Integrations
 APPROVED

Ankita
 5/4/2021 2:31:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 05:24:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.427	4.152	44511557	44424998	11.813	12.649
28)	SA Decachlor...	8.161	9.351	41299932	34305110	10.771	11.089
Target Compounds							
12)	B 4,4'-DDE	5.570	6.538	7788409	8766335	1.707m	2.310 #
17)	MA 4,4'-DDT	6.322	7.339	5317645	3175877	1.364	0.981 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050321\
Data File : PL066634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2021 13:51
Operator : AR\AJ
Sample : M2236-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
11991


Manual Integrations
APPROVED

Ankita
5/4/2021 2:31:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 05:24:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

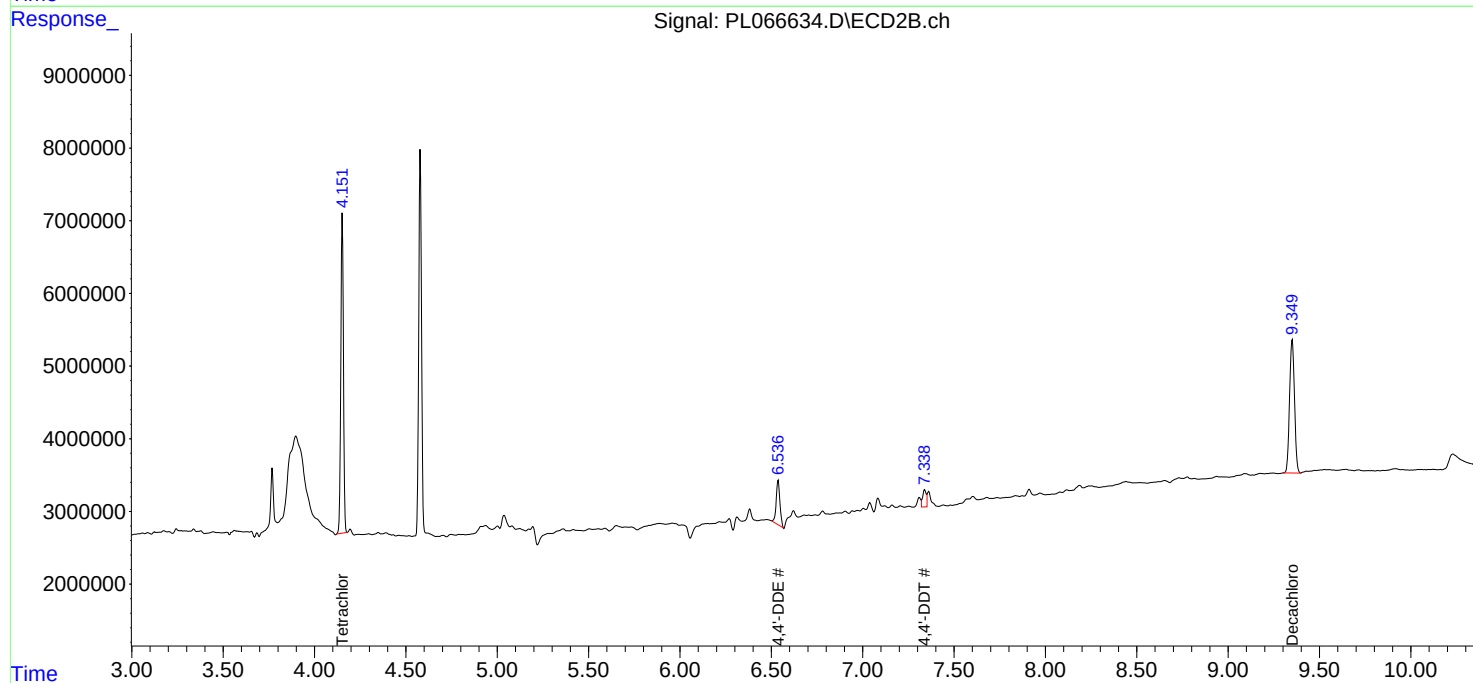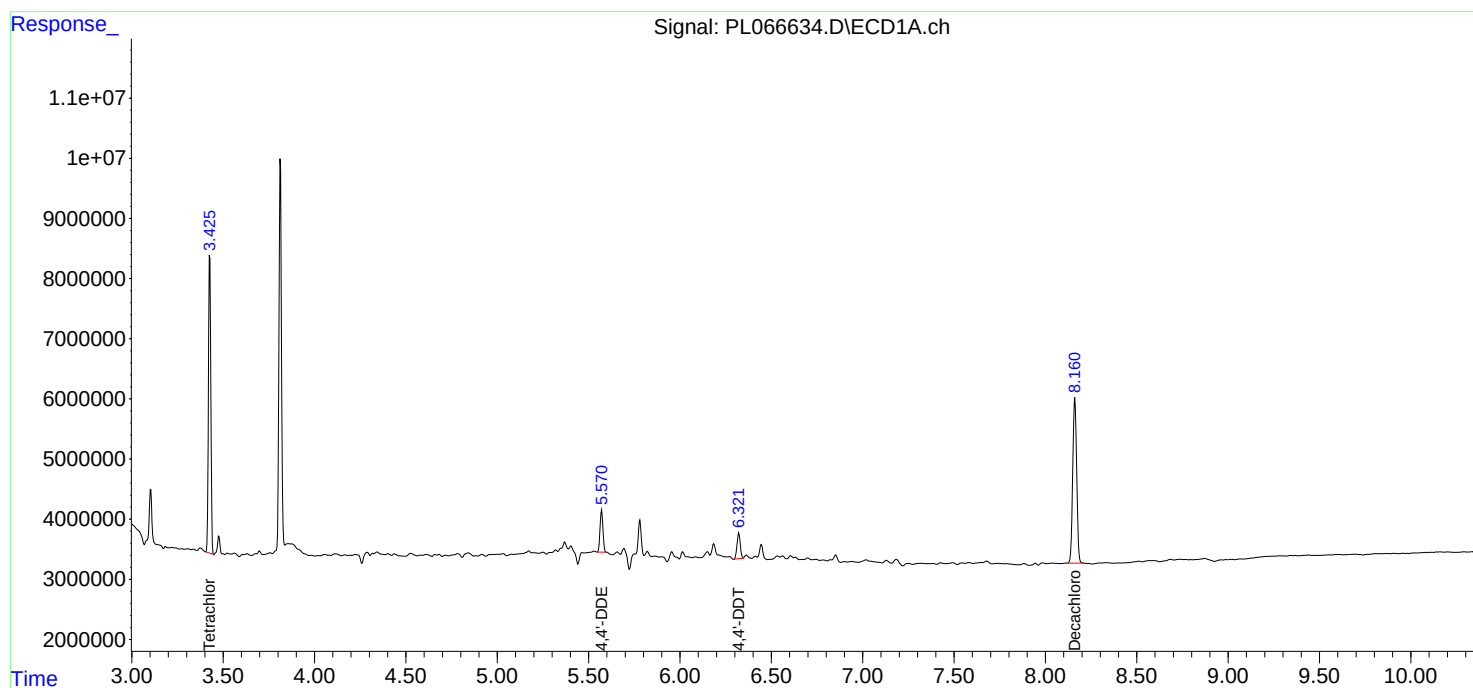

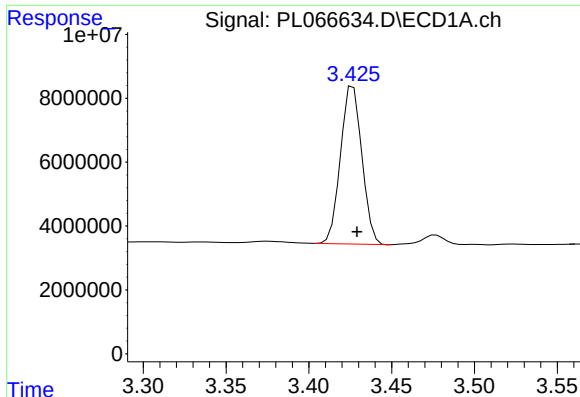


#1 Tetrachloro-m-xylene

R.T.: 3.427 min
Delta R.T.: -0.002 min
Response: 44511557
Conc: 11.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
11991


Manual Integrations
APPROVED

Ankita
5/4/2021 2:31:15 PM

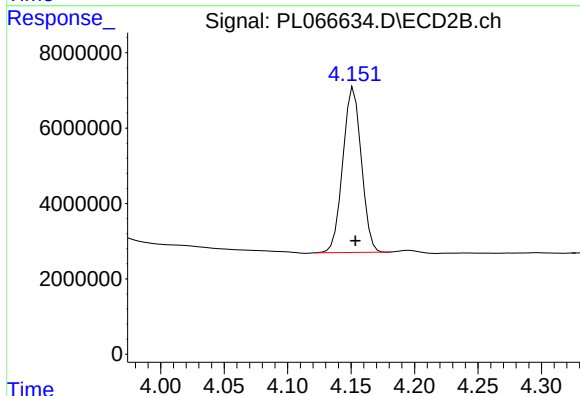


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: -0.001 min
Response: 44424998
Conc: 12.65 ng/ml

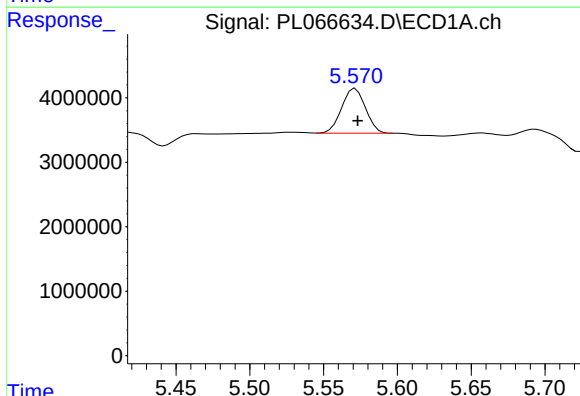


#12 4,4'-DDE

R.T.: 5.570 min
Delta R.T.: -0.003 min
Response: 7788409
Conc: 1.71 ng/ml m

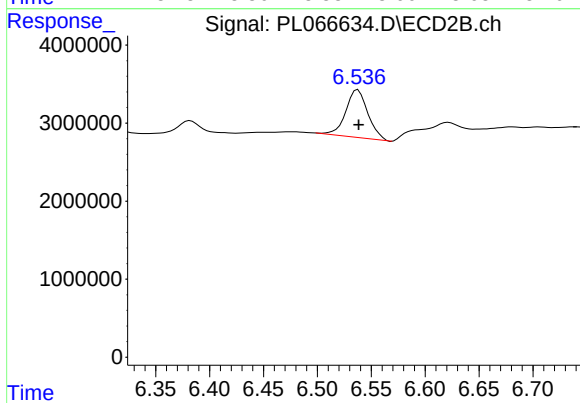

#12 4,4'-DDE

R.T.: 6.538 min
Delta R.T.: 0.000 min
Response: 8766335
Conc: 2.31 ng/ml

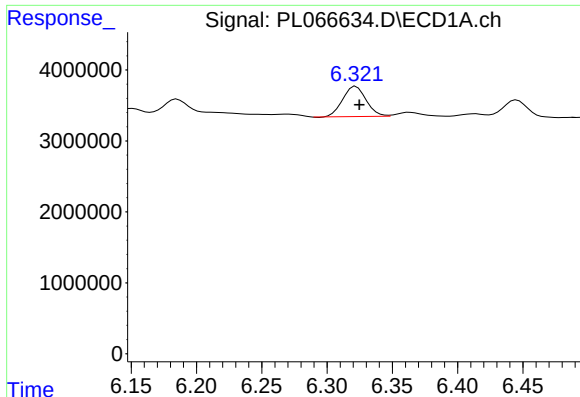


#17 4,4'-DDT

R.T.: 6.322 min
Delta R.T.: -0.003 min
Response: 5317645
Conc: 1.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
11991


Manual Integrations
APPROVED

Ankita
5/4/2021 2:31:15 PM

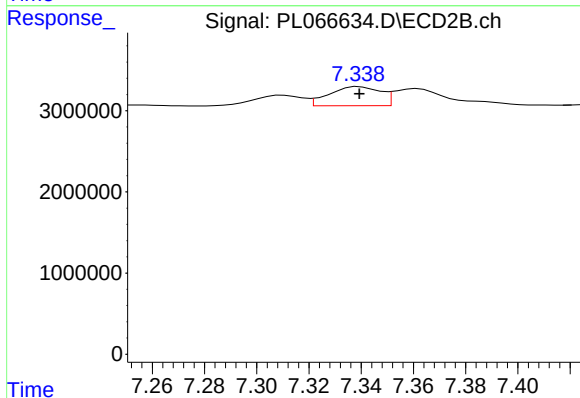


#17 4,4'-DDT

R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 3175877
Conc: 0.98 ng/ml

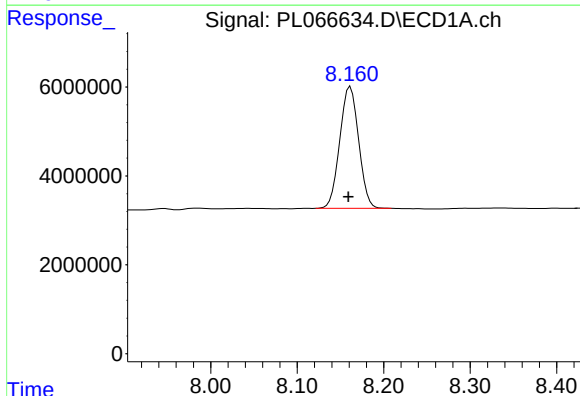

#28 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: 0.002 min
Response: 41299932
Conc: 10.77 ng/ml

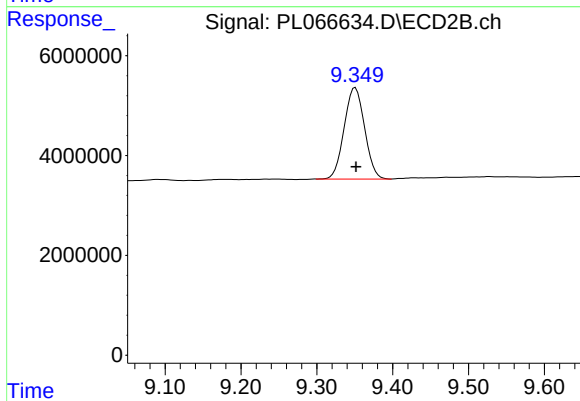

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: -0.001 min
Response: 34305110
Conc: 11.09 ng/ml