

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050322\
 Data File : PL074490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2022 16:43
 Operator : AR\AJ
 Sample : N2647-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 357

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/04/2022
 Supervised By : mohammad ahmed 05/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 04:53:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.489	2614492	12753566	8.092	7.153
28)	SA Decachlor...	10.400	11.330	2682520	8372446	5.158m	4.740
Target Compounds							
11)	B alpha-Chl...	7.421	8.281	198655	1878458	0.450	0.873 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050322\
Data File : PL074490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2022 16:43
Operator : AR\AJ
Sample : N2647-01
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
357


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/04/2022
Supervised By : mohammad ahmed 05/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 04:53:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

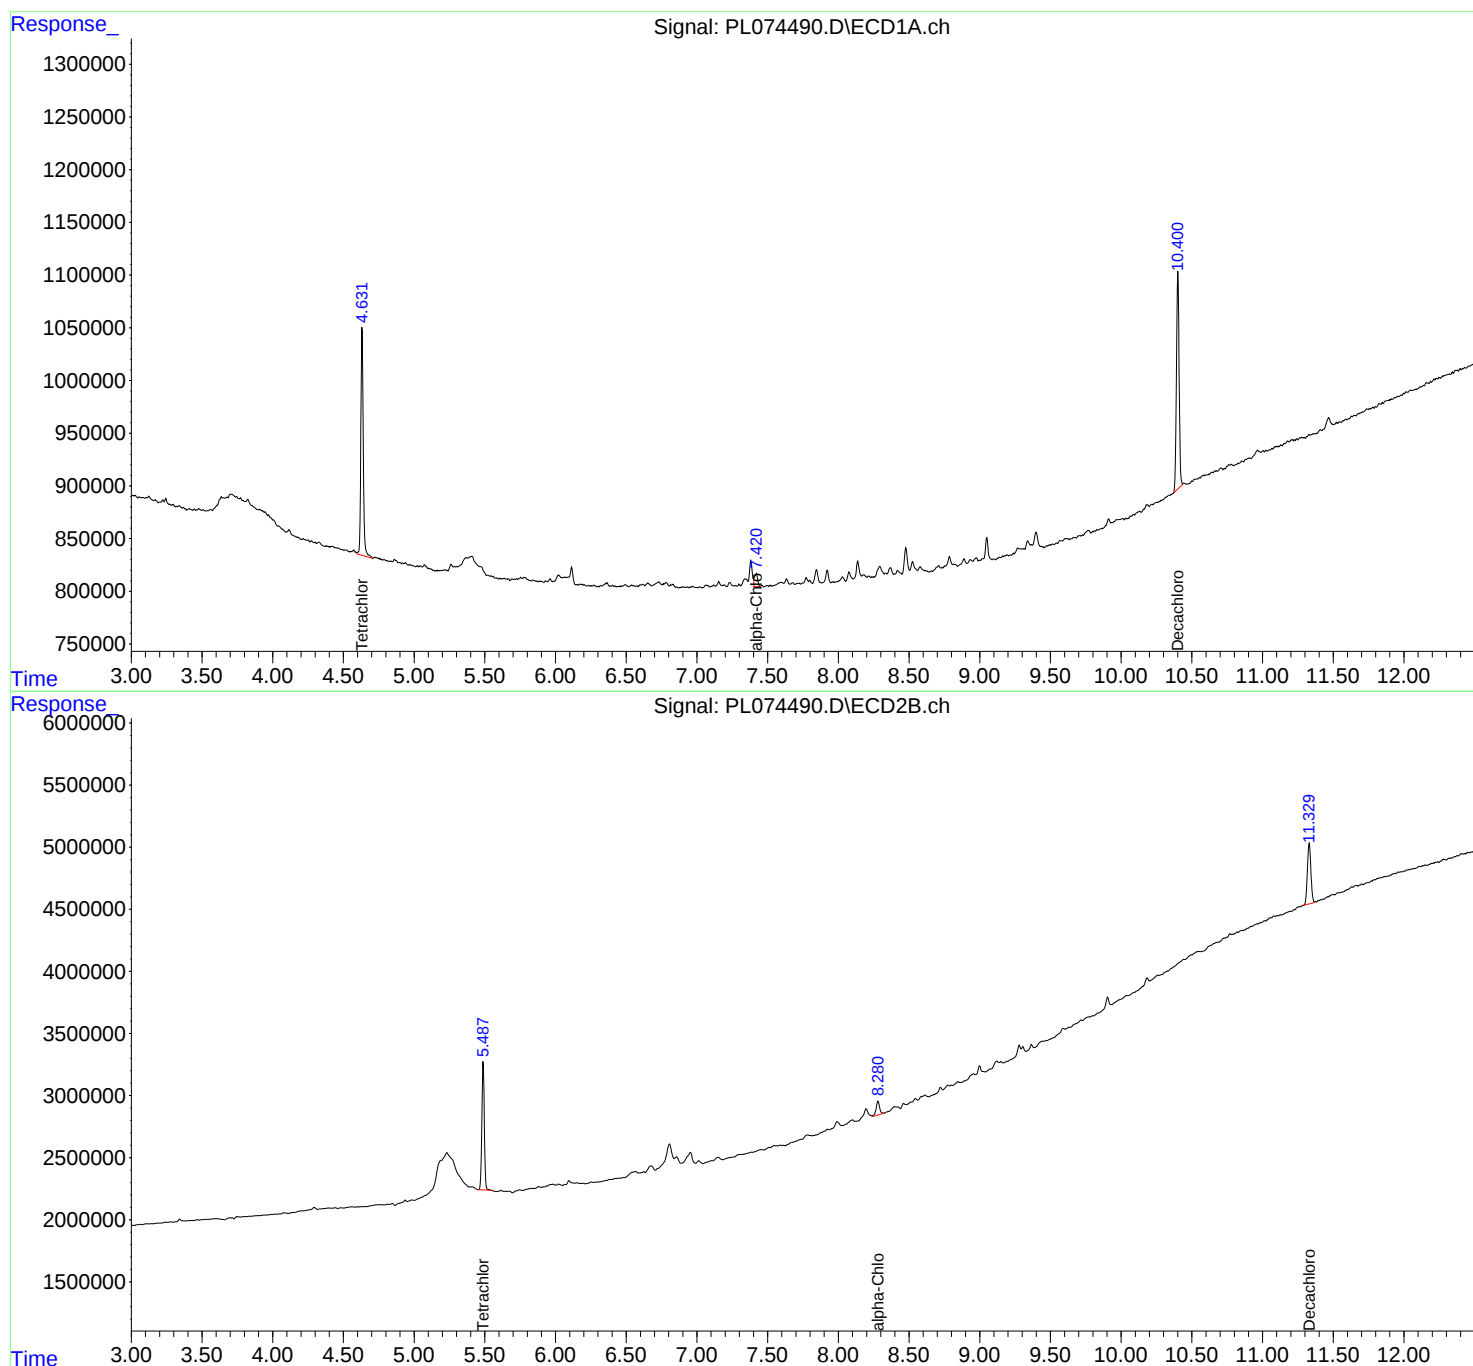

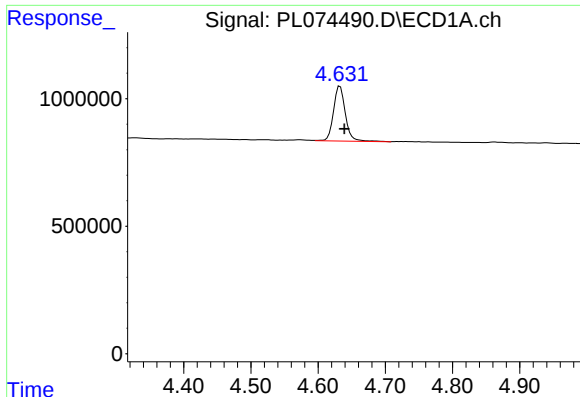


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: -0.006 min
Response: 2614492
Conc: 8.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
357


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2022
Supervised By :mohammad ahmed 05/04/2022

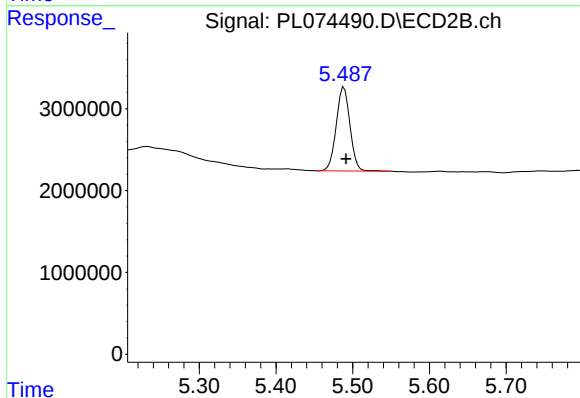


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.003 min
Response: 12753566
Conc: 7.15 ng/ml

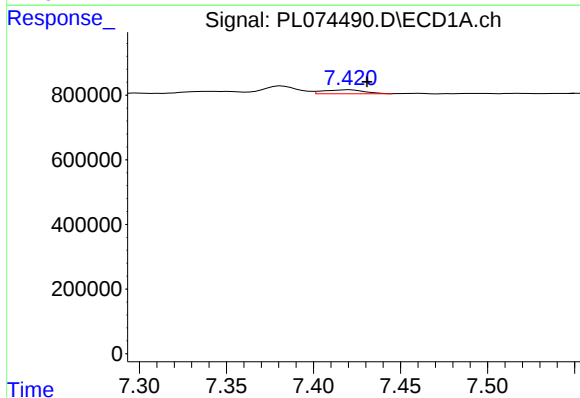


#11 alpha-Chlordane

R.T.: 7.421 min
Delta R.T.: -0.010 min
Response: 198655
Conc: 0.45 ng/ml

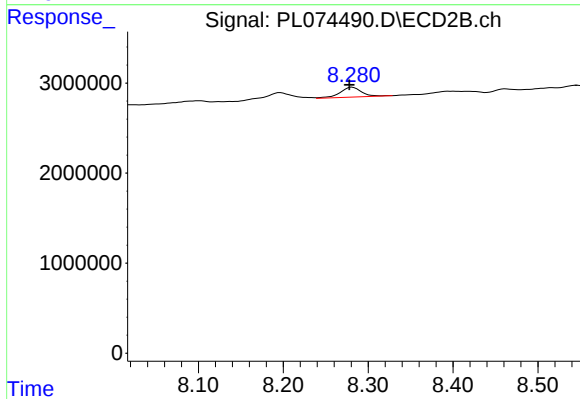

#11 alpha-Chlordane

R.T.: 8.281 min
Delta R.T.: 0.003 min
Response: 1878458
Conc: 0.87 ng/ml

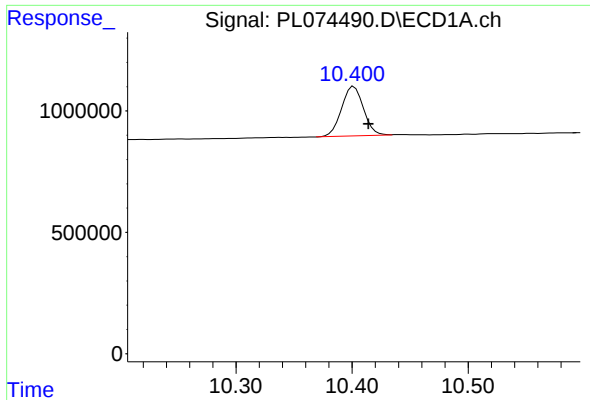


#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.014 min
Response: 2682520
Conc: 5.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
357

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2022
Supervised By :mohammad ahmed 05/04/2022

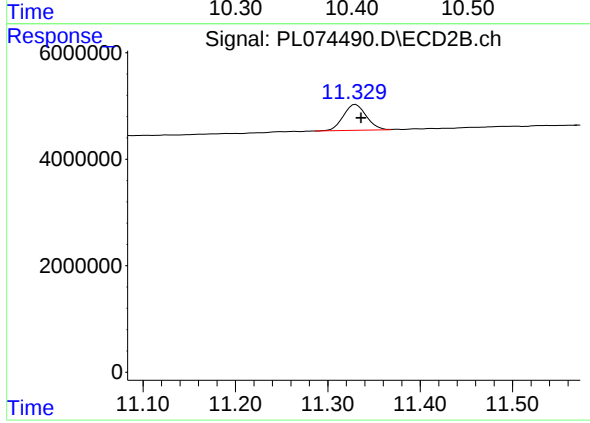

#28 Decachlorobiphenyl

R.T.: 11.330 min
Delta R.T.: -0.006 min
Response: 8372446
Conc: 4.74 ng/ml