

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050323\
 Data File : PL082456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2023 13:21
 Operator : AR\AJ
 Sample : PB152523BS
 Misc : CHLOR,BS
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB152523BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 21:43:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.645	50128268	51257534	18.766	22.125
28)	SA Decachlor...	8.746	7.758	39376808	43004603	20.626	18.841
Target Compounds							
23)	Chlordane-1	4.466	3.629	22768089	17715811	205.968	199.761
24)	Chlordane-2	4.993	4.203	25578190	22626940	214.848	201.769
25)	Chlordane-3	5.698	4.830	87685014	53747071	203.114	189.177
26)	Chlordane-4	5.779	4.891	107.7E6	57819918	207.095	193.762
27)	Chlordane-5	6.621	5.783	18421919	19832622	196.192	200.913



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050323\
Data File : PL082456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2023 13:21
Operator : AR\AJ
Sample : PB152523BS
Misc : CHLOR,BS
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB152523BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 21:43:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

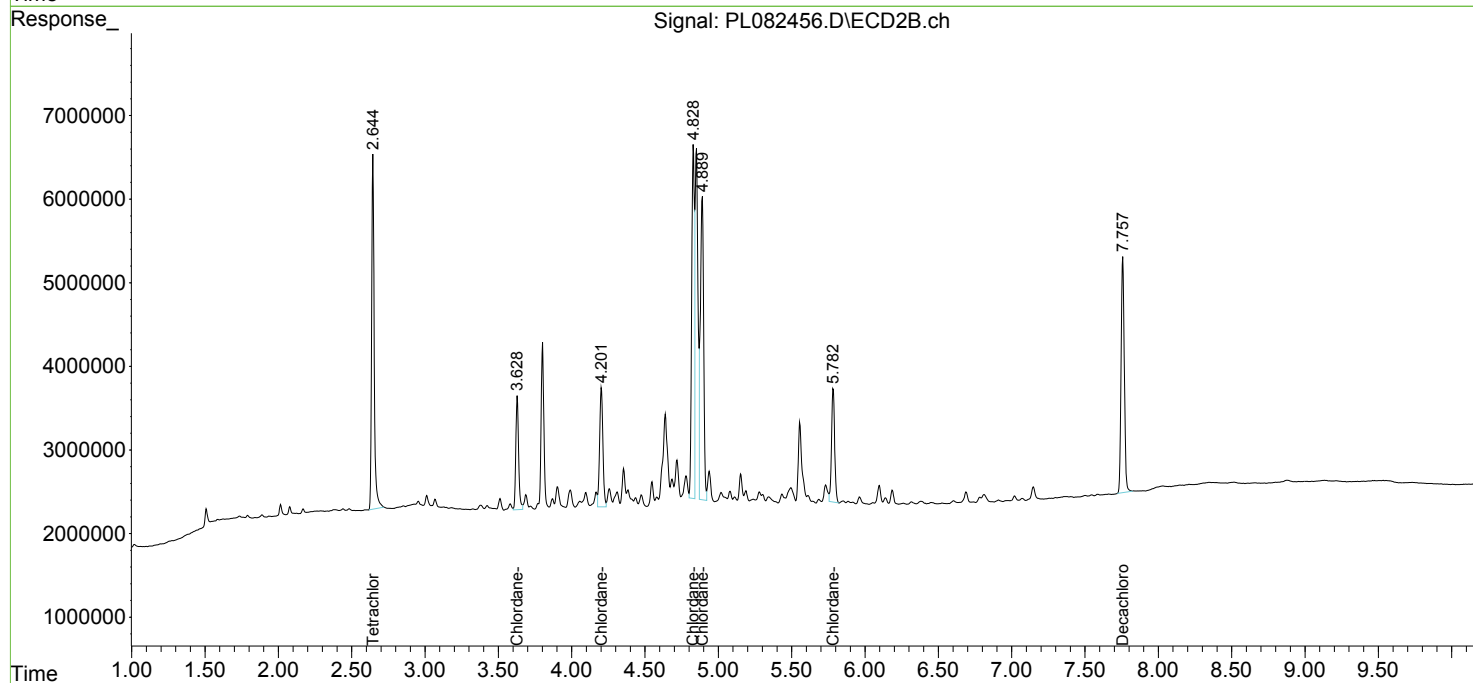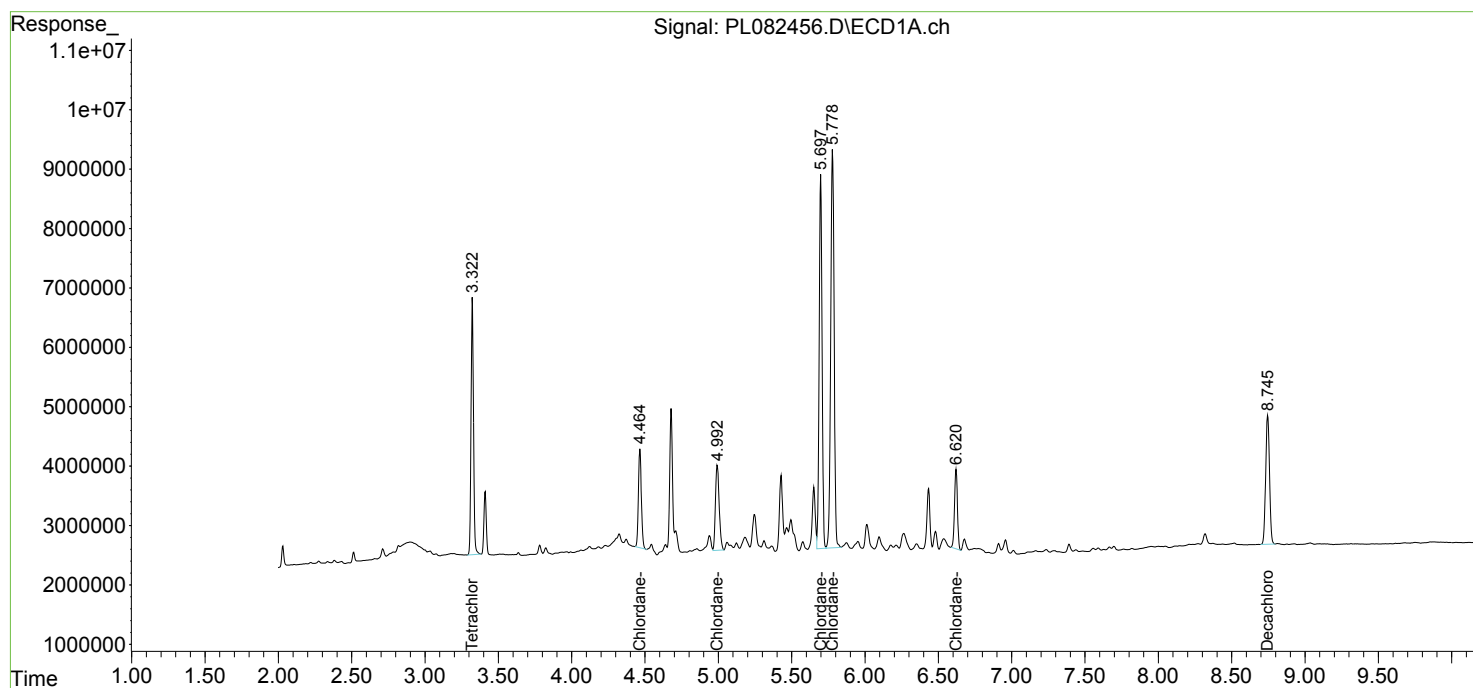


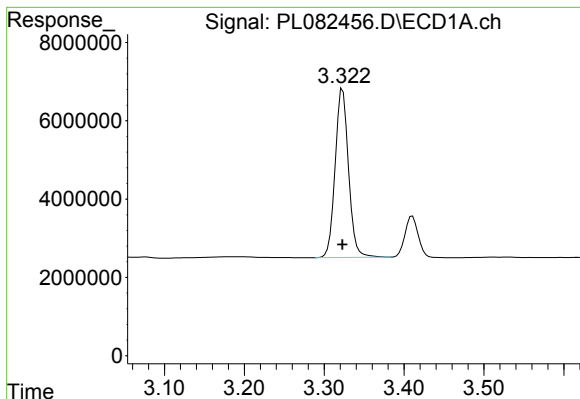

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 50128268
Conc: 18.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152523BS

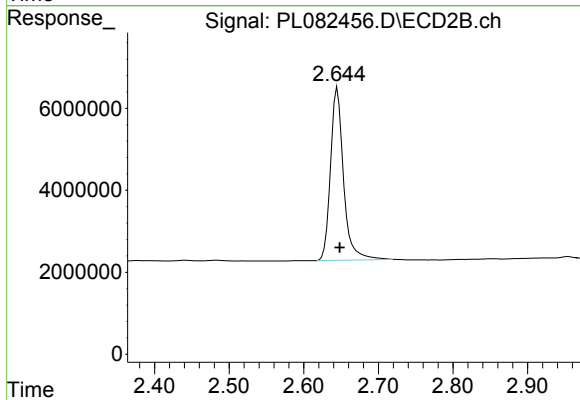


#1 Tetrachloro-m-xylene

R.T.: 2.645 min
Delta R.T.: -0.003 min
Response: 51257534
Conc: 22.12 ng/ml

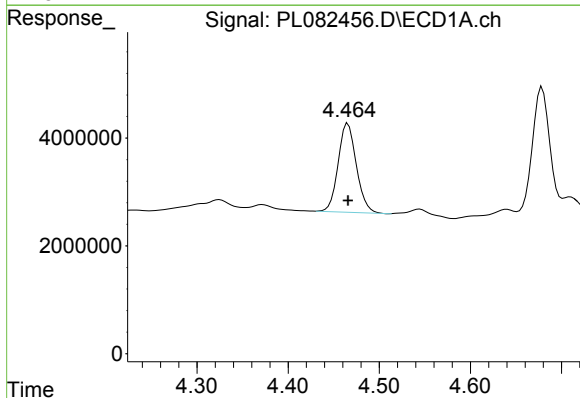


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 22768089
Conc: 205.97 ng/ml

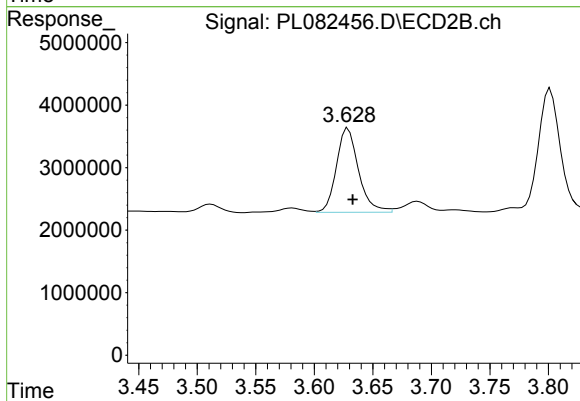

#23 Chlordane-1


R.T.: 3.629 min
Delta R.T.: -0.004 min
Response: 17715811
Conc: 199.76 ng/ml

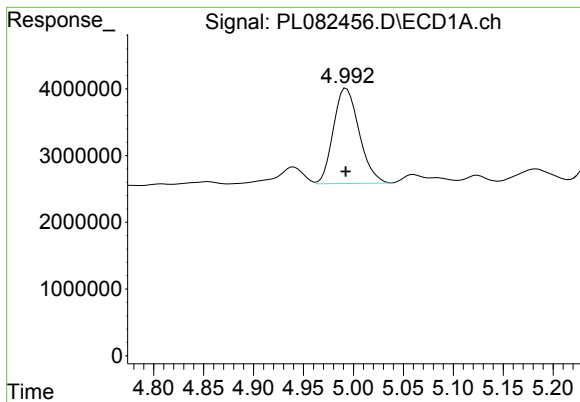

#24 Chlordane-2


R.T.: 4.993 min
Delta R.T.: 0.000 min
Response: 25578190
Conc: 214.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152523BS

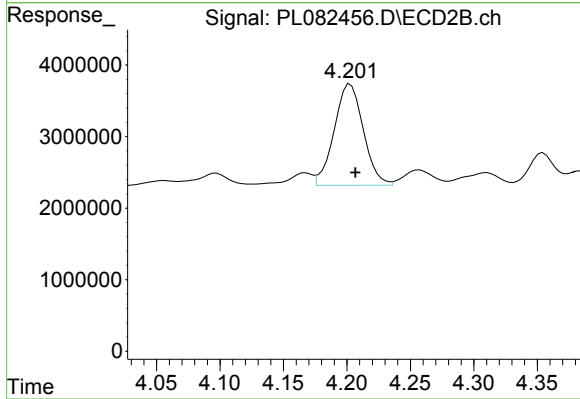


#24 Chlordane-2

R.T.: 4.203 min
Delta R.T.: -0.004 min
Response: 22626940
Conc: 201.77 ng/ml

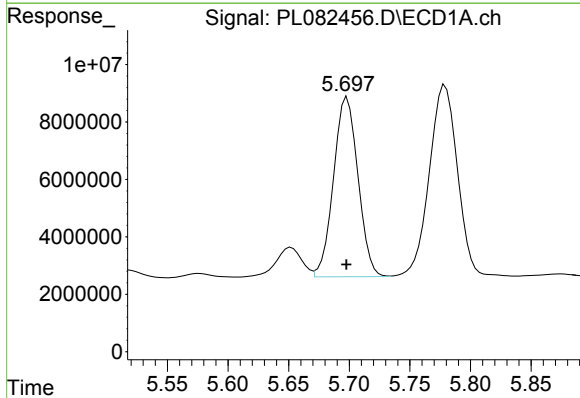


#25 Chlordane-3

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 87685014
Conc: 203.11 ng/ml

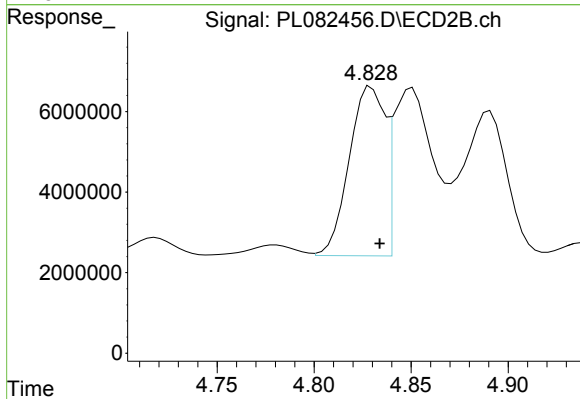

#25 Chlordane-3


R.T.: 4.830 min
Delta R.T.: -0.004 min
Response: 53747071
Conc: 189.18 ng/ml

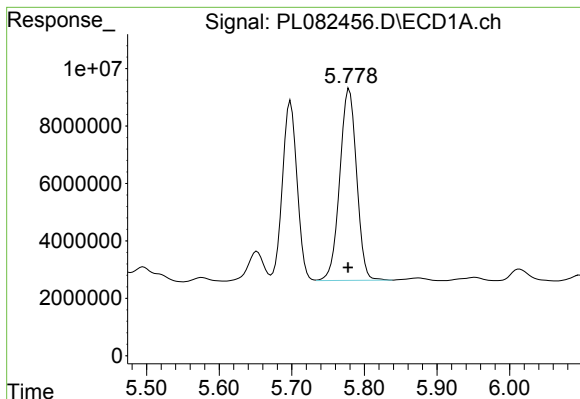

#26 Chlordane-4


R.T.: 5.779 min
Delta R.T.: 0.002 min
Response: 107671594
Conc: 207.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152523BS

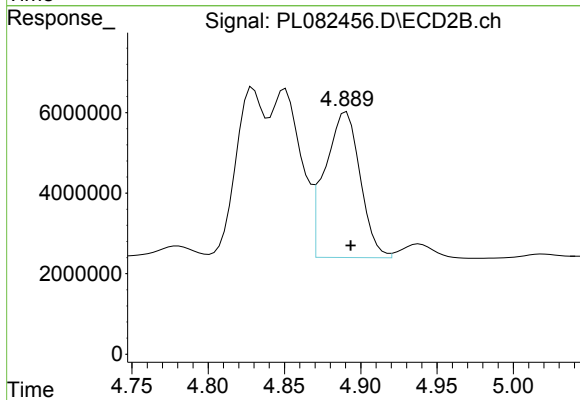


#26 Chlordane-4

R.T.: 4.891 min
Delta R.T.: -0.003 min
Response: 57819918
Conc: 193.76 ng/ml

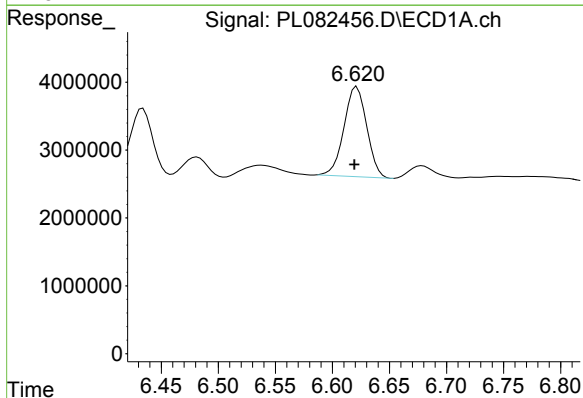


#27 Chlordane-5

R.T.: 6.621 min
Delta R.T.: 0.002 min
Response: 18421919
Conc: 196.19 ng/ml

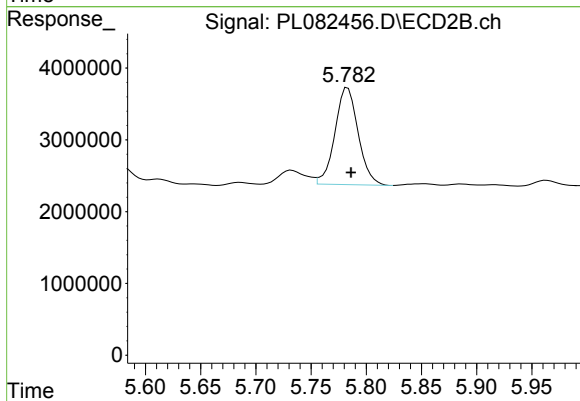

#27 Chlordane-5


R.T.: 5.783 min
Delta R.T.: -0.003 min
Response: 19832622
Conc: 200.91 ng/ml

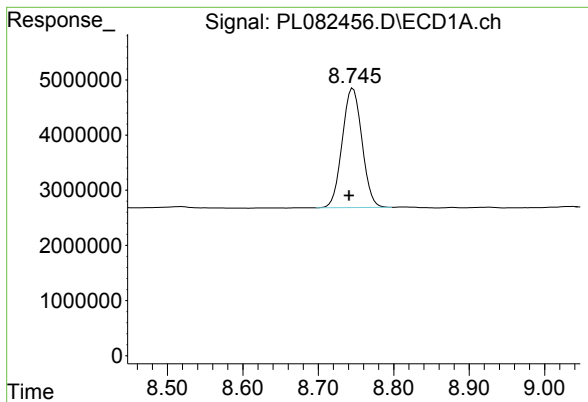

#28 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: 0.005 min
Response: 39376808
Conc: 20.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152523BS

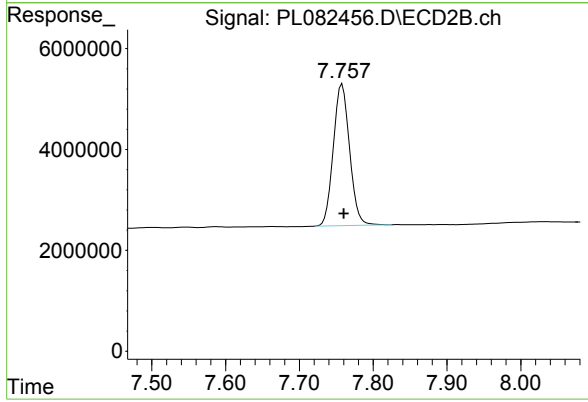

#28 Decachlorobiphenyl

R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 43004603
Conc: 18.84 ng/ml