

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050323\
 Data File : PL082465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2023 16:46
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 17:35:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.645	121.6E6	126.7E6	45.533	54.710
28)	SA Decachlor...	8.744	7.758	90320767	99540159	47.311	43.610
Target Compounds							
23)	Chlordane-1	4.466	3.629	55525956	42432933	502.308	478.467
24)	Chlordane-2	4.993	4.203	60528609	52339681	508.420	466.724
25)	Chlordane-3	5.698	4.830	219.3E6	135.9E6	507.909	478.299
26)	Chlordane-4	5.779	4.891	260.5E6	140.3E6	501.126	470.191
27)	Chlordane-5	6.621	5.784	43813987	47593938	466.615	482.147



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050323\
Data File : PL082465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2023 16:46
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 17:35:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

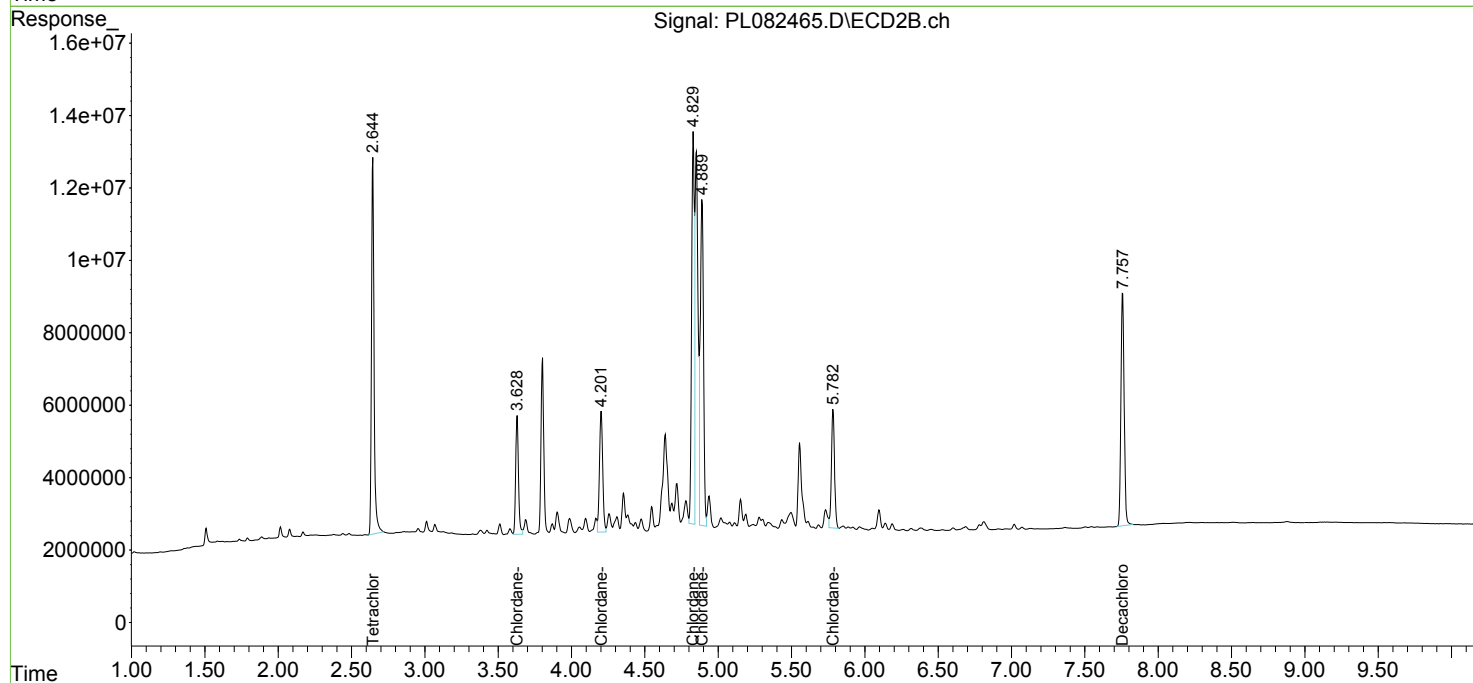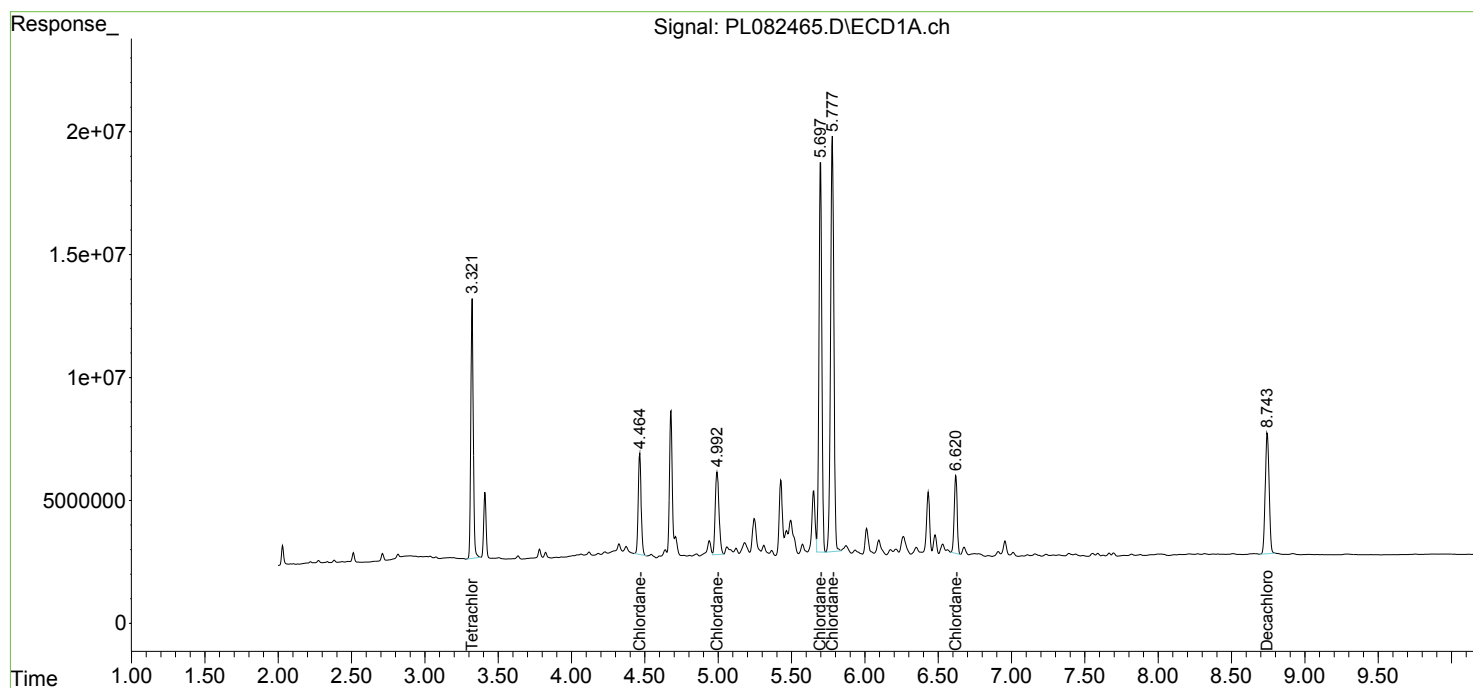


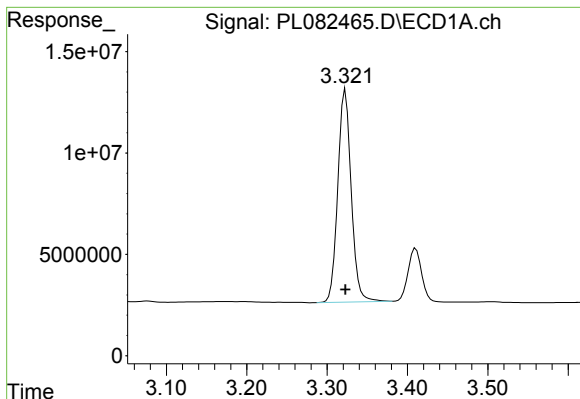

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 121628357
Conc: 45.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

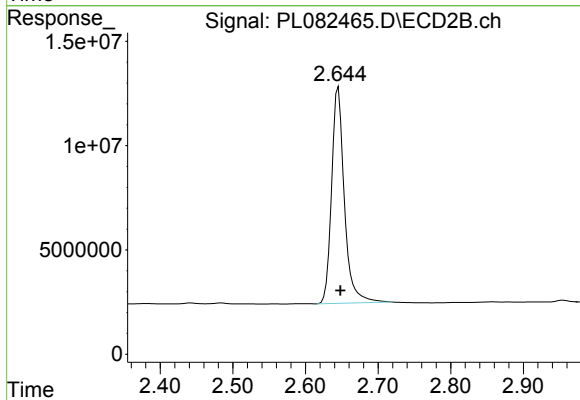


#1 Tetrachloro-m-xylene

R.T.: 2.645 min
Delta R.T.: -0.003 min
Response: 126749631
Conc: 54.71 ng/ml

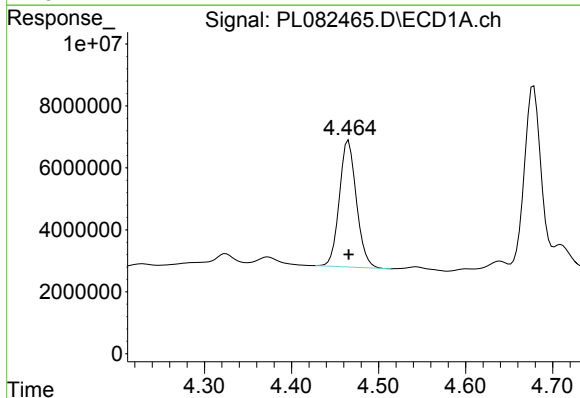


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 55525956
Conc: 502.31 ng/ml

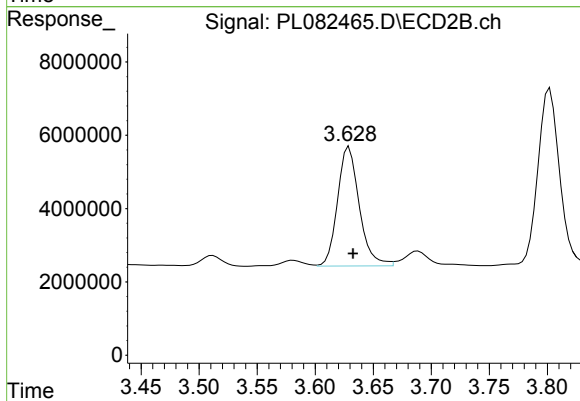

#23 Chlordane-1


R.T.: 3.629 min
Delta R.T.: -0.004 min
Response: 42432933
Conc: 478.47 ng/ml

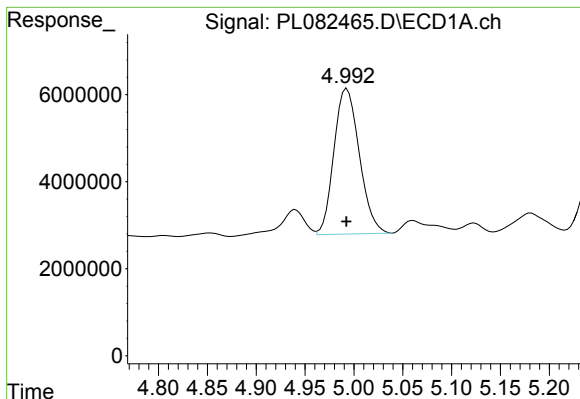

#24 Chlordane-2


R.T.: 4.993 min
Delta R.T.: 0.000 min
Response: 60528609
Conc: 508.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

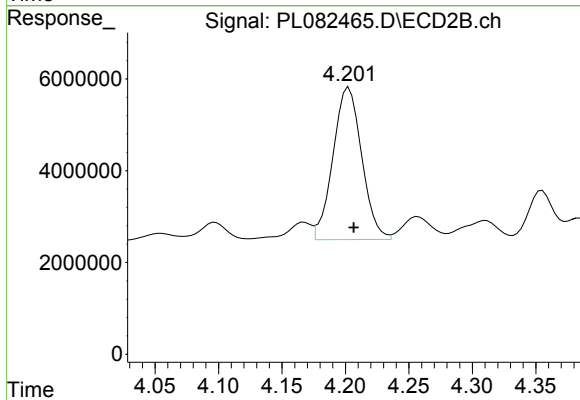


#24 Chlordane-2

R.T.: 4.203 min
Delta R.T.: -0.004 min
Response: 52339681
Conc: 466.72 ng/ml

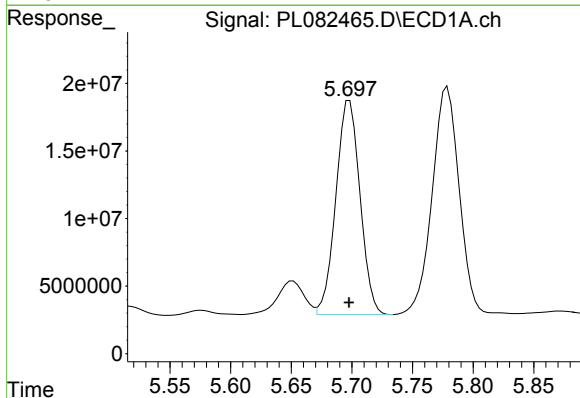


#25 Chlordane-3

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 219266050
Conc: 507.91 ng/ml

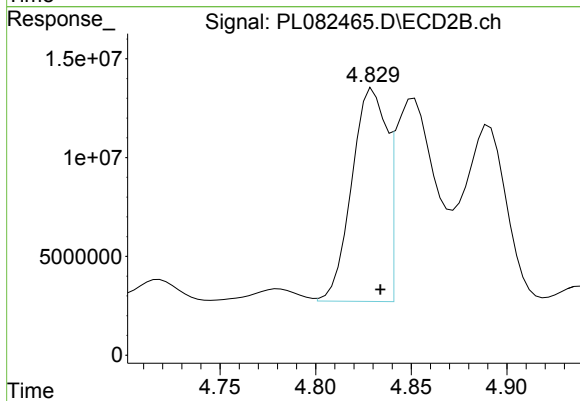

#25 Chlordane-3


R.T.: 4.830 min
Delta R.T.: -0.004 min
Response: 135889318
Conc: 478.30 ng/ml

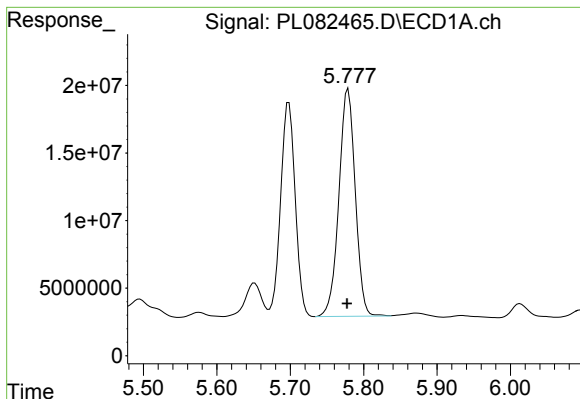

#26 Chlordane-4


R.T.: 5.779 min
Delta R.T.: 0.001 min
Response: 260543003
Conc: 501.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

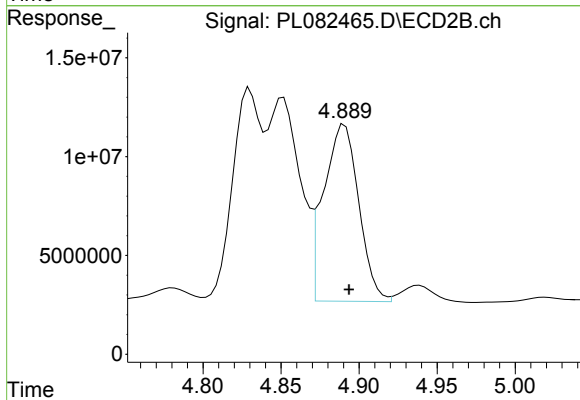


#26 Chlordane-4

R.T.: 4.891 min
Delta R.T.: -0.003 min
Response: 140308107
Conc: 470.19 ng/ml

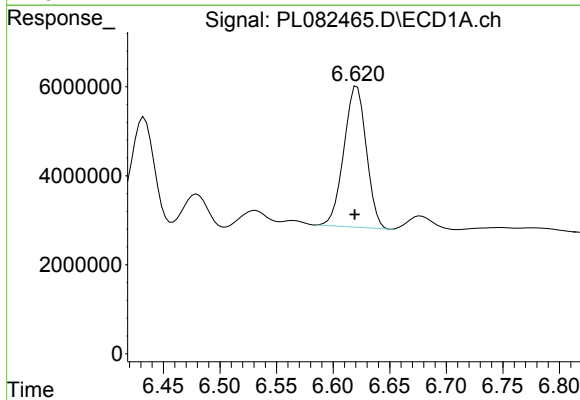


#27 Chlordane-5

R.T.: 6.621 min
Delta R.T.: 0.002 min
Response: 43813987
Conc: 466.61 ng/ml

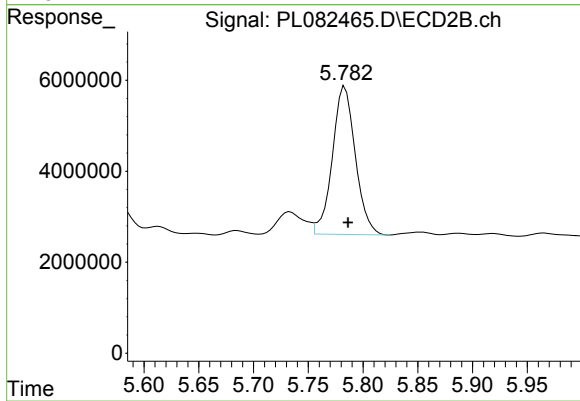

#27 Chlordane-5


R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 47593938
Conc: 482.15 ng/ml

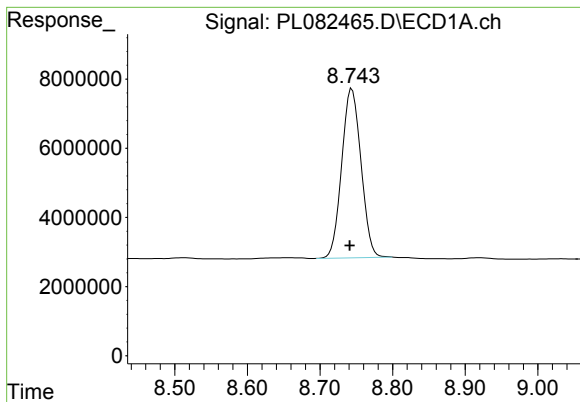

#28 Decachlorobiphenyl

R.T.: 8.744 min
Delta R.T.: 0.003 min
Response: 90320767
Conc: 47.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

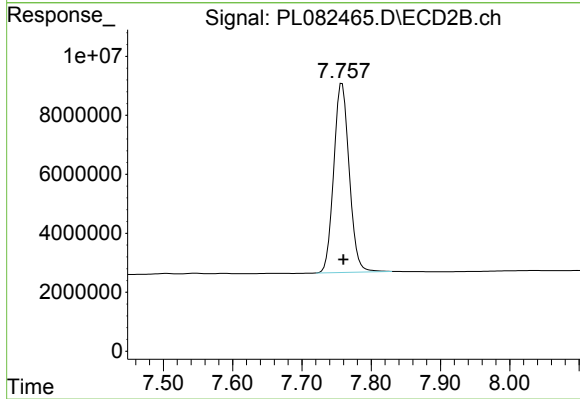

#28 Decachlorobiphenyl

R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 99540159
Conc: 43.61 ng/ml