

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050323\
 Data File : PL082473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2023 19:07
 Operator : AR\AJ
 Sample : 02583-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CF-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 21:49:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.646	46977635	39942055	17.587	17.241
28)	SA Decachlor...	8.743	7.757	26900427	29428468	14.091	12.893
Target Compounds							
11)	B alpha-Chl...	5.777	4.890	1721930	1472952	0.577	0.507



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050323\
Data File : PL082473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2023 19:07
Operator : AR\AJ
Sample : 02583-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CF-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 21:49:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

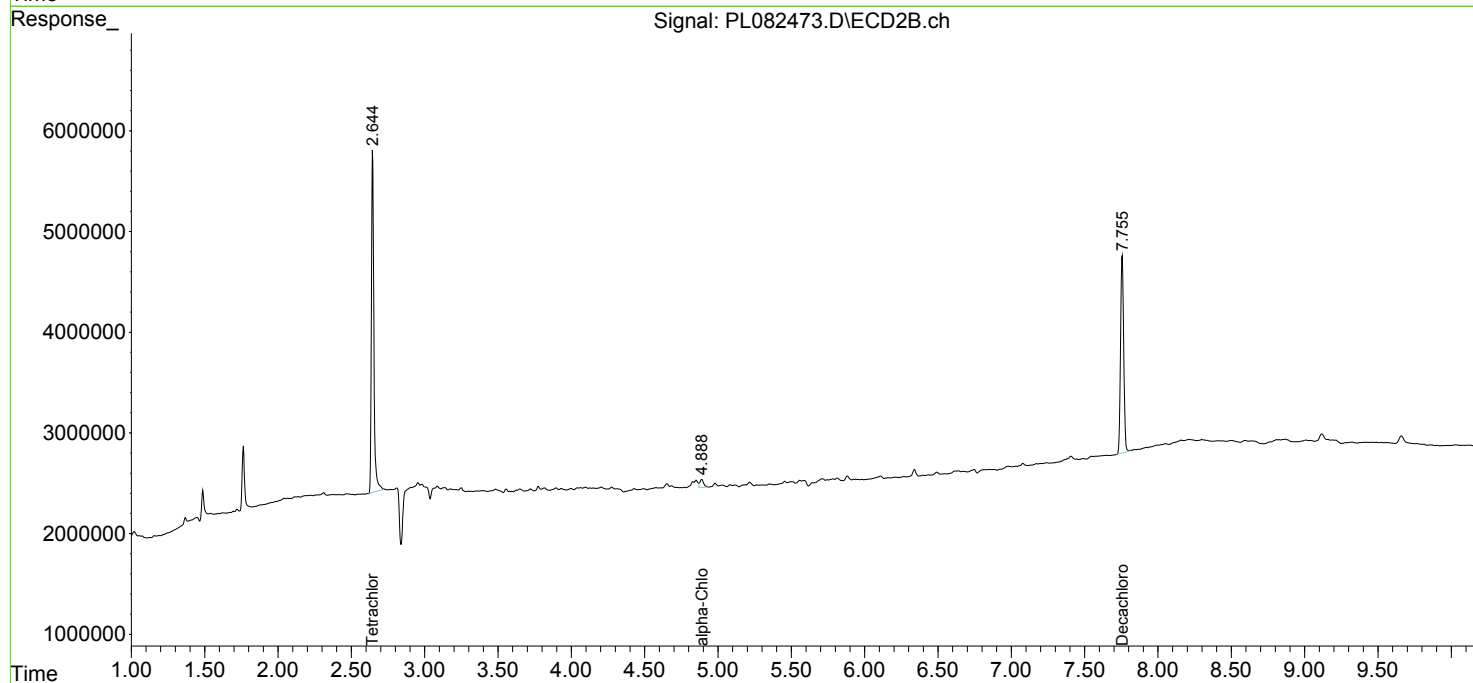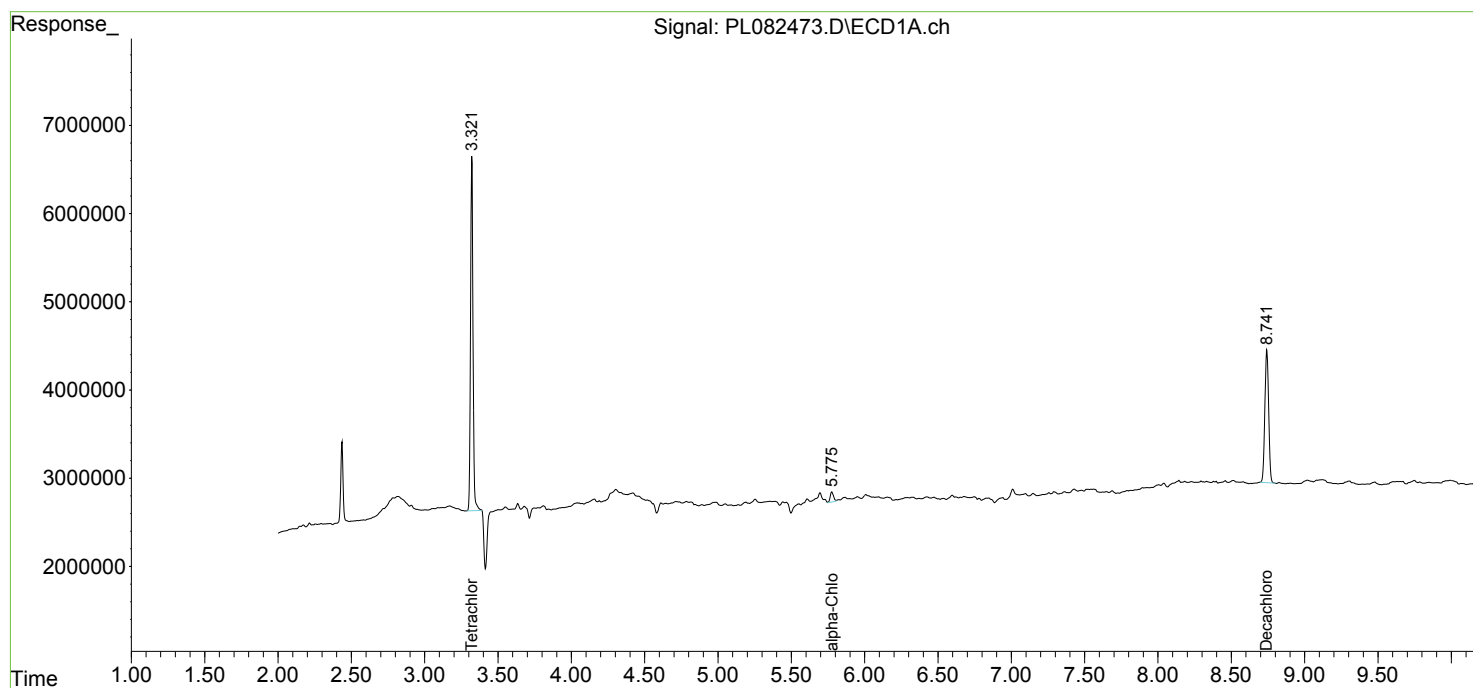


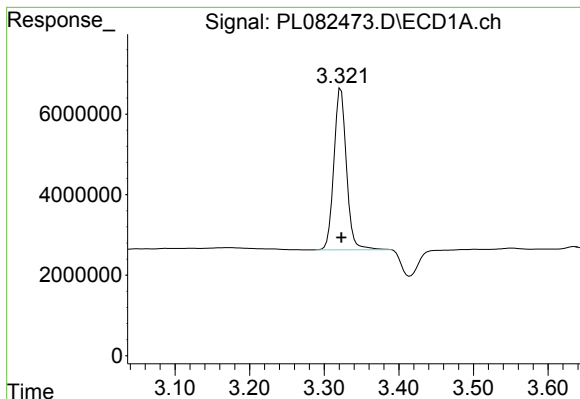

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.000 min
Response: 46977635
Conc: 17.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
CF-23

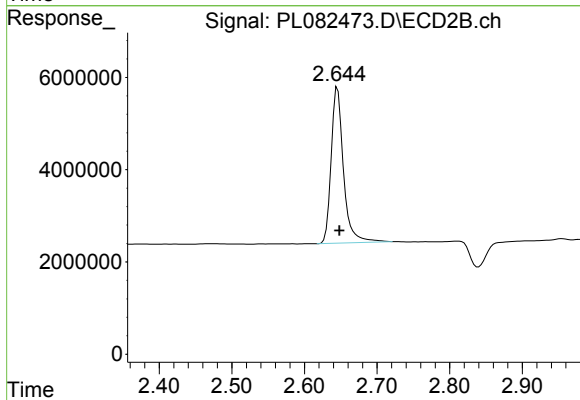


#1 Tetrachloro-m-xylene

R.T.: 2.646 min
Delta R.T.: -0.003 min
Response: 39942055
Conc: 17.24 ng/ml

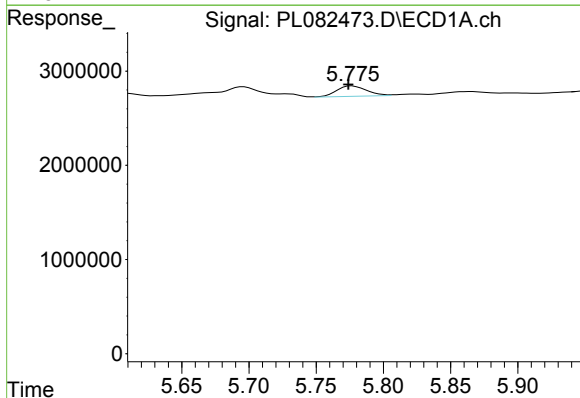


#11 alpha-Chlordane

R.T.: 5.777 min
Delta R.T.: 0.003 min
Response: 1721930
Conc: 0.58 ng/ml

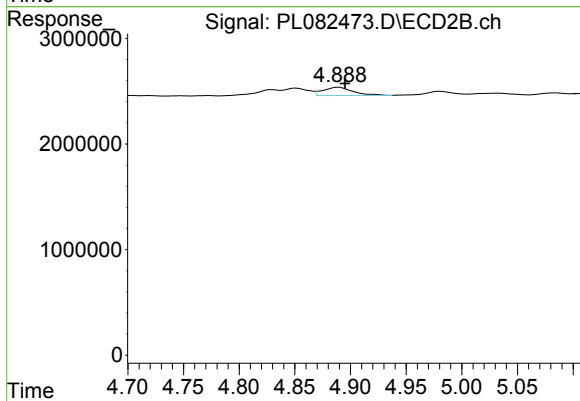

#11 alpha-Chlordane


R.T.: 4.890 min
Delta R.T.: -0.005 min
Response: 1472952
Conc: 0.51 ng/ml

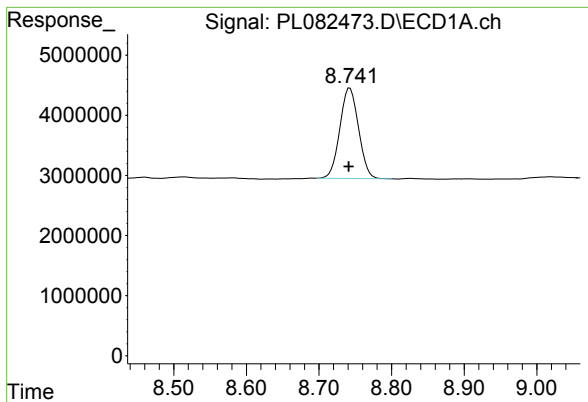

#28 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.002 min
Response: 26900427
Conc: 14.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
CF-23

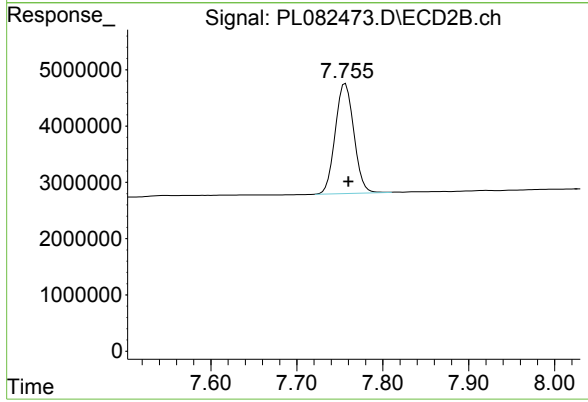

#28 Decachlorobiphenyl

R.T.: 7.757 min
Delta R.T.: -0.003 min
Response: 29428468
Conc: 12.89 ng/ml