

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050325\
 Data File : PL095496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2025 11:25
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 00:19:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	5.729	0.000	157.0E6	0	39.188	N.D.	#
12) B	4,4'-DDE	6.244	0.000	16899166	0	4.310	N.D.	#
13) MA	Dieldrin	0.000	5.545	0	28504893	N.D.	7.009	#
14) MA	Endrin	0.000	5.812	0	8914133	N.D.	2.448	#
15) B	Endosulfa...	6.851f	0.000	8552107	0	2.679	N.D.	#
22)	Mirex	0.000	7.219f	0	46299261	N.D.	16.063	#
24)	Chlordane-2	0.000	4.502	0	31494206	N.D.	171.138	#
27)	Chlordane-5	6.898f	0.000	1066690	0	7.037	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050325\
Data File : PL095496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2025 11:25
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 00:19:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

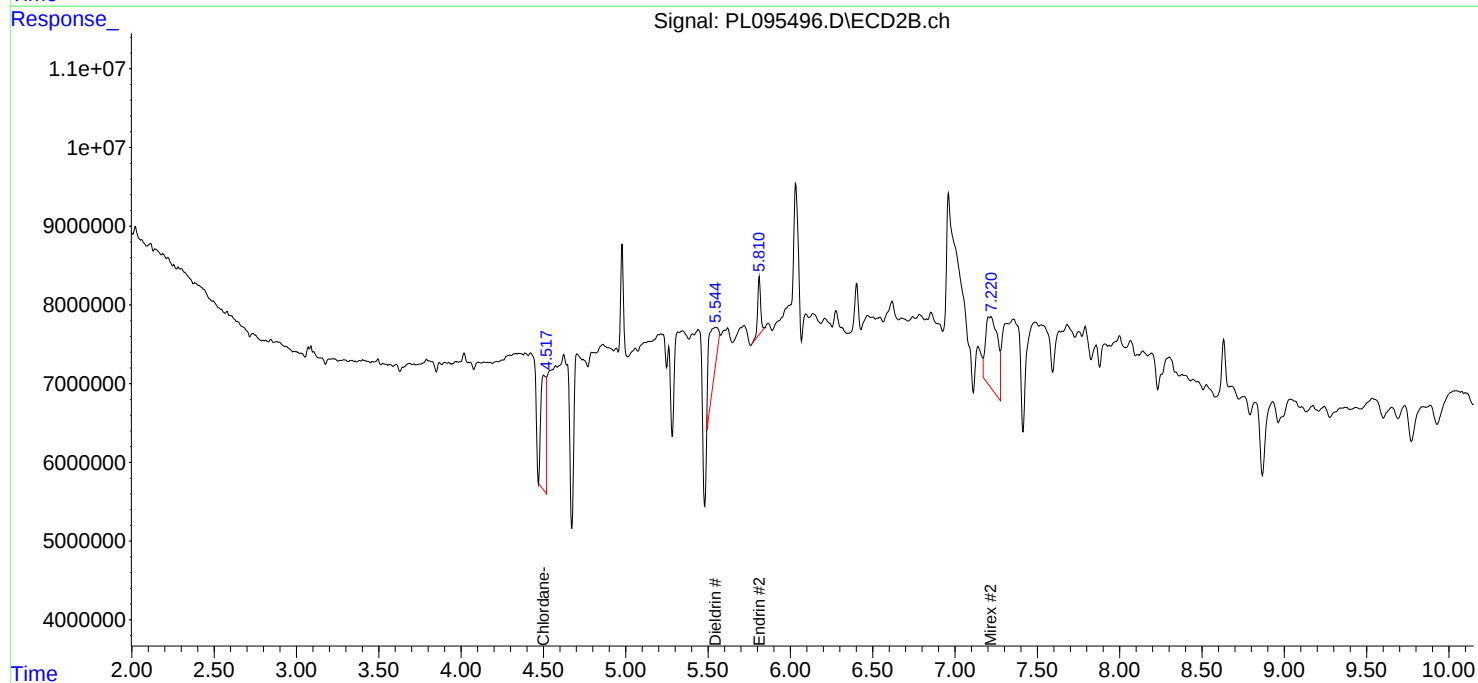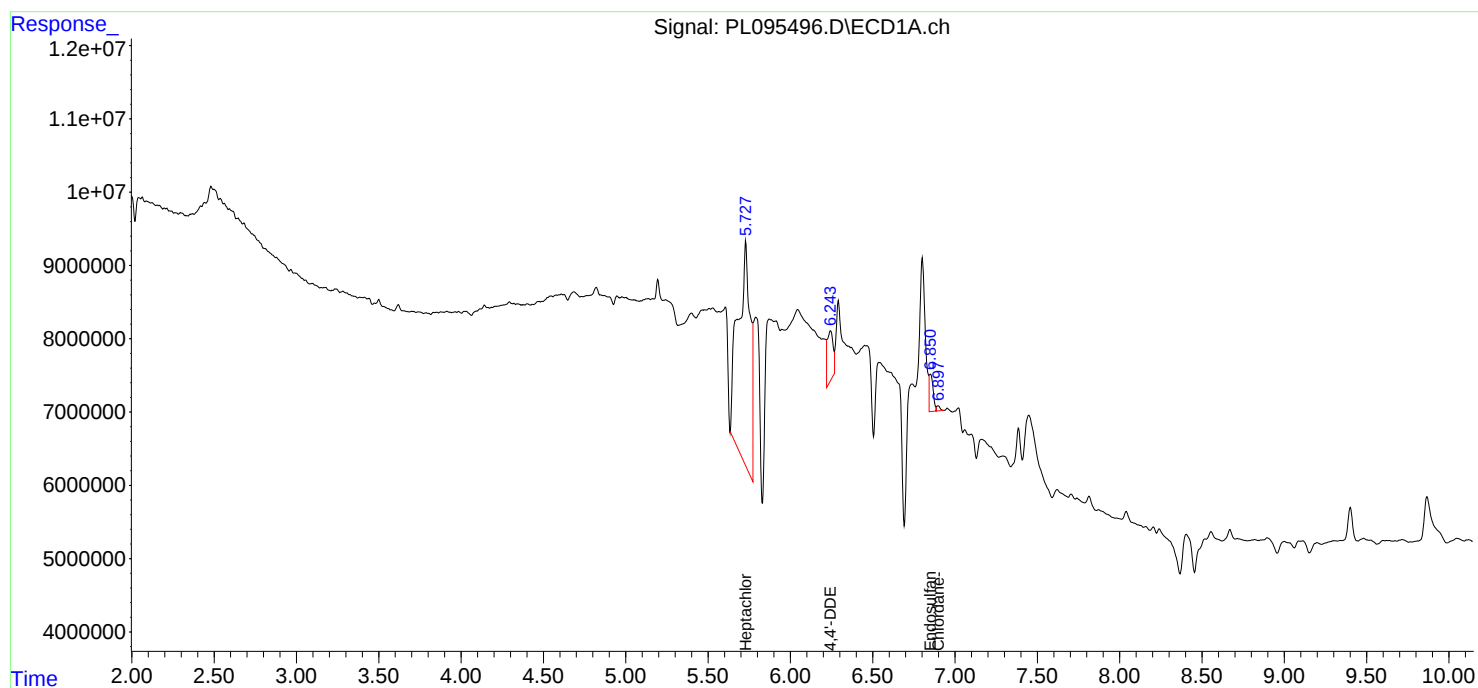


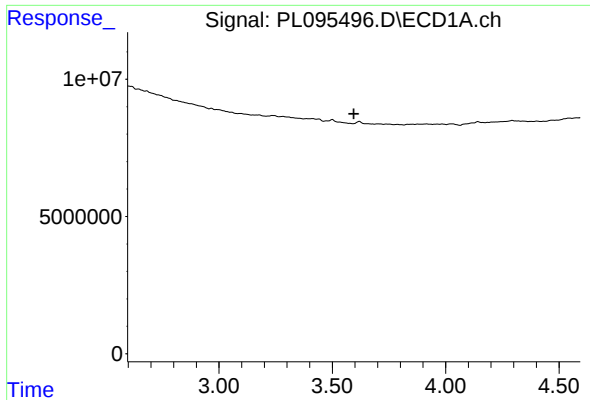

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

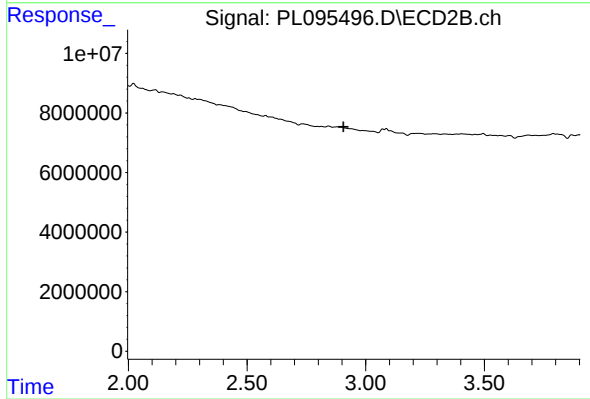


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.906 min
Response: 0
Conc: N.D.

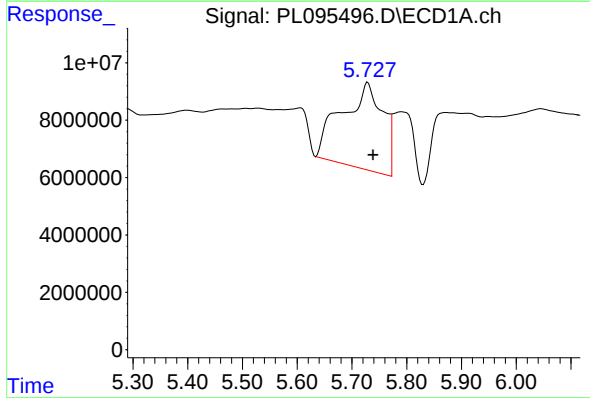


#8 Heptachlor epoxide

R.T.: 5.729 min
Delta R.T.: -0.010 min
Response: 156952232
Conc: 39.19 ng/ml

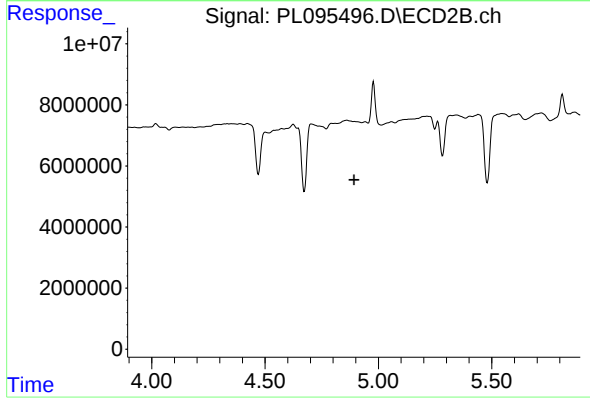

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.893 min
Response: 0
Conc: N.D.

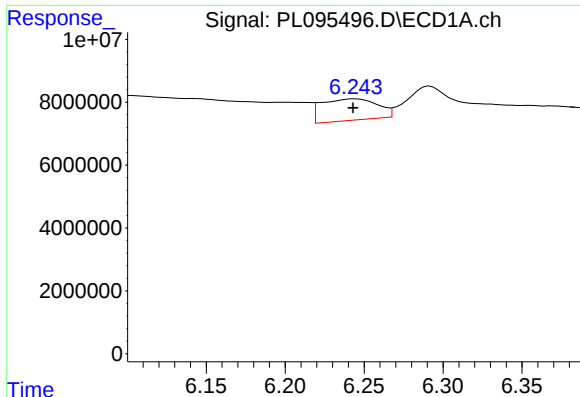

#12 4,4'-DDE


R.T.: 6.244 min
Delta R.T.: 0.001 min
Response: 16899166
Conc: 4.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

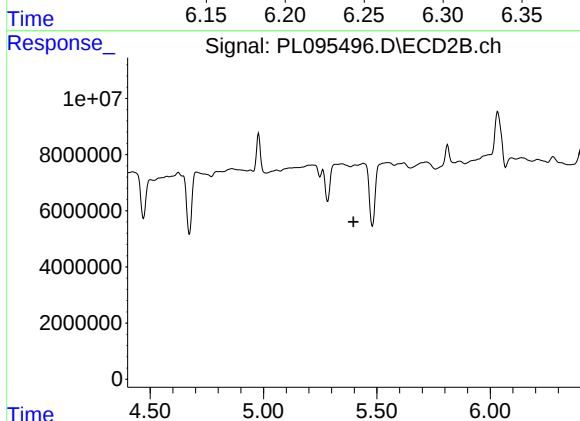


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

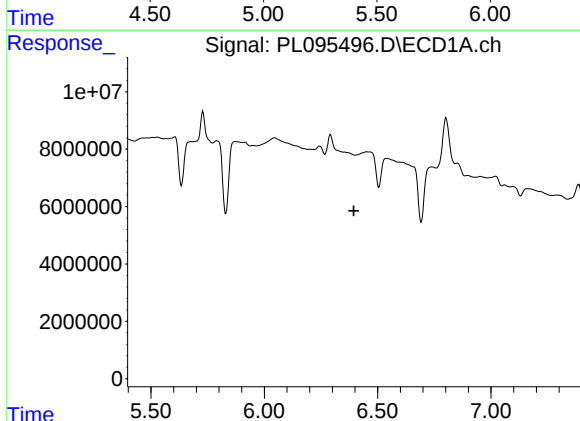


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

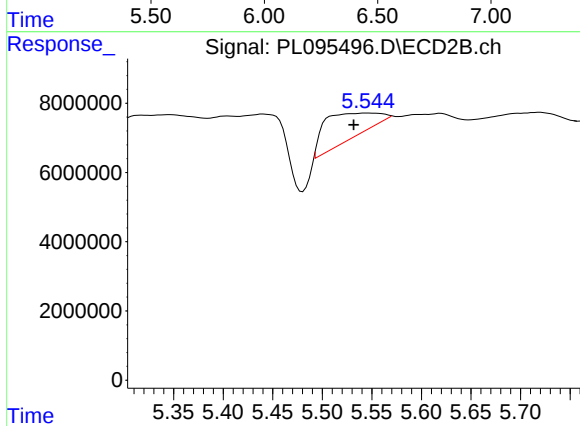

#13 Dieldrin


R.T.: 5.545 min
Delta R.T.: 0.013 min
Response: 28504893
Conc: 7.01 ng/ml

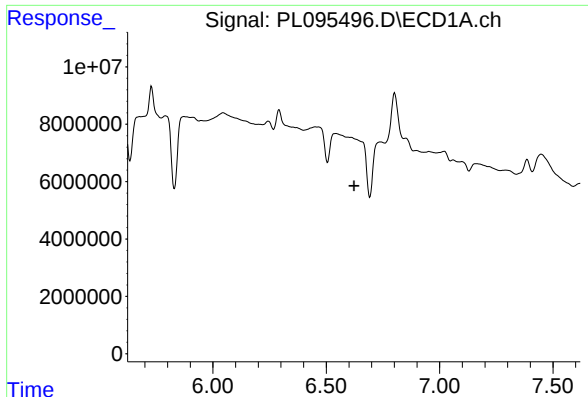

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.623 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

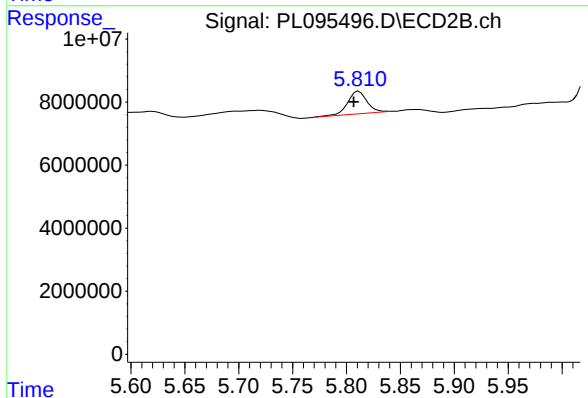


#14 Endrin

R.T.: 5.812 min
Delta R.T.: 0.005 min
Response: 8914133
Conc: 2.45 ng/ml

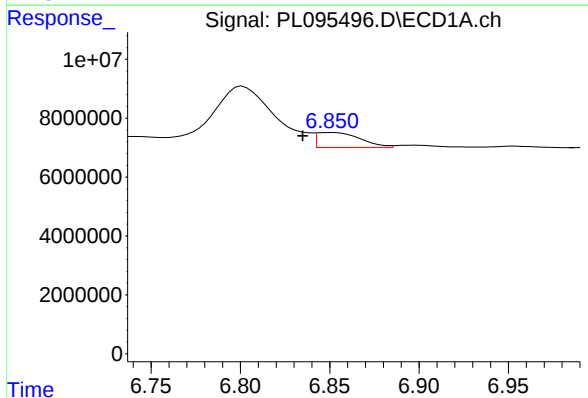


#15 Endosulfan II

R.T.: 6.851 min
Delta R.T.: 0.016 min
Response: 8552107
Conc: 2.68 ng/ml

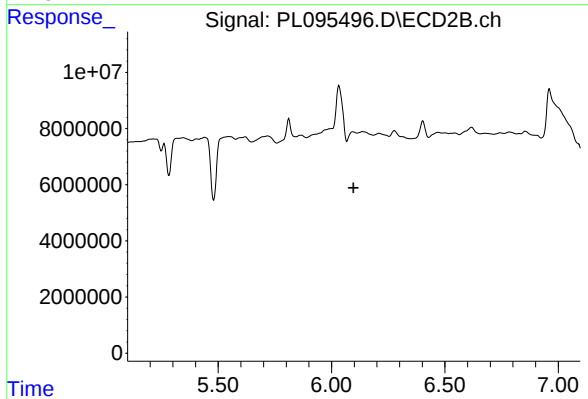

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.097 min
Response: 0
Conc: N.D.

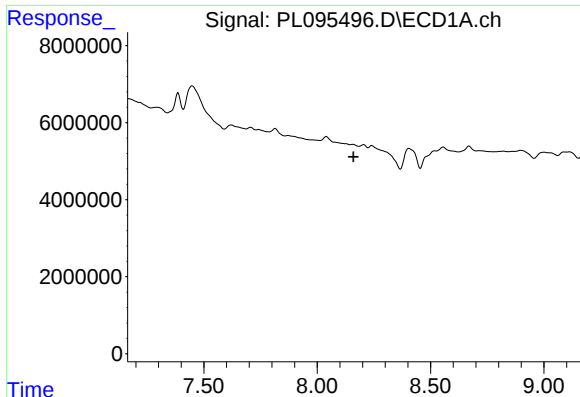

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

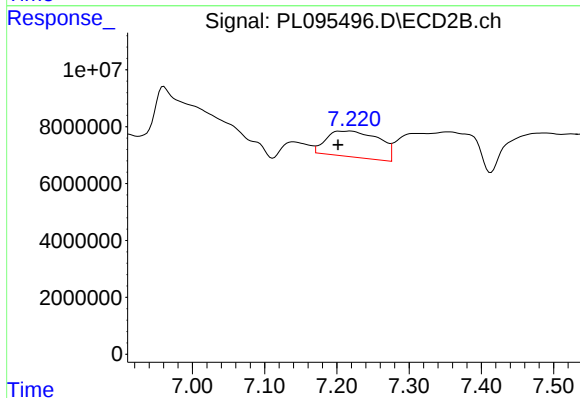


#22 Mirex

R.T.: 7.219 min
Delta R.T.: 0.017 min
Response: 46299261
Conc: 16.06 ng/ml

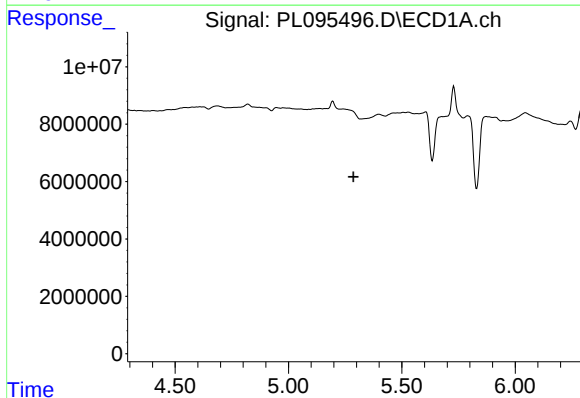


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.287 min
Response: 0
Conc: N.D.

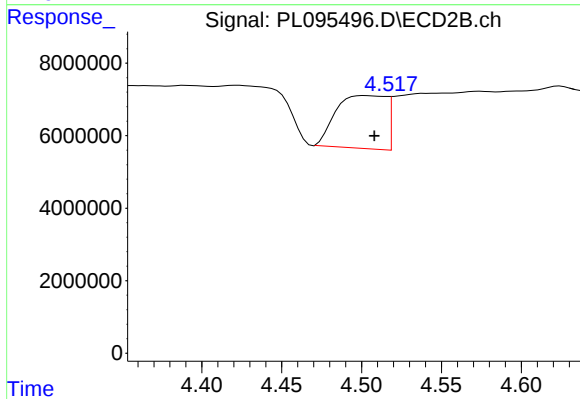

#24 Chlordane-2


R.T.: 4.502 min
Delta R.T.: -0.006 min
Response: 31494206
Conc: 171.14 ng/ml

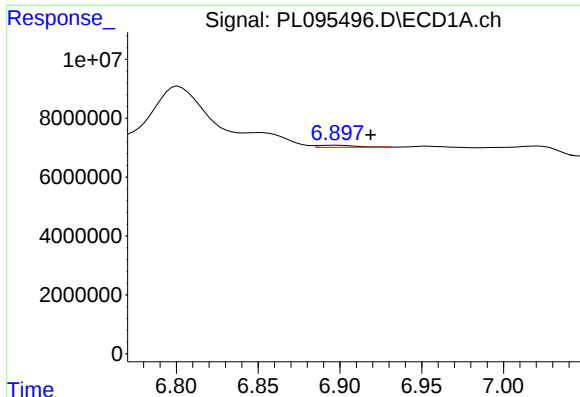

#27 Chlordane-5


R.T.: 6.898 min
Delta R.T.: -0.020 min
Response: 1066690
Conc: 7.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

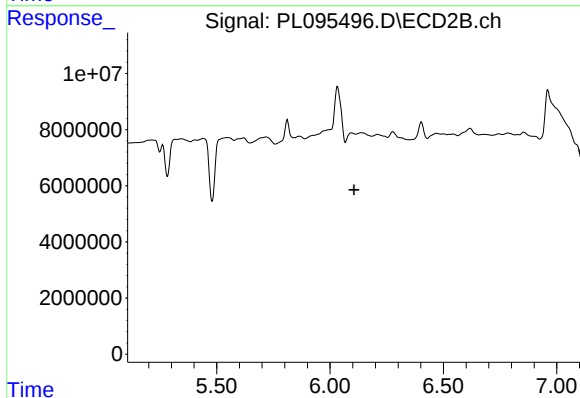


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.106 min
Response: 0
Conc: N.D.

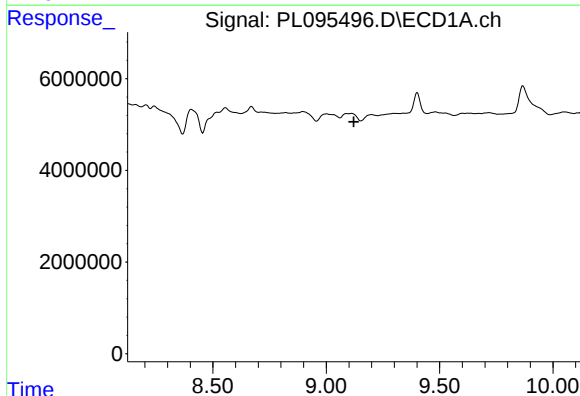

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.122 min
Response: 0
Conc: N.D.

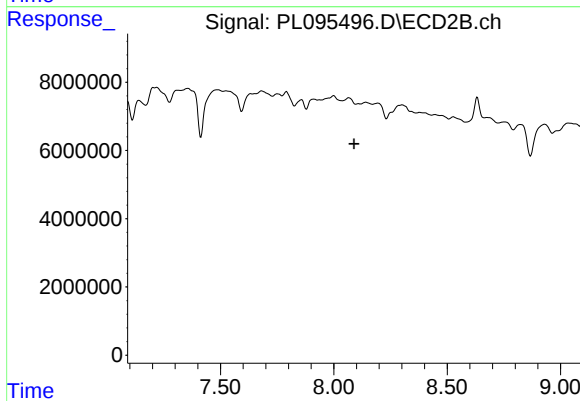

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.089 min
Response: 0
Conc: N.D.