

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050421\
 Data File : PL066661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2021 12:14
 Operator : AR\AJ
 Sample : PB136119BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB136119BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 12:52:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447f	4.153	51436602	61612483	13.651	17.543 #
28)	SA Decachlor...	8.182f	9.352	50879069	52117470	13.270	16.847 #
Target Compounds							
2)	A alpha-BHC	3.865	0.000	3094144	0	0.497	N.D. #
11)	B alpha-Chl...	5.388f	6.411f	2787964	-452943	0.566	N.D. #
13)	MA Dieldrin	5.694	0.000	8129015	0	1.676	N.D. #
14)	MA Endrin	5.977f	0.000	126930	0	0.029	N.D. #
15)	B Endosulfa...	6.206f	0.000	3785777	0	0.917	N.D. #
22)	Mirex	7.297f	0.000	1261739	0	0.343	N.D. #
26)	Chlordane-4	5.388f	6.411f	2787964	-452943	6.606	N.D. #
27)	Chlordane-5	6.206f	7.213	3785777	614612	22.481	5.234 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050421\
Data File : PL066661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2021 12:14
Operator : AR\AJ
Sample : PB136119BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB136119BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 12:52:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

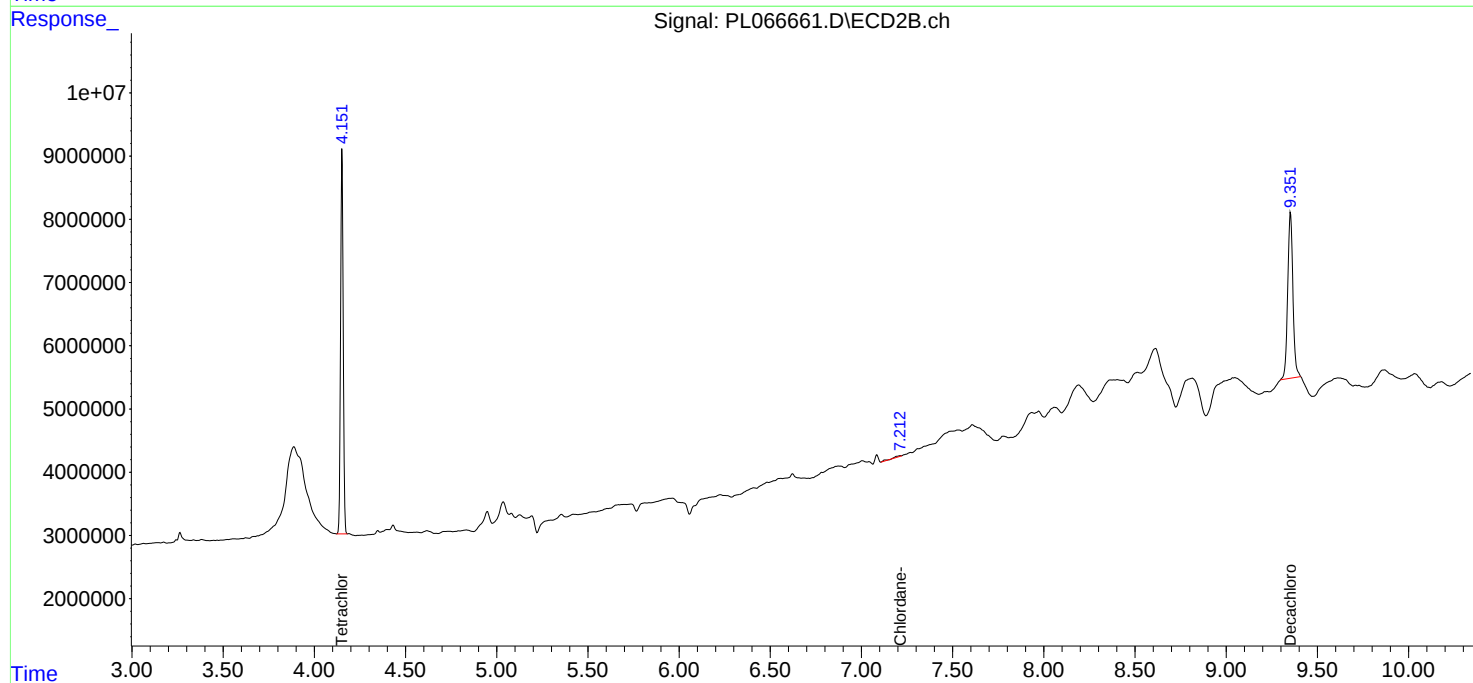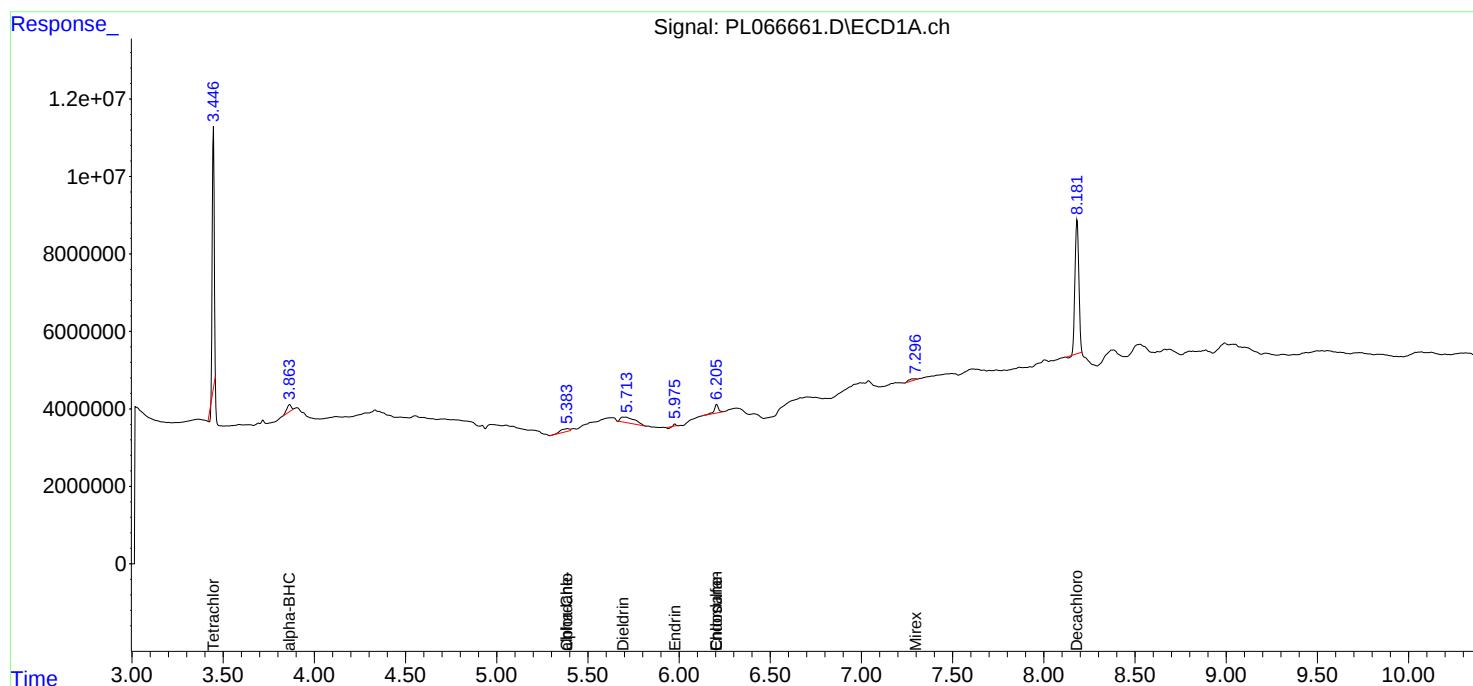


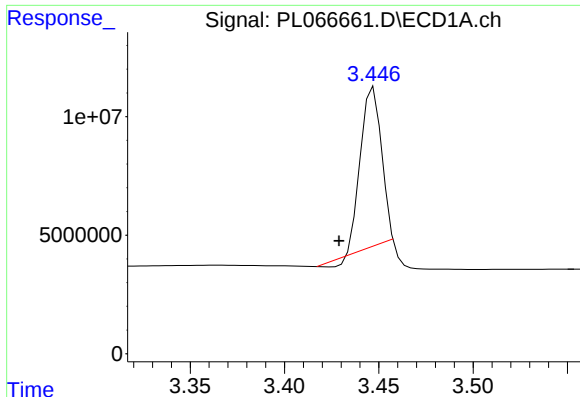

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: 0.018 min
Response: 51436602
Conc: 13.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136119BL

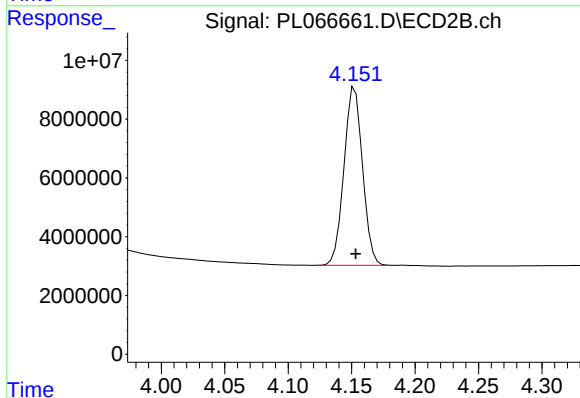


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 61612483
Conc: 17.54 ng/ml

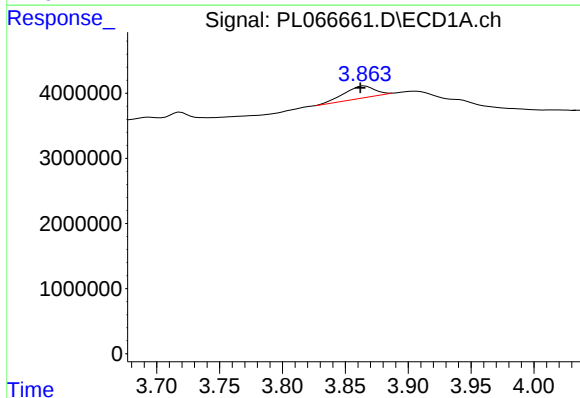


#2 alpha-BHC

R.T.: 3.865 min
Delta R.T.: 0.003 min
Response: 3094144
Conc: 0.50 ng/ml

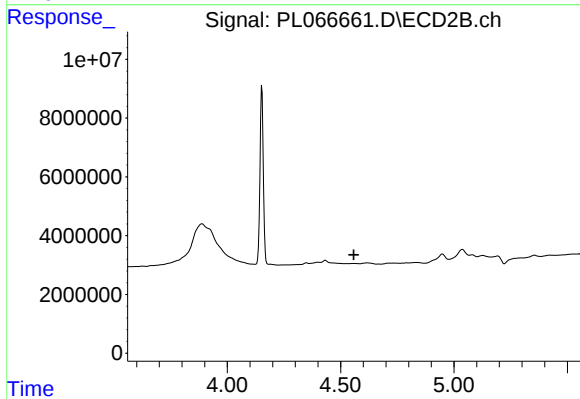

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.557 min
Response: 0
Conc: N.D.

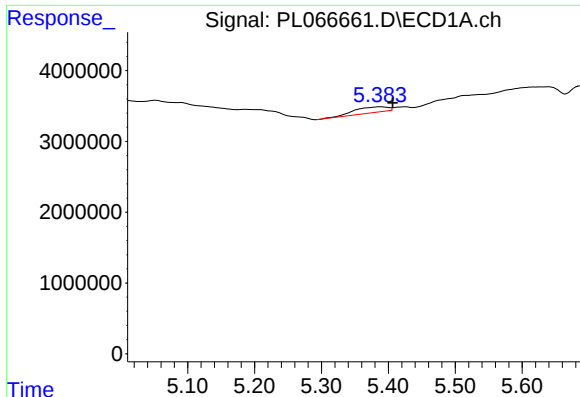

#11 alpha-Chlordane


R.T.: 5.388 min
Delta R.T.: -0.018 min
Response: 2787964
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136119BL

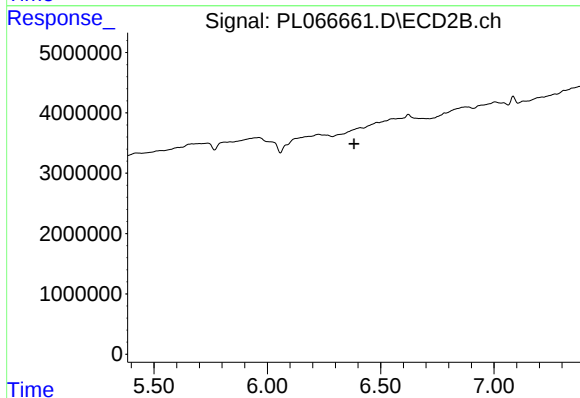


#11 alpha-Chlordane

R.T.: 6.411 min
Delta R.T.: 0.028 min
Response: -452943
Conc: N.D.

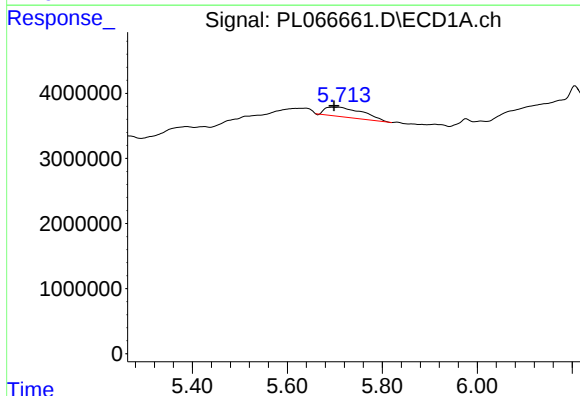


#13 Dieldrin

R.T.: 5.694 min
Delta R.T.: -0.005 min
Response: 8129015
Conc: 1.68 ng/ml

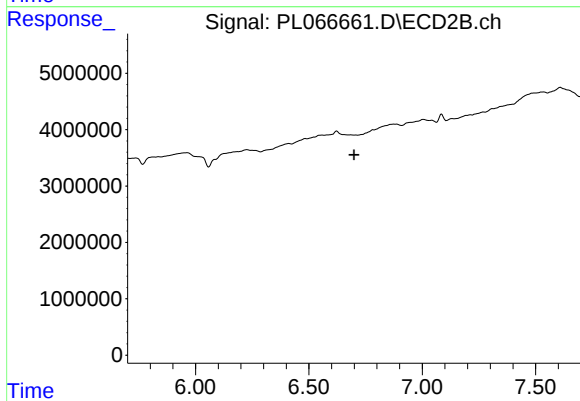

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.699 min
Response: 0
Conc: N.D.

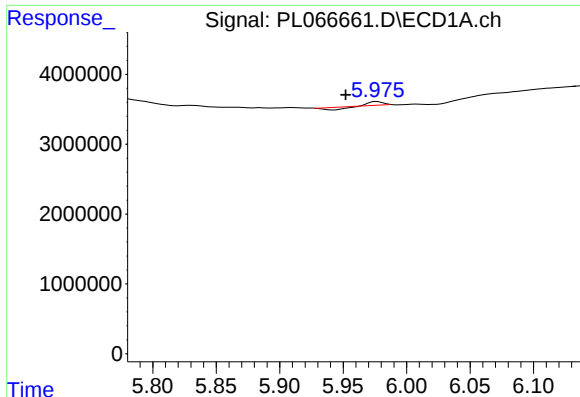

#14 Endrin


R.T.: 5.977 min
Delta R.T.: 0.024 min
Response: 126930
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136119BL

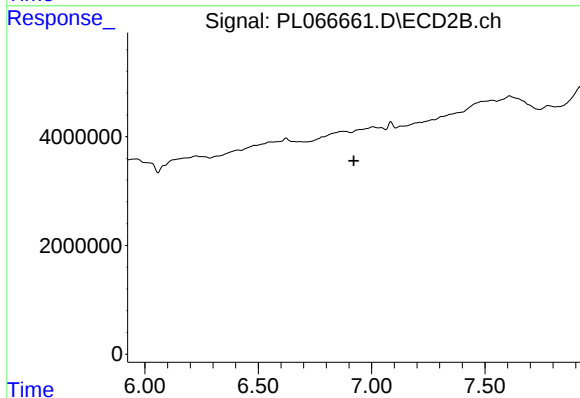


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

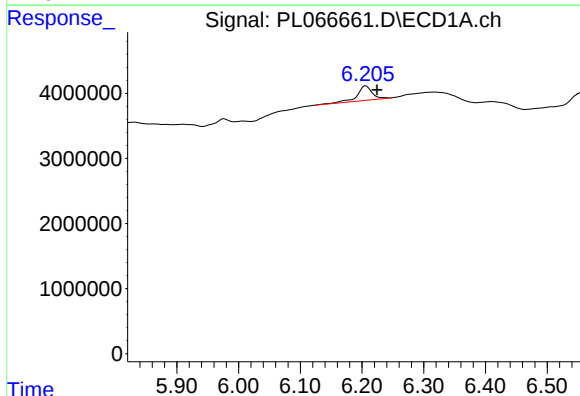


#15 Endosulfan II

R.T.: 6.206 min
Delta R.T.: -0.018 min
Response: 3785777
Conc: 0.92 ng/ml

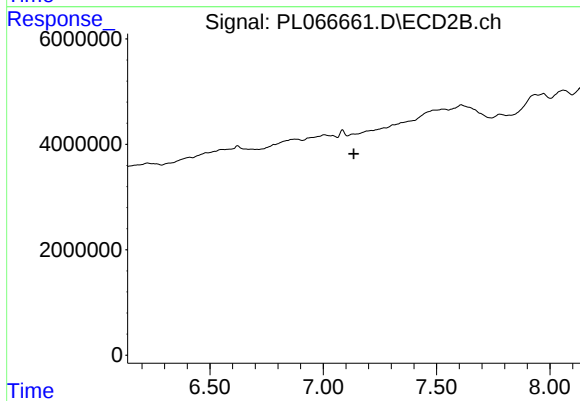

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.136 min
Response: 0
Conc: N.D.

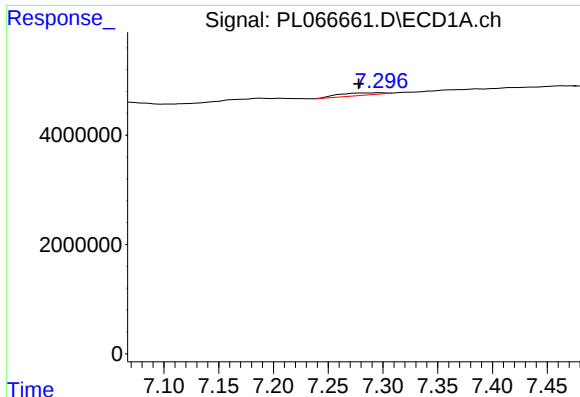

#22 Mirex


R.T.: 7.297 min
Delta R.T.: 0.019 min
Response: 1261739
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136119BL

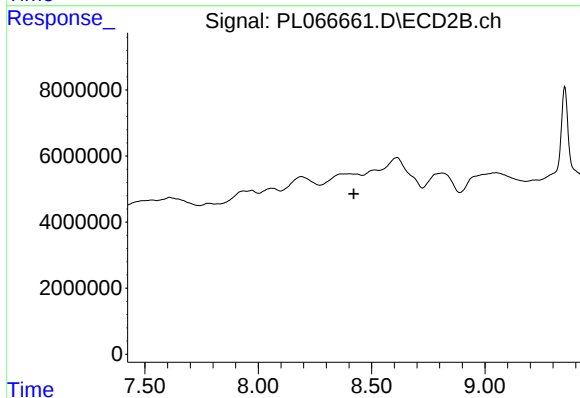


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.421 min
Response: 0
Conc: N.D.

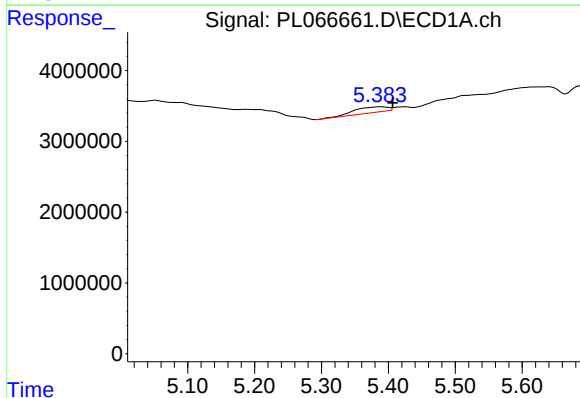


#26 Chlordane-4

R.T.: 5.388 min
Delta R.T.: -0.019 min
Response: 2787964
Conc: 6.61 ng/ml

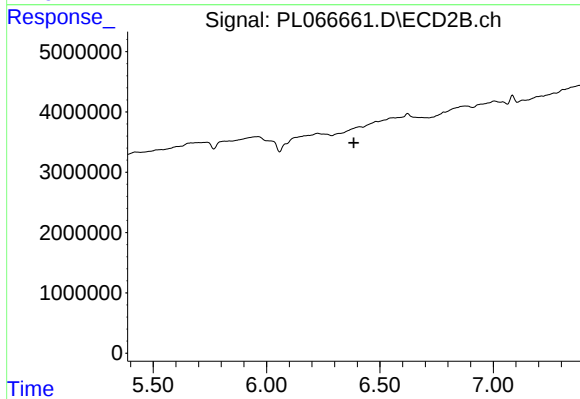

#26 Chlordane-4


R.T.: 6.411 min
Delta R.T.: 0.027 min
Response: -452943
Conc: N.D.

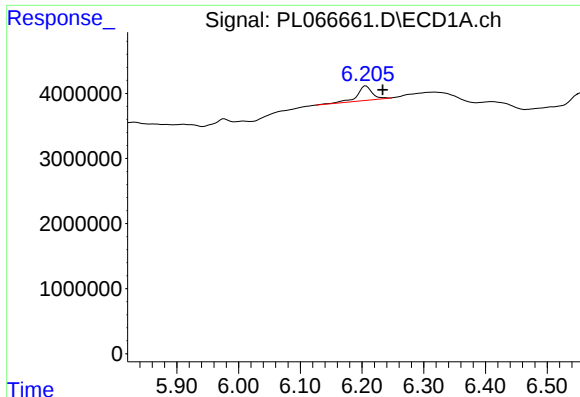

#27 Chlordane-5


R.T.: 6.206 min
Delta R.T.: -0.027 min
Response: 3785777
Conc: 22.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136119BL

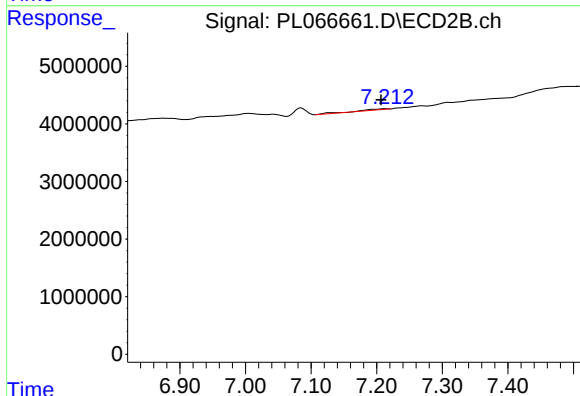


#27 Chlordane-5

R.T.: 7.213 min
Delta R.T.: 0.007 min
Response: 614612
Conc: 5.23 ng/ml

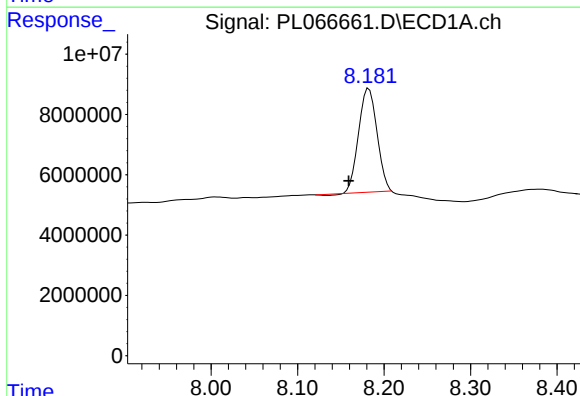

#28 Decachlorobiphenyl

R.T.: 8.182 min
Delta R.T.: 0.023 min
Response: 50879069
Conc: 13.27 ng/ml

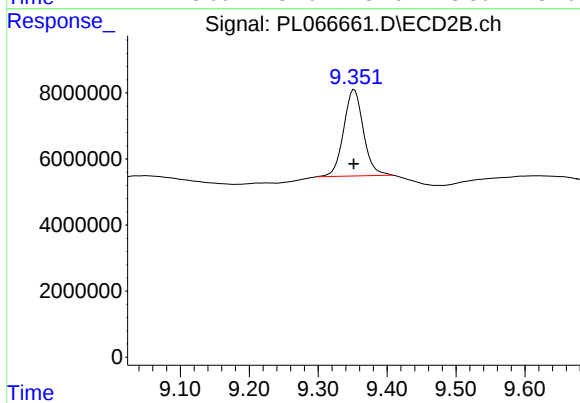

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 52117470
Conc: 16.85 ng/ml