

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050421\
 Data File : PL066664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2021 12:56
 Operator : AR\AJ
 Sample : M2237-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 17:19:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.153	44027240	40627407	11.684	11.568
28)	SA Decachlor...	8.163	9.353	38092545	34986877	9.935	11.309
Target Compounds							
10)	B gamma-Chl...	5.347	6.309	3197782	2026384	0.628	0.487
11)	B alpha-Chl...	5.404	6.383	4177527	4591331	0.848	1.107 #
12)	B 4,4'-DDE	5.572	6.539	3324242	3971833	0.729	1.047 #
14)	MA Endrin	0.000	6.942f	0	816149	N.D.	0.260 #
16)	A 4,4'-DDD	0.000	7.038	0	1910019	N.D.	0.613 #
17)	MA 4,4'-DDT	6.321	7.340	1384316	419852	0.355	0.130 #
23)	Chlordane-1	4.288	0.000	2513711	0	14.871	N.D. #
25)	Chlordane-3	5.347	6.309	3197782	2026384	6.426	3.615 #
26)	Chlordane-4	5.404	6.383	4177527	4591331	9.899	6.839 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050421\
Data File : PL066664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2021 12:56
Operator : AR\AJ
Sample : M2237-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 17:19:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

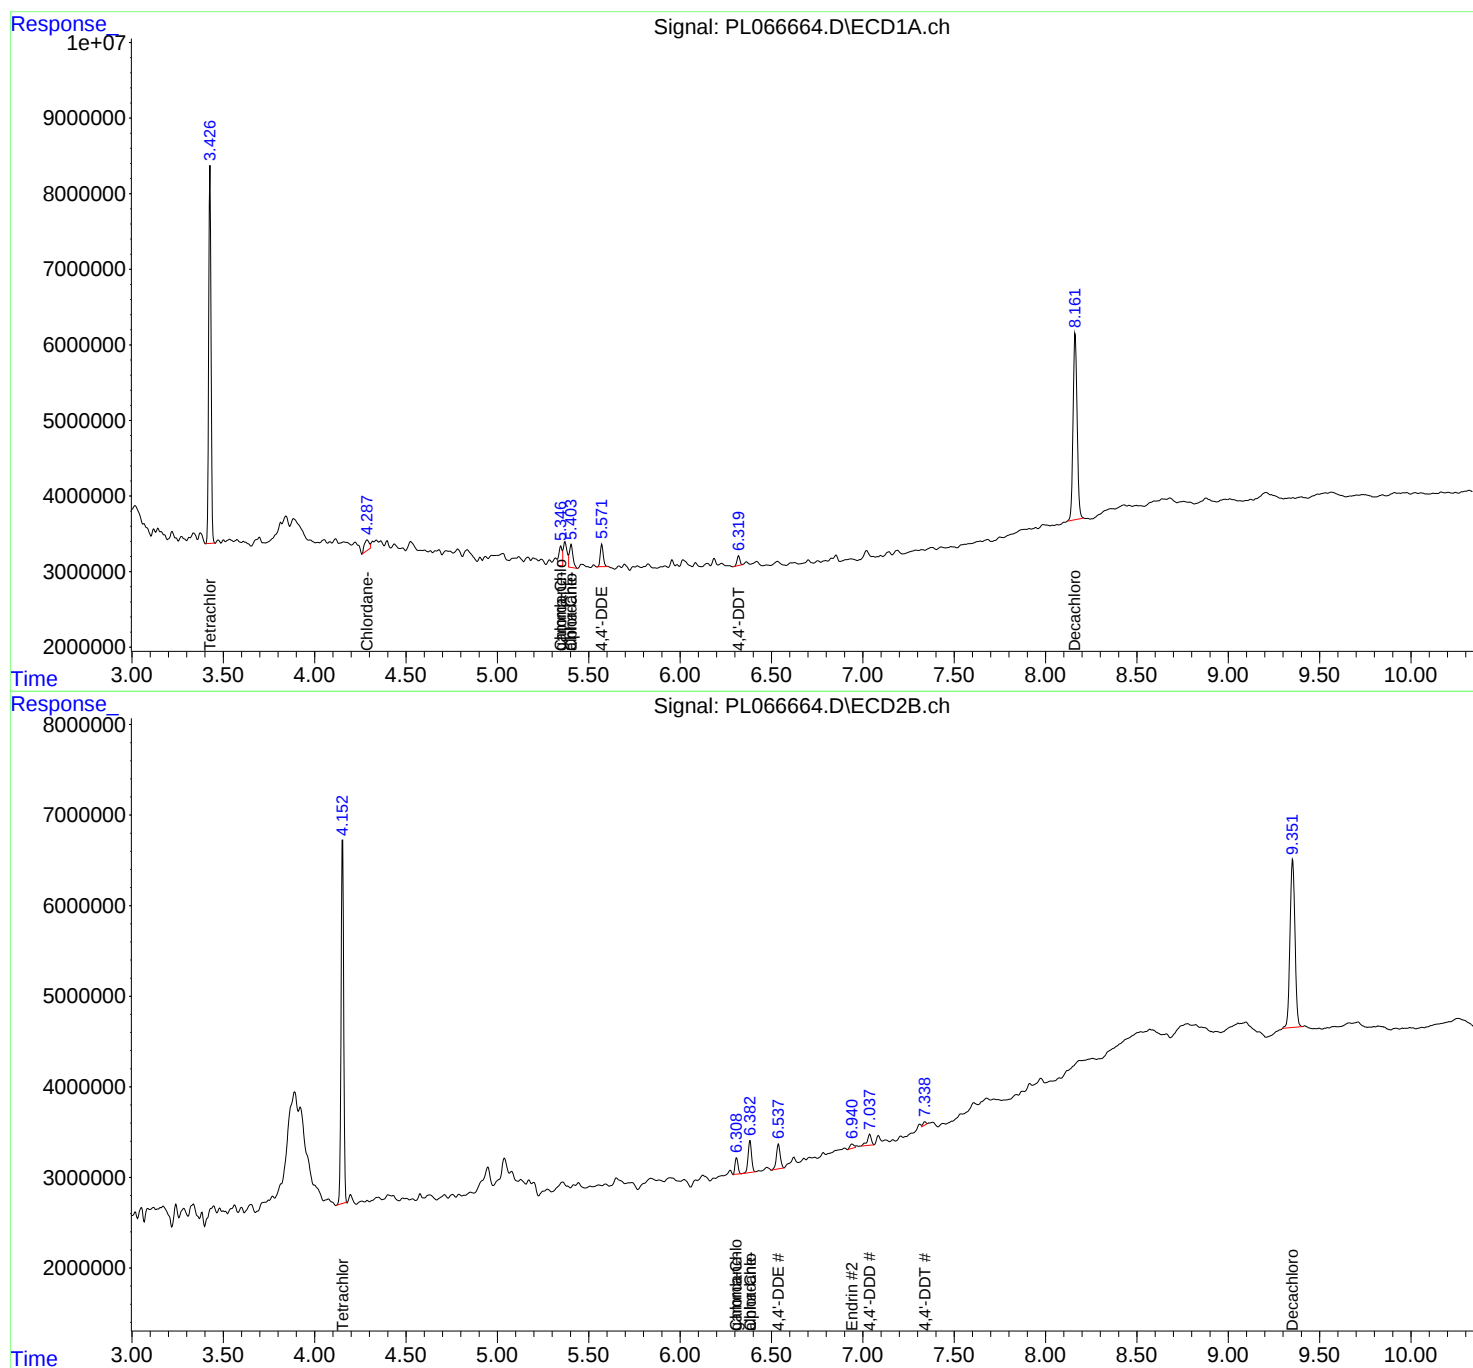


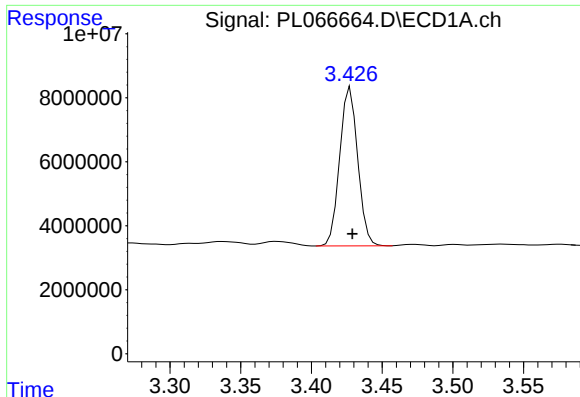

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: -0.001 min
Response: 44027240
Conc: 11.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

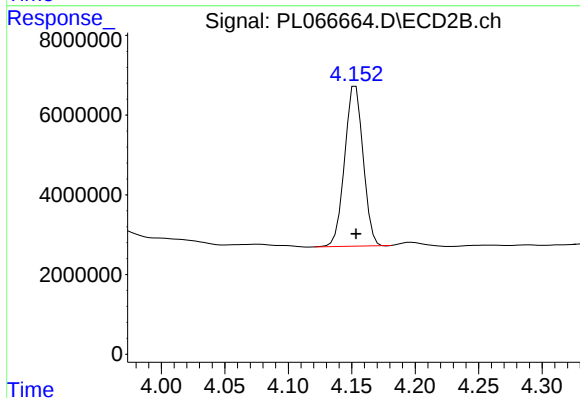


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 40627407
Conc: 11.57 ng/ml

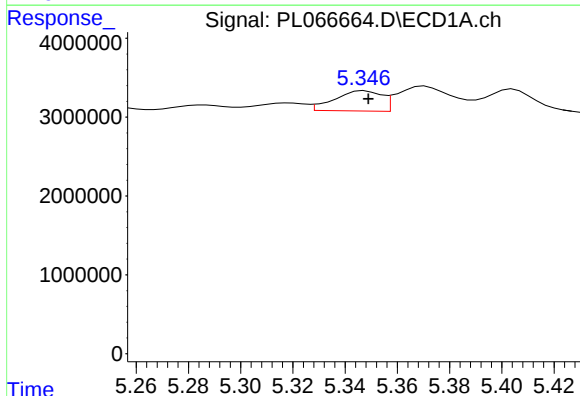


#10 gamma-Chlordane

R.T.: 5.347 min
Delta R.T.: -0.001 min
Response: 3197782
Conc: 0.63 ng/ml

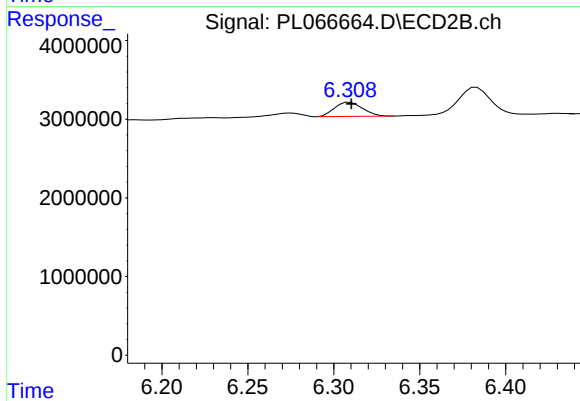

#10 gamma-Chlordane


R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 2026384
Conc: 0.49 ng/ml

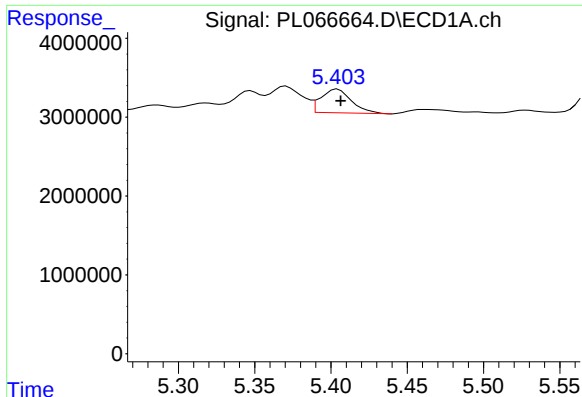

#11 alpha-Chlordane


R.T.: 5.404 min
Delta R.T.: -0.002 min
Response: 4177527
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

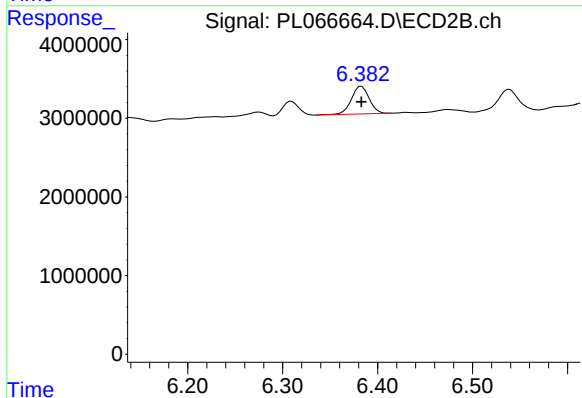


#11 alpha-Chlordane

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 4591331
Conc: 1.11 ng/ml

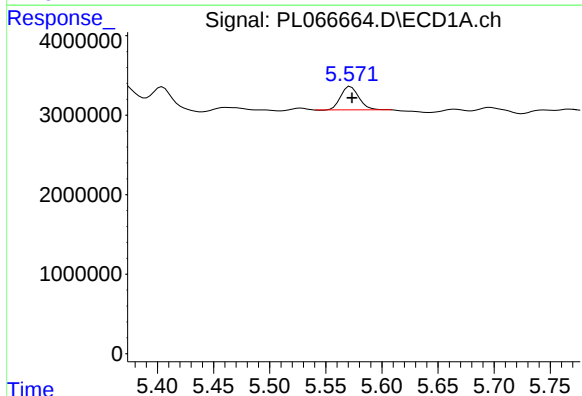


#12 4,4'-DDE

R.T.: 5.572 min
Delta R.T.: -0.001 min
Response: 3324242
Conc: 0.73 ng/ml

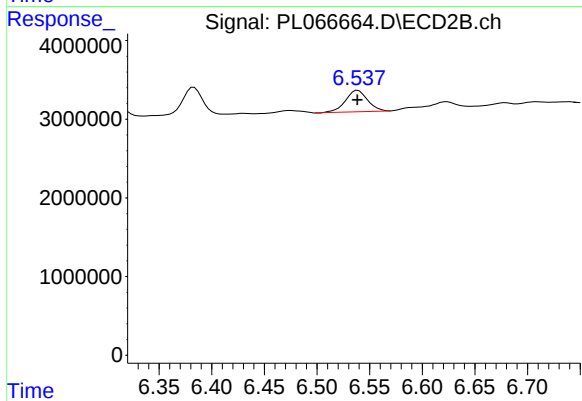

#12 4,4'-DDE


R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 3971833
Conc: 1.05 ng/ml

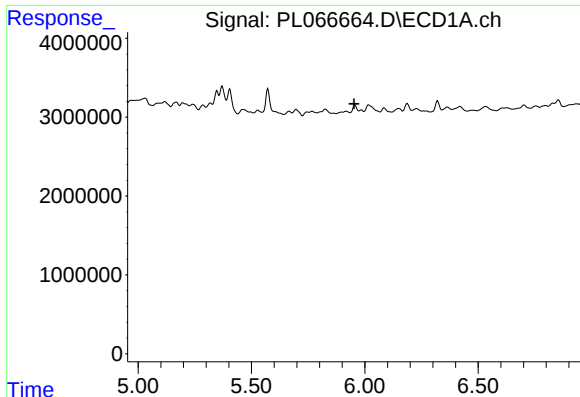

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.952 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

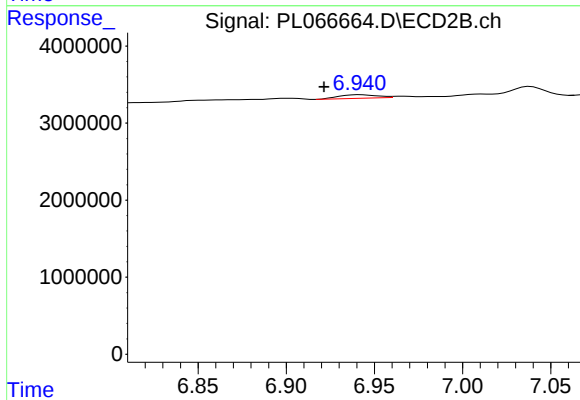


#14 Endrin

R.T.: 6.942 min
Delta R.T.: 0.020 min
Response: 816149
Conc: 0.26 ng/ml

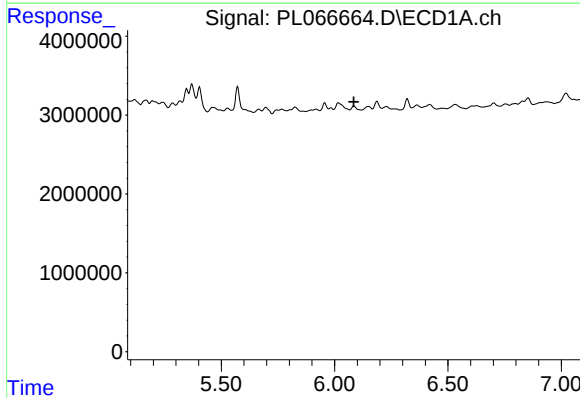


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.085 min
Response: 0
Conc: N.D.

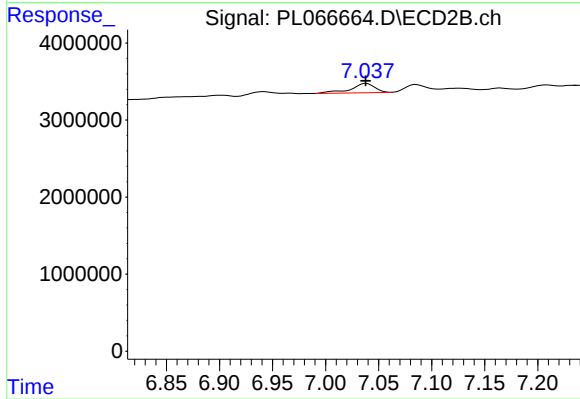

#16 4,4'-DDD


R.T.: 7.038 min
Delta R.T.: 0.000 min
Response: 1910019
Conc: 0.61 ng/ml

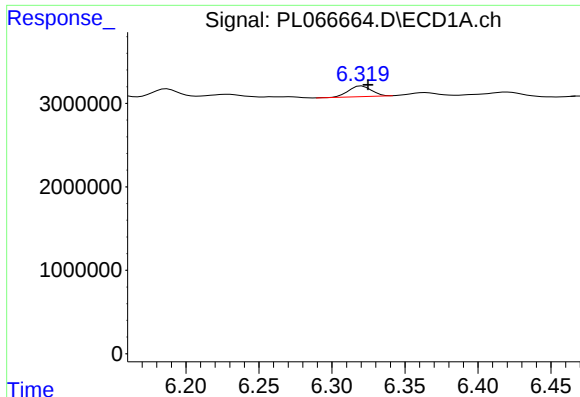

#17 4,4'-DDT


R.T.: 6.321 min
Delta R.T.: -0.004 min
Response: 1384316
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

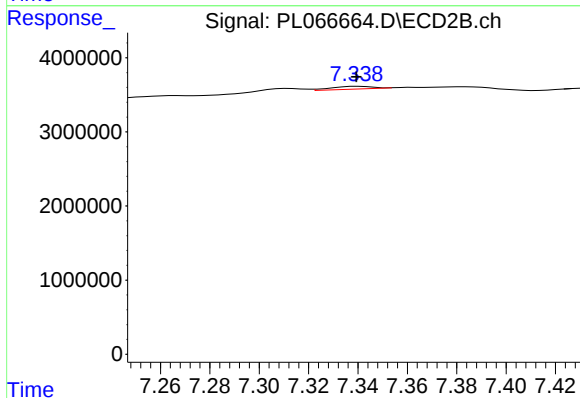


#17 4,4'-DDT

R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 419852
Conc: 0.13 ng/ml

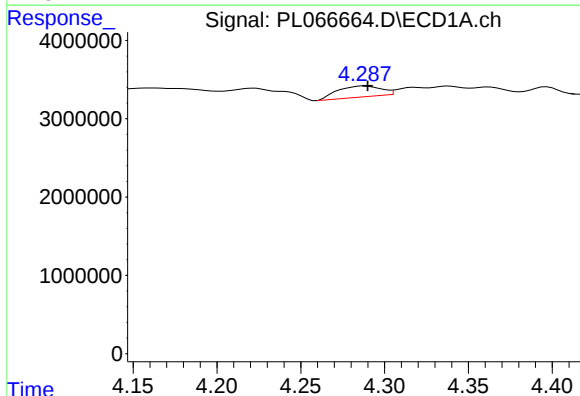


#23 Chlordane-1

R.T.: 4.288 min
Delta R.T.: -0.002 min
Response: 2513711
Conc: 14.87 ng/ml

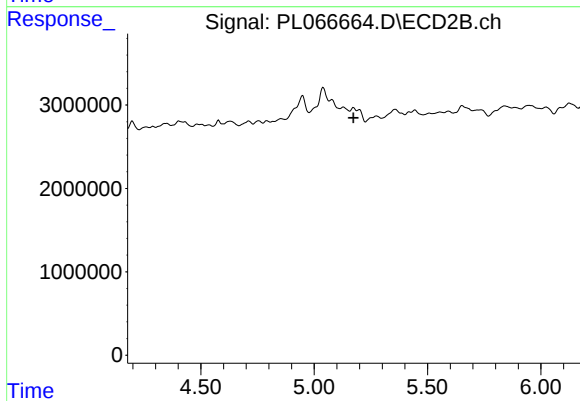

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.174 min
Response: 0
Conc: N.D.

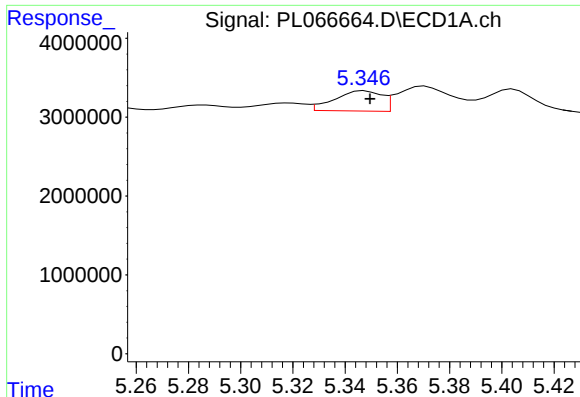

#25 Chlordane-3


R.T.: 5.347 min
Delta R.T.: -0.002 min
Response: 3197782
Conc: 6.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

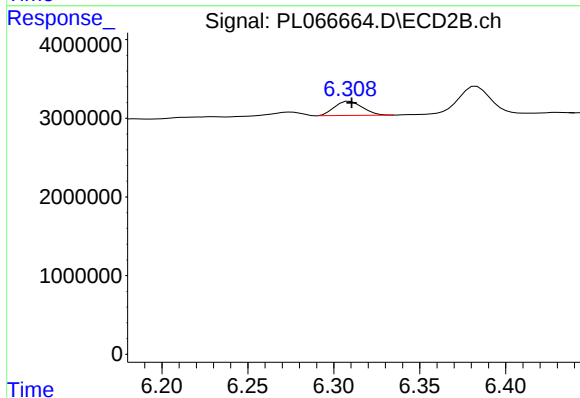


#25 Chlordane-3

R.T.: 6.309 min
Delta R.T.: -0.001 min
Response: 2026384
Conc: 3.62 ng/ml

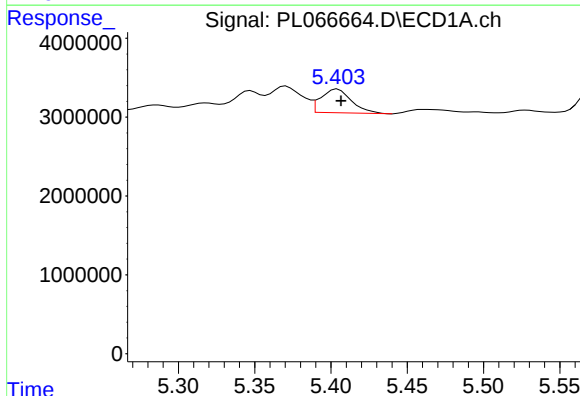


#26 Chlordane-4

R.T.: 5.404 min
Delta R.T.: -0.002 min
Response: 4177527
Conc: 9.90 ng/ml

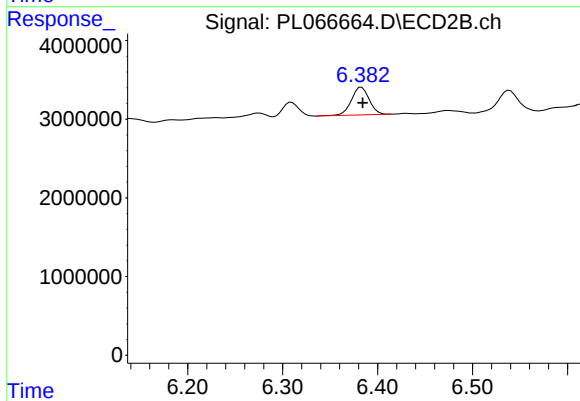

#26 Chlordane-4


R.T.: 6.383 min
Delta R.T.: -0.001 min
Response: 4591331
Conc: 6.84 ng/ml

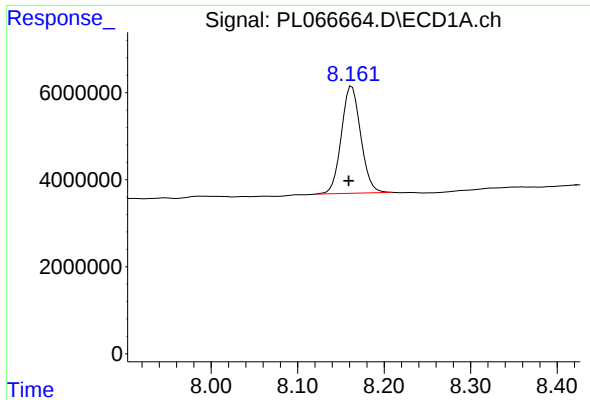

#28 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: 0.004 min
Response: 38092545
Conc: 9.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

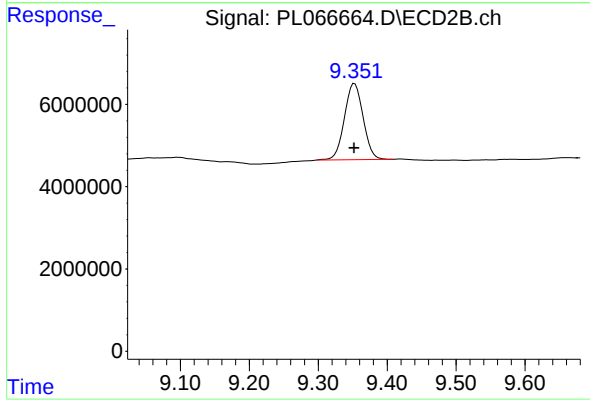

#28 Decachlorobiphenyl

R.T.: 9.353 min
Delta R.T.: 0.000 min
Response: 34986877
Conc: 11.31 ng/ml