

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050421\
 Data File : PL066674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2021 17:41
 Operator : AR\AJ
 Sample : M2263-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 02:26:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.427	4.152	76437010	81528003	20.285	23.214
28)	SA Decachlor...	8.151	9.349	69442796	58814004	18.111	19.012
Target Compounds							
2)	A alpha-BHC	3.887f	0.000	5165197	0	0.830	N.D. #
5)	MB Aldrin	0.000	5.649f	0	1817032	N.D.	0.389 #
6)	B beta-BHC	0.000	5.042	0	15476270	N.D.	3.817 #
14)	MA Endrin	0.000	6.946f	0	1367743	N.D.	0.436 #
16)	A 4,4'-DDD	6.110f	0.000	1496636	0	0.394	N.D. #
17)	MA 4,4'-DDT	0.000	7.366f	0	1578401	N.D.	0.488 #
23)	Chlordane-1	4.296	0.000	2108818	0	12.476	N.D. #
24)	Chlordane-2	0.000	5.649	0	1817032	N.D.	11.188 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050421\
Data File : PL066674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2021 17:41
Operator : AR\AJ
Sample : M2263-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 02:26:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

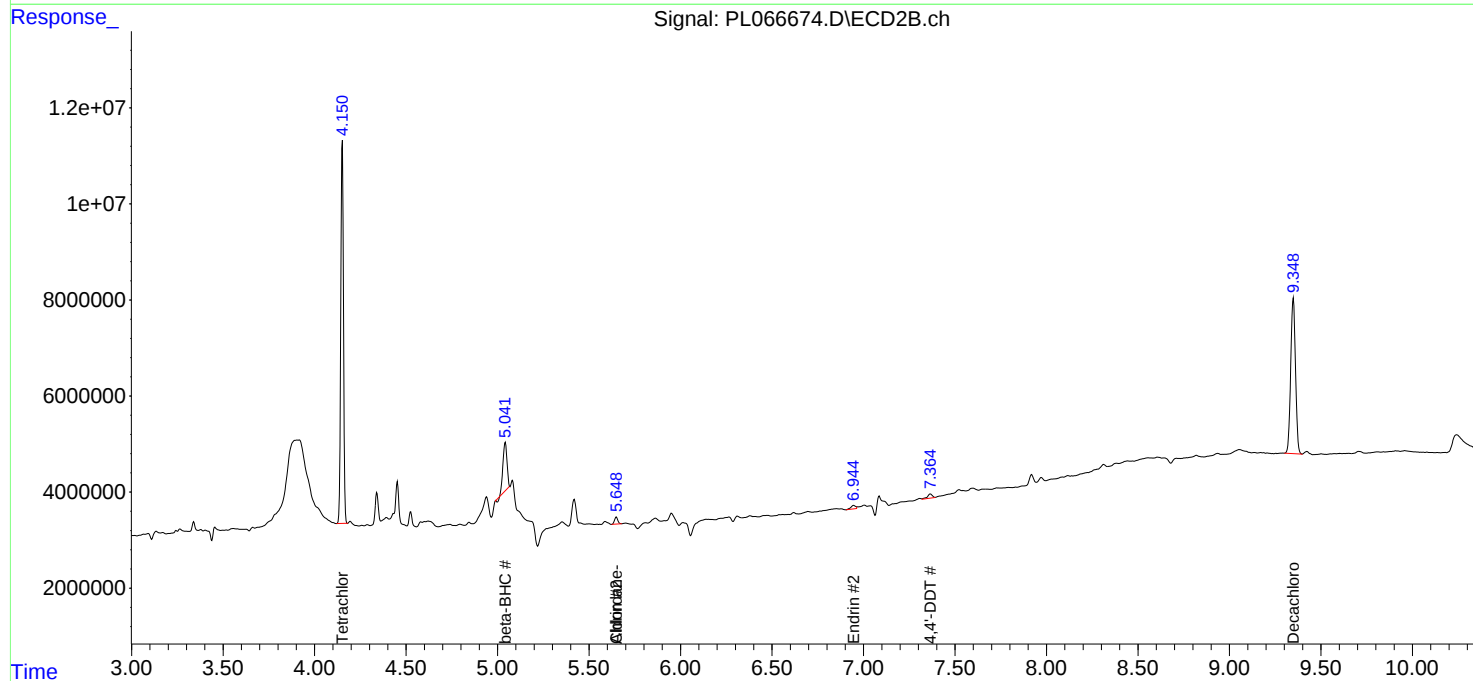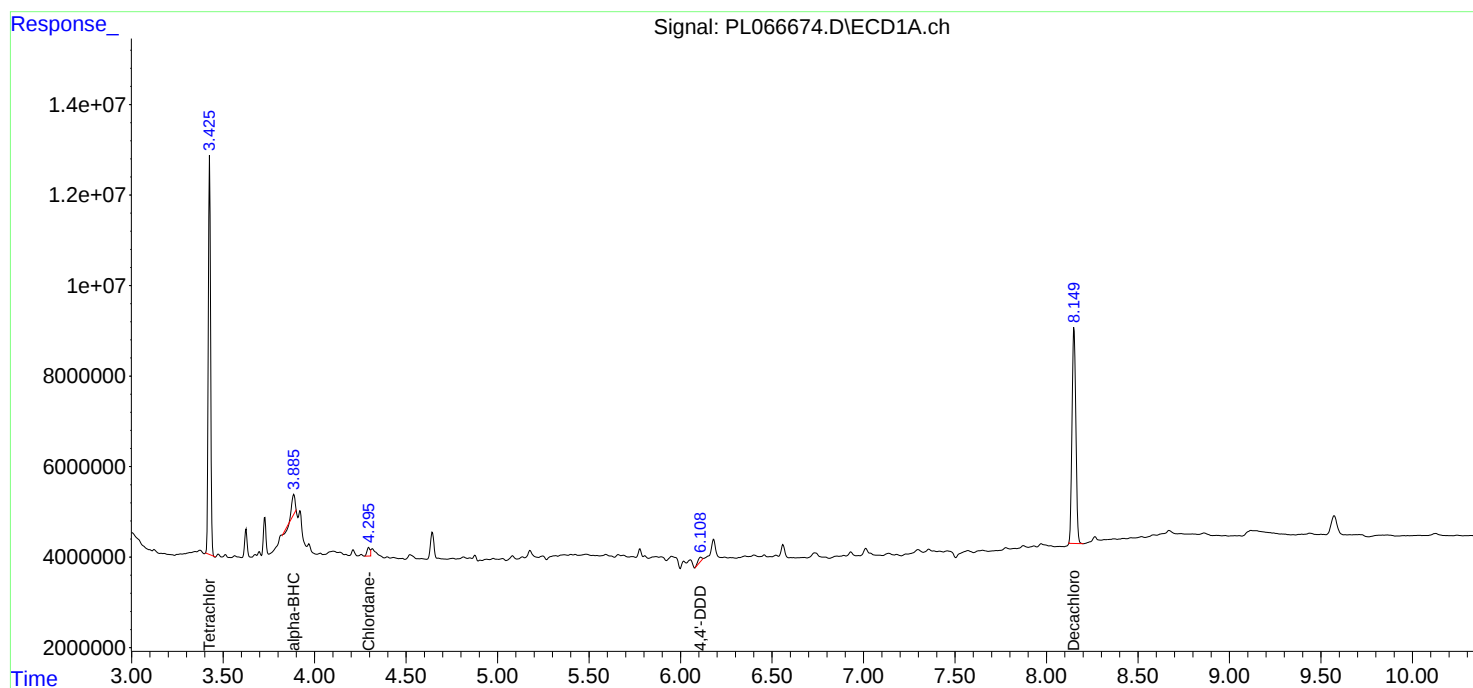


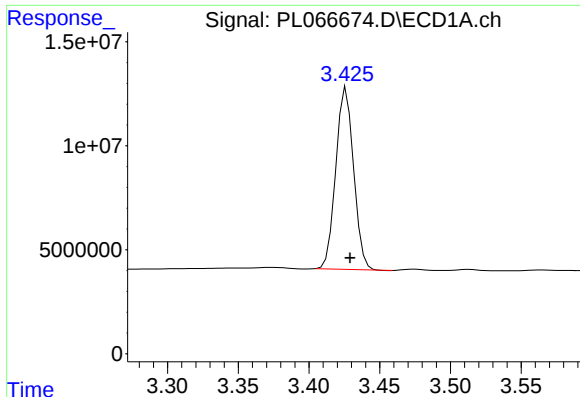

#1 Tetrachloro-m-xylene


R.T.: 3.427 min
Delta R.T.: -0.002 min
Response: 76437010
Conc: 20.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

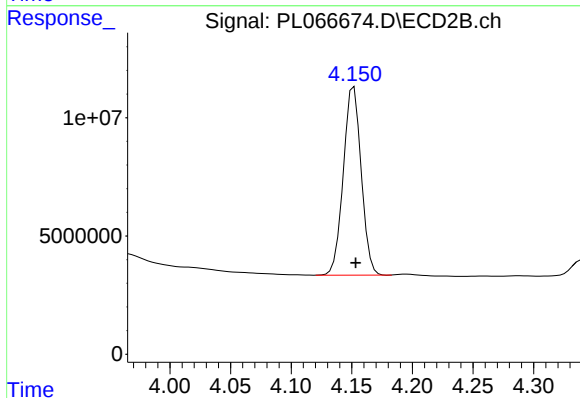


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: -0.002 min
Response: 81528003
Conc: 23.21 ng/ml

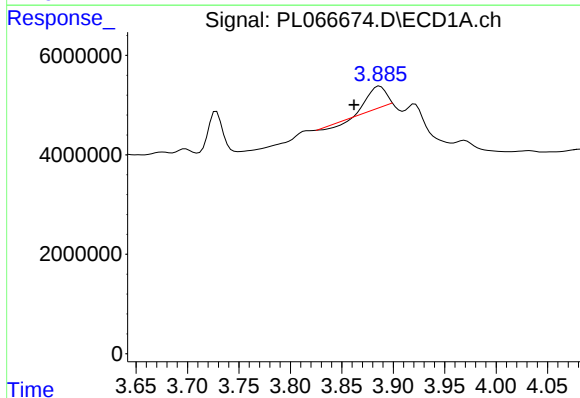


#2 alpha-BHC

R.T.: 3.887 min
Delta R.T.: 0.025 min
Response: 5165197
Conc: 0.83 ng/ml

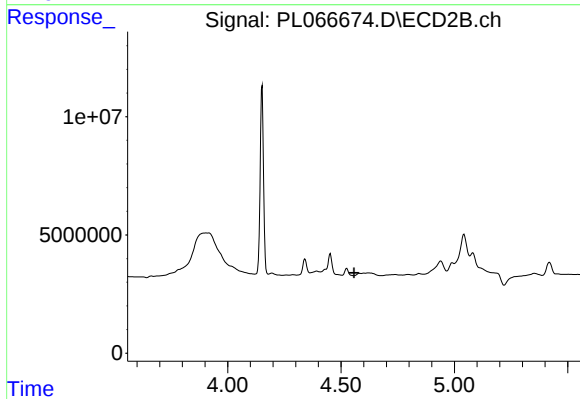

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.557 min
Response: 0
Conc: N.D.

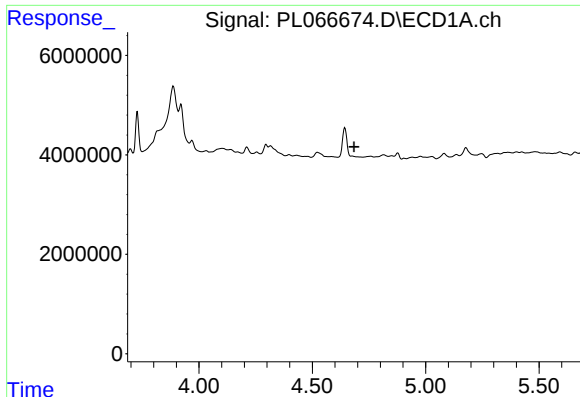

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.684 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

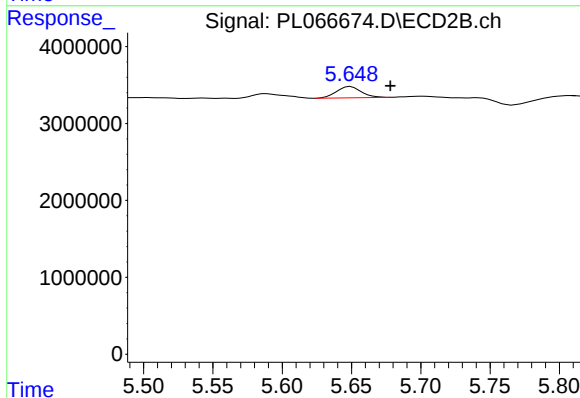


#5 Aldrin

R.T.: 5.649 min
Delta R.T.: -0.029 min
Response: 1817032
Conc: 0.39 ng/ml

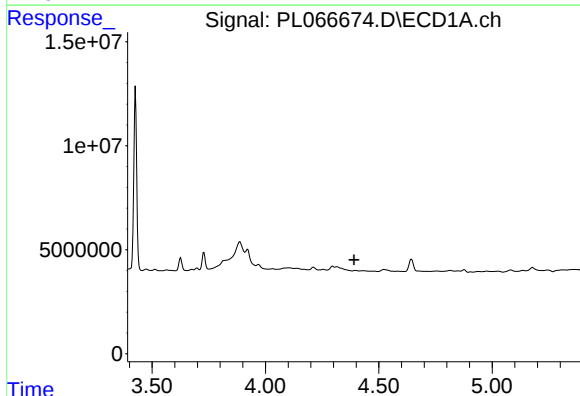


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.391 min
Response: 0
Conc: N.D.

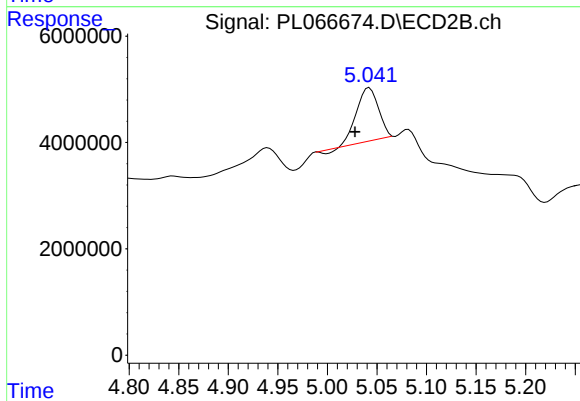

#6 beta-BHC


R.T.: 5.042 min
Delta R.T.: 0.014 min
Response: 15476270
Conc: 3.82 ng/ml

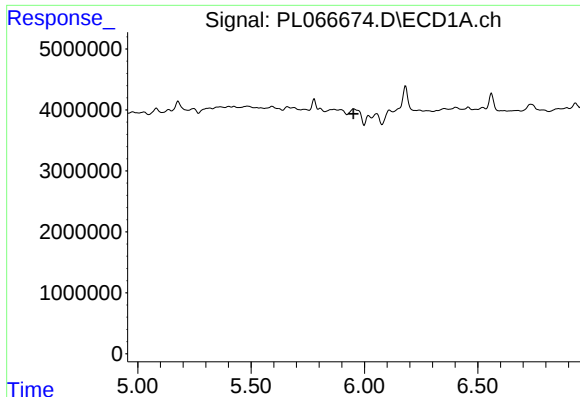

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.952 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

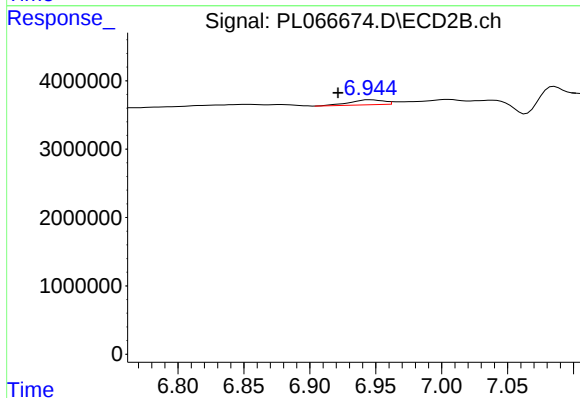


#14 Endrin

R.T.: 6.946 min
Delta R.T.: 0.024 min
Response: 1367743
Conc: 0.44 ng/ml

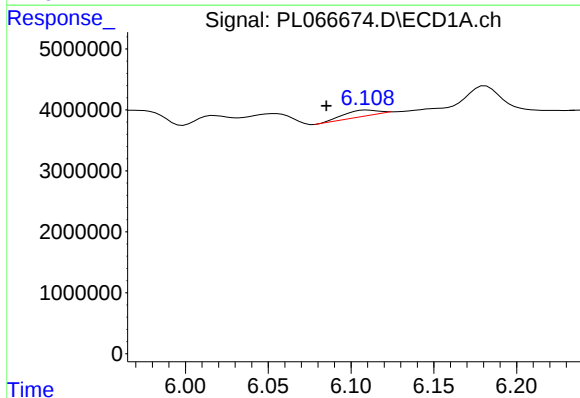


#16 4,4'-DDD

R.T.: 6.110 min
Delta R.T.: 0.025 min
Response: 1496636
Conc: 0.39 ng/ml

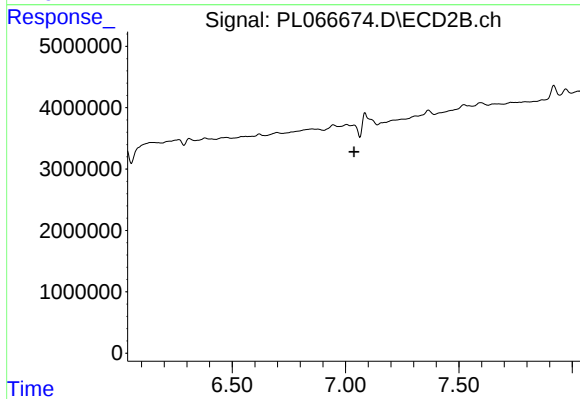

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 7.038 min
Response: 0
Conc: N.D.

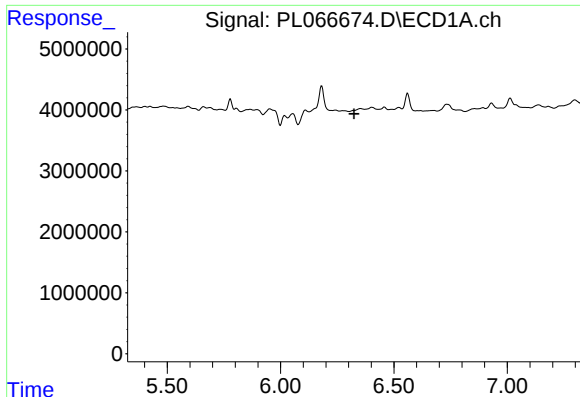

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.325 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

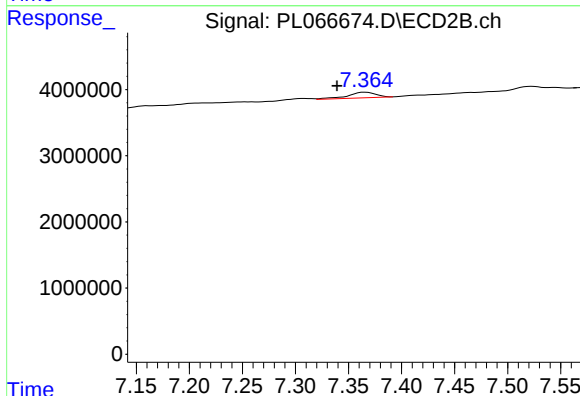


#17 4,4'-DDT

R.T.: 7.366 min
Delta R.T.: 0.026 min
Response: 1578401
Conc: 0.49 ng/ml

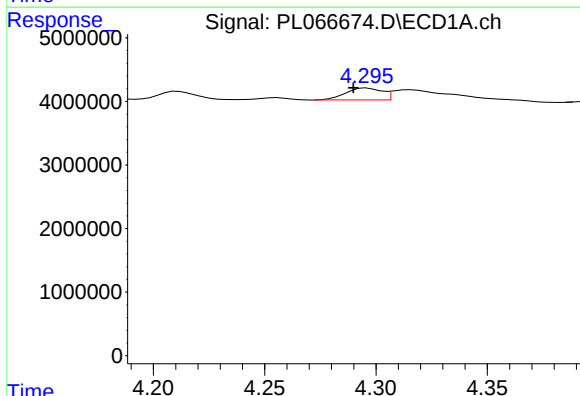


#23 Chlordane-1

R.T.: 4.296 min
Delta R.T.: 0.006 min
Response: 2108818
Conc: 12.48 ng/ml

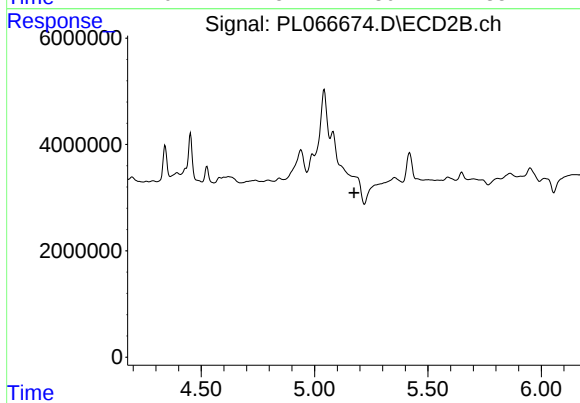

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.174 min
Response: 0
Conc: N.D.

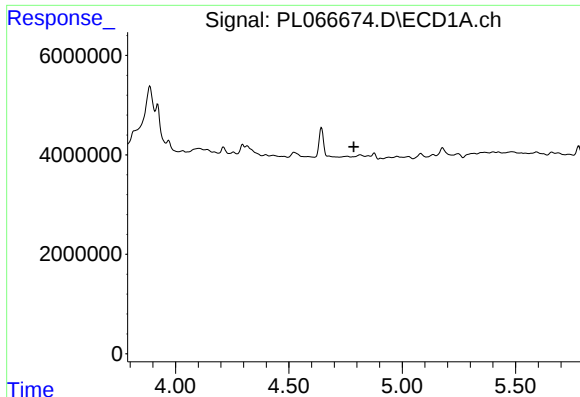

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.786 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

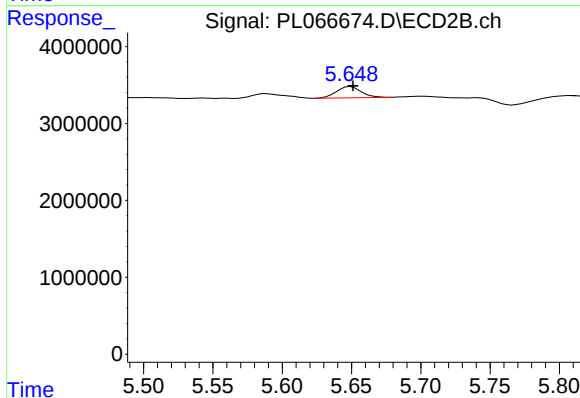


#24 Chlordane-2

R.T.: 5.649 min
Delta R.T.: -0.002 min
Response: 1817032
Conc: 11.19 ng/ml

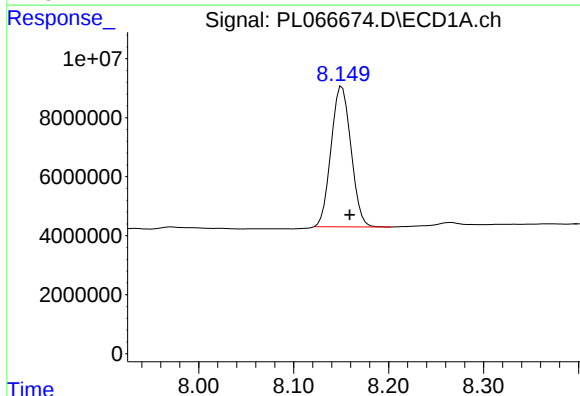

#28 Decachlorobiphenyl

R.T.: 8.151 min
Delta R.T.: -0.008 min
Response: 69442796
Conc: 18.11 ng/ml

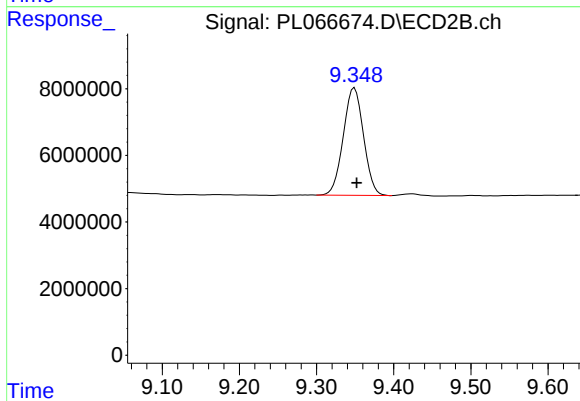

#28 Decachlorobiphenyl

R.T.: 9.349 min
Delta R.T.: -0.003 min
Response: 58814004
Conc: 19.01 ng/ml