

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050421\
 Data File : PL066681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2021 19:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 02:27:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.152	73333220	69279177	19.462	19.726
28)	SA Decachlor...	8.151	9.348	66737083	52273598	17.406	16.897
Target Compounds							
2)	A alpha-BHC	3.888f	0.000	1999055	0	0.321	N.D. #
6)	B beta-BHC	4.399	5.044f	1156576	12028240	0.437	2.225 #
8)	B Heptachlo...	0.000	6.069	0	1340831	N.D.	0.362 #
14)	MA Endrin	5.952	0.000	2106190	0	0.484	N.D. #
23)	Chlordane-1	4.312f	0.000	422811	0	2.501	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050421\
Data File : PL066681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2021 19:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 02:27:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

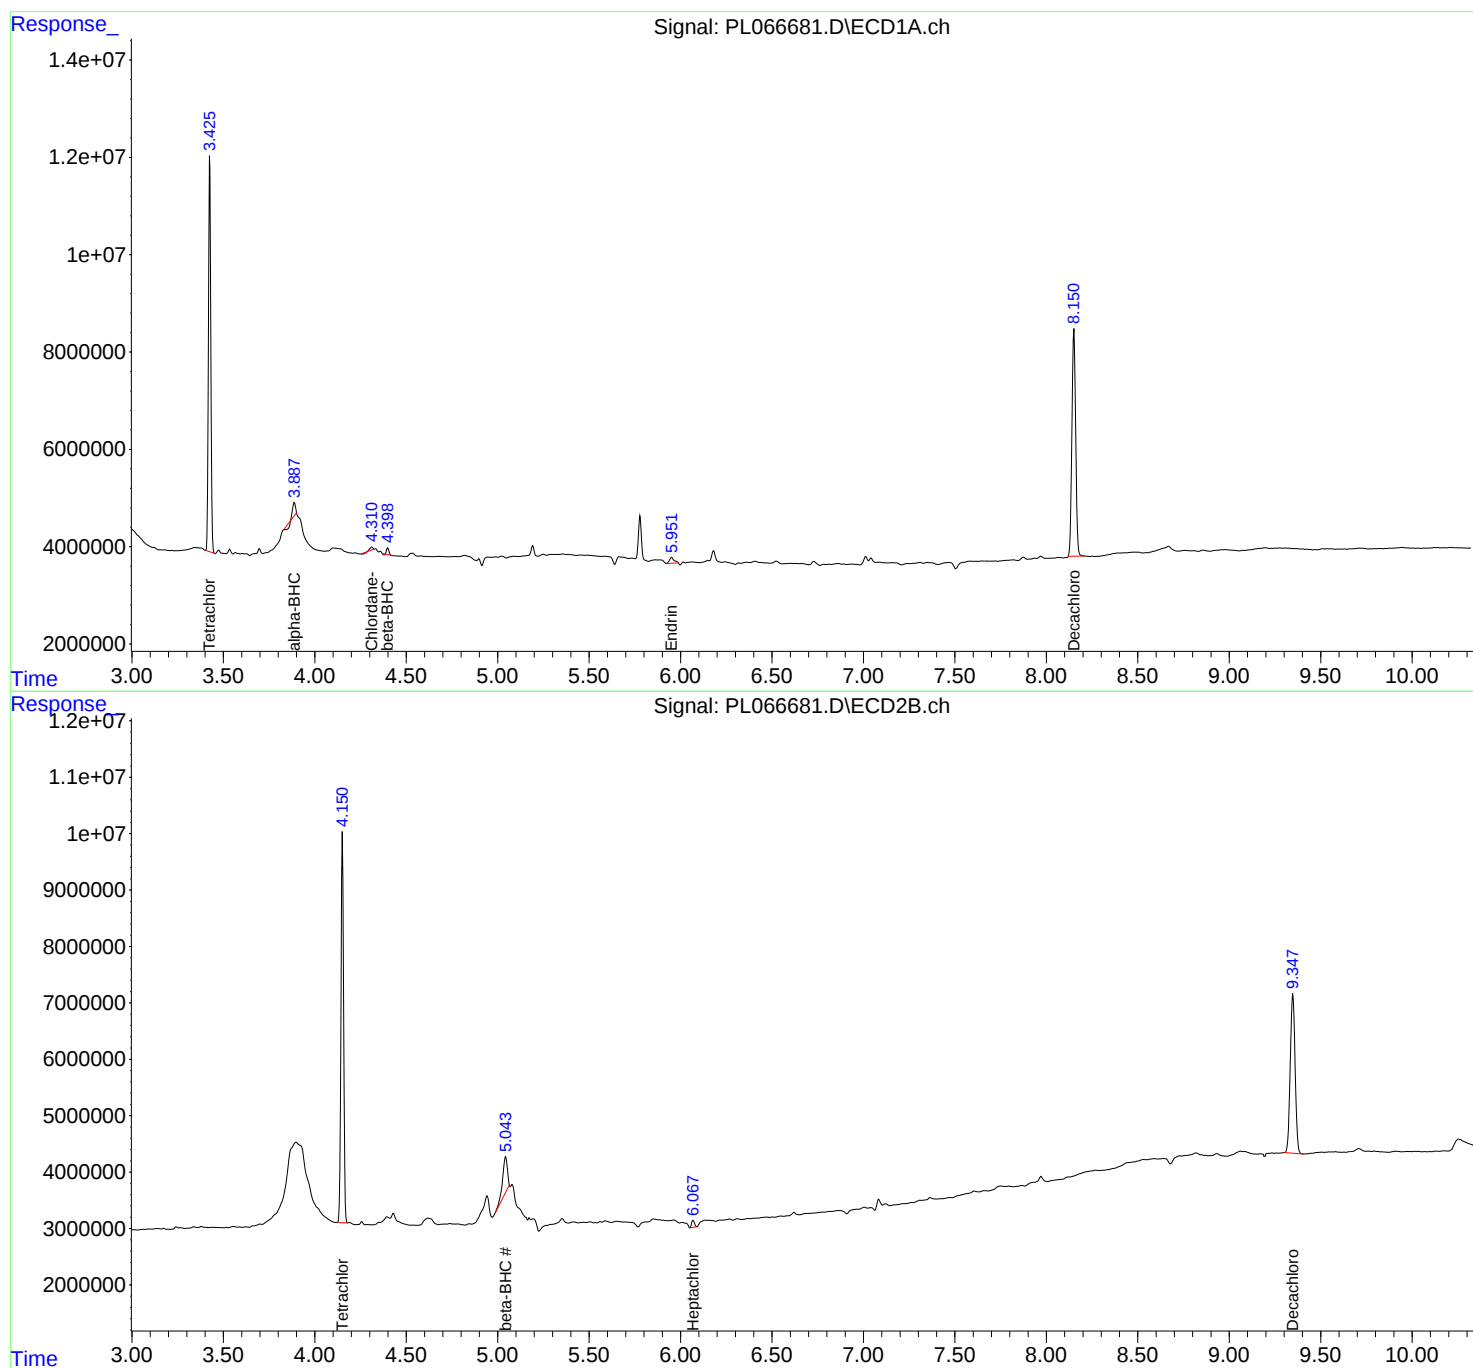


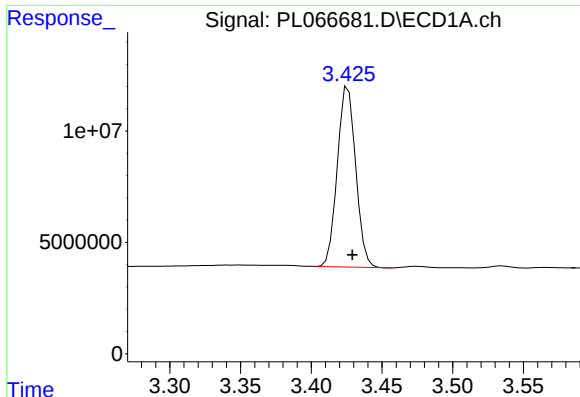

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: -0.003 min
Response: 73333220
Conc: 19.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

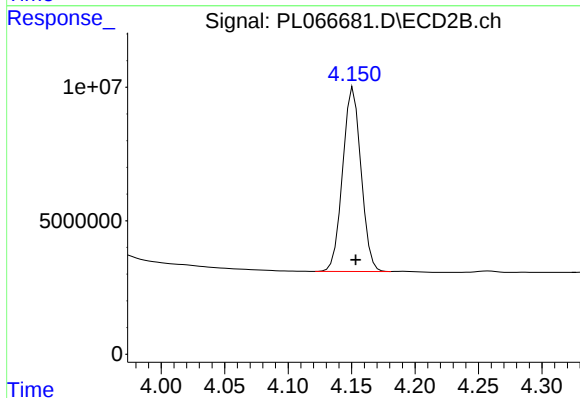


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: -0.002 min
Response: 69279177
Conc: 19.73 ng/ml

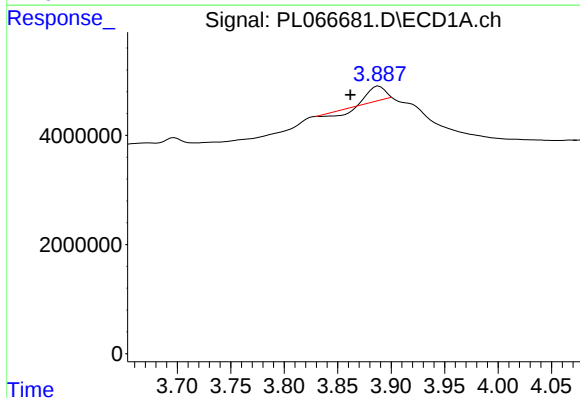


#2 alpha-BHC

R.T.: 3.888 min
Delta R.T.: 0.027 min
Response: 1999055
Conc: 0.32 ng/ml

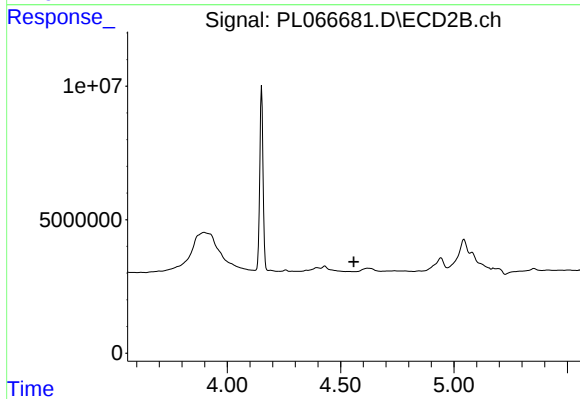

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.557 min
Response: 0
Conc: N.D.

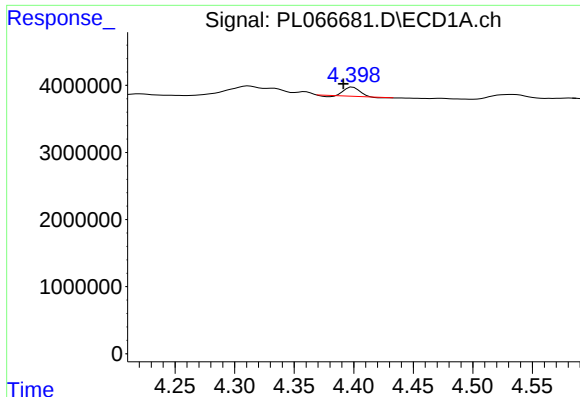

#6 beta-BHC


R.T.: 4.399 min
Delta R.T.: 0.008 min
Response: 1156576
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

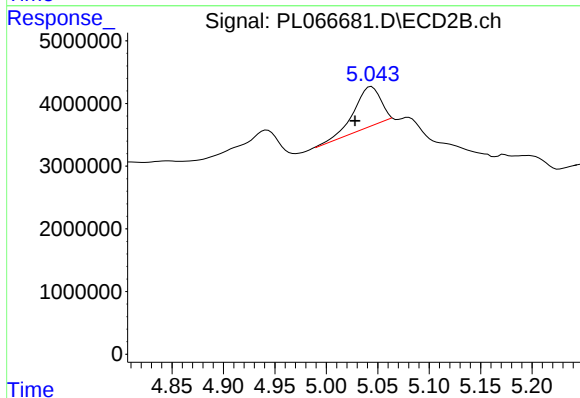


#6 beta-BHC

R.T.: 5.044 min
Delta R.T.: 0.016 min
Response: 12028240
Conc: 2.22 ng/ml

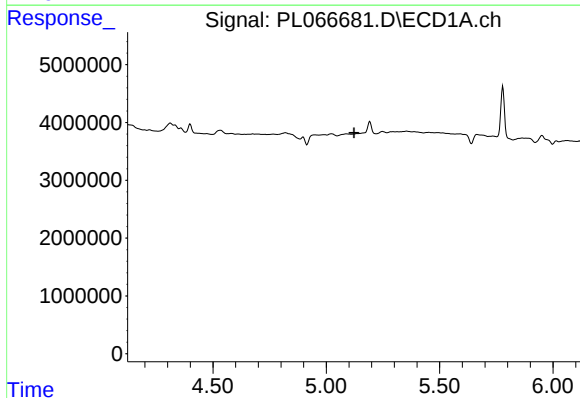


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

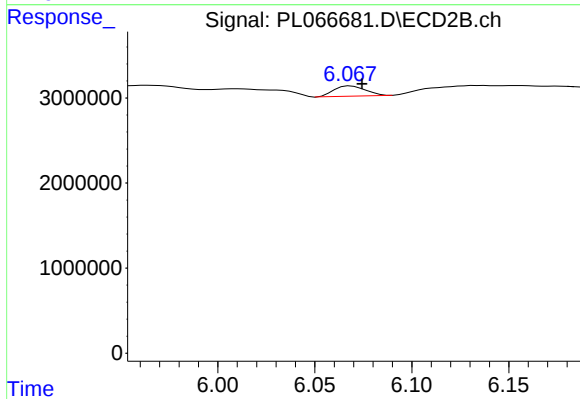

#8 Heptachlor epoxide


R.T.: 6.069 min
Delta R.T.: -0.006 min
Response: 1340831
Conc: 0.36 ng/ml

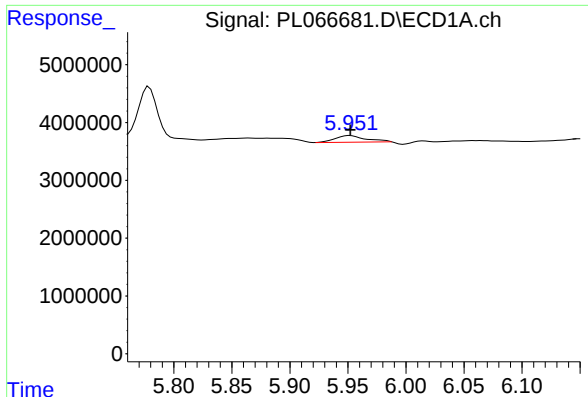

#14 Endrin


R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 2106190
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

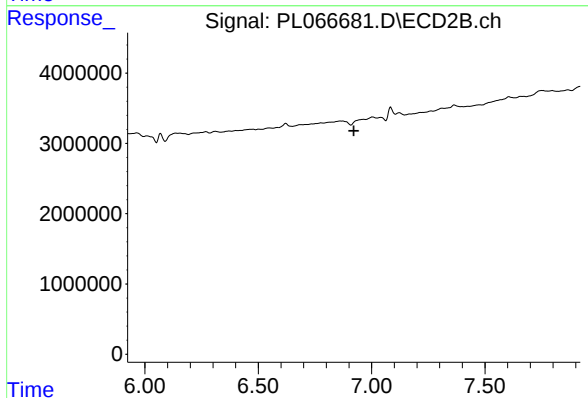


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

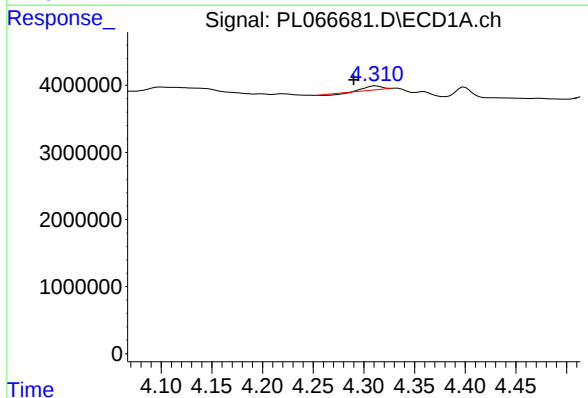


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.022 min
Response: 422811
Conc: 2.50 ng/ml

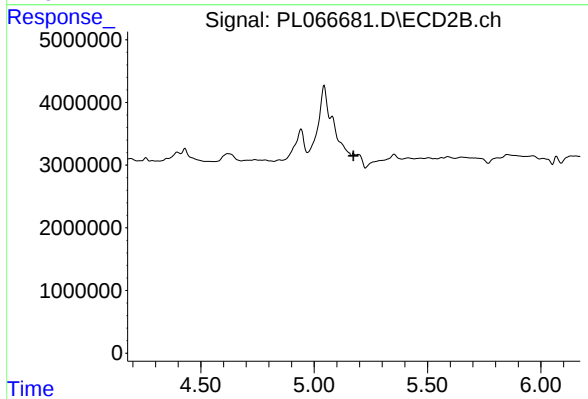

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

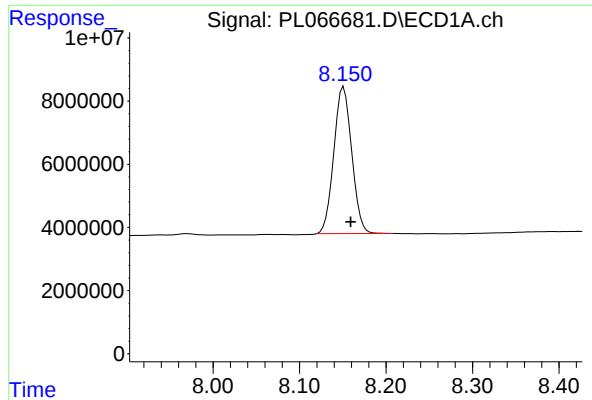

#28 Decachlorobiphenyl

R.T.: 8.151 min
Delta R.T.: -0.008 min
Response: 66737083
Conc: 17.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

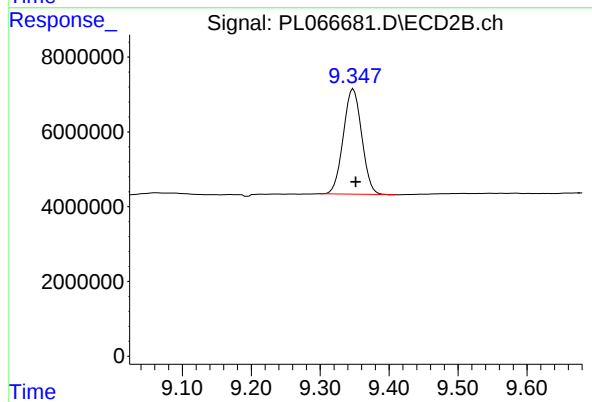

#28 Decachlorobiphenyl

R.T.: 9.348 min
Delta R.T.: -0.004 min
Response: 52273598
Conc: 16.90 ng/ml