

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050422\
 Data File : PL074509.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2022 13:09
 Operator : AR\AJ
 Sample : PB144563BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 23:24:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.484	7242782	38298866	22.416	21.480
28)	SA Decachlor...	10.411	11.334	12163729	41661780	23.390	23.587
Target Compounds							
5)	MB Aldrin	0.000	7.489f	0	145409	N.D.	0.062 #
7)	B delta-BHC	0.000	6.955	0	889289	N.D.	0.364 #
11)	B alpha-Chl...	0.000	8.294f	0	46371	N.D.	0.022 #
14)	MA Endrin	8.088f	0.000	402642	0	0.991	N.D. #
17)	MA 4,4'-DDT	0.000	9.309	0	40839	N.D.	0.023 #
18)	B Endrin al...	0.000	9.180f	0	3795	N.D.	0.003 #
20)	A Methoxychlor	0.000	9.801	0	132579	N.D.	0.138 #
22)	Mirex	9.531f	0.000	23694	0	0.051	N.D. #
24)	Chlordane-2	0.000	7.422f	0	97120	N.D.	1.175 #
26)	Chlordane-4	0.000	8.294	0	46371	N.D.	0.117 #
27)	Chlordane-5	0.000	9.180f	0	3795	N.D.	0.063 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050422\
Data File : PL074509.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2022 13:09
Operator : AR\AJ
Sample : PB144563BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 23:24:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

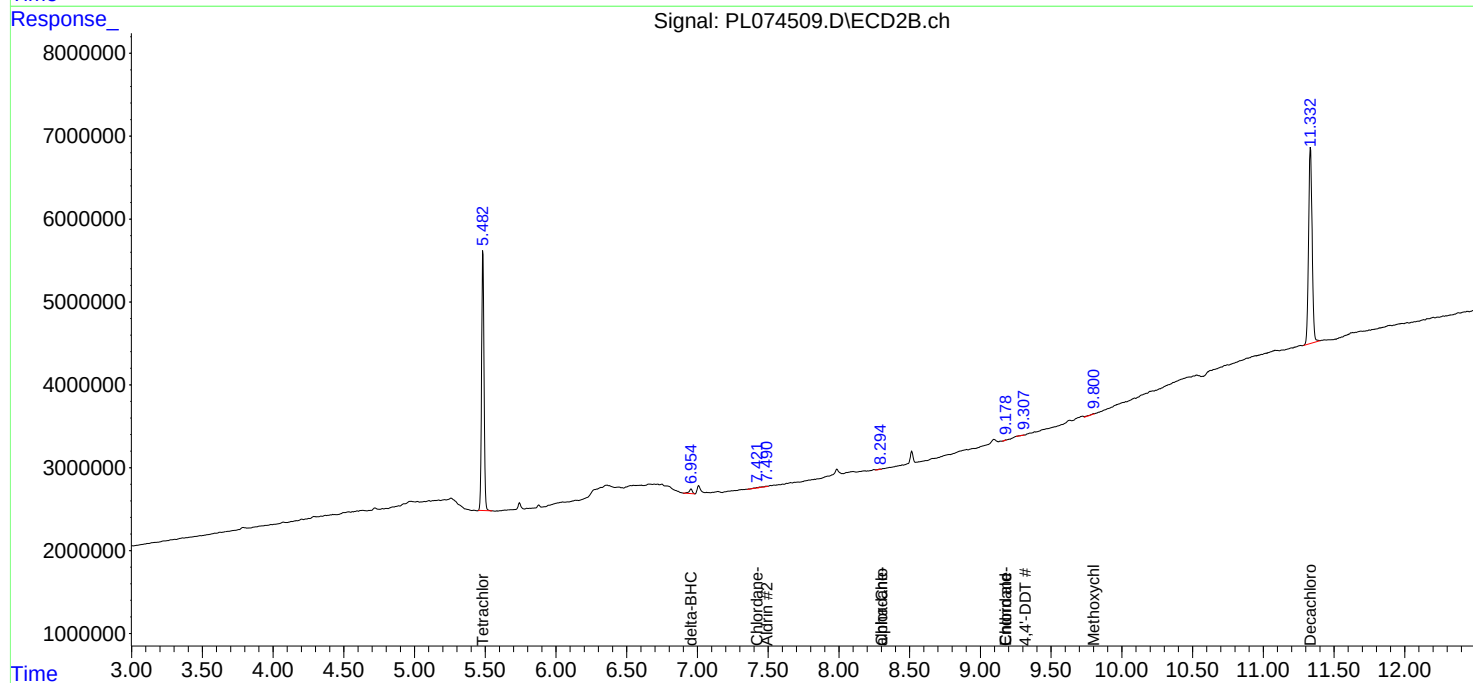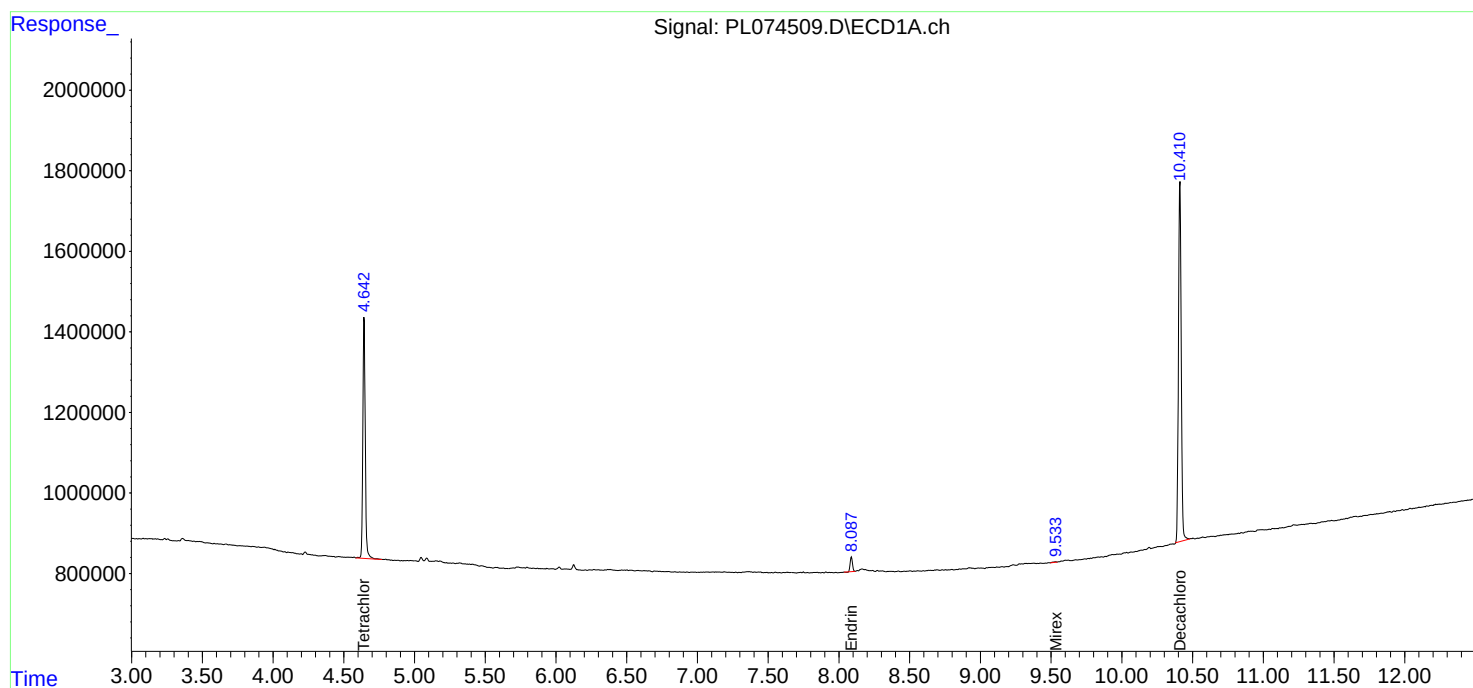


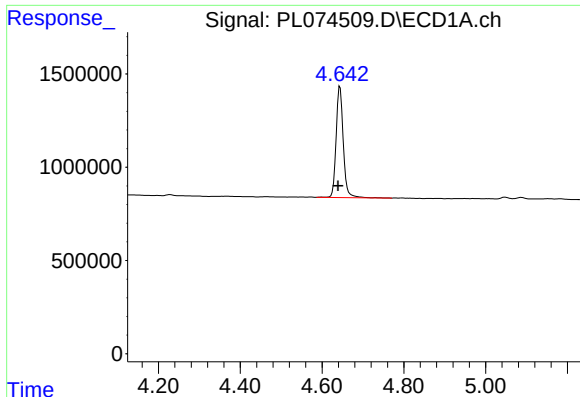

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: 0.005 min
Response: 7242782
Conc: 22.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

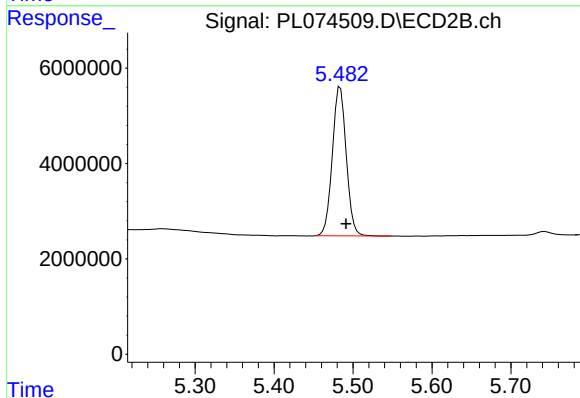


#1 Tetrachloro-m-xylene

R.T.: 5.484 min
Delta R.T.: -0.008 min
Response: 38298866
Conc: 21.48 ng/ml

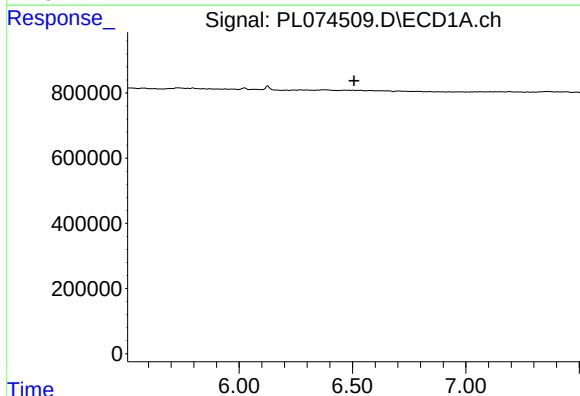


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

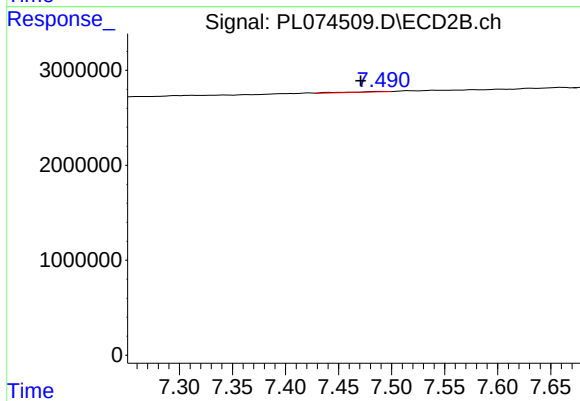

#5 Aldrin


R.T.: 7.489 min
Delta R.T.: 0.019 min
Response: 145409
Conc: 0.06 ng/ml

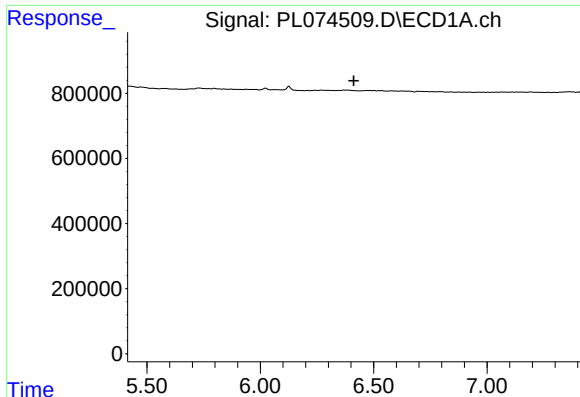

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

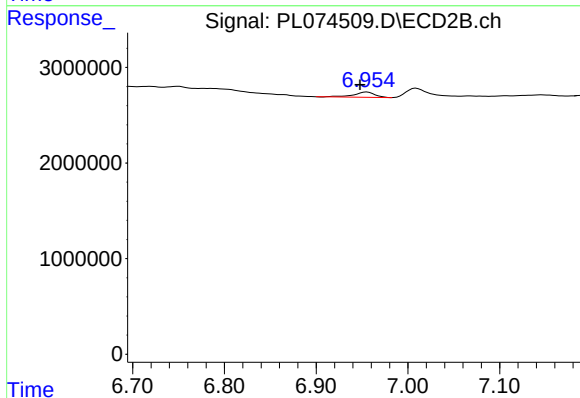


#7 delta-BHC

R.T.: 6.955 min
Delta R.T.: 0.008 min
Response: 889289
Conc: 0.36 ng/ml

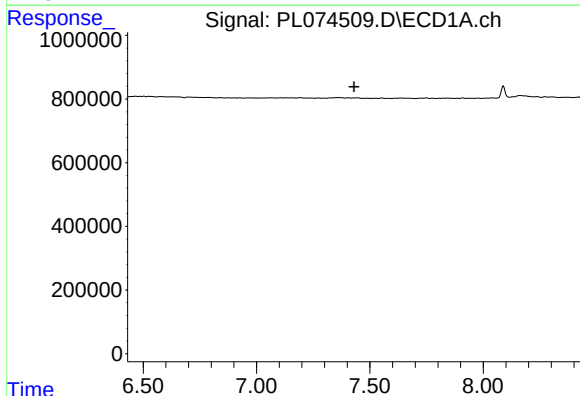


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.431 min
Response: 0
Conc: N.D.

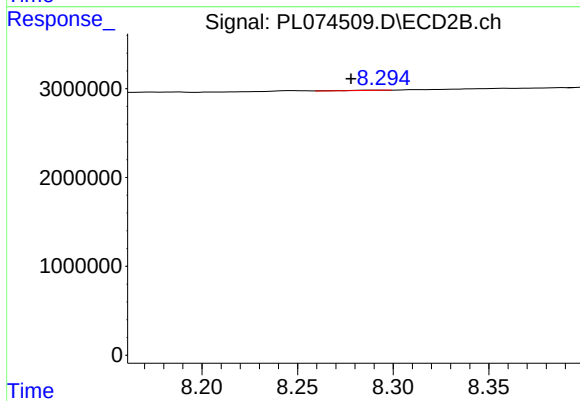

#11 alpha-Chlordane


R.T.: 8.294 min
Delta R.T.: 0.016 min
Response: 46371
Conc: 0.02 ng/ml

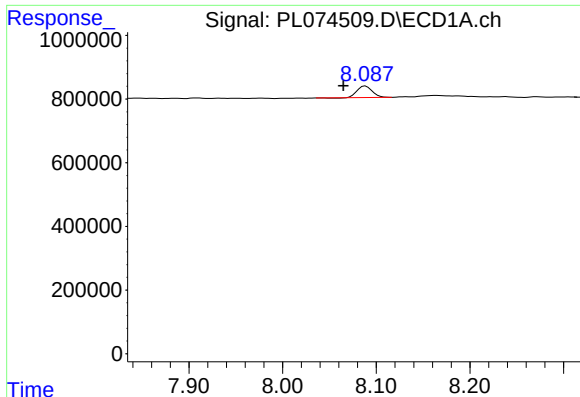

#14 Endrin


R.T.: 8.088 min
Delta R.T.: 0.024 min
Response: 402642
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

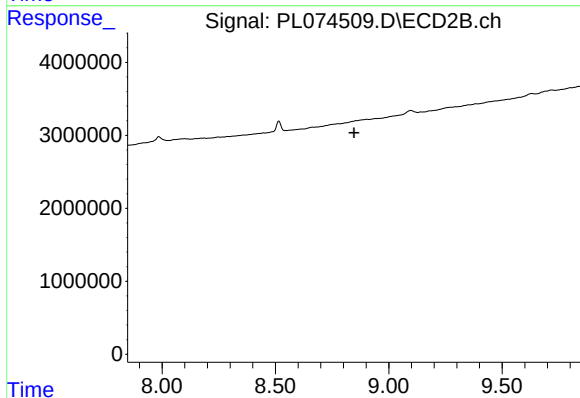


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.847 min
Response: 0
Conc: N.D.

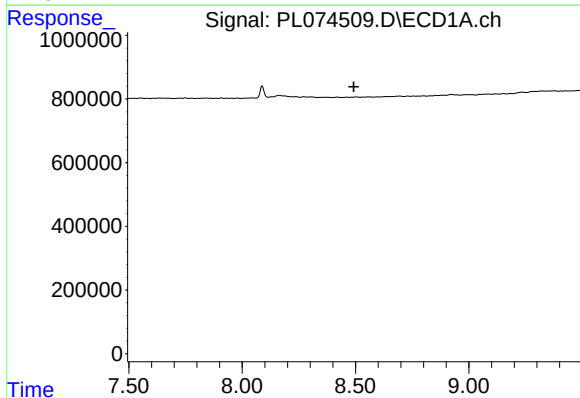


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.492 min
Response: 0
Conc: N.D.

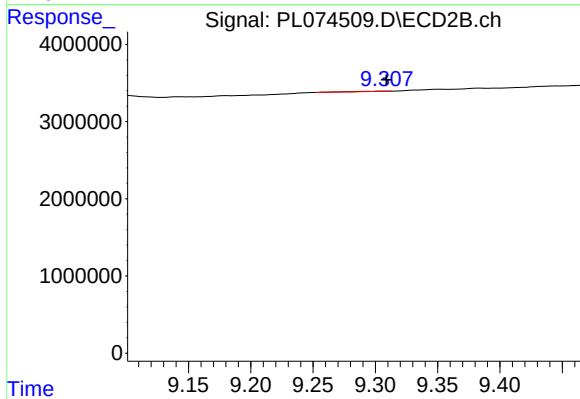

#17 4,4'-DDT


R.T.: 9.309 min
Delta R.T.: 0.000 min
Response: 40839
Conc: 0.02 ng/ml

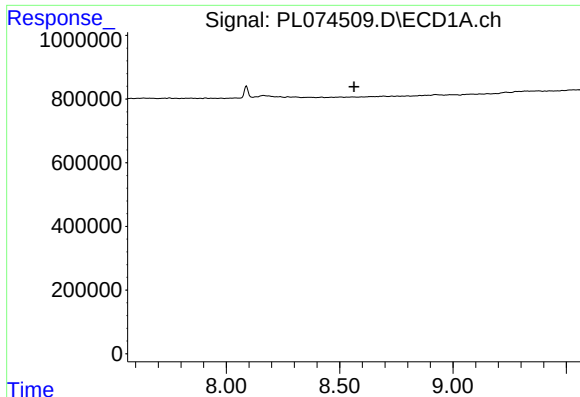

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

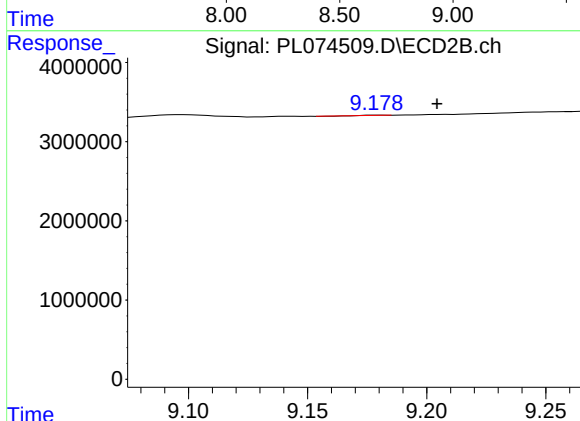


#18 Endrin aldehyde

R.T.: 9.180 min
Delta R.T.: -0.024 min
Response: 3795
Conc: 0.00 ng/ml

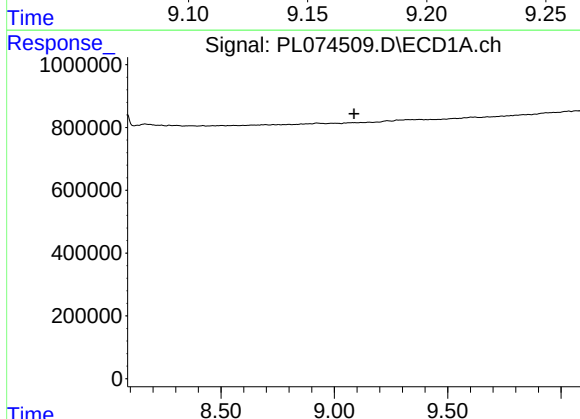


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.087 min
Response: 0
Conc: N.D.

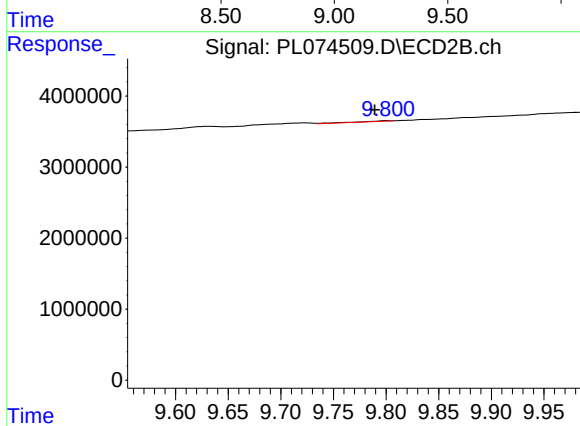

#20 Methoxychlor


R.T.: 9.801 min
Delta R.T.: 0.012 min
Response: 132579
Conc: 0.14 ng/ml

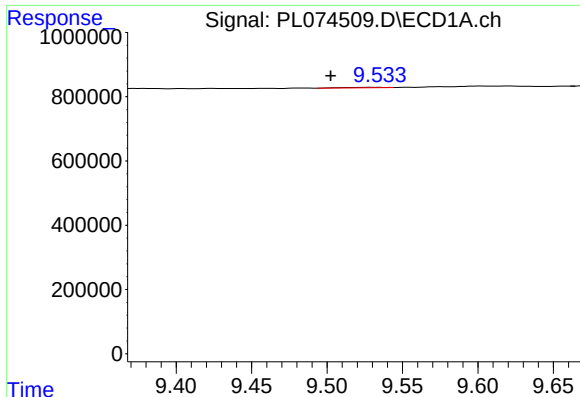

#22 Mirex


R.T.: 9.531 min
Delta R.T.: 0.029 min
Response: 23694
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

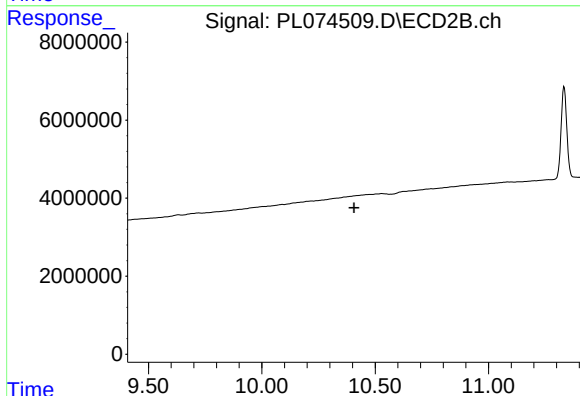


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.407 min
Response: 0
Conc: N.D.

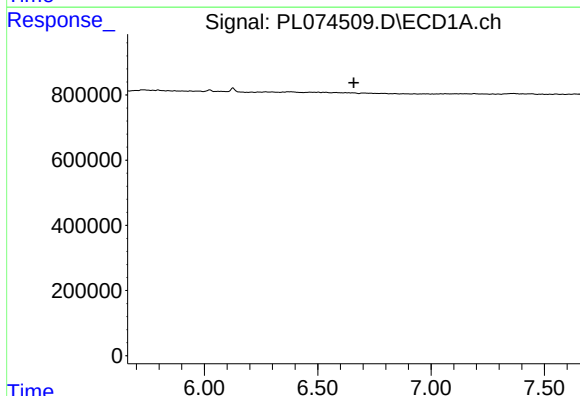


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.659 min
Response: 0
Conc: N.D.

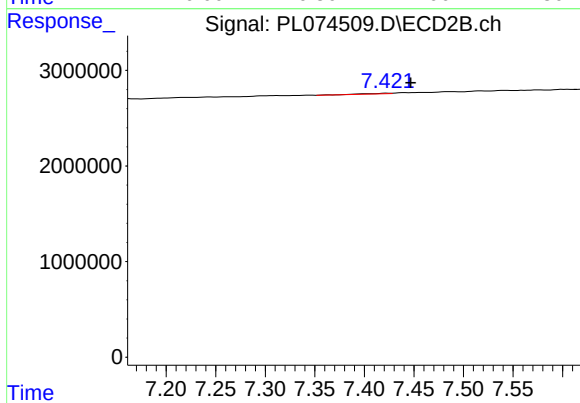

#24 Chlordane-2


R.T.: 7.422 min
Delta R.T.: -0.025 min
Response: 97120
Conc: 1.18 ng/ml

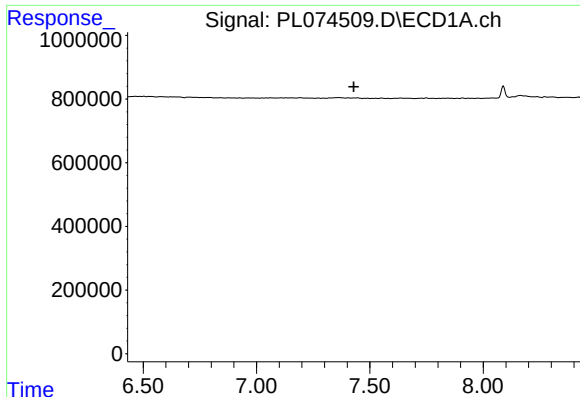

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

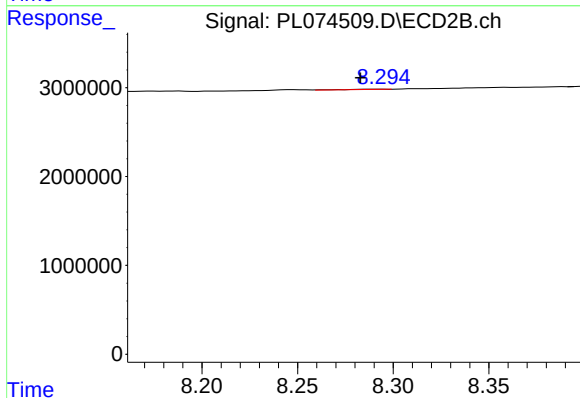


#26 Chlordane-4

R.T.: 8.294 min
Delta R.T.: 0.011 min
Response: 46371
Conc: 0.12 ng/ml

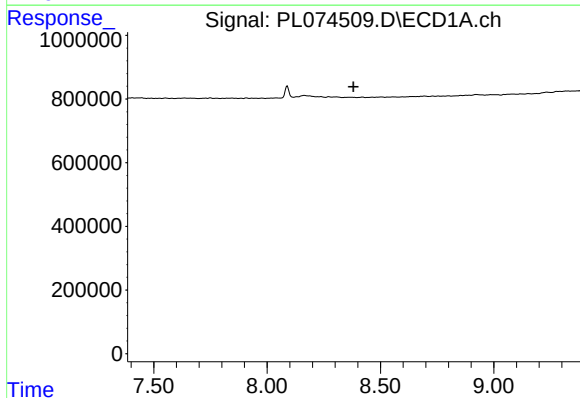


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.381 min
Response: 0
Conc: N.D.

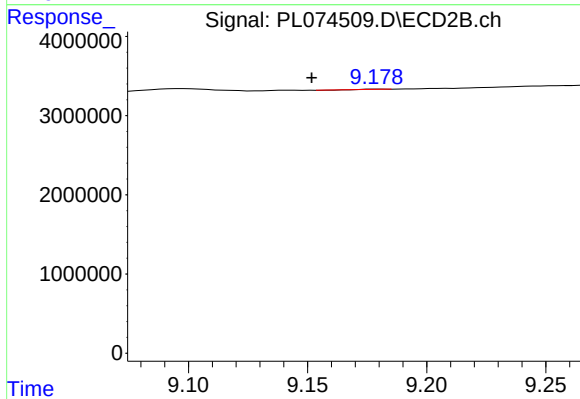

#27 Chlordane-5


R.T.: 9.180 min
Delta R.T.: 0.028 min
Response: 3795
Conc: 0.06 ng/ml

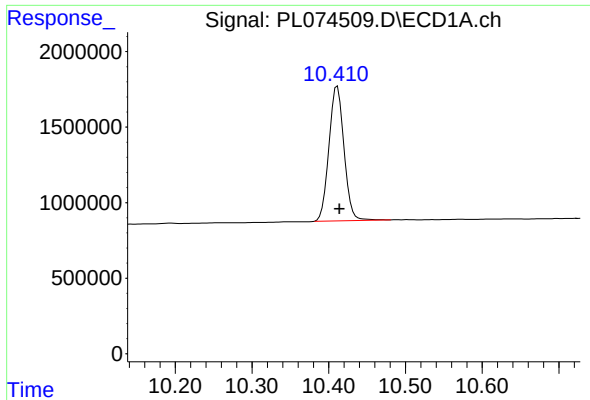

#28 Decachlorobiphenyl

R.T.: 10.411 min
Delta R.T.: -0.003 min
Response: 12163729
Conc: 23.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

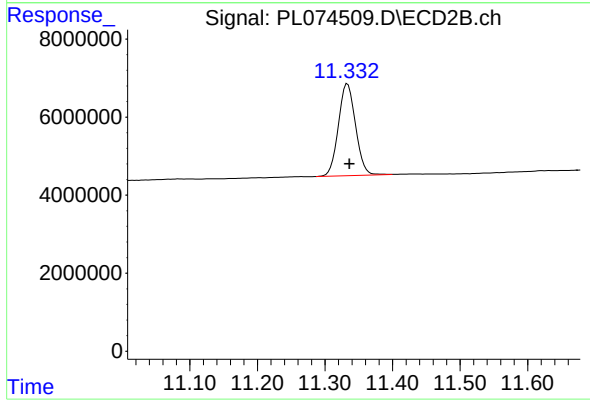

#28 Decachlorobiphenyl

R.T.: 11.334 min
Delta R.T.: -0.003 min
Response: 41661780
Conc: 23.59 ng/ml