

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050422\
 Data File : PL074522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2022 17:42
 Operator : AR\AJ
 Sample : N2665-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 23:28:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.489	7586300	41346348	23.479	23.190
28)	SA Decachlor...	10.403	11.333	10912367	40262969	20.984	22.795
Target Compounds							
6)	B beta-BHC	0.000	6.676	0	689354	N.D.	0.612 #
7)	B delta-BHC	0.000	6.954	0	2208634	N.D.	0.904 #
10)	B gamma-Chl...	0.000	8.196	0	320137	N.D.	0.144 #
13)	MA Dieldrin	0.000	8.606	0	68877	N.D.	0.034 #
14)	MA Endrin	8.079	8.850	65355	147444	0.161	0.087 #
16)	A 4,4'-DDD	0.000	9.000	0	206527	N.D.	0.134 #
17)	MA 4,4'-DDT	0.000	9.321	0	203713	N.D.	0.115 #
20)	A Methoxychlor	0.000	9.789	0	100087	N.D.	0.104 #
21)	B Endrin ke...	0.000	9.960f	0	178043	N.D.	0.103 #
23)	Chlordane-1	0.000	6.855	0	1312521	N.D.	16.447 #
25)	Chlordane-3	0.000	8.196	0	320137	N.D.	0.946 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050422\
Data File : PL074522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2022 17:42
Operator : AR\AJ
Sample : N2665-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 23:28:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

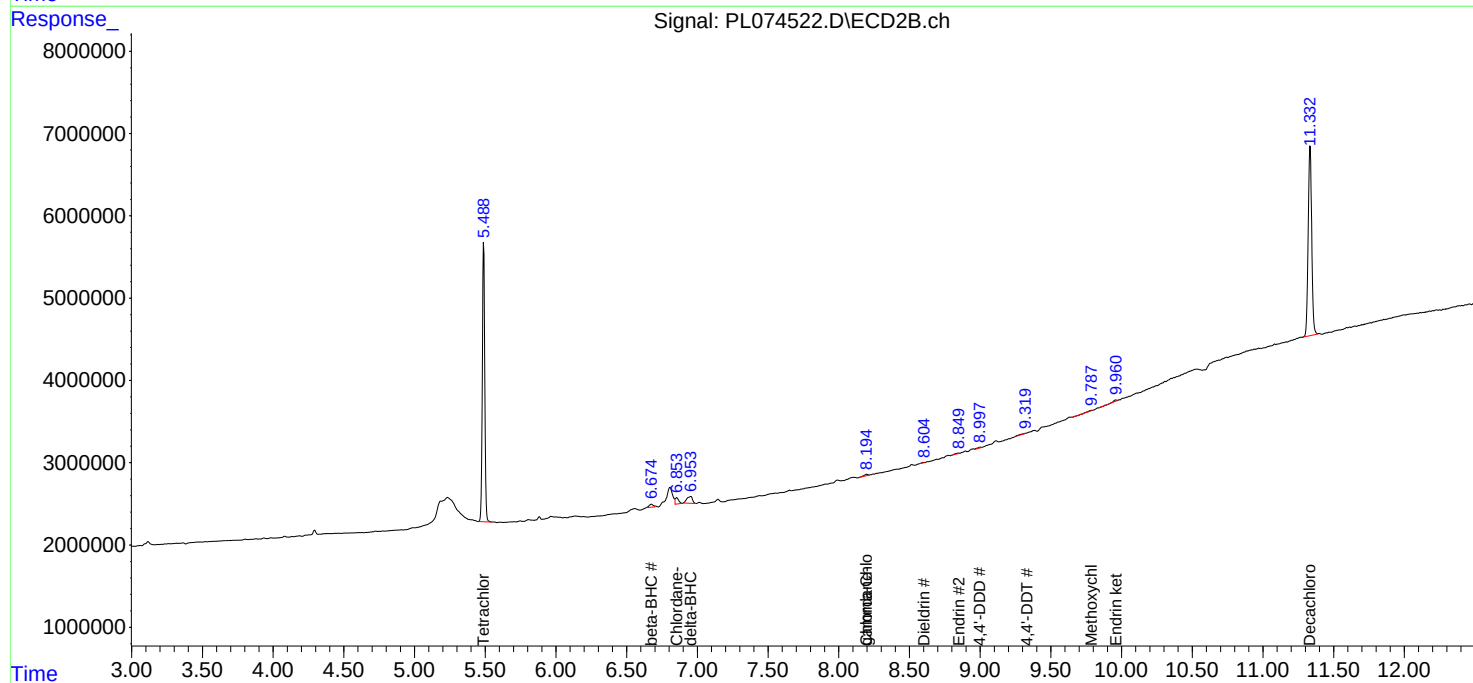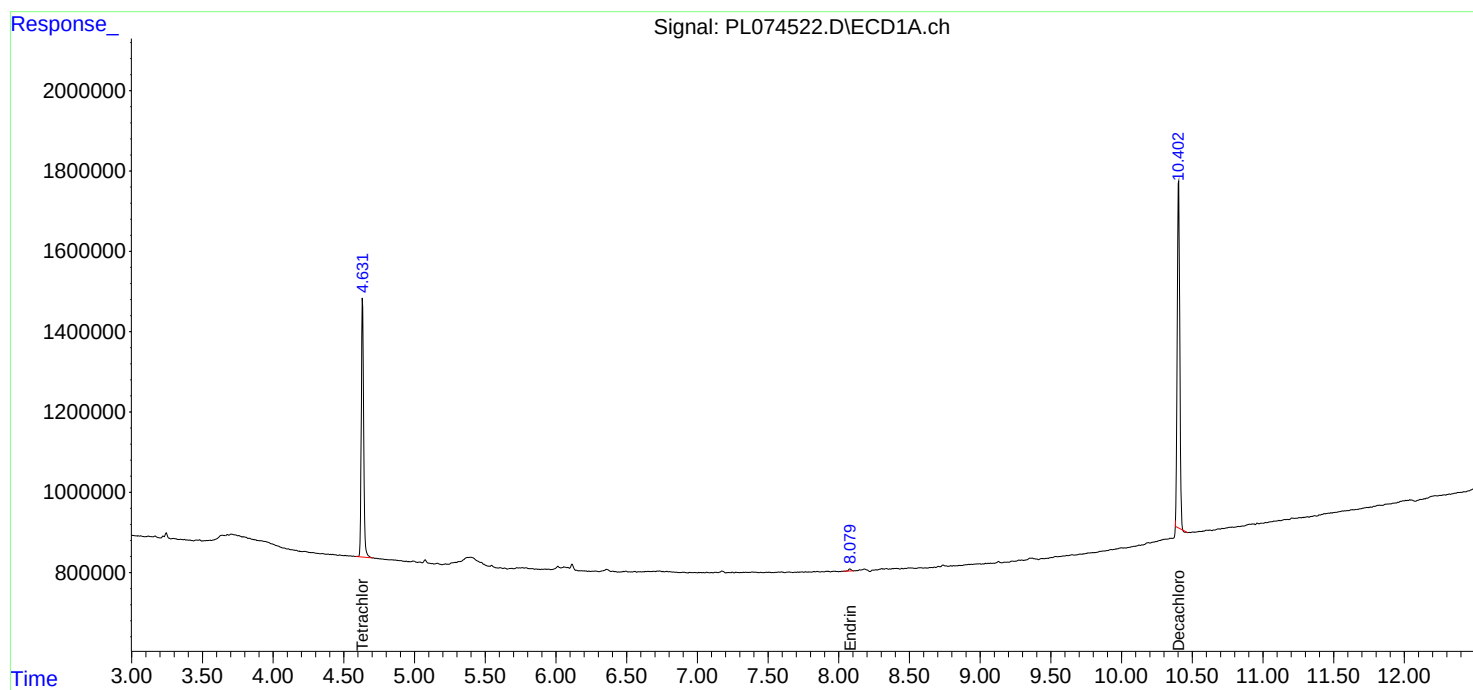


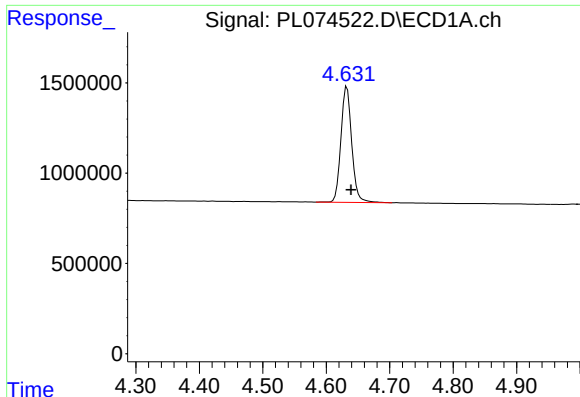

#1 Tetrachloro-m-xylene


R.T.: 4.633 min
Delta R.T.: -0.006 min
Response: 7586300
Conc: 23.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

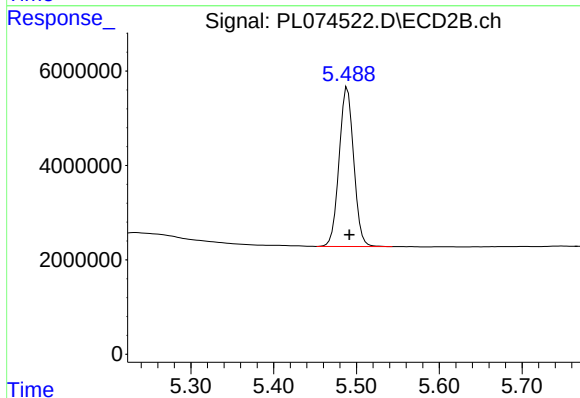


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 41346348
Conc: 23.19 ng/ml

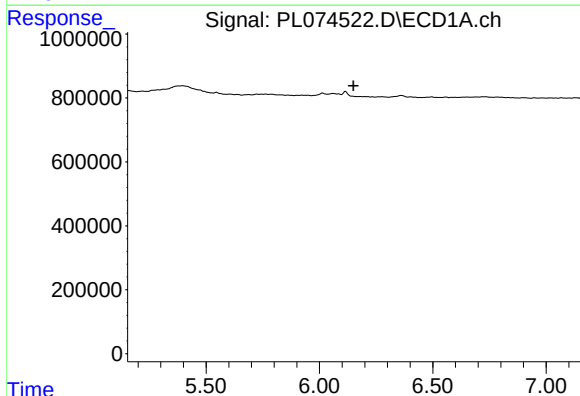


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.151 min
Response: 0
Conc: N.D.

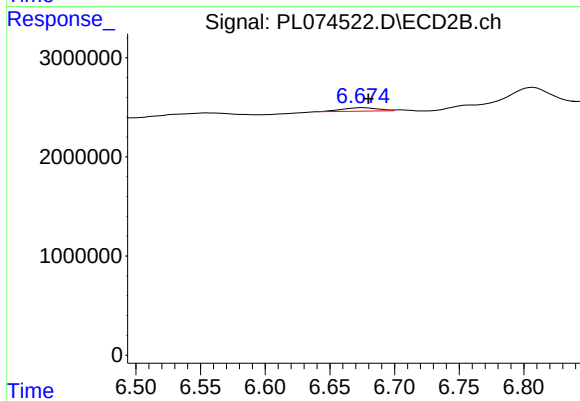

#6 beta-BHC


R.T.: 6.676 min
Delta R.T.: -0.004 min
Response: 689354
Conc: 0.61 ng/ml

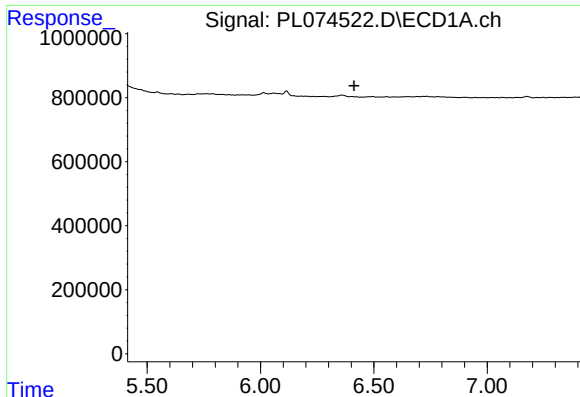

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

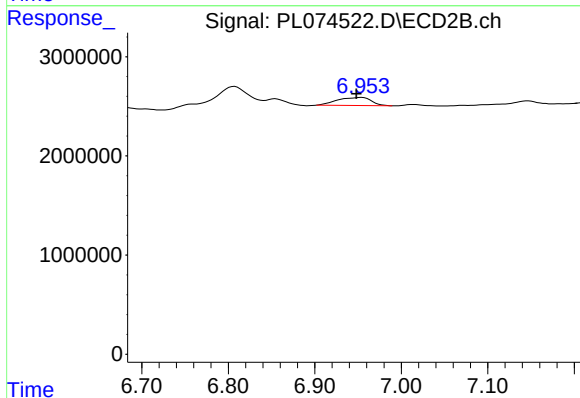


#7 delta-BHC

R.T.: 6.954 min
Delta R.T.: 0.006 min
Response: 2208634
Conc: 0.90 ng/ml

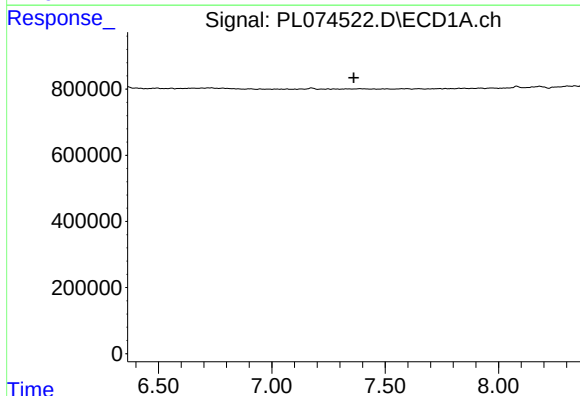


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

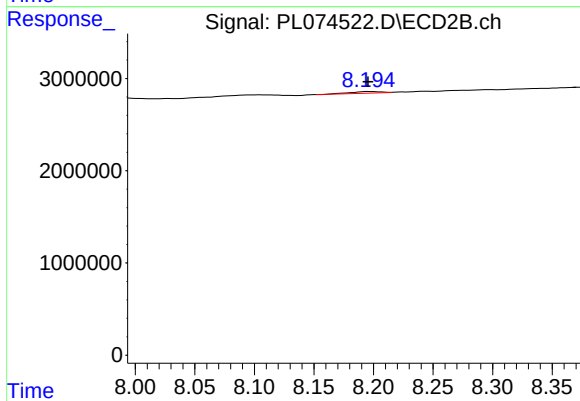

#10 gamma-Chlordane


R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 320137
Conc: 0.14 ng/ml

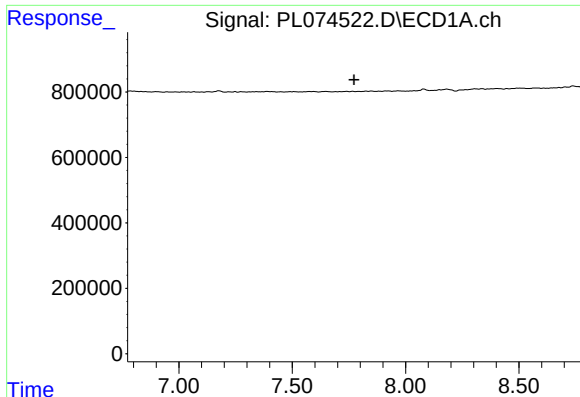

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

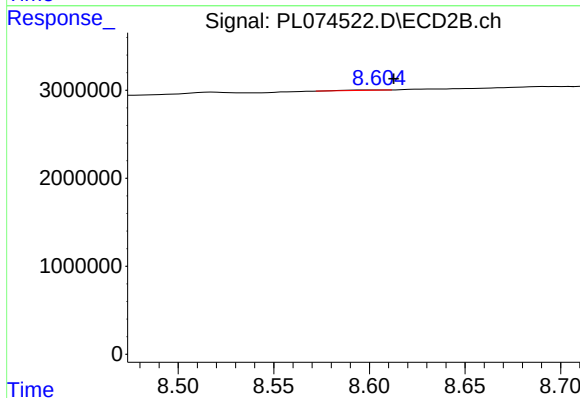


#13 Dieldrin

R.T.: 8.606 min
Delta R.T.: -0.007 min
Response: 68877
Conc: 0.03 ng/ml

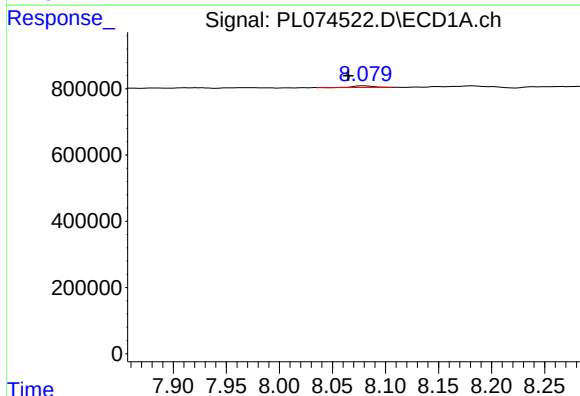


#14 Endrin

R.T.: 8.079 min
Delta R.T.: 0.015 min
Response: 65355
Conc: 0.16 ng/ml

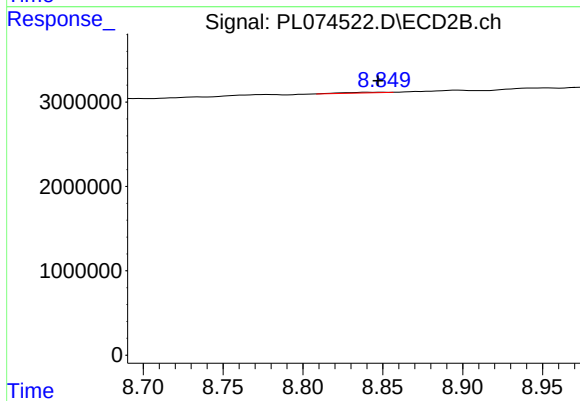

#14 Endrin


R.T.: 8.850 min
Delta R.T.: 0.003 min
Response: 147444
Conc: 0.09 ng/ml

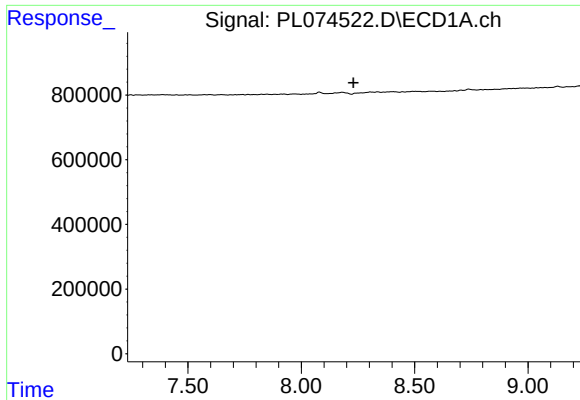

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

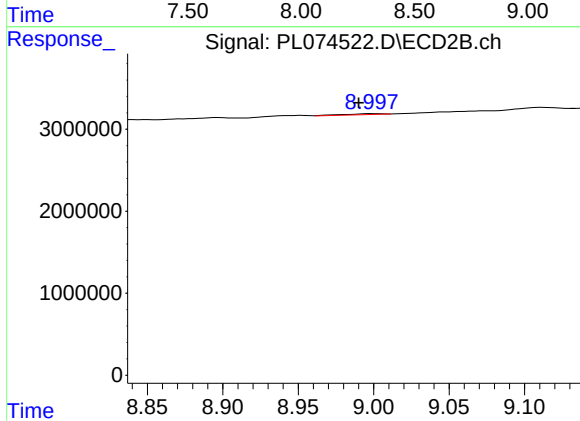


#16 4,4'-DDD

R.T.: 9.000 min
Delta R.T.: 0.010 min
Response: 206527
Conc: 0.13 ng/ml

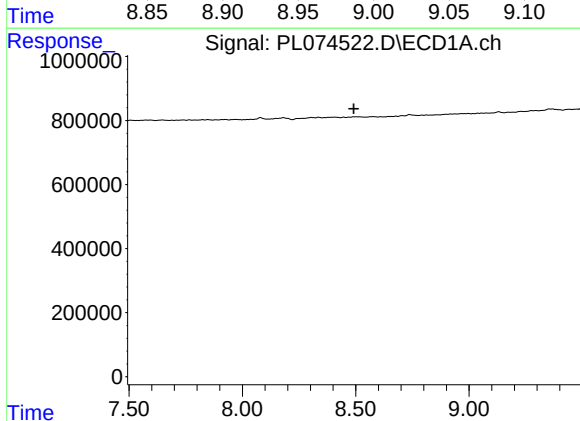


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

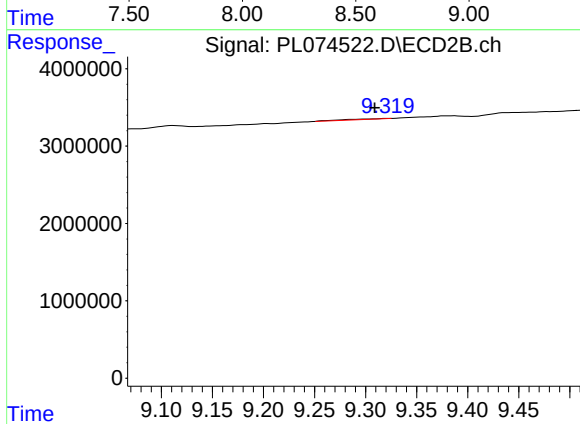

#17 4,4'-DDT


R.T.: 9.321 min
Delta R.T.: 0.012 min
Response: 203713
Conc: 0.11 ng/ml

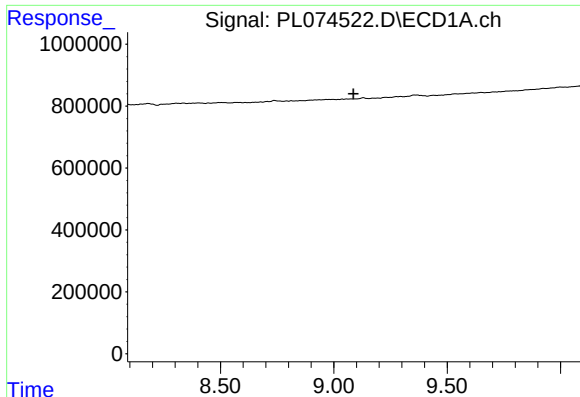

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

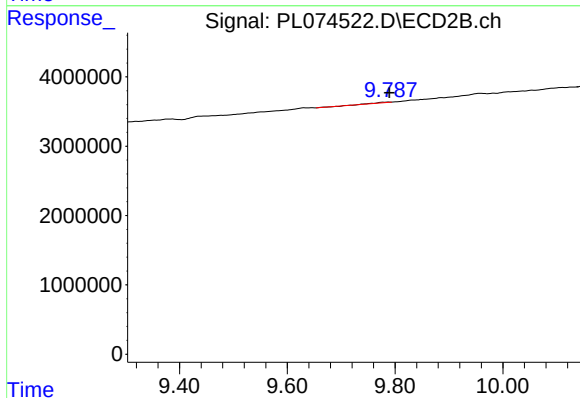


#20 Methoxychlor

R.T.: 9.789 min
Delta R.T.: 0.000 min
Response: 100087
Conc: 0.10 ng/ml

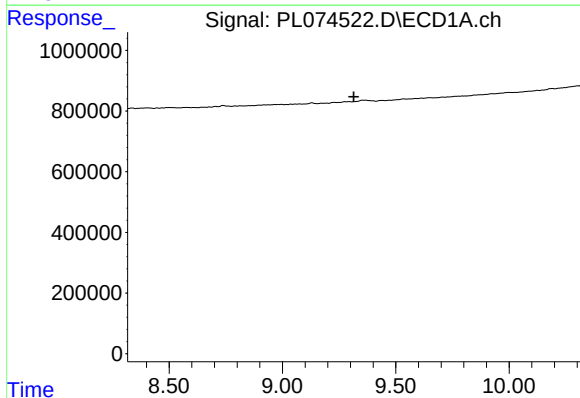


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.314 min
Response: 0
Conc: N.D.

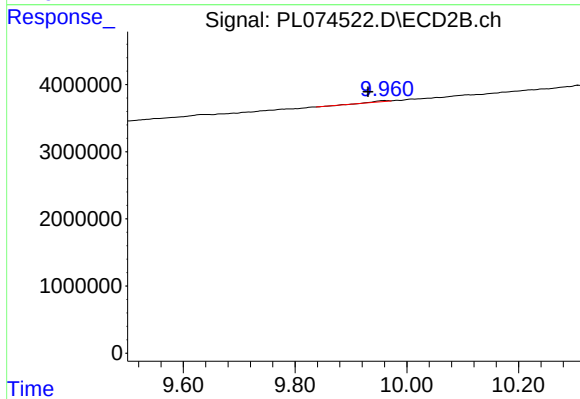

#21 Endrin ketone


R.T.: 9.960 min
Delta R.T.: 0.030 min
Response: 178043
Conc: 0.10 ng/ml

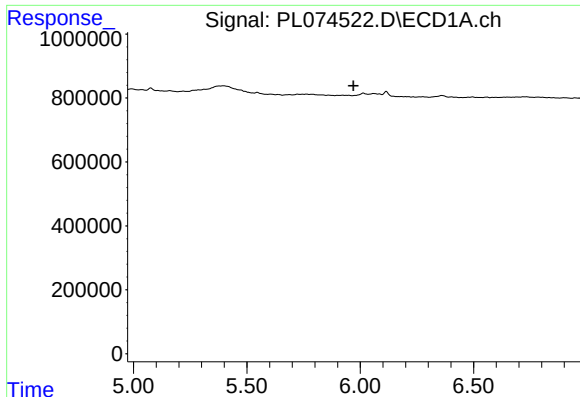

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

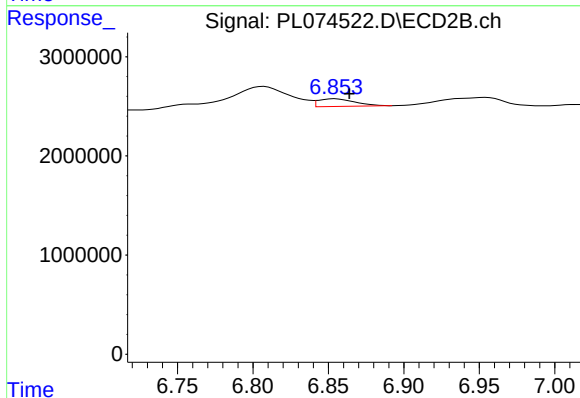


#23 Chlordane-1

R.T.: 6.855 min
Delta R.T.: -0.009 min
Response: 1312521
Conc: 16.45 ng/ml

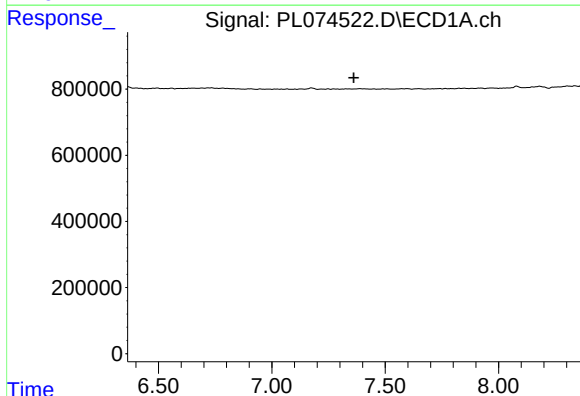


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

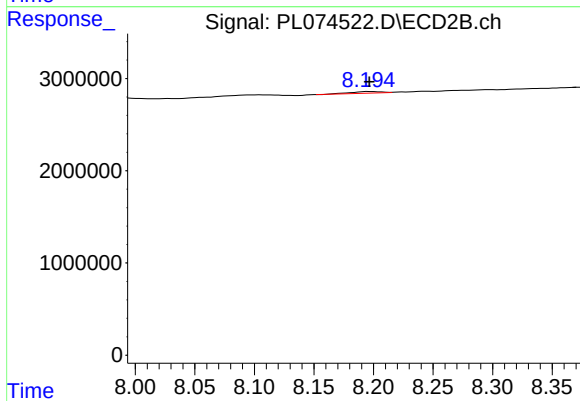

#25 Chlordane-3


R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 320137
Conc: 0.95 ng/ml

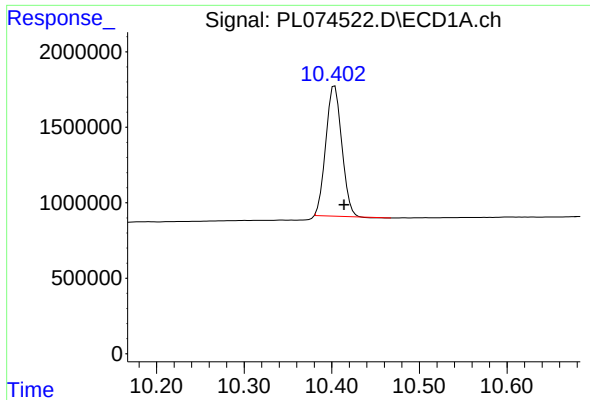

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.010 min
Response: 10912367
Conc: 20.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

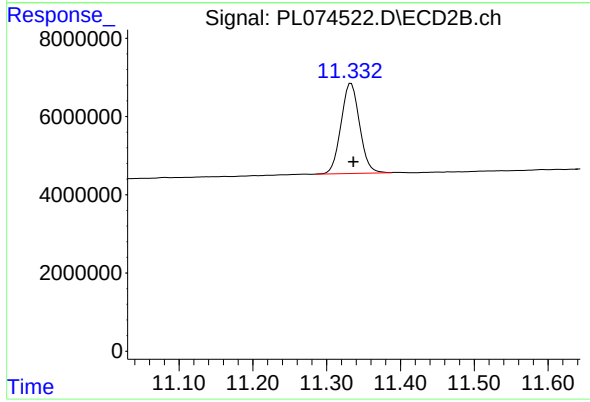

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: -0.003 min
Response: 40262969
Conc: 22.80 ng/ml