

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050423\
 Data File : PL082514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2023 17:03
 Operator : AR\AJ
 Sample : 02588-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ZONE-A-0-3-05022023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 21:20:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	2.643	26260954	22742489	9.831	9.817
28)	SA Decachlor...	8.739	7.753	18729939	21899043	9.811	9.594

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050423\
Data File : PL082514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2023 17:03
Operator : AR\AJ
Sample : 02588-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ZONE-A-0-3-05022023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 21:20:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

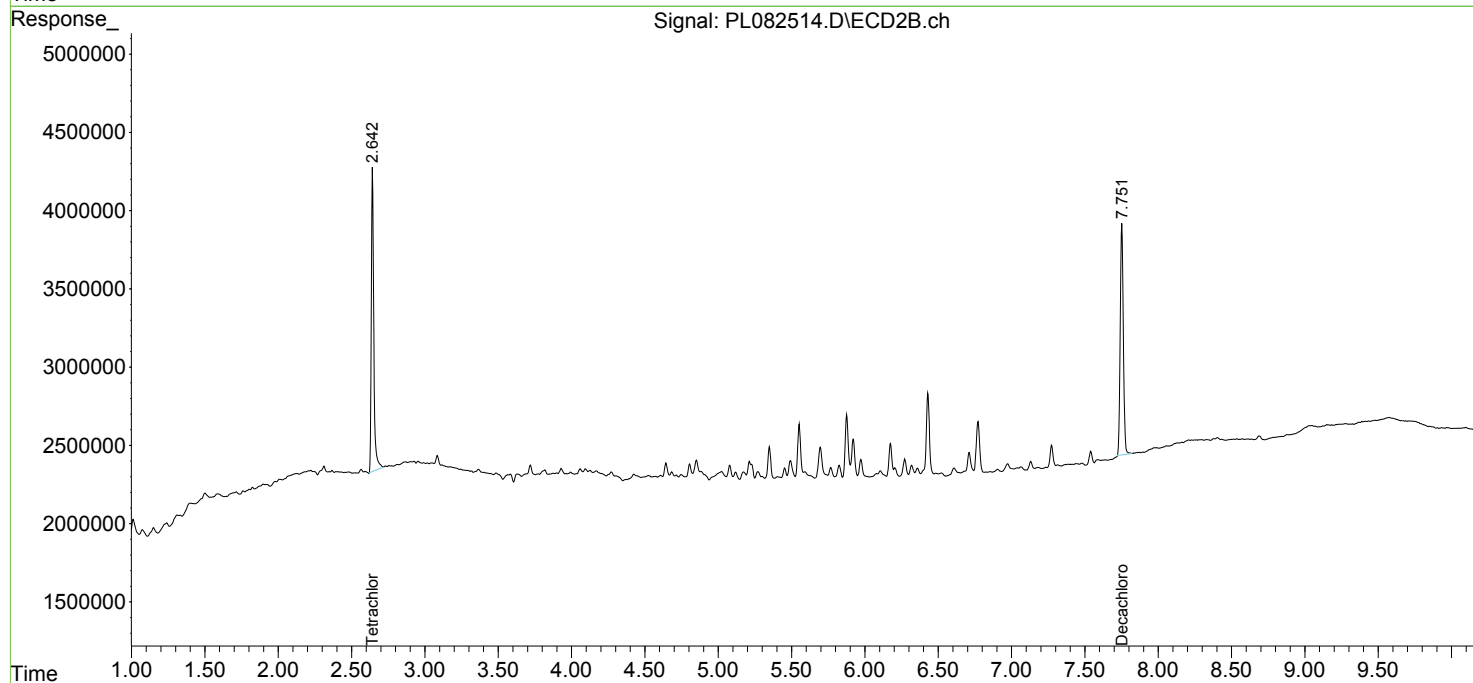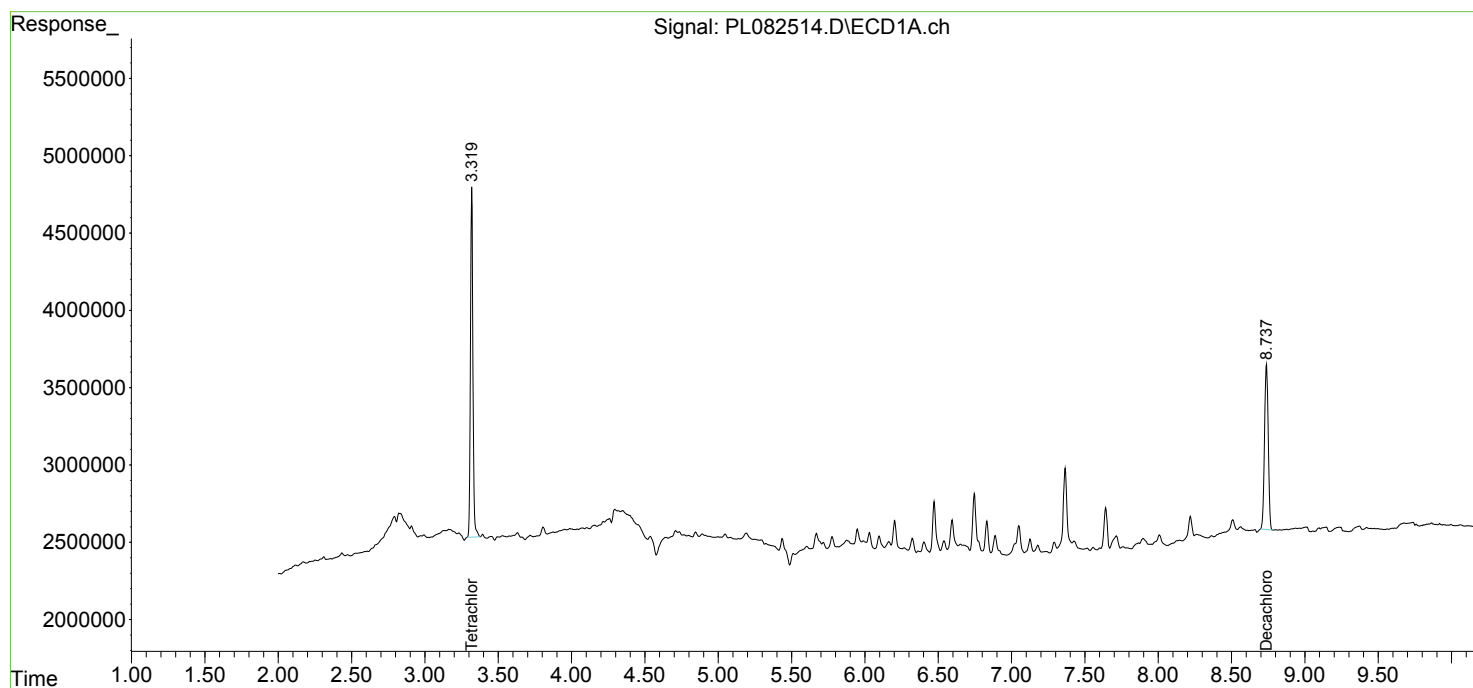


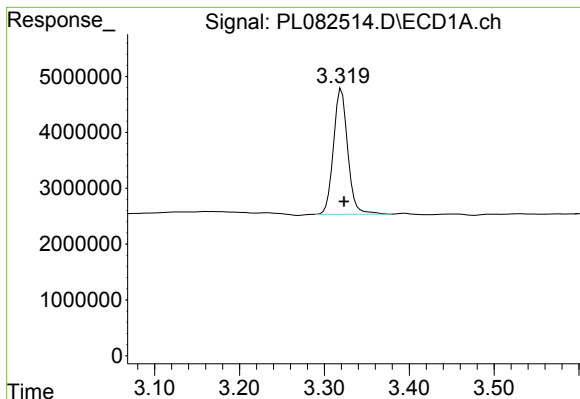

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.003 min
Response: 26260954
Conc: 9.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
ZONE-A-0-3-05022023

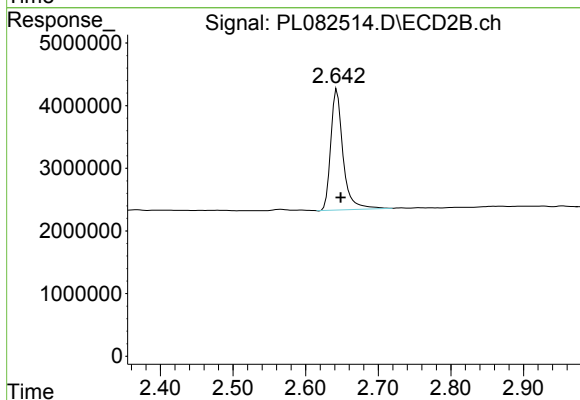


#1 Tetrachloro-m-xylene

R.T.: 2.643 min
Delta R.T.: -0.005 min
Response: 22742489
Conc: 9.82 ng/ml

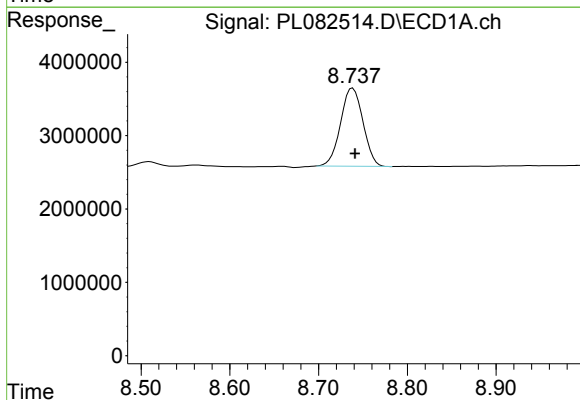

#28 Decachlorobiphenyl

R.T.: 8.739 min
Delta R.T.: -0.002 min
Response: 18729939
Conc: 9.81 ng/ml

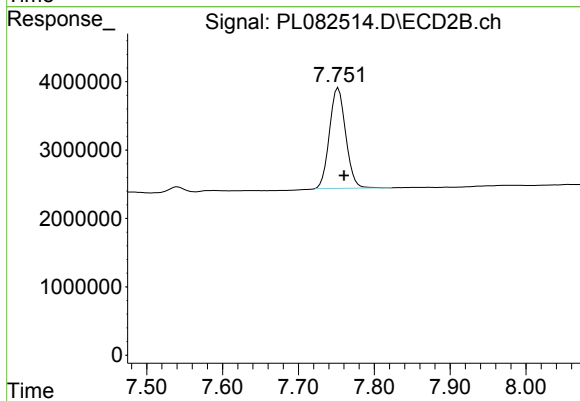

#28 Decachlorobiphenyl

R.T.: 7.753 min
Delta R.T.: -0.007 min
Response: 21899043
Conc: 9.59 ng/ml