

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050425\
 Data File : PL095505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2025 09:33
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 12:36:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.735	0.000	223.7E6	0	55.861	N.D. #
10) B	gamma-Chl...	5.981	0.000	28856065	0	7.074	N.D. #
13) MA	Dieldrin	0.000	5.555f	0	41683862	N.D.	10.249 #
14) MA	Endrin	0.000	5.813	0	13763066	N.D.	3.780 #
15) B	Endosulfa...	6.819f	6.099	58055643	6940452	18.187	1.933 #
16) A	4,4'-DDD	6.752	0.000	87390723	0	30.870	N.D. #
24)	Chlordane-2	0.000	4.503	0	34304770	N.D.	186.410 #
25)	Chlordane-3	5.981	0.000	28856065	0	37.046	N.D. #
27)	Chlordane-5	0.000	6.099	0	6940452	N.D.	37.569 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050425\
Data File : PL095505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2025 09:33
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 12:36:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

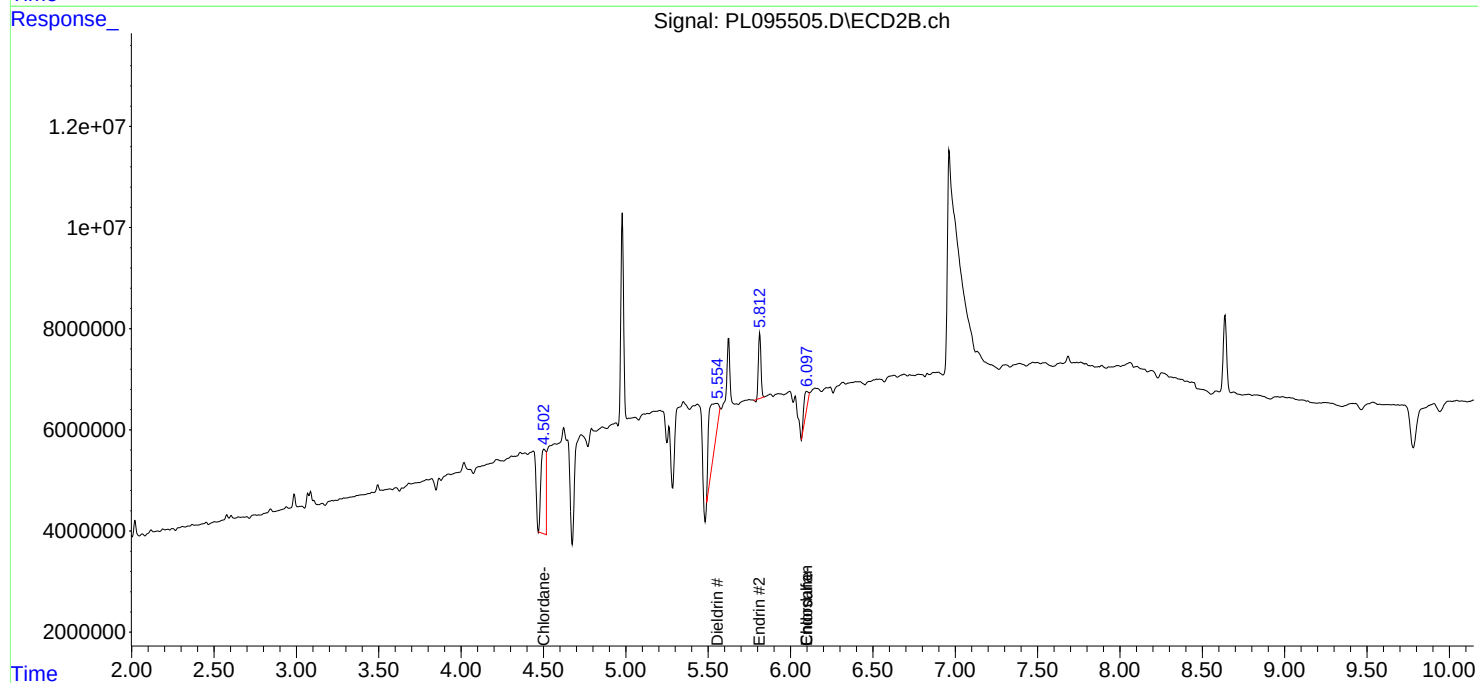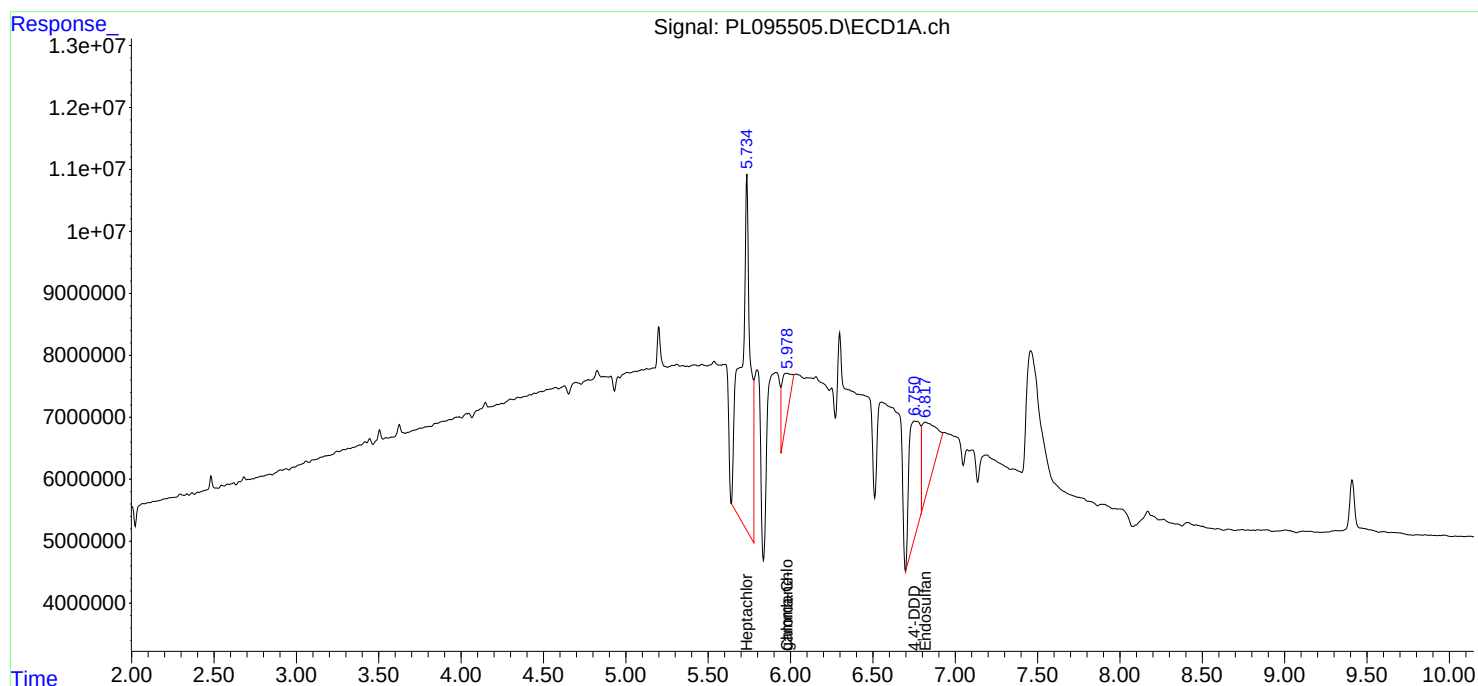


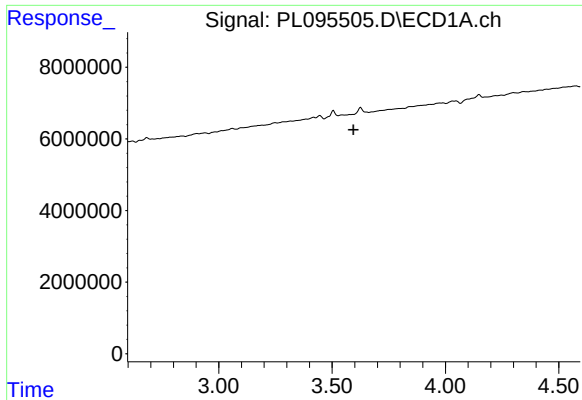

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

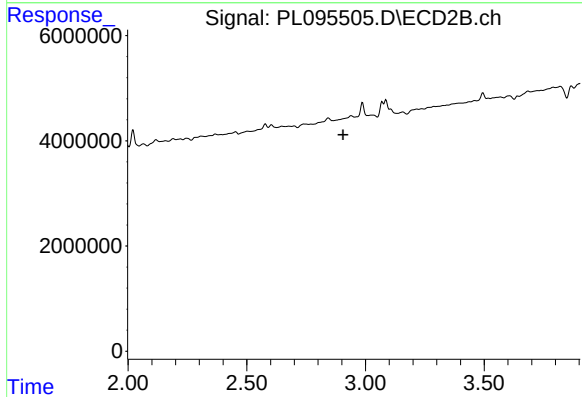


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.906 min
Response: 0
Conc: N.D.

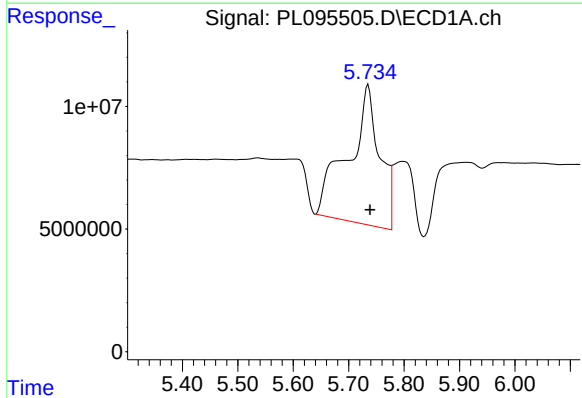


#8 Heptachlor epoxide

R.T.: 5.735 min
Delta R.T.: -0.004 min
Response: 223731081
Conc: 55.86 ng/ml

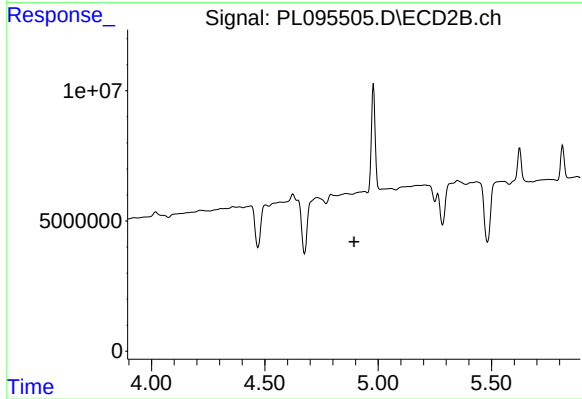

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.893 min
Response: 0
Conc: N.D.

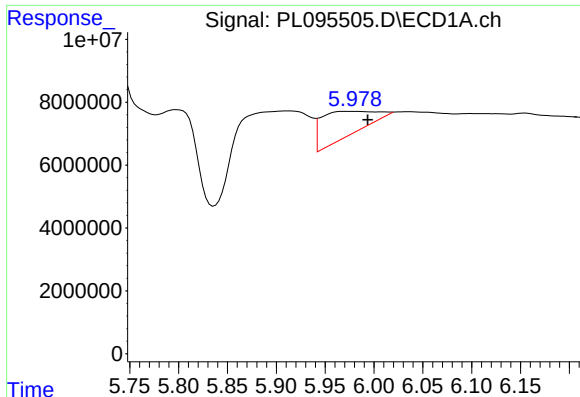

#10 gamma-Chlordane


R.T.: 5.981 min
Delta R.T.: -0.013 min
Response: 28856065
Conc: 7.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

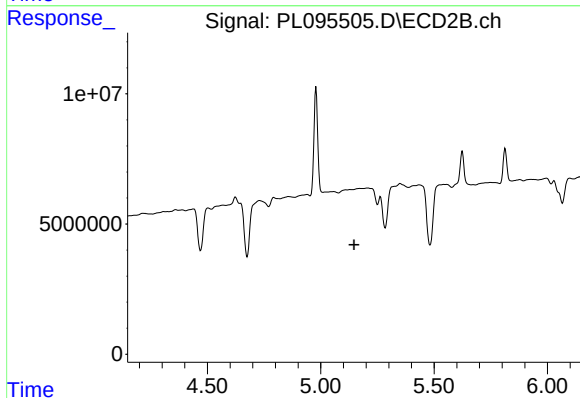


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.147 min
Response: 0
Conc: N.D.

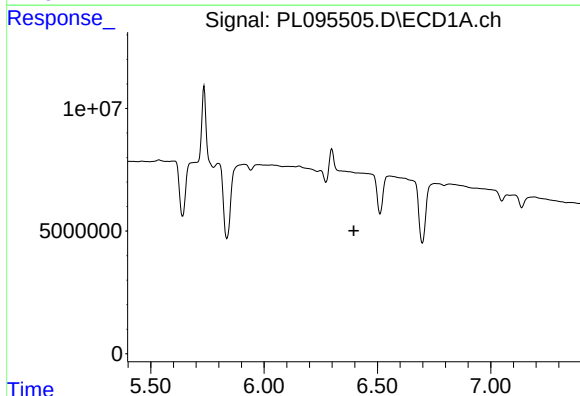


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

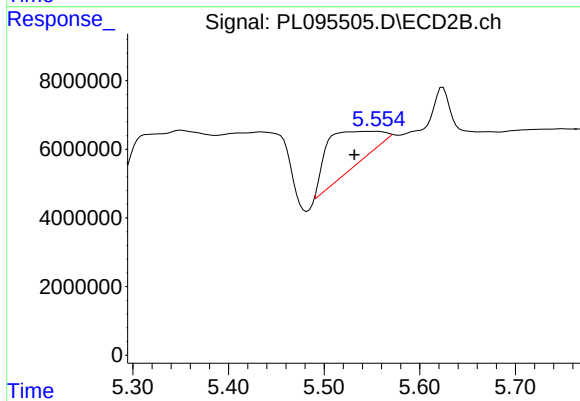

#13 Dieldrin


R.T.: 5.555 min
Delta R.T.: 0.024 min
Response: 41683862
Conc: 10.25 ng/ml

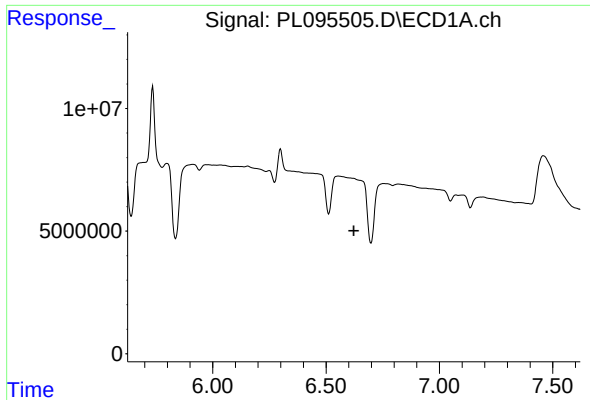

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.623 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

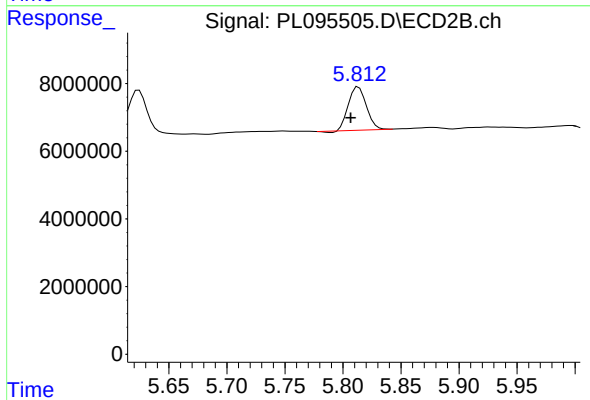


#14 Endrin

R.T.: 5.813 min
Delta R.T.: 0.007 min
Response: 13763066
Conc: 3.78 ng/ml

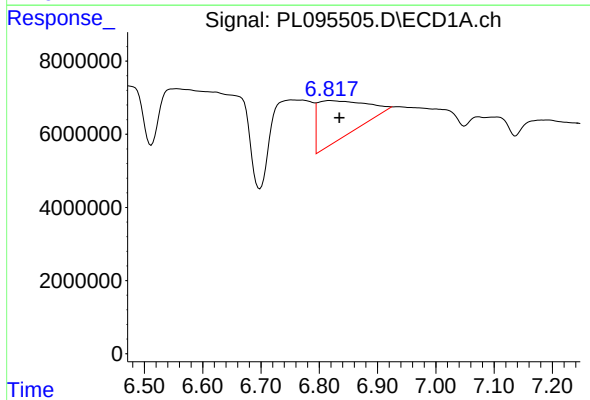


#15 Endosulfan II

R.T.: 6.819 min
Delta R.T.: -0.016 min
Response: 58055643
Conc: 18.19 ng/ml

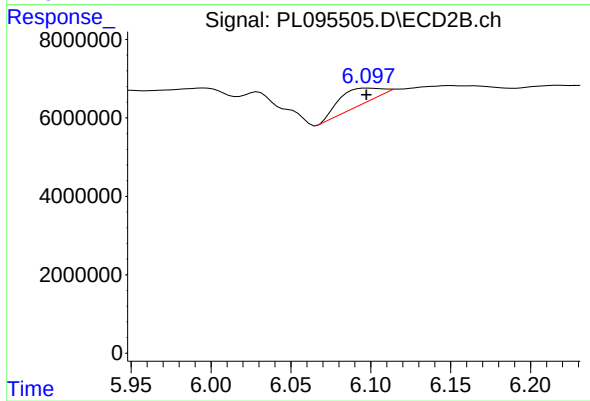

#15 Endosulfan II


R.T.: 6.099 min
Delta R.T.: 0.001 min
Response: 6940452
Conc: 1.93 ng/ml

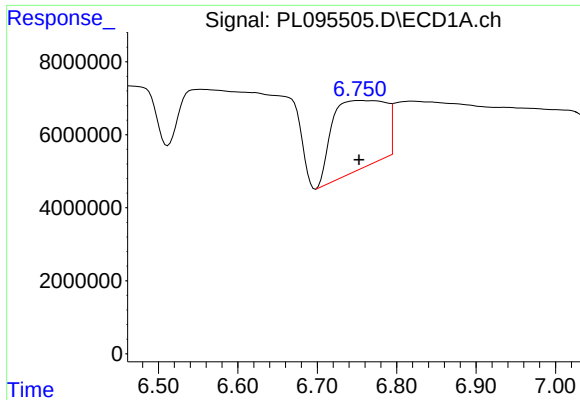

#16 4,4'-DDD


R.T.: 6.752 min
Delta R.T.: 0.000 min
Response: 87390723
Conc: 30.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

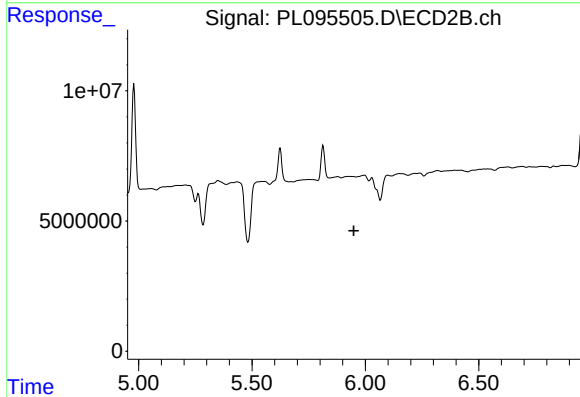


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

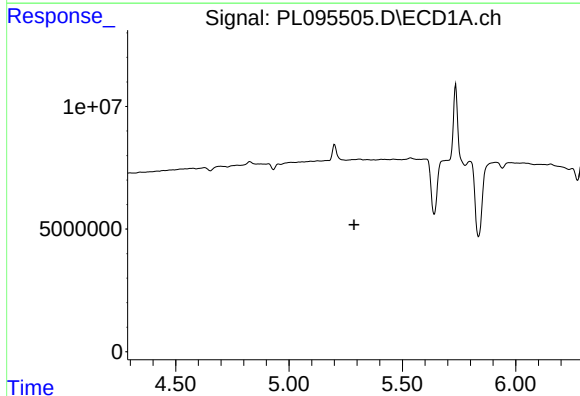


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.287 min
Response: 0
Conc: N.D.

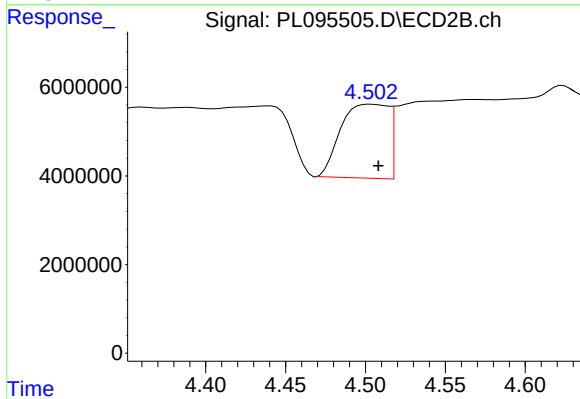

#24 Chlordane-2


R.T.: 4.503 min
Delta R.T.: -0.005 min
Response: 34304770
Conc: 186.41 ng/ml

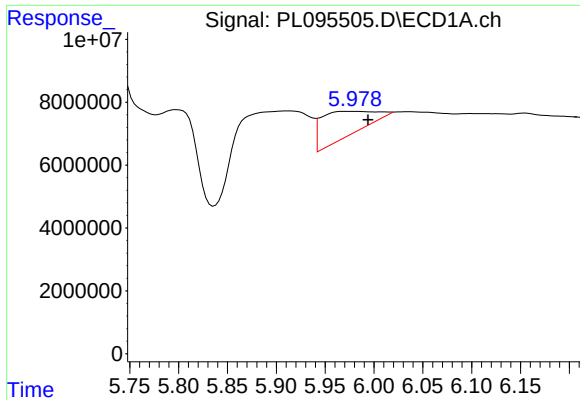

#25 Chlordane-3


R.T.: 5.981 min
Delta R.T.: -0.013 min
Response: 28856065
Conc: 37.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

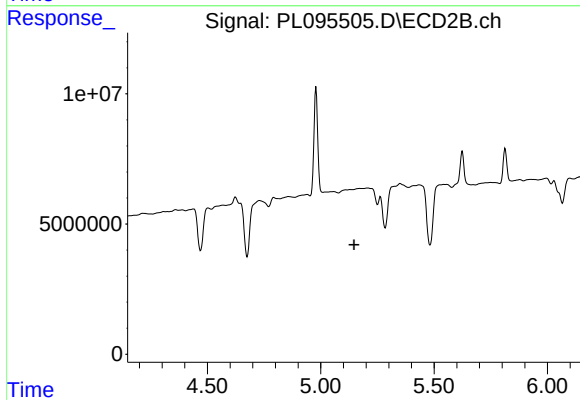


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.147 min
Response: 0
Conc: N.D.

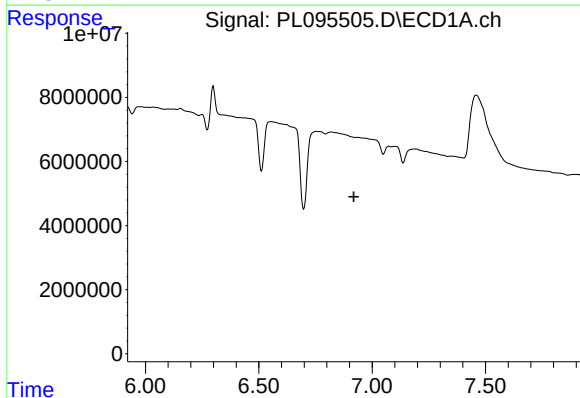


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.919 min
Response: 0
Conc: N.D.

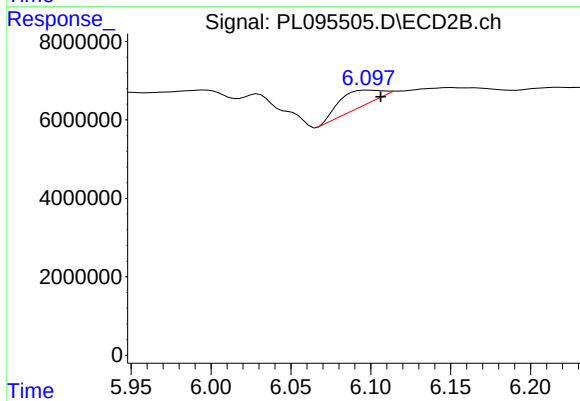

#27 Chlordane-5


R.T.: 6.099 min
Delta R.T.: -0.008 min
Response: 6940452
Conc: 37.57 ng/ml

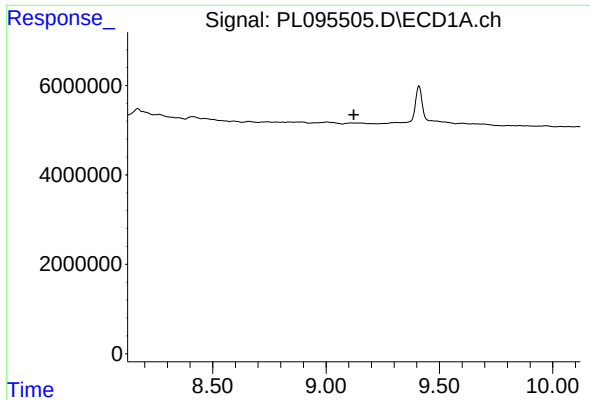

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.122 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

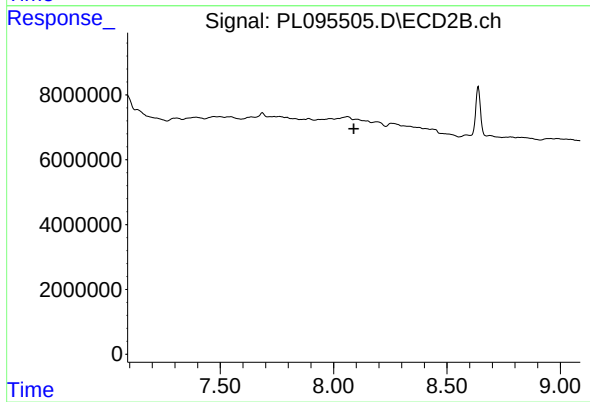

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.089 min
Response: 0
Conc: N.D.