

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050425\
 Data File : PL095512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2025 13:32
 Operator : AR\AJ
 Sample : Q1923-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-04302025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 01:31:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.594	2.909	26042160	38798788	7.977	12.202 #
28)	SA Decachlor...	9.118	8.087	34973705	34540172	12.622	11.672
Target Compounds							
2)	A alpha-BHC	0.000	3.439f	0	4002672	N.D.	0.900 #
10)	B gamma-Chl...	5.990	5.173f	26008747	11964256	6.376	2.952 #
11)	B alpha-Chl...	6.076	5.211	28448926	13164258	6.997	3.307 #
17)	MA 4,4'-DDT	0.000	6.200	0	3611407	N.D.	1.051 #
24)	Chlordane-2	0.000	4.537f	0	3500337	N.D.	19.021 #
25)	Chlordane-3	5.990	5.173f	26008747	11964256	33.391	23.159 #
26)	Chlordane-4	6.076	5.211	28448926	13164258	30.171	30.290



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050425\
Data File : PL095512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2025 13:32
Operator : AR\AJ
Sample : Q1923-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-05-04302025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 01:31:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

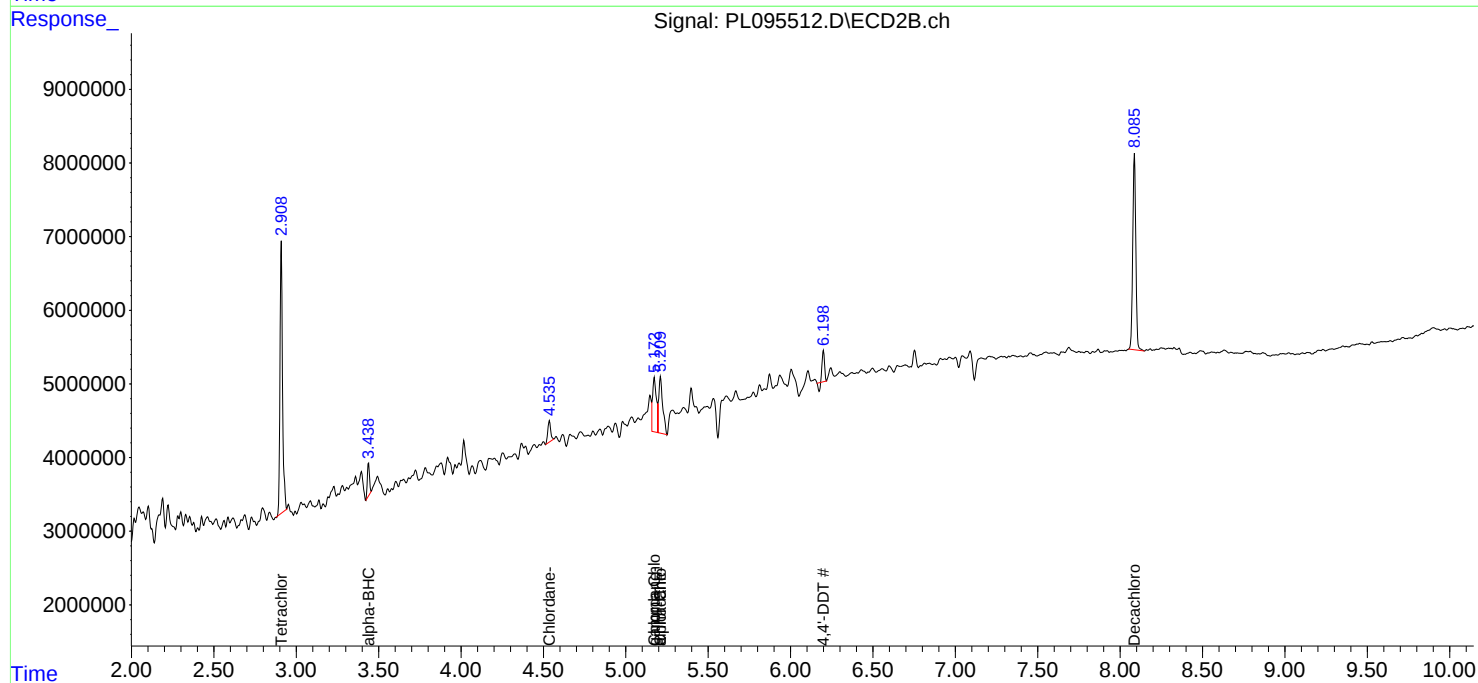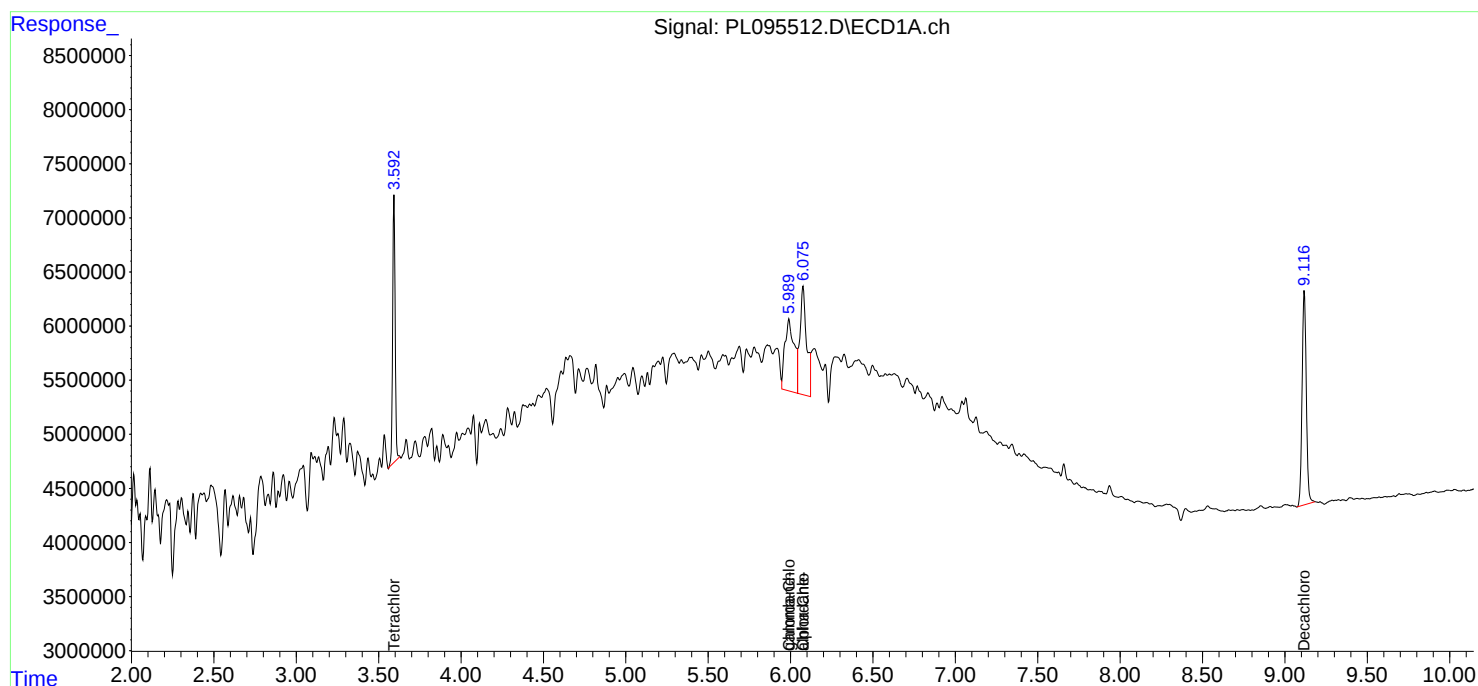


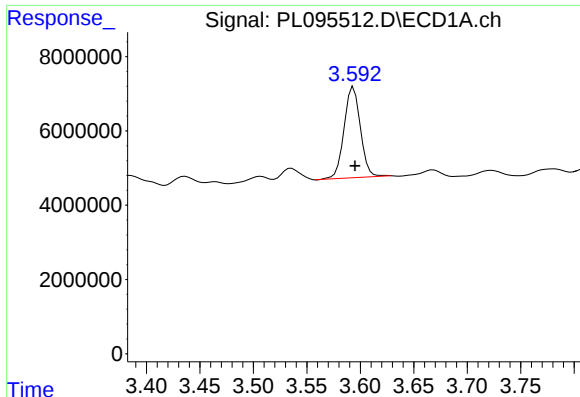

#1 Tetrachloro-m-xylene


R.T.: 3.594 min
Delta R.T.: -0.001 min
Response: 26042160
Conc: 7.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-04302025

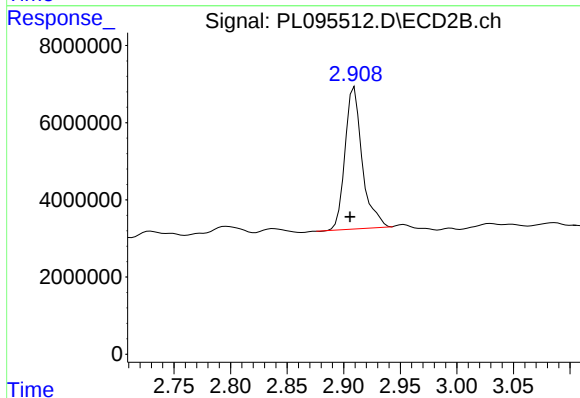


#1 Tetrachloro-m-xylene

R.T.: 2.909 min
Delta R.T.: 0.004 min
Response: 38798788
Conc: 12.20 ng/ml

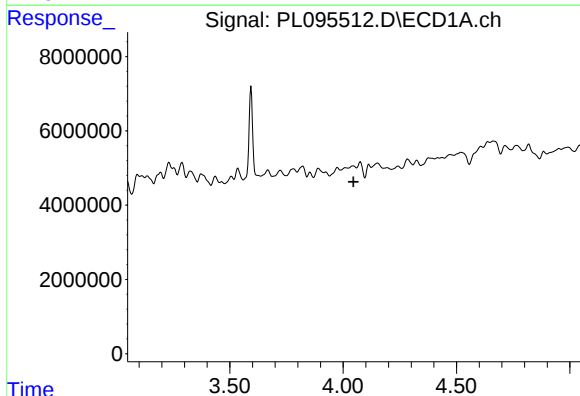


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.046 min
Response: 0
Conc: N.D.

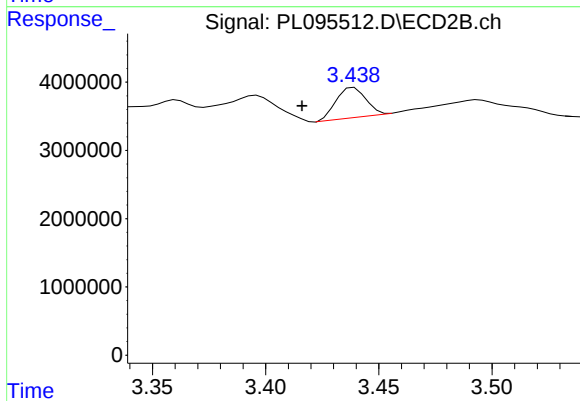

#2 alpha-BHC


R.T.: 3.439 min
Delta R.T.: 0.023 min
Response: 4002672
Conc: 0.90 ng/ml

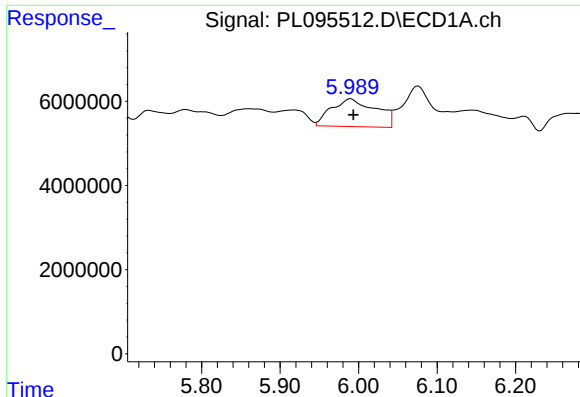

#10 gamma-Chlordane


R.T.: 5.990 min
Delta R.T.: -0.003 min
Response: 26008747
Conc: 6.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-04302025

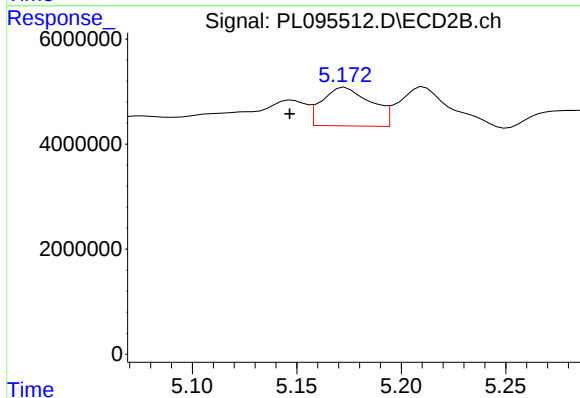


#10 gamma-Chlordane

R.T.: 5.173 min
Delta R.T.: 0.027 min
Response: 11964256
Conc: 2.95 ng/ml

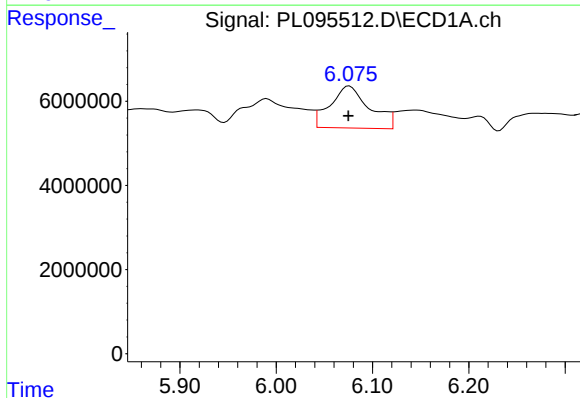


#11 alpha-Chlordane

R.T.: 6.076 min
Delta R.T.: 0.001 min
Response: 28448926
Conc: 7.00 ng/ml

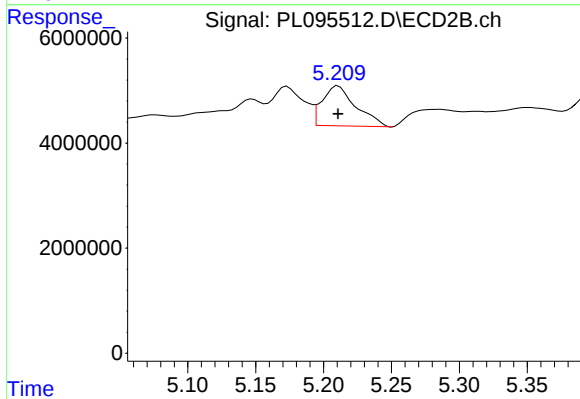

#11 alpha-Chlordane


R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 13164258
Conc: 3.31 ng/ml

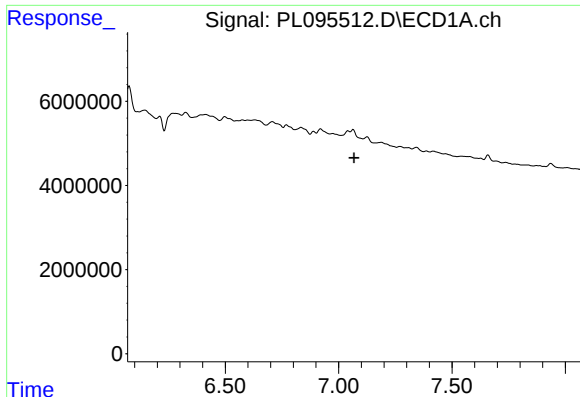

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR-05-04302025

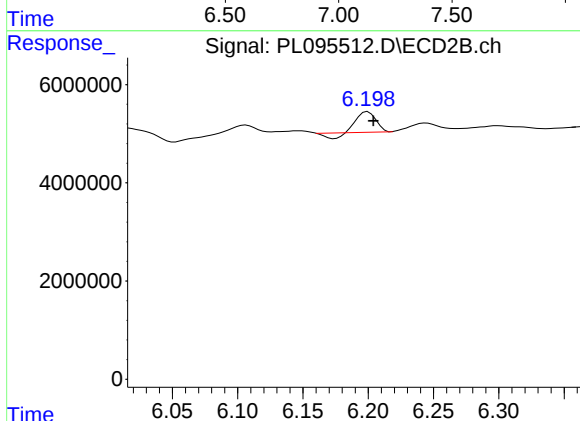


#17 4,4'-DDT

R.T.: 6.200 min
Delta R.T.: -0.004 min
Response: 3611407
Conc: 1.05 ng/ml

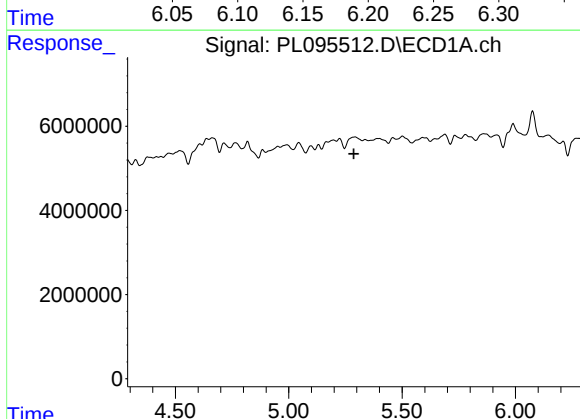


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.287 min
Response: 0
Conc: N.D.

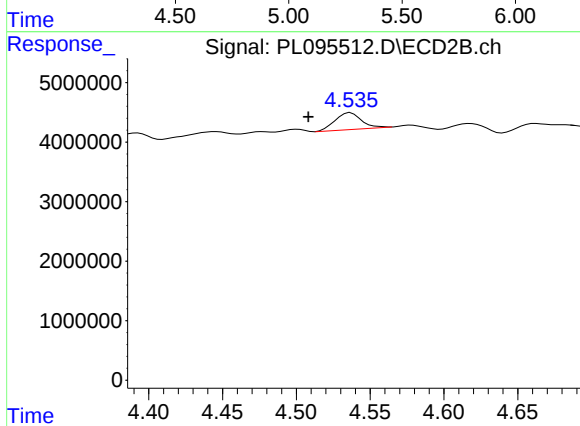

#24 Chlordane-2


R.T.: 4.537 min
Delta R.T.: 0.029 min
Response: 3500337
Conc: 19.02 ng/ml

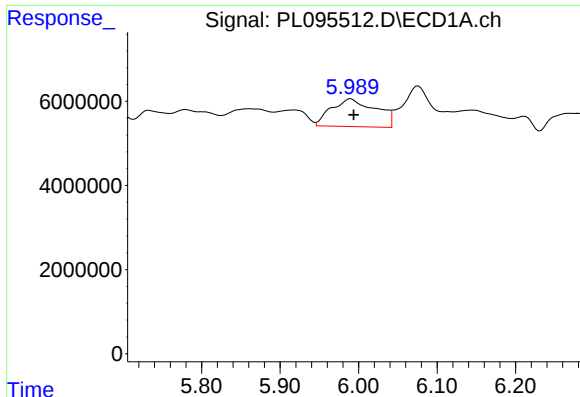

#25 Chlordane-3


R.T.: 5.990 min
Delta R.T.: -0.004 min
Response: 26008747
Conc: 33.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-04302025

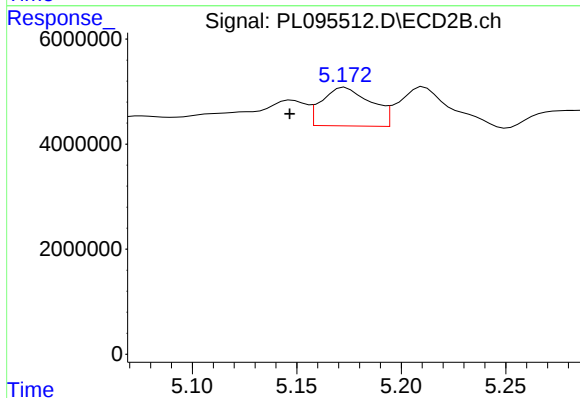


#25 Chlordane-3

R.T.: 5.173 min
Delta R.T.: 0.027 min
Response: 11964256
Conc: 23.16 ng/ml

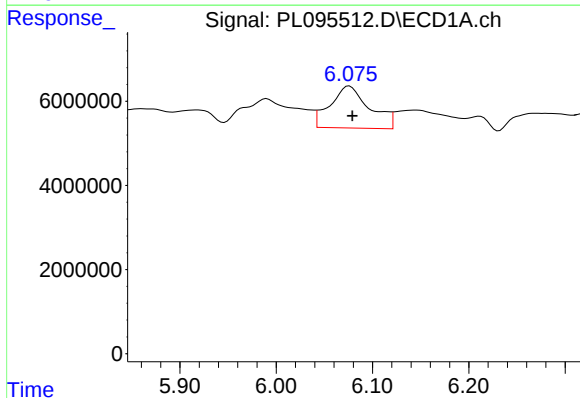


#26 Chlordane-4

R.T.: 6.076 min
Delta R.T.: -0.003 min
Response: 28448926
Conc: 30.17 ng/ml

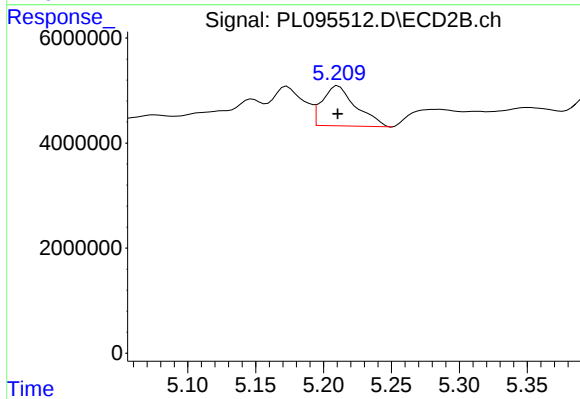

#26 Chlordane-4


R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 13164258
Conc: 30.29 ng/ml

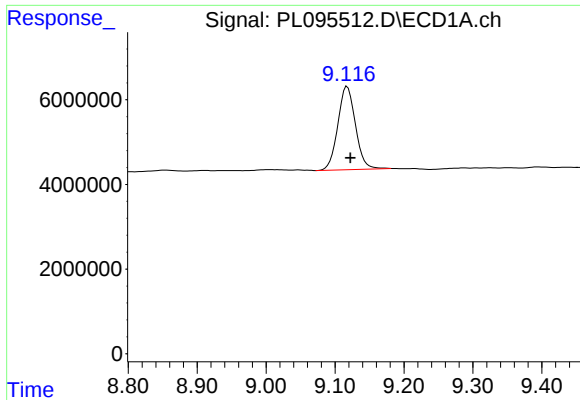

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.005 min
Response: 34973705
Conc: 12.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-04302025

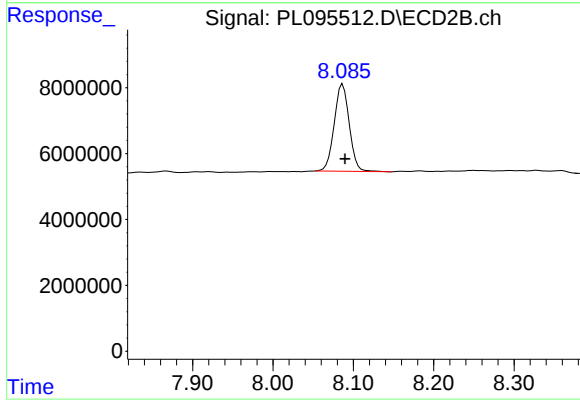

#28 Decachlorobiphenyl

R.T.: 8.087 min
Delta R.T.: -0.003 min
Response: 34540172
Conc: 11.67 ng/ml