

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050520\
 Data File : PL058531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2020 15:35
 Operator : AJ\MA
 Sample : L2483-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 6FT-TP-5

Manual Integrations
 APPROVED

mohammad
 5/6/2020 2:39:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 00:39:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 29 00:55:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.455	3.954	233.1E6	47173370	21.903	21.825
28)	SA Decachlor...	8.200	8.975	161.9E6	35640720	14.973	16.063
Target Compounds							
12)	B 4,4'-DDE	5.612	6.274	32215160	5283604	2.131	1.732
16)	A 4,4'-DDD	6.129	6.763	20403270	4044233	1.740	1.779m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050520\
Data File : PL058531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2020 15:35
Operator : AJ\MA
Sample : L2483-10
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
6FT-TP-5


Manual Integrations
APPROVED

mohammad
5/6/2020 2:39:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 00:39:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
Quant Title : GC Extractables
QLast Update : Wed Apr 29 00:55:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

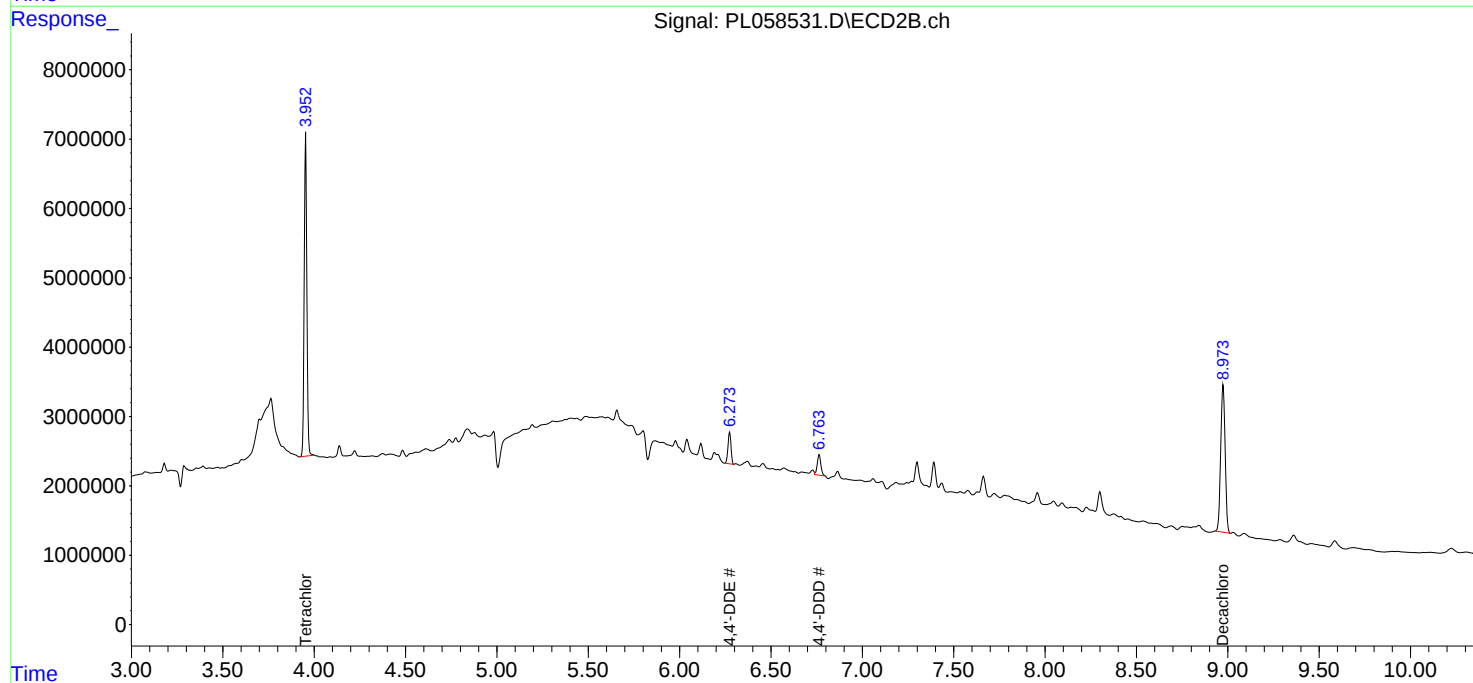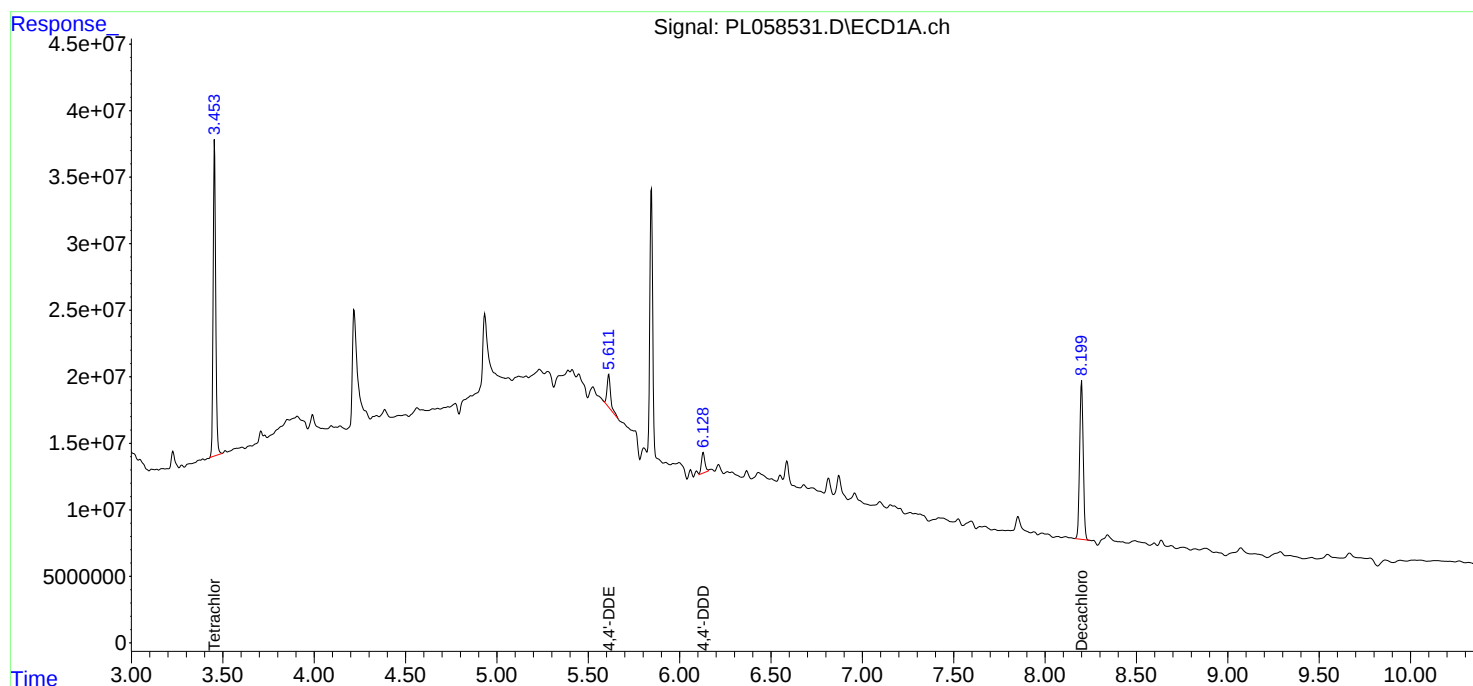

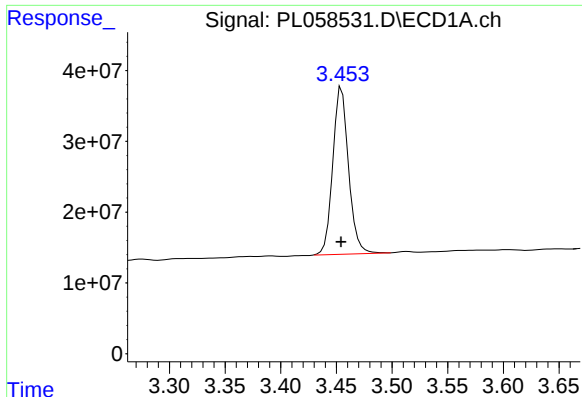


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: 0.000 min
Response: 233094362
Conc: 21.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
6FT-TP-5


Manual Integrations
APPROVED

mohammad
5/6/2020 2:39:55 PM

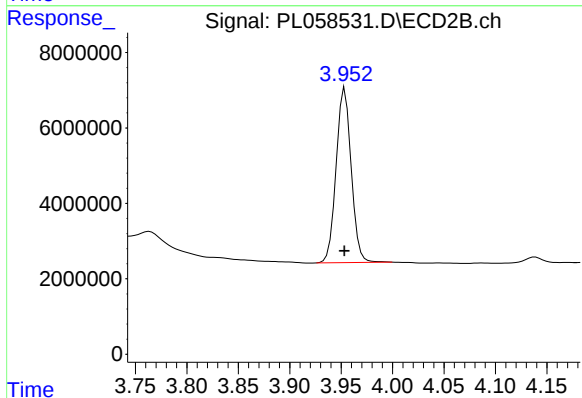


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: 0.000 min
Response: 47173370
Conc: 21.83 ng/ml

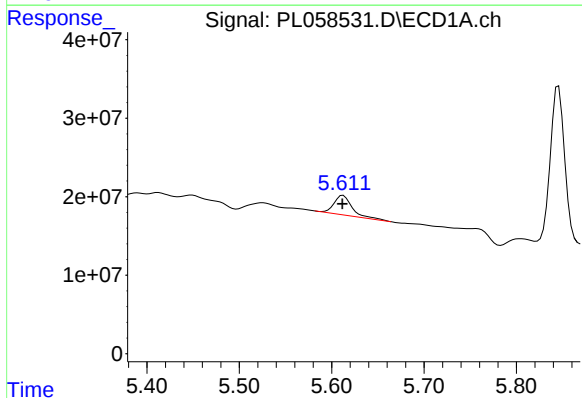


#12 4,4'-DDE

R.T.: 5.612 min
Delta R.T.: 0.000 min
Response: 32215160
Conc: 2.13 ng/ml

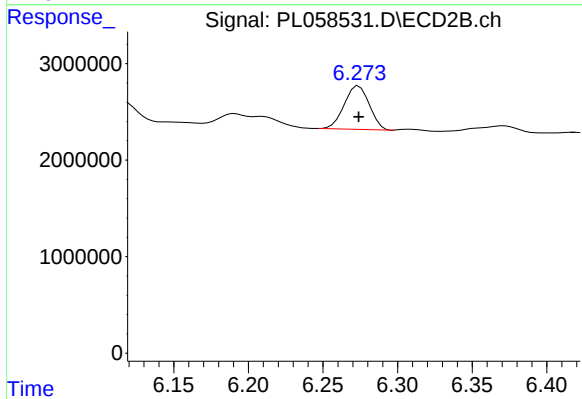

#12 4,4'-DDE

R.T.: 6.274 min
Delta R.T.: 0.000 min
Response: 5283604
Conc: 1.73 ng/ml

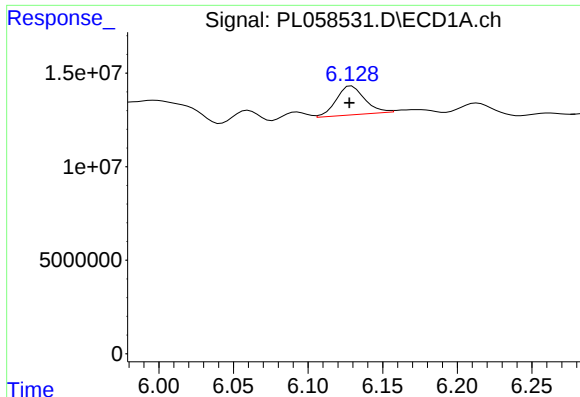


#16 4,4'-DDD

R.T.: 6.129 min
Delta R.T.: 0.002 min
Response: 20403270
Conc: 1.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
6FT-TP-5


Manual Integrations
APPROVED

mohammad
5/6/2020 2:39:55 PM

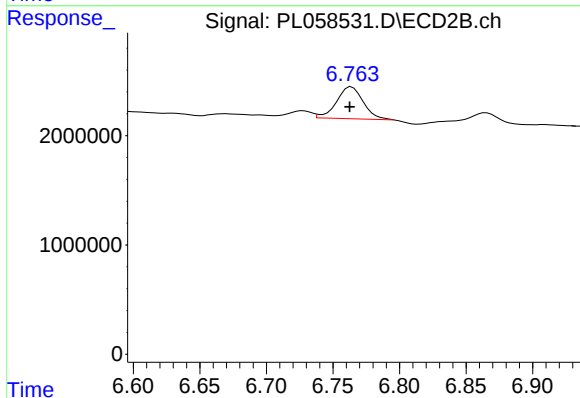


#16 4,4'-DDD

R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 4044233
Conc: 1.78 ng/ml m

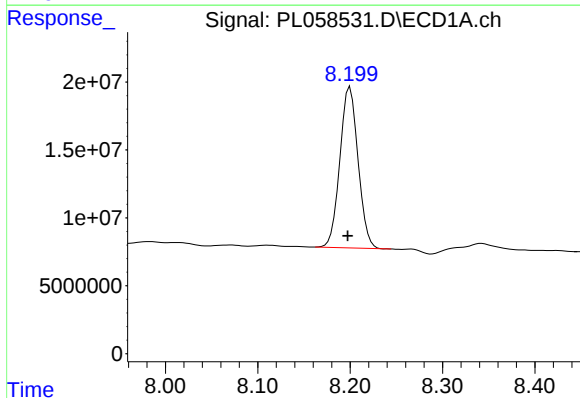

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: 0.003 min
Response: 161925592
Conc: 14.97 ng/ml

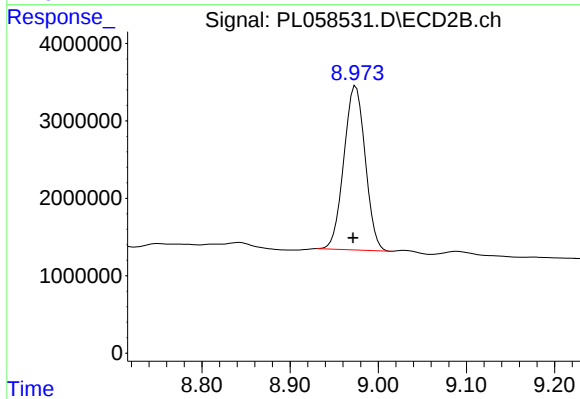

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.003 min
Response: 35640720
Conc: 16.06 ng/ml