

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050521\
 Data File : PL066697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2021 14:38
 Operator : AR\AJ
 Sample : M2275-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT-020

Manual Integrations
 APPROVED

Ankita
 5/6/2021 1:48:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 16:42:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.426	4.151	63551080	63923715	16.866	18.201
28) SA Decachlor...	8.144	9.347	64523284	48506717	16.828m	15.680
Target Compounds						
12) B 4,4'-DDE	5.566	6.535	6110968	6783817	1.339m	1.788 #
17) MA 4,4'-DDT	6.314	7.335	6127148	8107808	1.571m	2.505 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050521\
Data File : PL066697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2021 14:38
Operator : AR\AJ
Sample : M2275-09
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
CRT-020


Manual Integrations
APPROVED

Ankita
5/6/2021 1:48:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 16:42:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

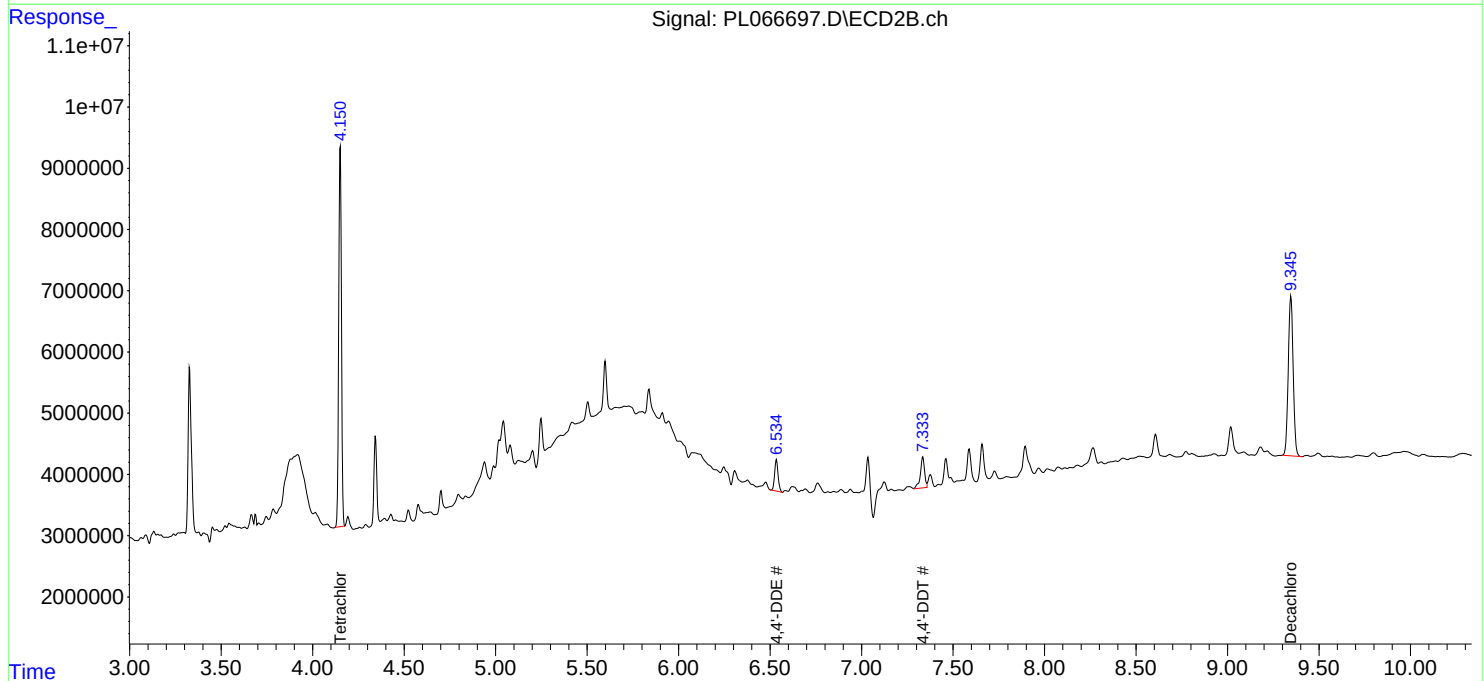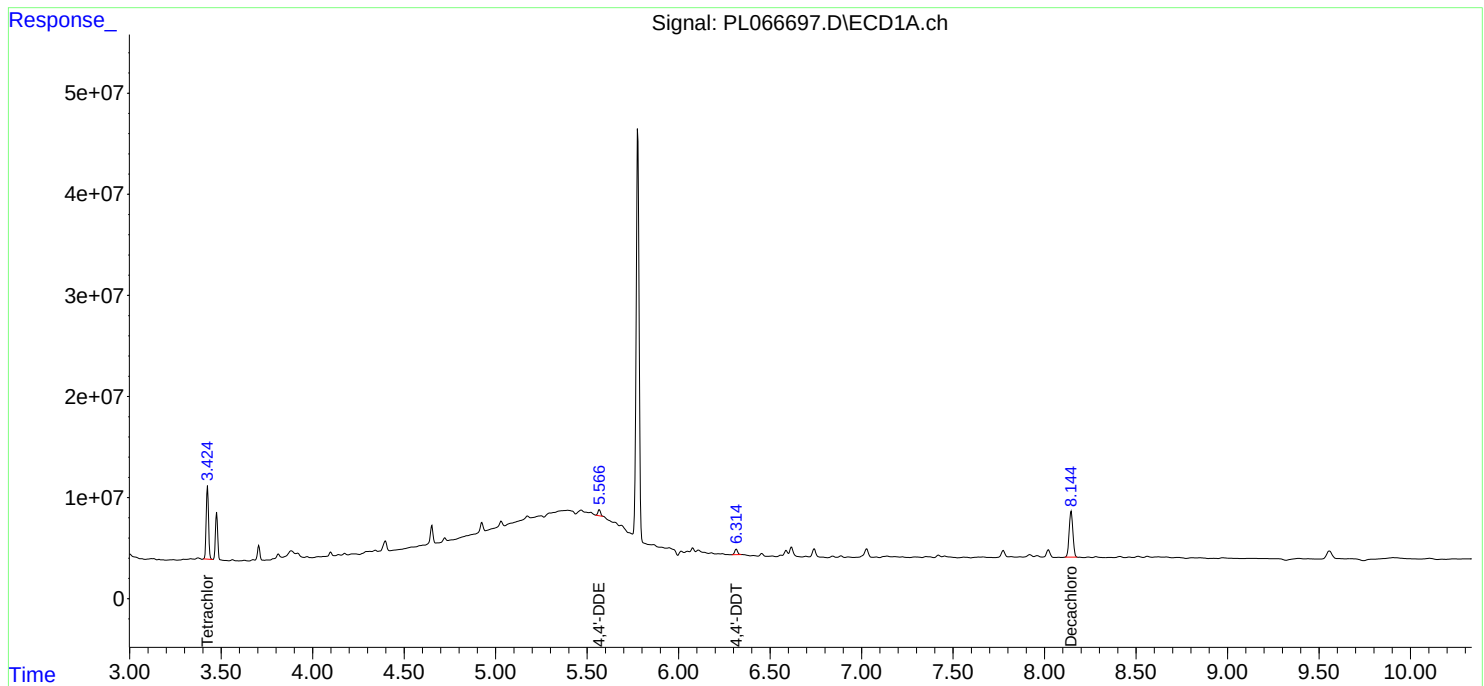

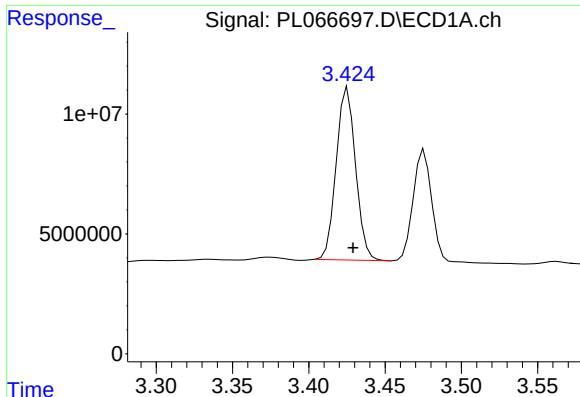


#1 Tetrachloro-m-xylene

R.T.: 3.426 min
Delta R.T.: -0.003 min
Response: 63551080
Conc: 16.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-020


Manual Integrations
APPROVED

Ankita
5/6/2021 1:48:05 PM

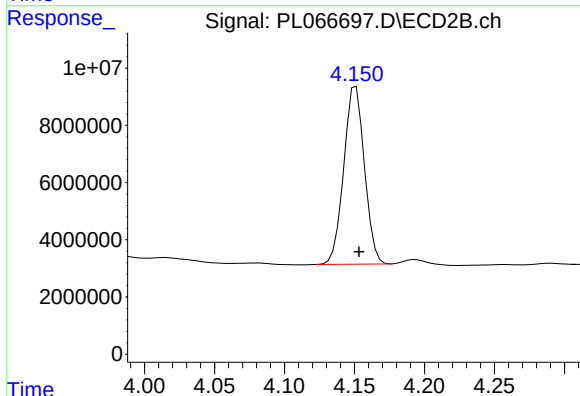


#1 Tetrachloro-m-xylene

R.T.: 4.151 min
Delta R.T.: -0.002 min
Response: 63923715
Conc: 18.20 ng/ml

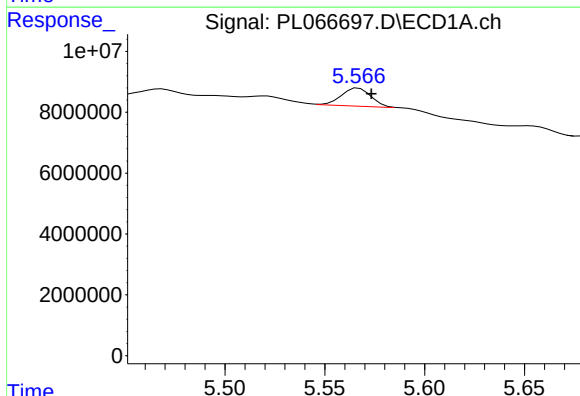


#12 4,4'-DDE

R.T.: 5.566 min
Delta R.T.: -0.008 min
Response: 6110968
Conc: 1.34 ng/ml m

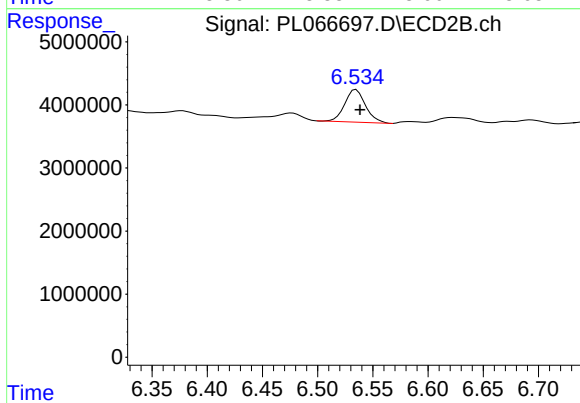

#12 4,4'-DDE

R.T.: 6.535 min
Delta R.T.: -0.004 min
Response: 6783817
Conc: 1.79 ng/ml

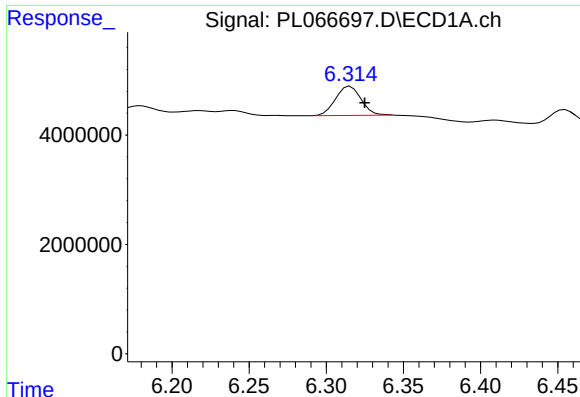


#17 4,4'-DDT

R.T.: 6.314 min
Delta R.T.: -0.011 min
Response: 6127148
Conc: 1.57 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CRT-020


Manual Integrations
APPROVED

Ankita
5/6/2021 1:48:05 PM

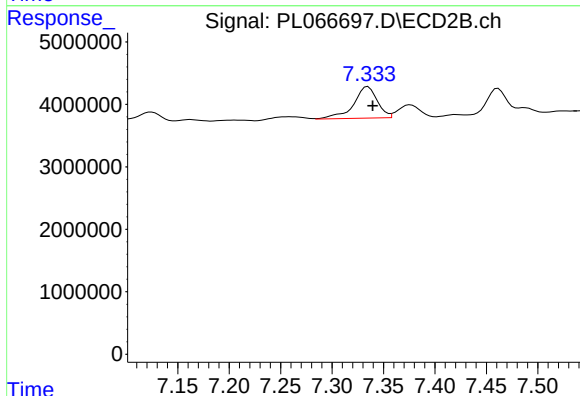


#17 4,4'-DDT

R.T.: 7.335 min
Delta R.T.: -0.005 min
Response: 8107808
Conc: 2.51 ng/ml

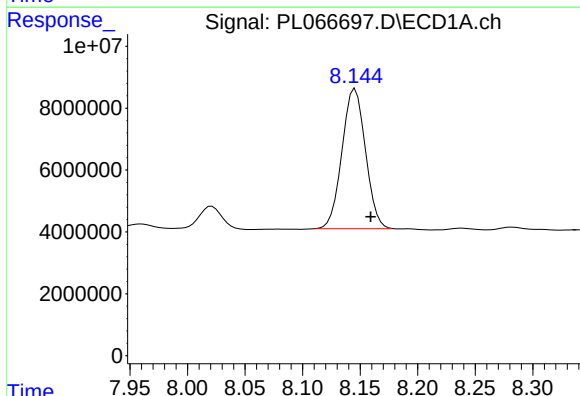

#28 Decachlorobiphenyl

R.T.: 8.144 min
Delta R.T.: -0.015 min
Response: 64523284
Conc: 16.83 ng/ml m

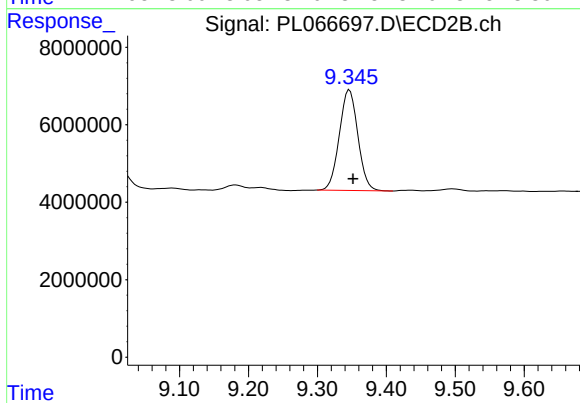

#28 Decachlorobiphenyl

R.T.: 9.347 min
Delta R.T.: -0.005 min
Response: 48506717
Conc: 15.68 ng/ml