

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050521\
 Data File : PL066701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2021 15:36
 Operator : AR\AJ
 Sample : M2277-01MS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-01-A3-A3A-B3-B3AMS

Manual Integrations
 APPROVED

Ankita
 5/6/2021 1:48:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 07:42:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.151	55775390	58144547	14.802	16.556
28)	SA Decachlor...	8.144	9.348	77017476	54920938	20.087m	17.753

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050521\
Data File : PL066701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2021 15:36
Operator : AR\AJ
Sample : M2277-01MS
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-A3-A3A-B3-B3AMS


Manual Integrations
APPROVED

Ankita
5/6/2021 1:48:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 07:42:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

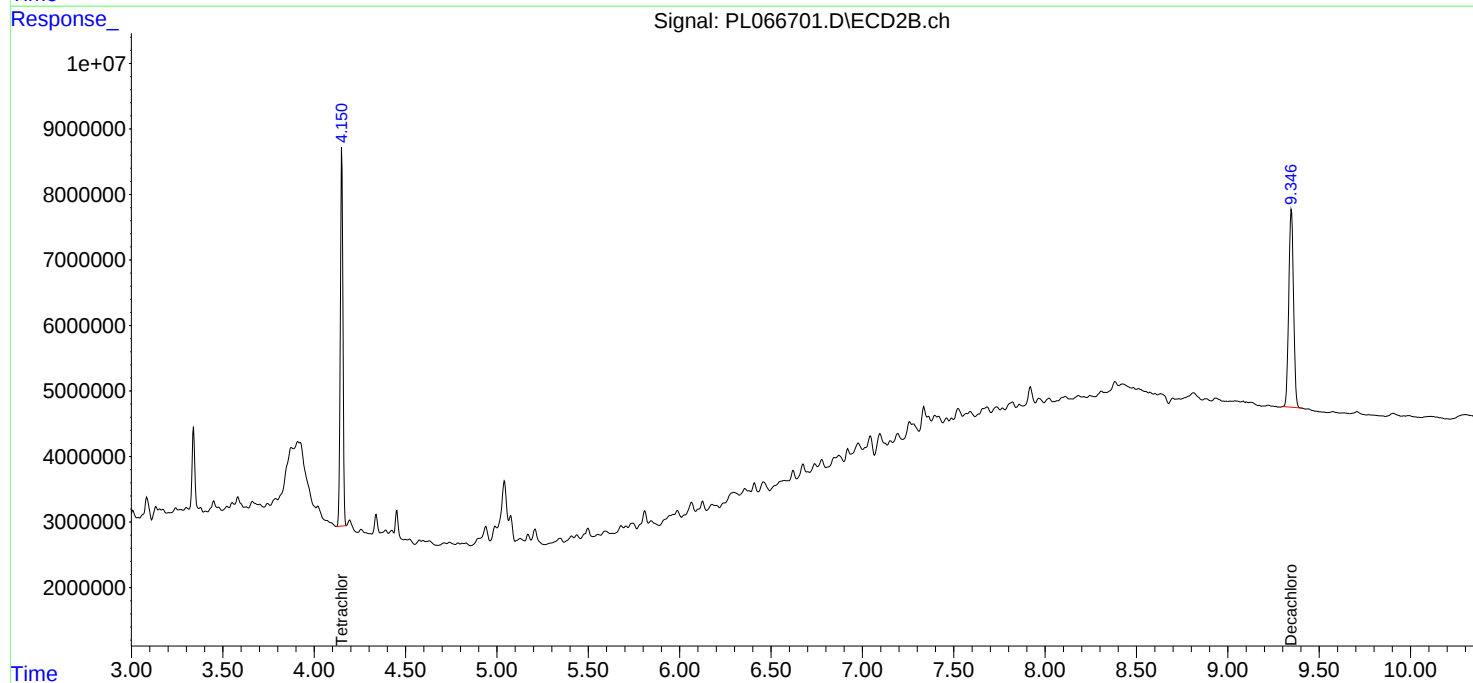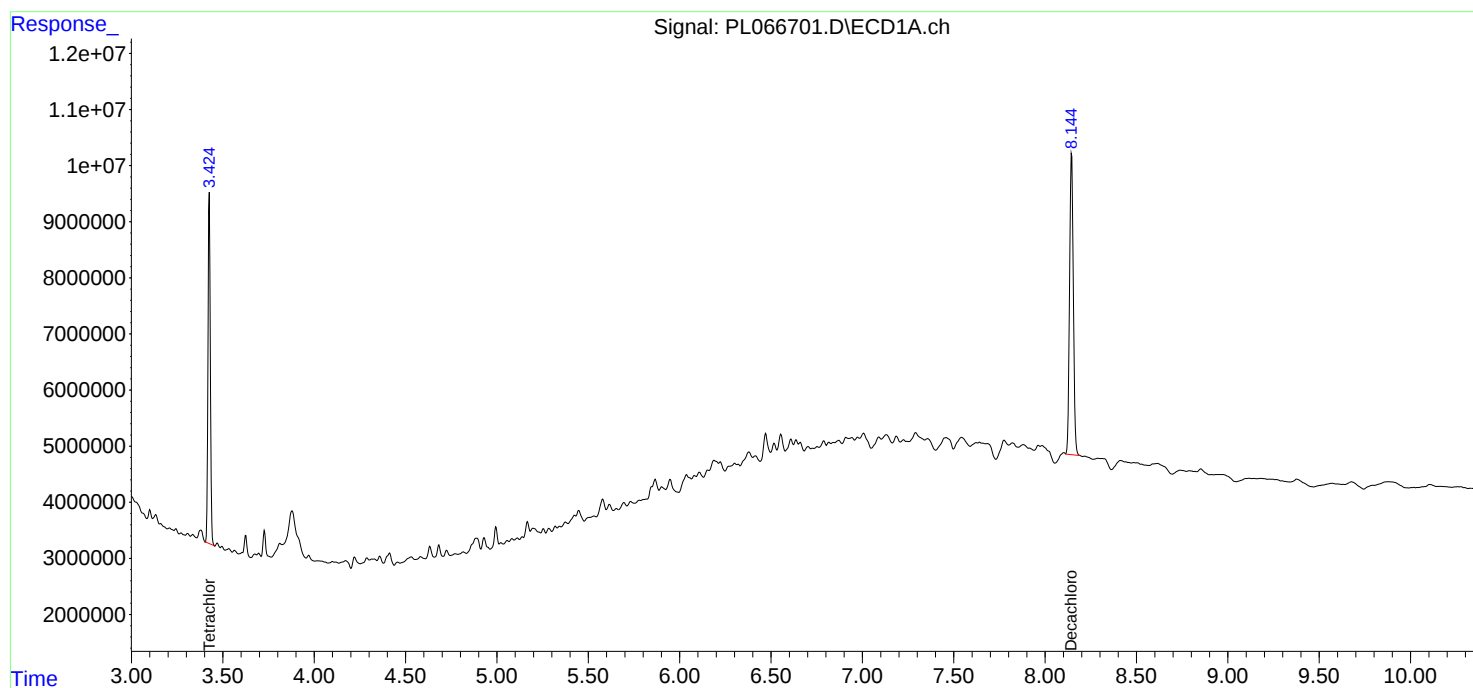

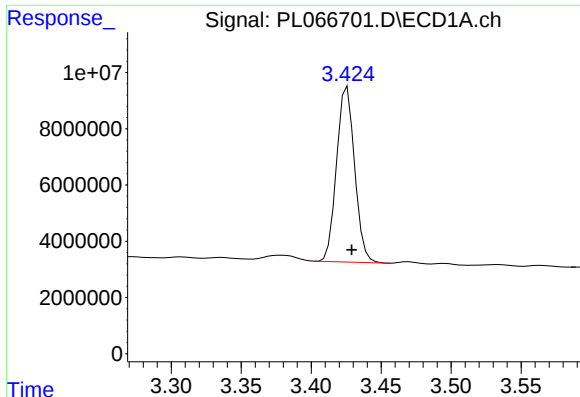


#1 Tetrachloro-m-xylene

R.T.: 3.426 min
Delta R.T.: -0.003 min
Response: 55775390
Conc: 14.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-A3-A3A-B3-B3AMS


Manual Integrations
APPROVED

Ankita
5/6/2021 1:48:15 PM

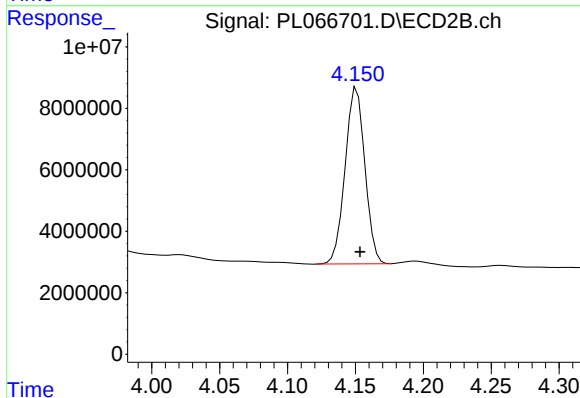


#1 Tetrachloro-m-xylene

R.T.: 4.151 min
Delta R.T.: -0.002 min
Response: 58144547
Conc: 16.56 ng/ml

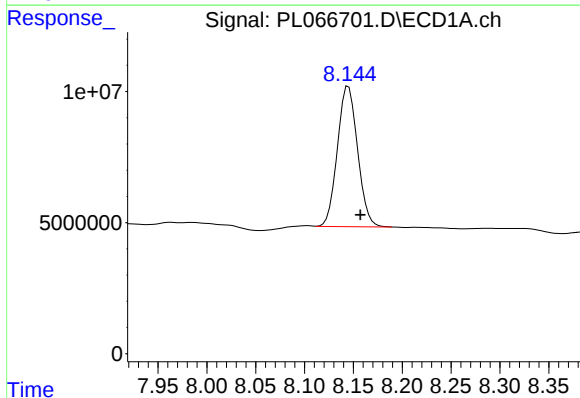

#28 Decachlorobiphenyl

R.T.: 8.144 min
Delta R.T.: -0.013 min
Response: 77017476
Conc: 20.09 ng/ml m

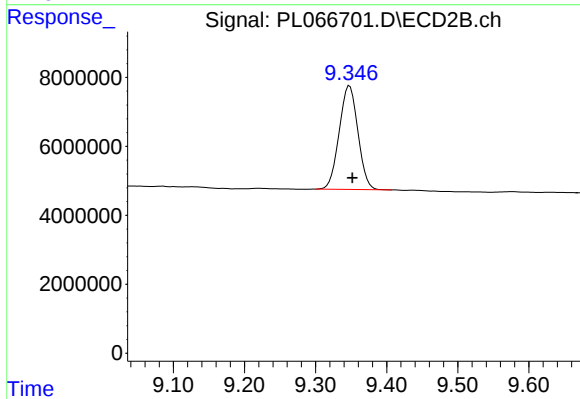

#28 Decachlorobiphenyl

R.T.: 9.348 min
Delta R.T.: -0.004 min
Response: 54920938
Conc: 17.75 ng/ml