

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050522\
 Data File : PL074558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2022 17:39
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 01:15:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.489	8756827	46747174	27.102	26.219
28)	SA Decachlor...	10.403	11.332	12955009	49884835	24.912	28.243
Target Compounds							
6)	B beta-BHC	0.000	6.678	0	754679	N.D.	0.670 #
7)	B delta-BHC	0.000	6.955	0	1965473	N.D.	0.805 #
8)	B Heptachlo...	0.000	7.926	0	1445967	N.D.	0.642 #
9)	A Endosulfan I	0.000	8.332	0	228372	N.D.	0.116 #
10)	B gamma-Chl...	0.000	8.206	0	505082	N.D.	0.226 #
11)	B alpha-Chl...	0.000	8.252f	0	134830	N.D.	0.063 #
13)	MA Dieldrin	7.757f	8.600	27321	70487	0.064	0.035 #
14)	MA Endrin	8.079	8.840	159407	555400	0.392	0.328
20)	A Methoxychlor	0.000	9.789	0	1372970	N.D.	1.427 #
22)	Mirex	9.518f	0.000	39700	0	0.085	N.D. #
23)	Chlordane-1	0.000	6.856	0	796090	N.D.	9.976 #
25)	Chlordane-3	0.000	8.206	0	505082	N.D.	1.493 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050522\
Data File : PL074558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2022 17:39
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 01:15:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

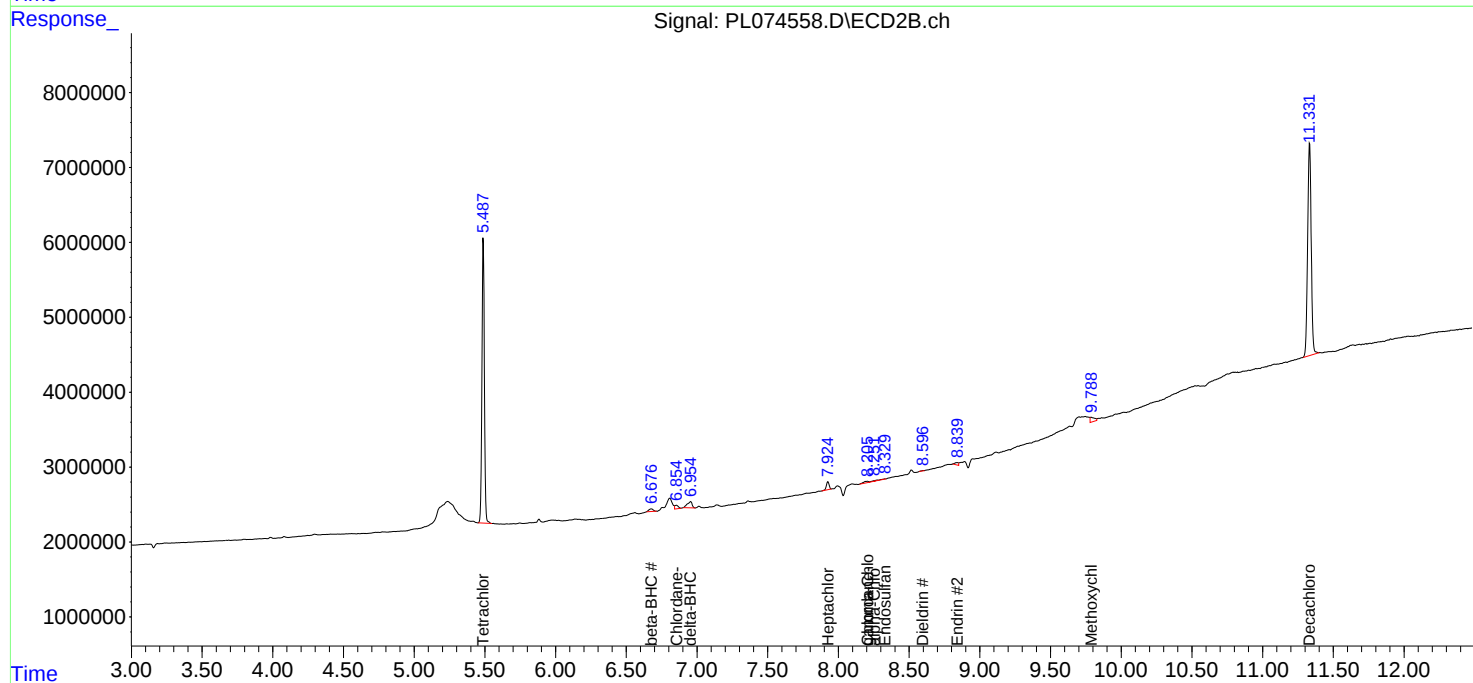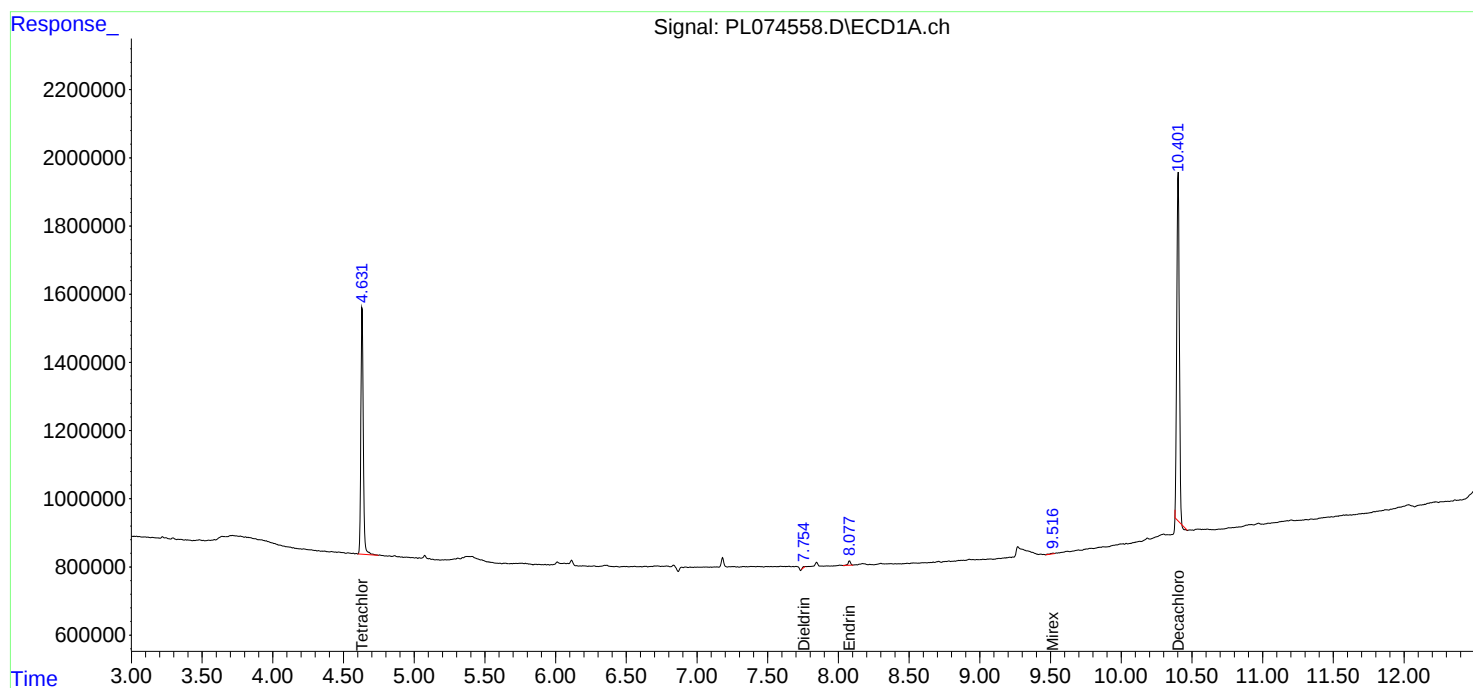


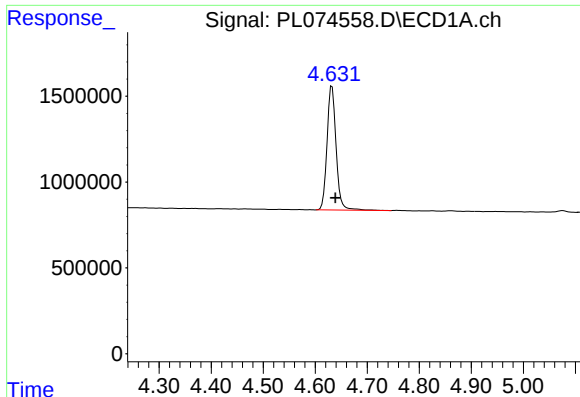

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: -0.007 min
Response: 8756827
Conc: 27.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

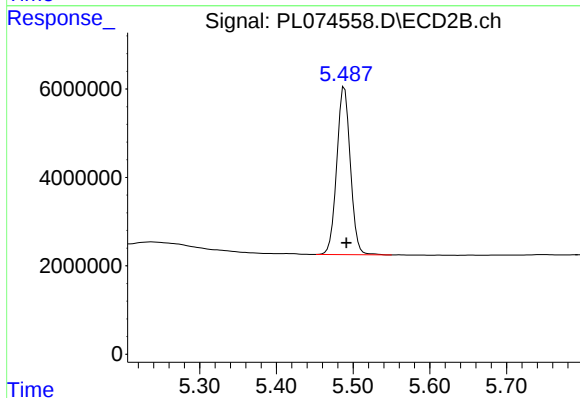


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.003 min
Response: 46747174
Conc: 26.22 ng/ml

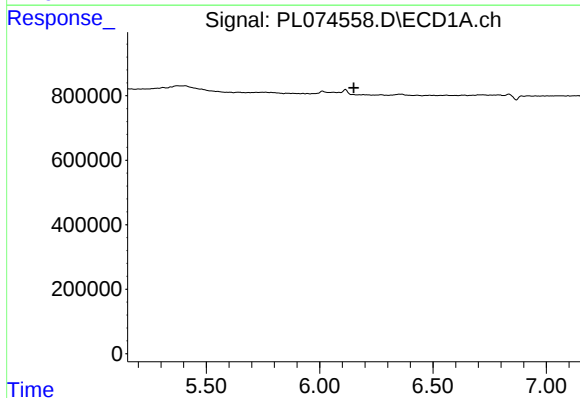


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.151 min
Response: 0
Conc: N.D.

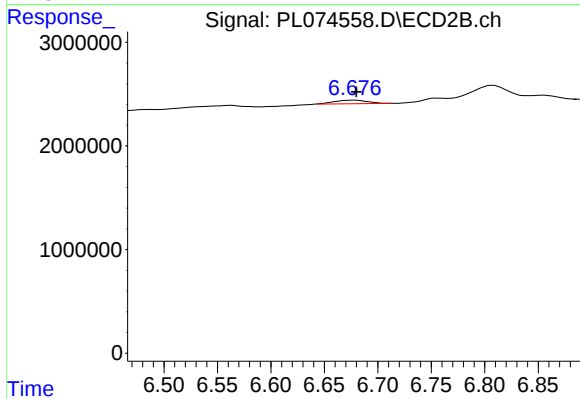

#6 beta-BHC


R.T.: 6.678 min
Delta R.T.: -0.002 min
Response: 754679
Conc: 0.67 ng/ml

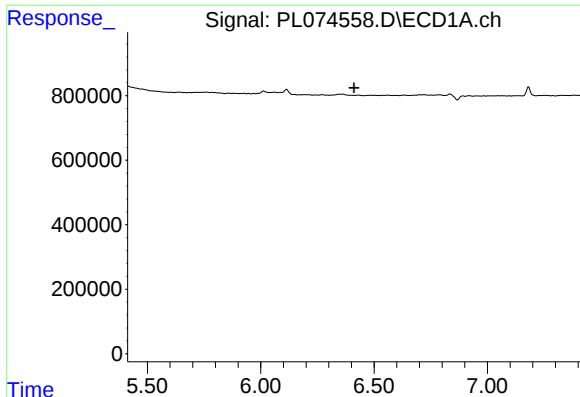

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

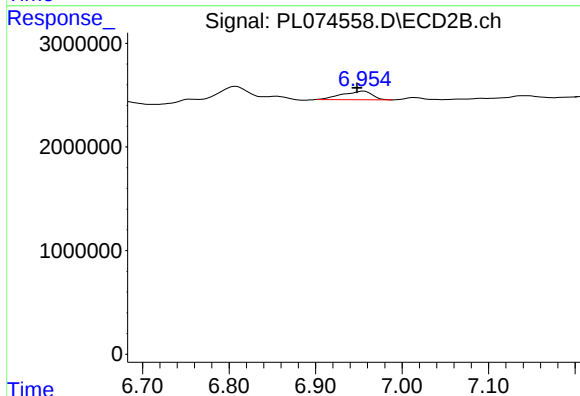


#7 delta-BHC

R.T.: 6.955 min
Delta R.T.: 0.007 min
Response: 1965473
Conc: 0.80 ng/ml

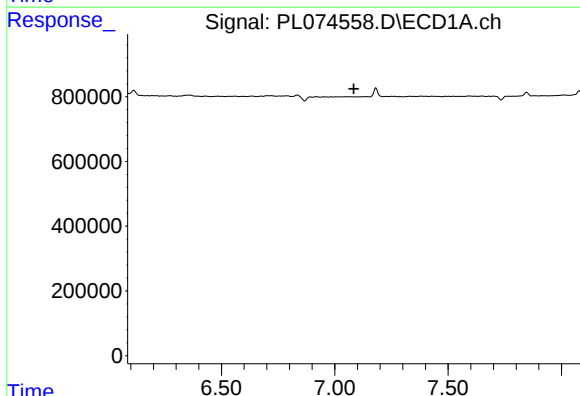


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

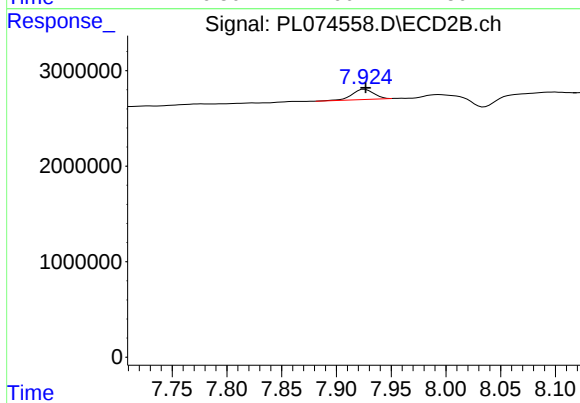

#8 Heptachlor epoxide


R.T.: 7.926 min
Delta R.T.: 0.000 min
Response: 1445967
Conc: 0.64 ng/ml

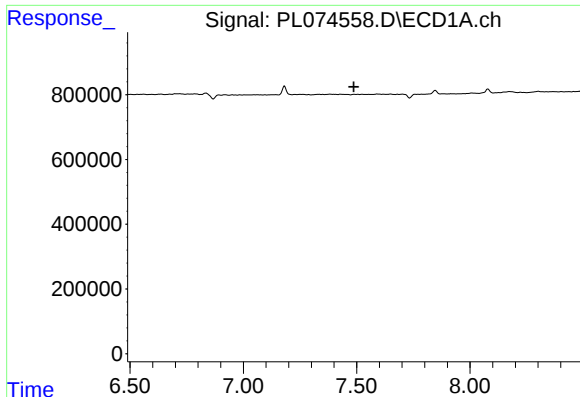

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

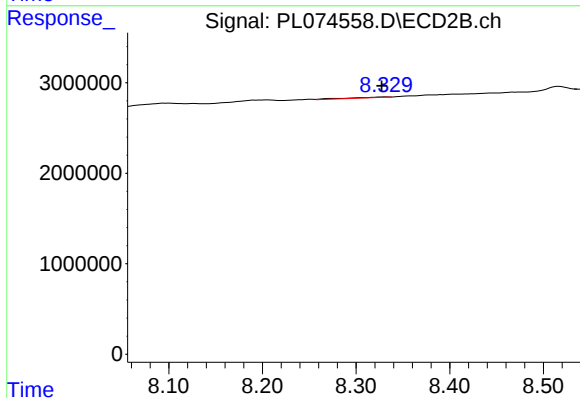


#9 Endosulfan I

R.T.: 8.332 min
Delta R.T.: 0.005 min
Response: 228372
Conc: 0.12 ng/ml

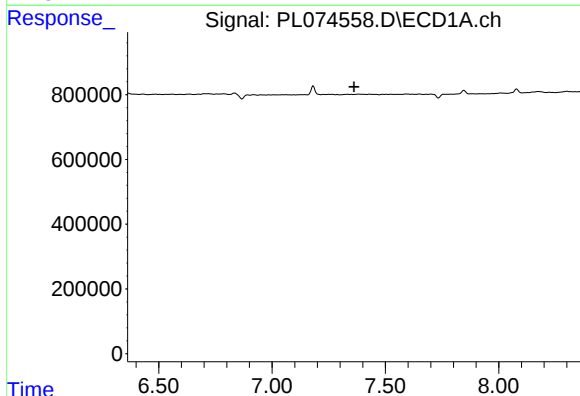


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

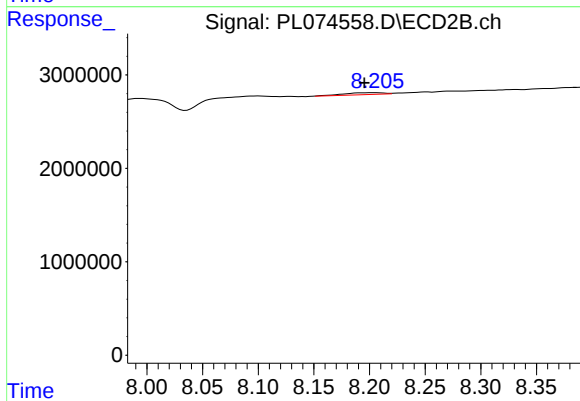

#10 gamma-Chlordane


R.T.: 8.206 min
Delta R.T.: 0.010 min
Response: 505082
Conc: 0.23 ng/ml

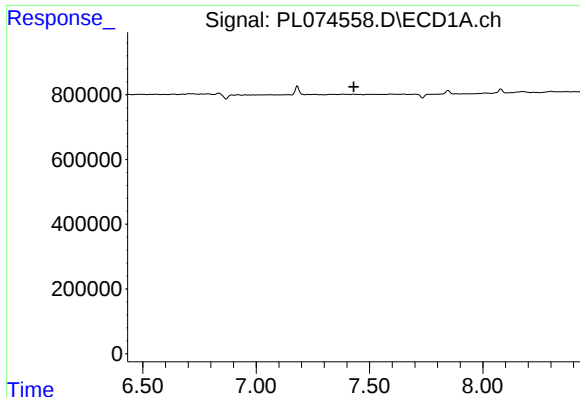

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

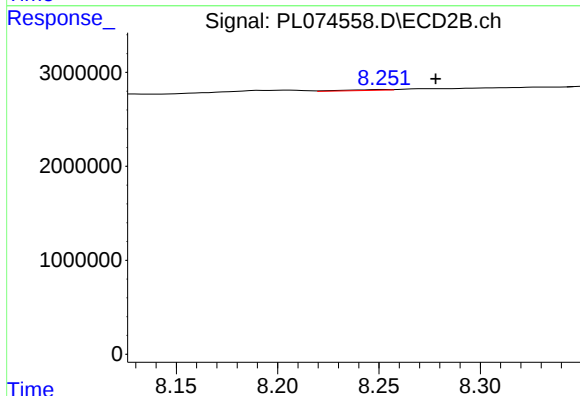


#11 alpha-Chlordane

R.T.: 8.252 min
Delta R.T.: -0.025 min
Response: 134830
Conc: 0.06 ng/ml

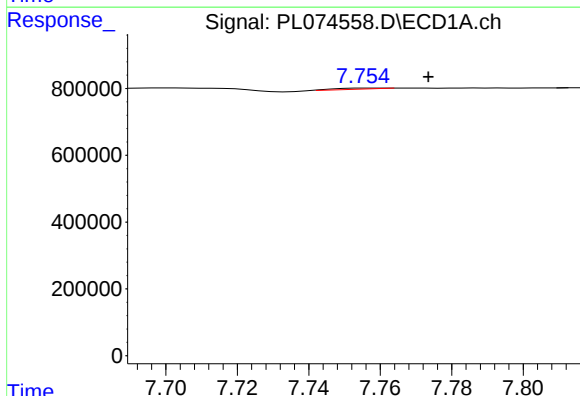


#13 Dieldrin

R.T.: 7.757 min
Delta R.T.: -0.016 min
Response: 27321
Conc: 0.06 ng/ml

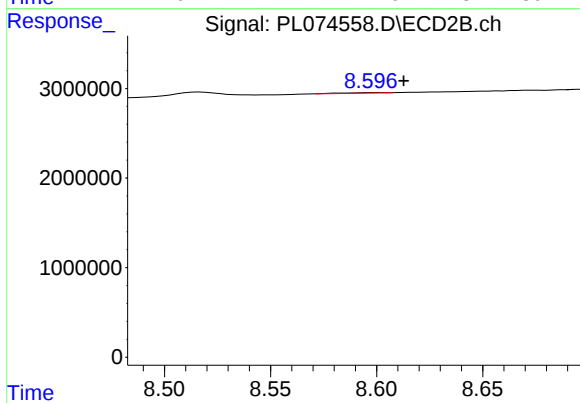

#13 Dieldrin


R.T.: 8.600 min
Delta R.T.: -0.013 min
Response: 70487
Conc: 0.04 ng/ml

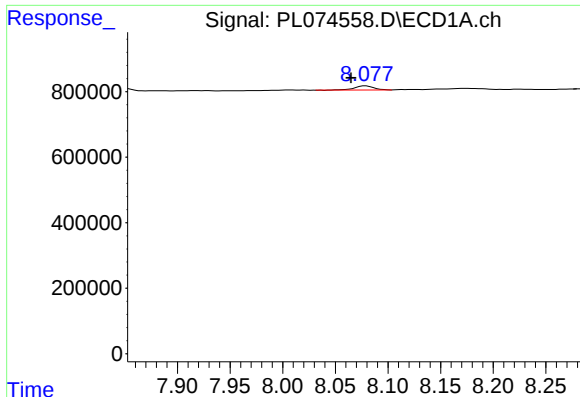

#14 Endrin


R.T.: 8.079 min
Delta R.T.: 0.014 min
Response: 159407
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

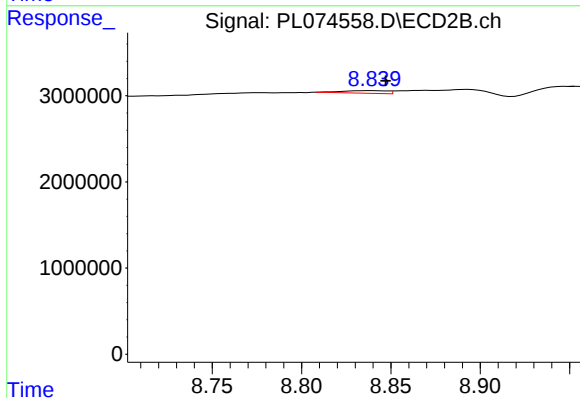


#14 Endrin

R.T.: 8.840 min
Delta R.T.: -0.007 min
Response: 555400
Conc: 0.33 ng/ml

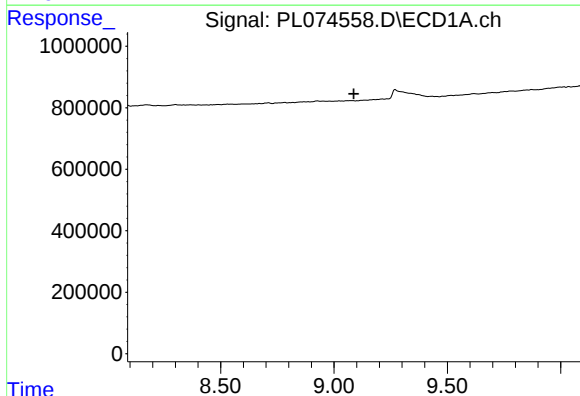


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.087 min
Response: 0
Conc: N.D.

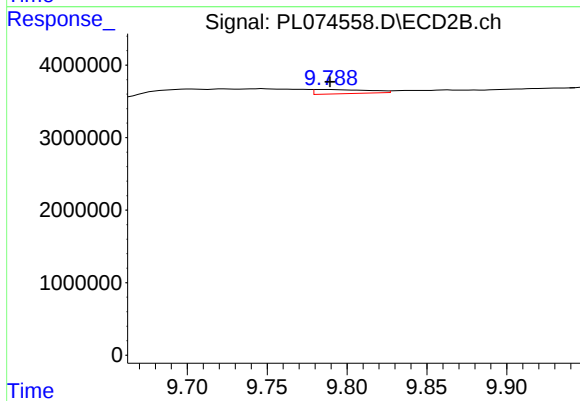

#20 Methoxychlor


R.T.: 9.789 min
Delta R.T.: 0.000 min
Response: 1372970
Conc: 1.43 ng/ml

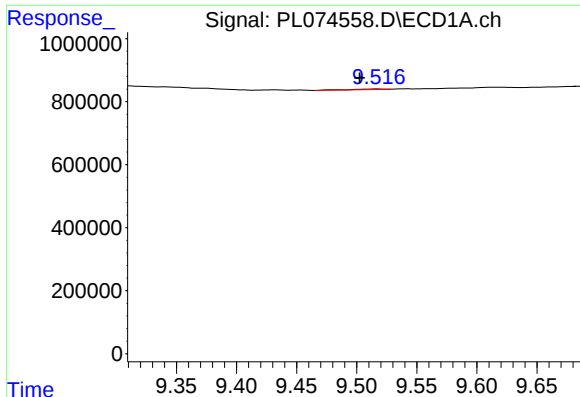

#22 Mirex


R.T.: 9.518 min
Delta R.T.: 0.016 min
Response: 39700
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

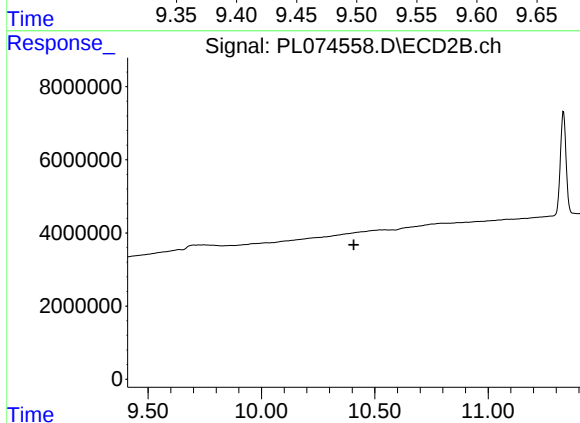


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.407 min
Response: 0
Conc: N.D.

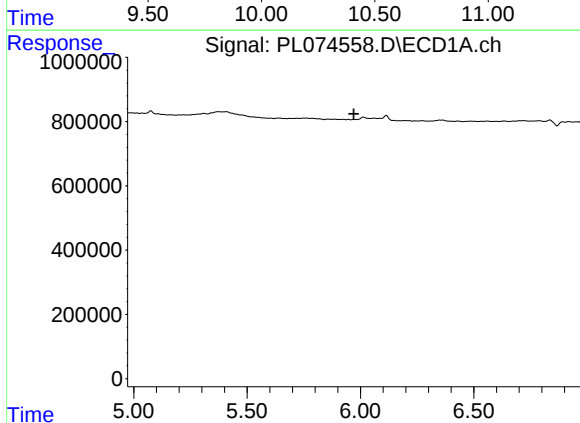


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.970 min
Response: 0
Conc: N.D.

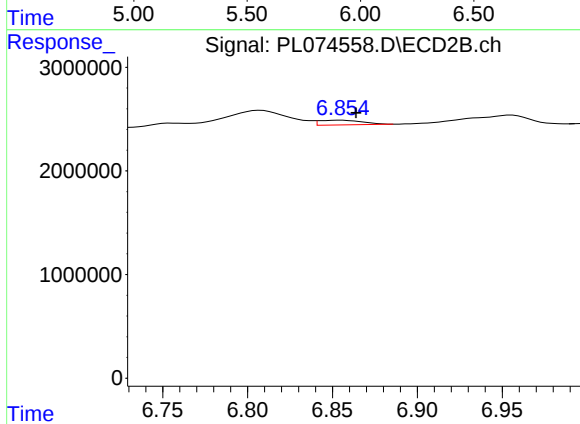

#23 Chlordane-1


R.T.: 6.856 min
Delta R.T.: -0.008 min
Response: 796090
Conc: 9.98 ng/ml

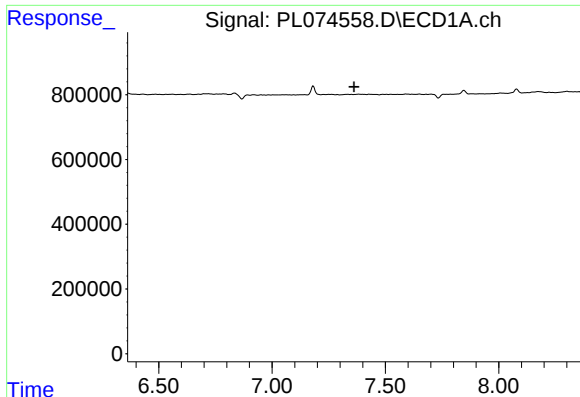

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

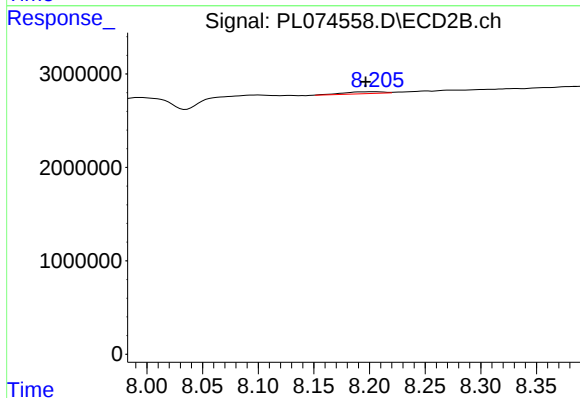


#25 Chlordane-3

R.T.: 8.206 min
Delta R.T.: 0.009 min
Response: 505082
Conc: 1.49 ng/ml

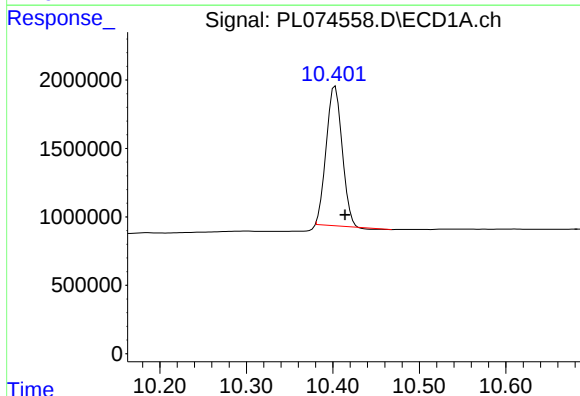

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.011 min
Response: 12955009
Conc: 24.91 ng/ml

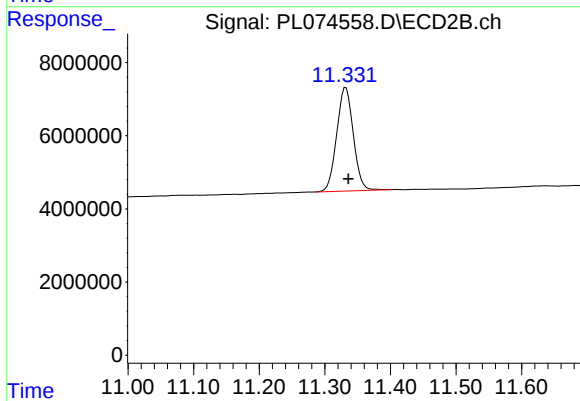

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: -0.004 min
Response: 49884835
Conc: 28.24 ng/ml