

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050522\
 Data File : PL074568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2022 23:03
 Operator : AR\AJ
 Sample : N2703-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 01:19:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.489	3664068	18163947	11.340	10.187
28)	SA Decachlor...	10.405	11.332	5831793	19485259	11.214	11.032
Target Compounds							
2)	A alpha-BHC	5.372f	0.000	47464	0	0.113	N.D. #
6)	B beta-BHC	0.000	6.680	0	515997	N.D.	0.458 #
7)	B delta-BHC	0.000	6.957	0	2744468	N.D.	1.124 #
10)	B gamma-Chl...	7.381f	8.198	76931	500520	0.175	0.224 #
11)	B alpha-Chl...	0.000	8.282	0	477823	N.D.	0.222 #
17)	MA 4,4'-DDT	0.000	9.318	0	53271	N.D.	0.030 #
19)	B Endosulfa...	0.000	9.471f	0	139658	N.D.	0.084 #
20)	A Methoxychlor	0.000	9.773f	0	27338	N.D.	0.028 #
23)	Chlordane-1	0.000	6.853	0	956488	N.D.	11.986 #
25)	Chlordane-3	7.381f	8.198	76931	500520	1.778	1.480
26)	Chlordane-4	0.000	8.282	0	477823	N.D.	1.205 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050522\
Data File : PL074568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2022 23:03
Operator : AR\AJ
Sample : N2703-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 01:19:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

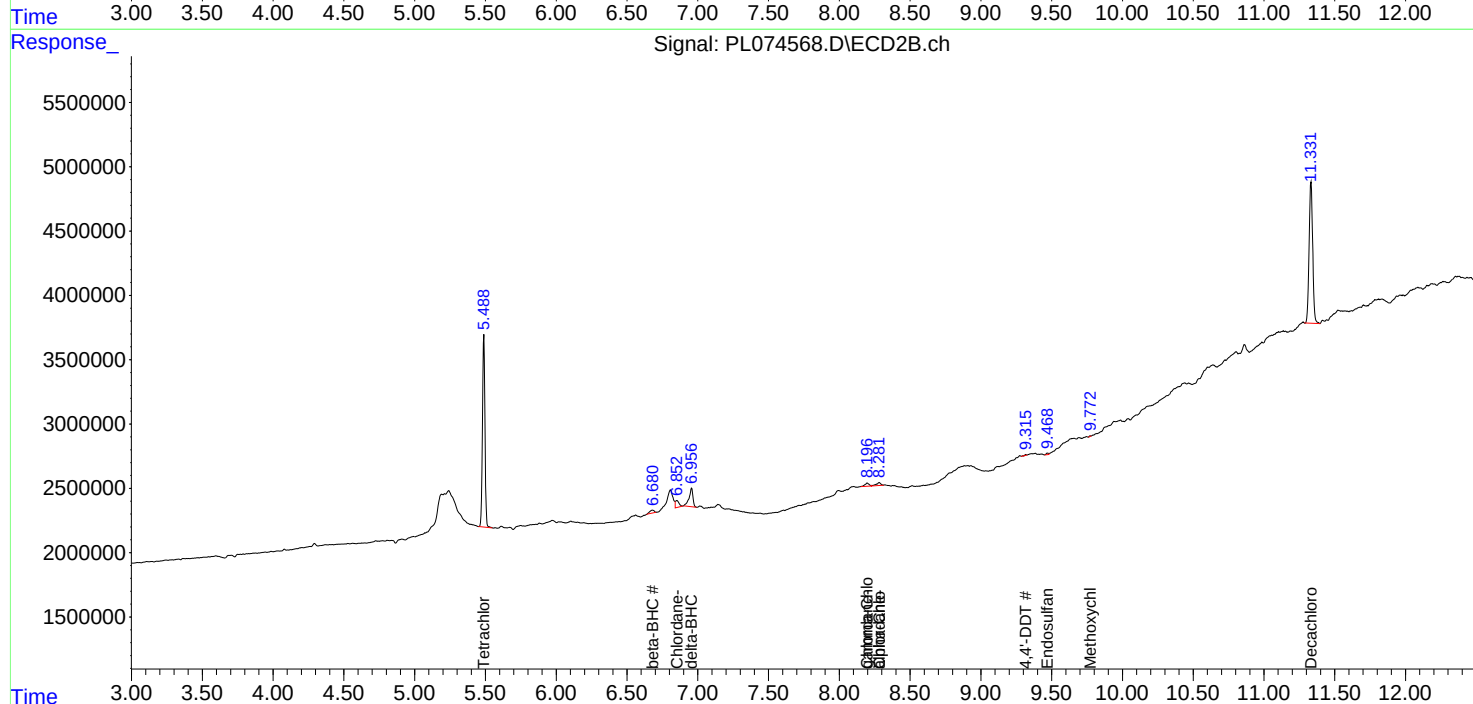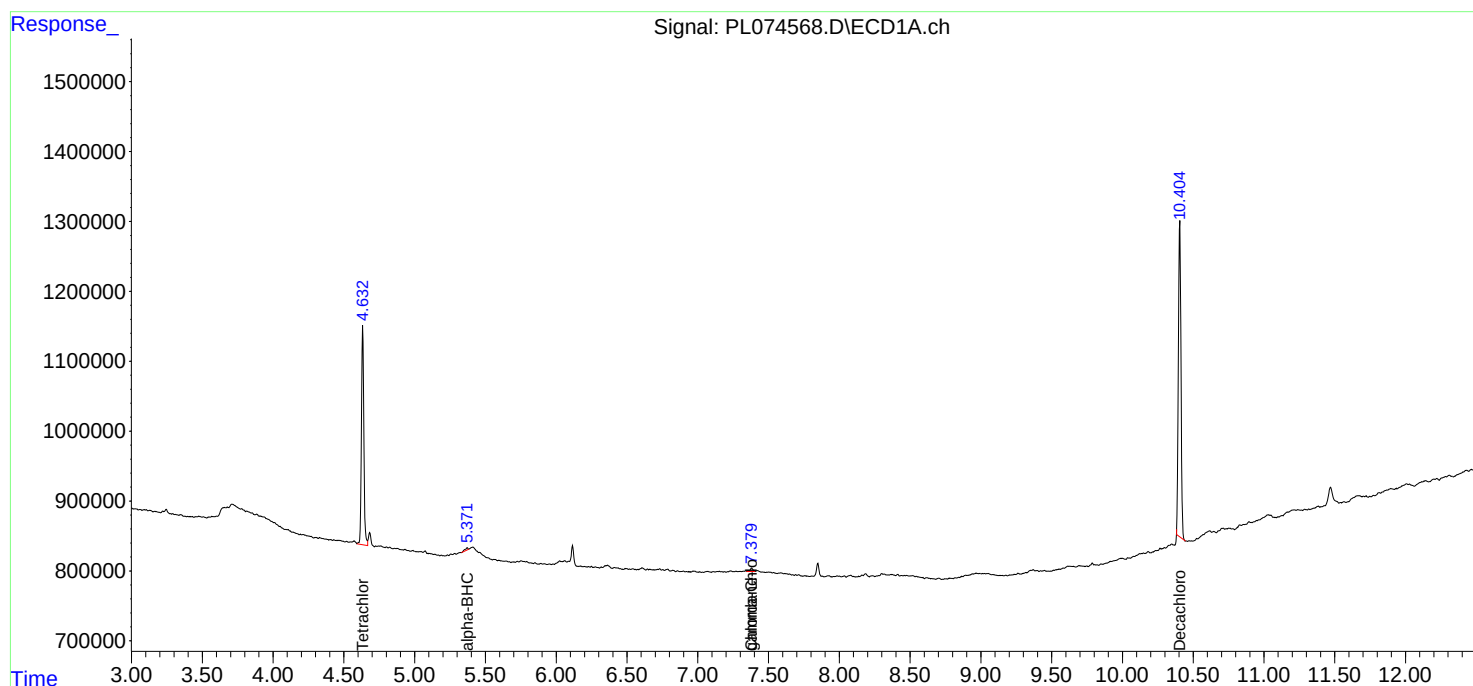


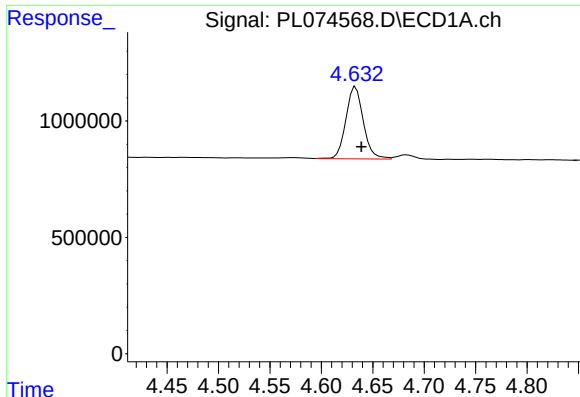

#1 Tetrachloro-m-xylene


R.T.: 4.633 min
Delta R.T.: -0.006 min
Response: 3664068
Conc: 11.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

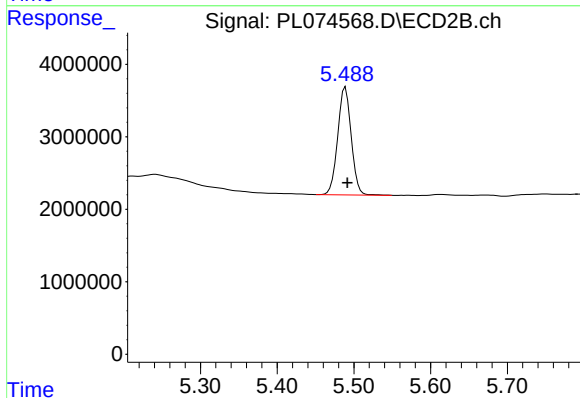


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 18163947
Conc: 10.19 ng/ml

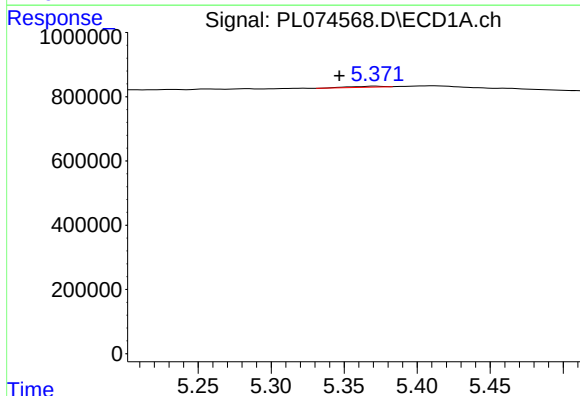


#2 alpha-BHC

R.T.: 5.372 min
Delta R.T.: 0.025 min
Response: 47464
Conc: 0.11 ng/ml

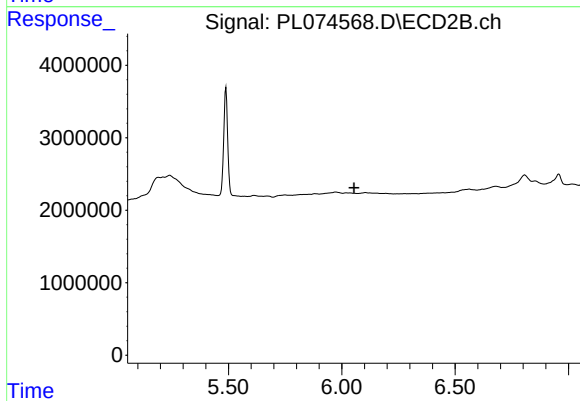

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

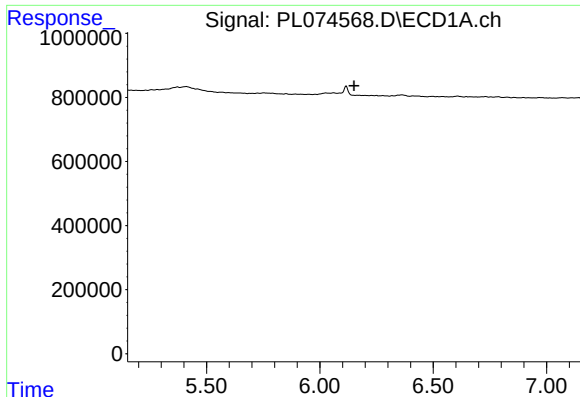

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

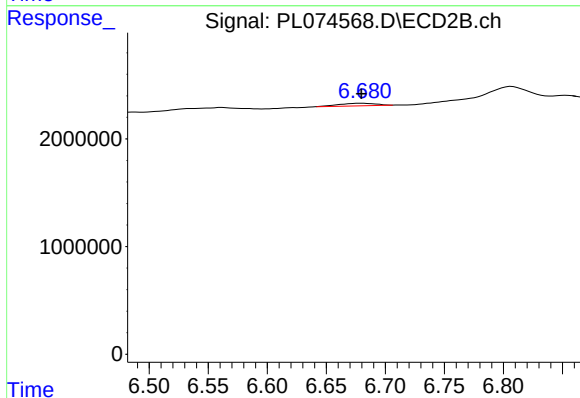


#6 beta-BHC

R.T.: 6.680 min
Delta R.T.: 0.000 min
Response: 515997
Conc: 0.46 ng/ml

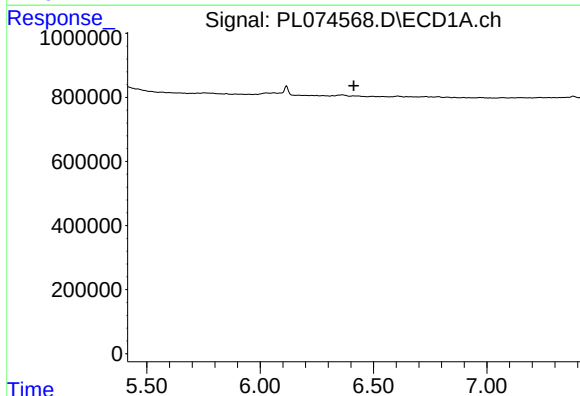


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

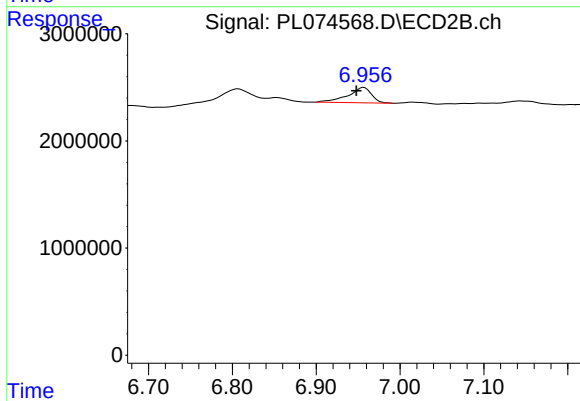

#7 delta-BHC


R.T.: 6.957 min
Delta R.T.: 0.009 min
Response: 2744468
Conc: 1.12 ng/ml

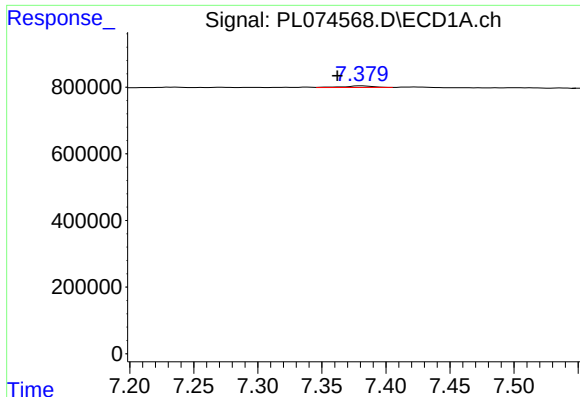

#10 gamma-Chlordane


R.T.: 7.381 min
Delta R.T.: 0.019 min
Response: 76931
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

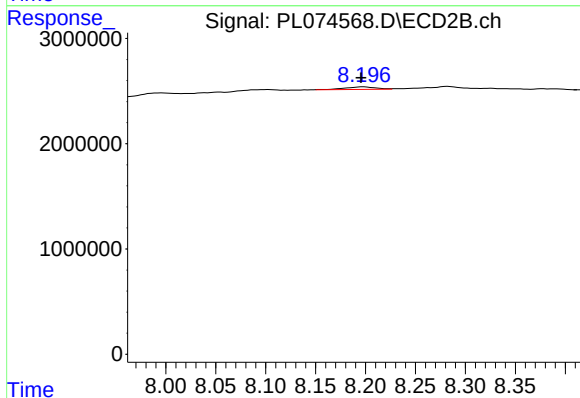


#10 gamma-Chlordane

R.T.: 8.198 min
Delta R.T.: 0.002 min
Response: 500520
Conc: 0.22 ng/ml

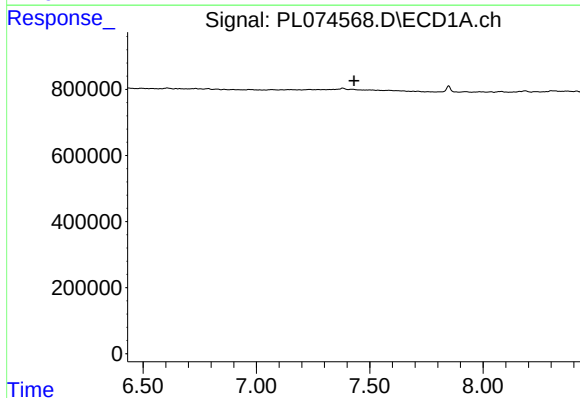


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.431 min
Response: 0
Conc: N.D.

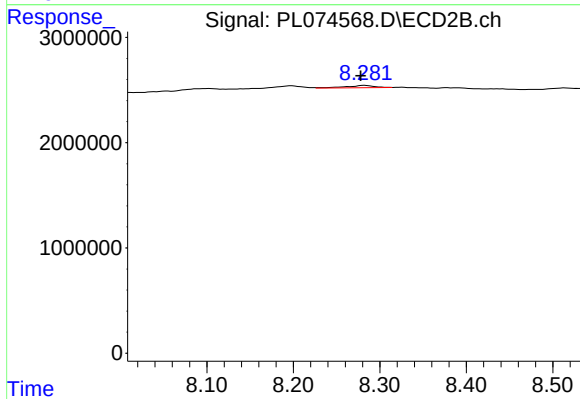

#11 alpha-Chlordane


R.T.: 8.282 min
Delta R.T.: 0.004 min
Response: 477823
Conc: 0.22 ng/ml

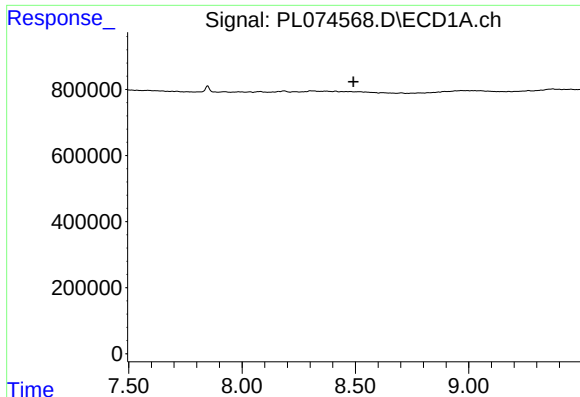

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

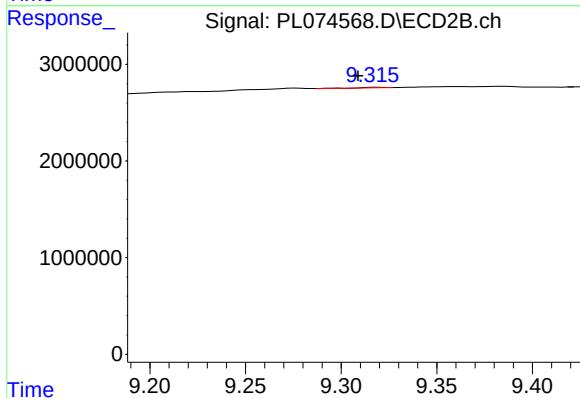


#17 4,4'-DDT

R.T.: 9.318 min
Delta R.T.: 0.009 min
Response: 53271
Conc: 0.03 ng/ml

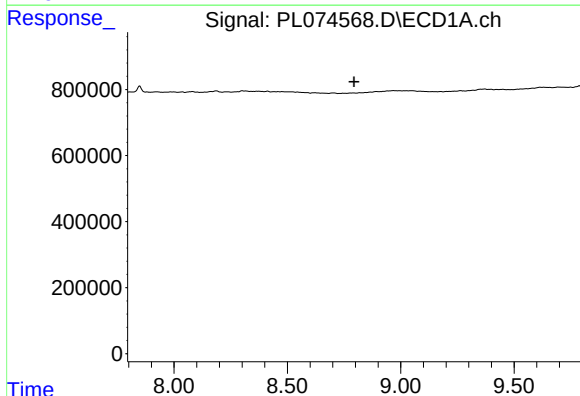


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

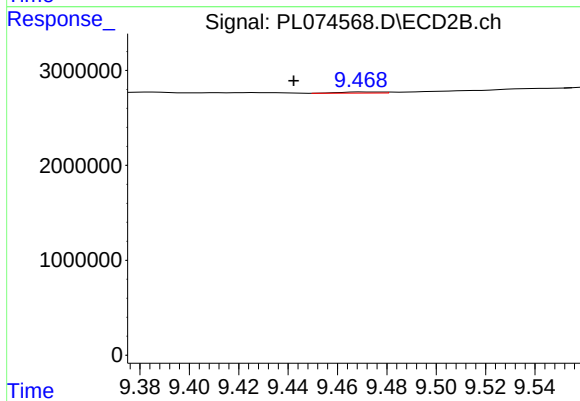

#19 Endosulfan Sulfate


R.T.: 9.471 min
Delta R.T.: 0.028 min
Response: 139658
Conc: 0.08 ng/ml

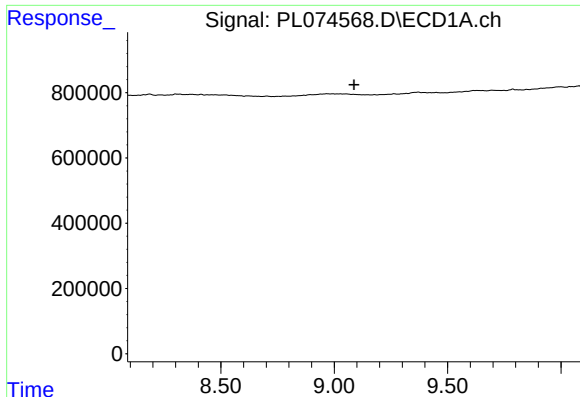

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

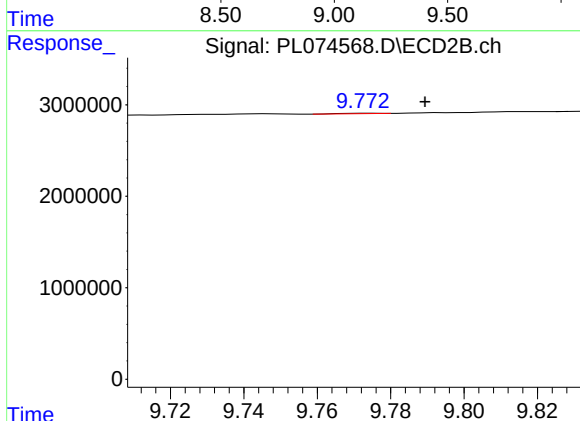


#20 Methoxychlor

R.T.: 9.773 min
Delta R.T.: -0.016 min
Response: 27338
Conc: 0.03 ng/ml

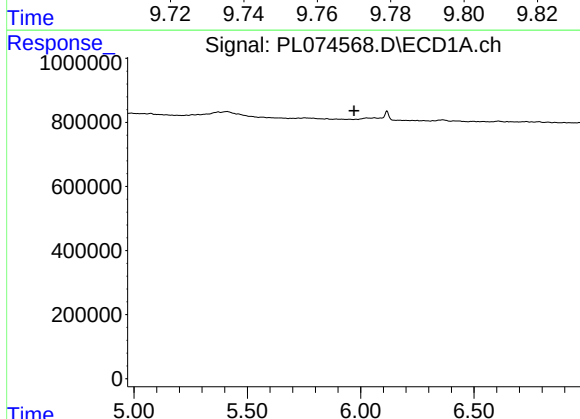


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.970 min
Response: 0
Conc: N.D.

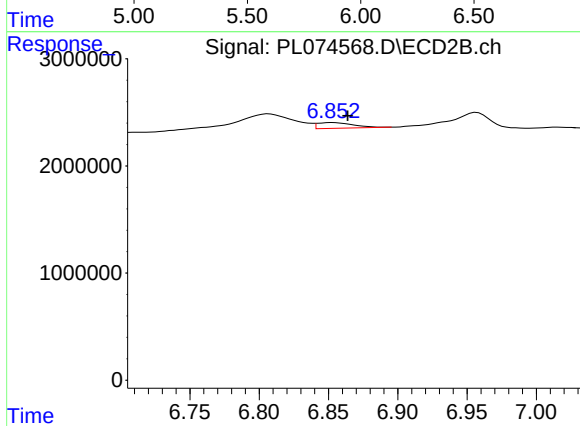

#23 Chlordane-1


R.T.: 6.853 min
Delta R.T.: -0.011 min
Response: 956488
Conc: 11.99 ng/ml

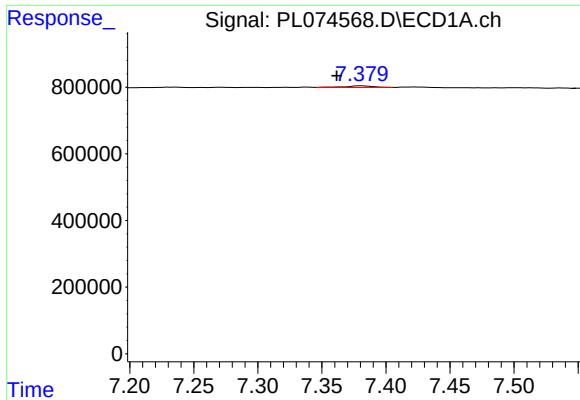

#25 Chlordane-3


R.T.: 7.381 min
Delta R.T.: 0.019 min
Response: 76931
Conc: 1.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

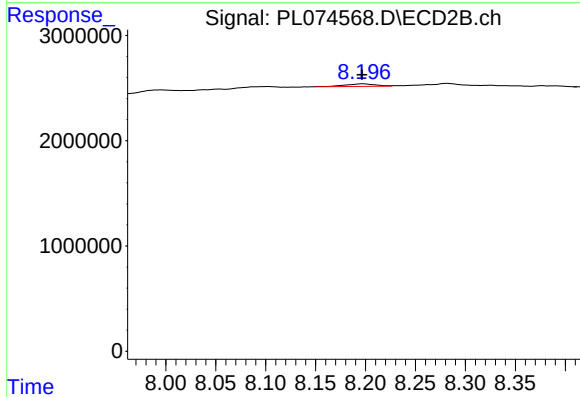


#25 Chlordane-3

R.T.: 8.198 min
Delta R.T.: 0.001 min
Response: 500520
Conc: 1.48 ng/ml

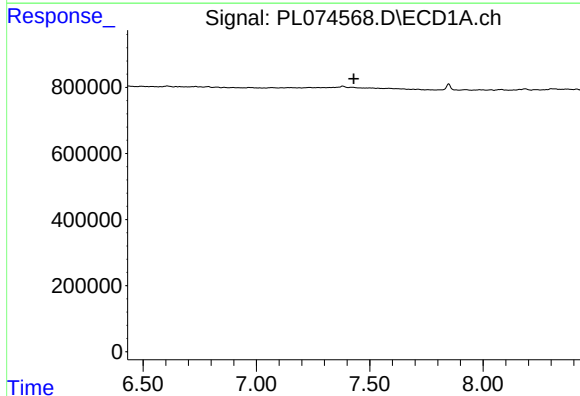


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

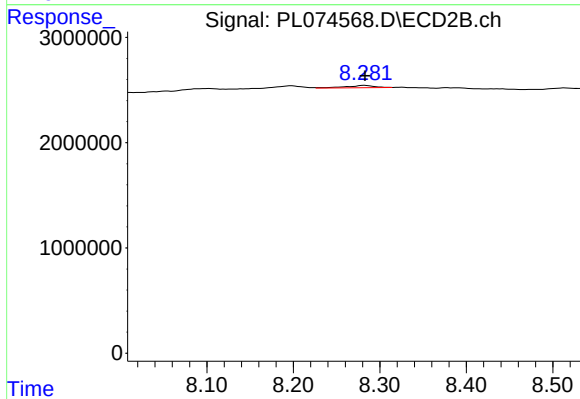

#26 Chlordane-4


R.T.: 8.282 min
Delta R.T.: 0.000 min
Response: 477823
Conc: 1.20 ng/ml

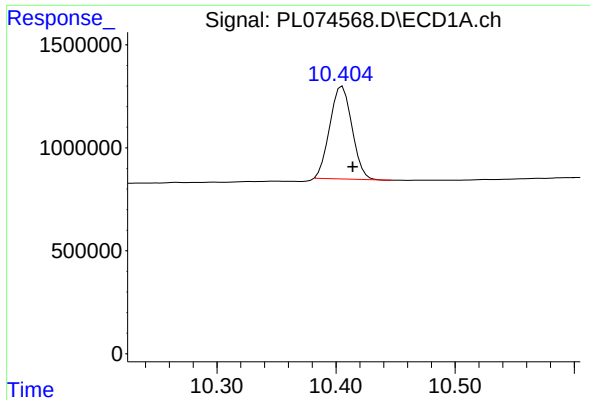

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.009 min
Response: 5831793
Conc: 11.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

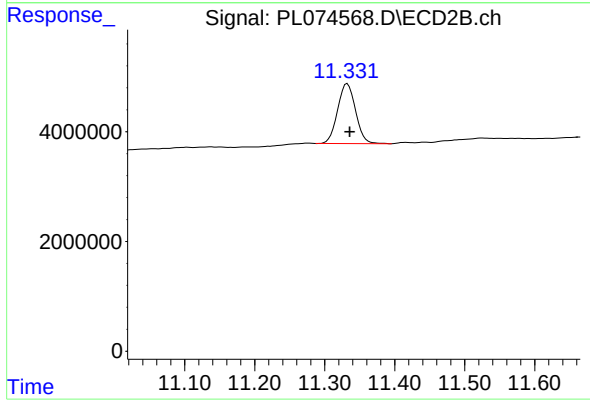

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: -0.004 min
Response: 19485259
Conc: 11.03 ng/ml