

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050522\
 Data File : PL074571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2022 23:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 01:20:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.489	8878307	47589564	27.478	26.691
28)	SA Decachlor...	10.405	11.332	12535430	43565875	24.105	24.665
Target Compounds							
6)	B beta-BHC	0.000	6.673	0	681291	N.D.	0.605 #
7)	B delta-BHC	0.000	6.955	0	1942836	N.D.	0.796 #
8)	B Heptachlo...	0.000	7.926	0	1632577	N.D.	0.725 #
9)	A Endosulfan I	0.000	8.324	0	22	N.D.	0.000 #
10)	B gamma-Chl...	0.000	8.197	0	267058	N.D.	0.120 #
11)	B alpha-Chl...	0.000	8.270	0	42220	N.D.	0.020 #
13)	MA Dieldrin	7.769	0.000	151338	0	0.352	N.D. #
14)	MA Endrin	8.081f	8.842	177549	640760	0.437	0.378
15)	B Endosulfa...	0.000	9.055f	0	3666754	N.D.	2.111 #
20)	A Methoxychlor	0.000	9.797	0	58402	N.D.	0.061 #
22)	Mirex	0.000	10.388f	0	52510	N.D.	0.038 #
23)	Chlordane-1	0.000	6.854	0	1047440	N.D.	13.126 #
25)	Chlordane-3	0.000	8.197	0	267058	N.D.	0.789 #
26)	Chlordane-4	0.000	8.270	0	42220	N.D.	0.106 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050522\
Data File : PL074571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2022 23:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 01:20:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

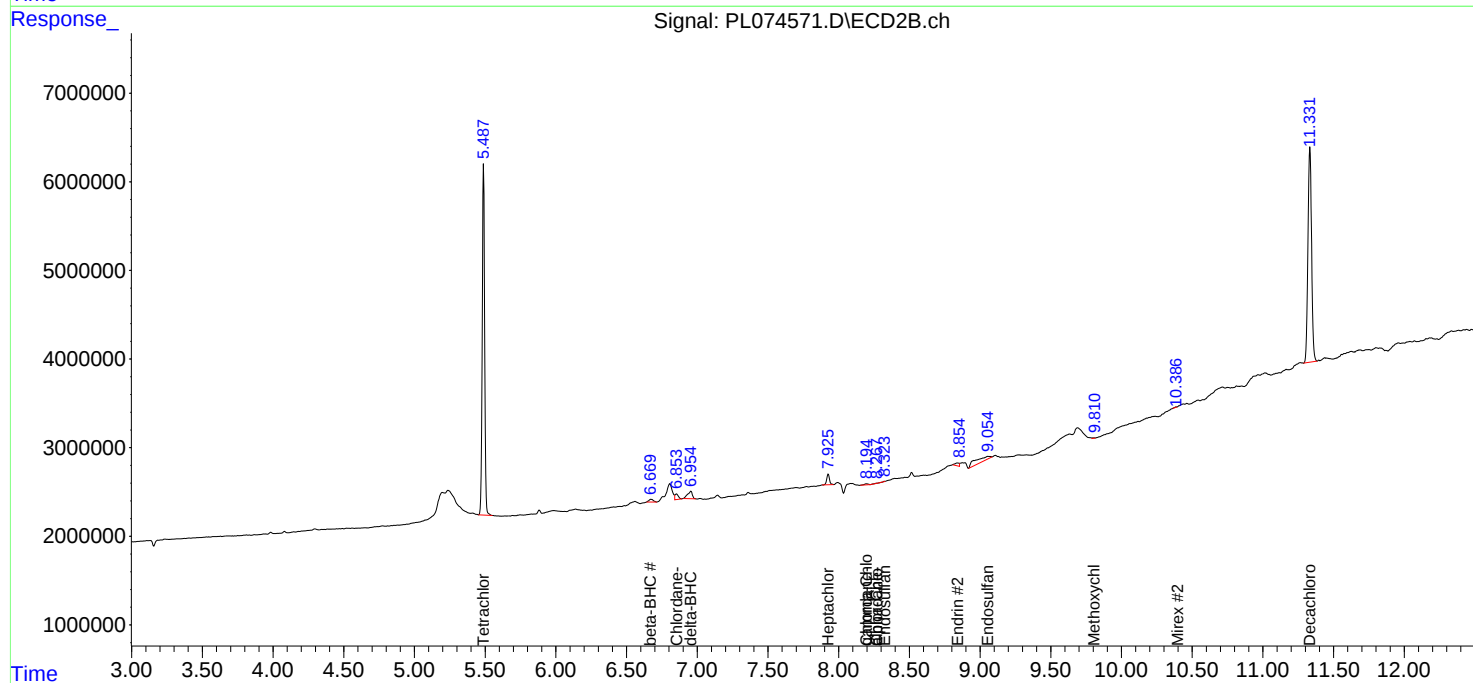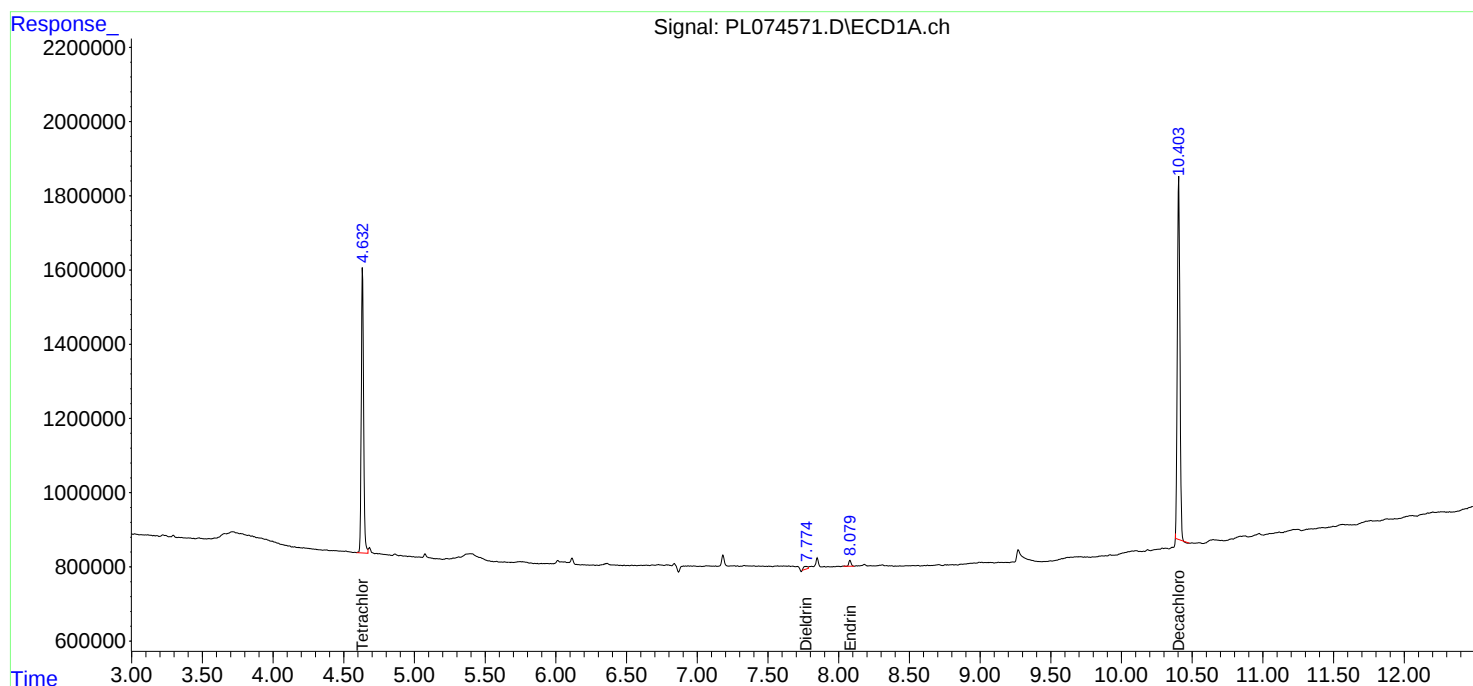


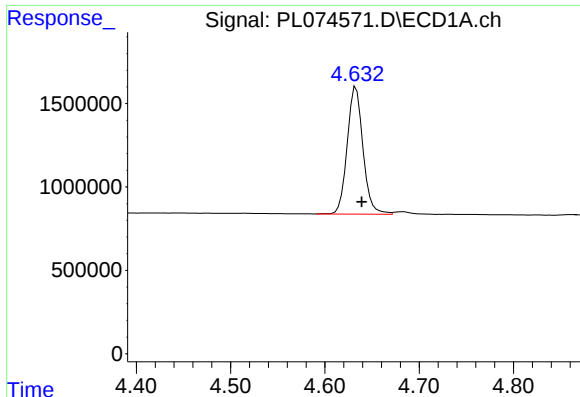

#1 Tetrachloro-m-xylene


R.T.: 4.633 min
Delta R.T.: -0.006 min
Response: 8878307
Conc: 27.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

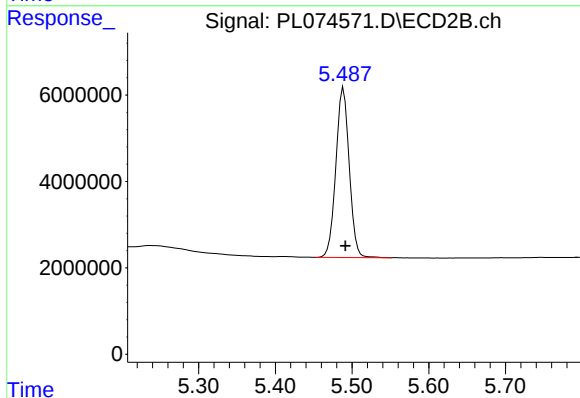


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.003 min
Response: 47589564
Conc: 26.69 ng/ml

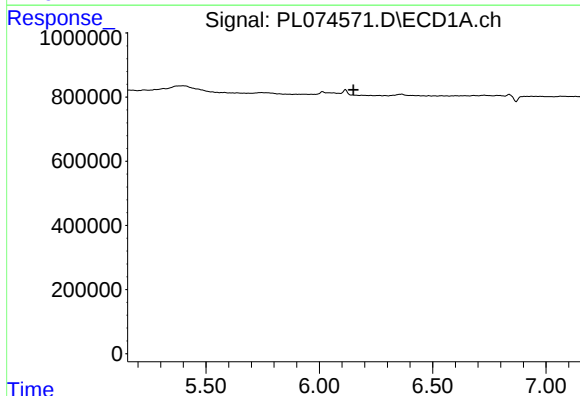


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.151 min
Response: 0
Conc: N.D.

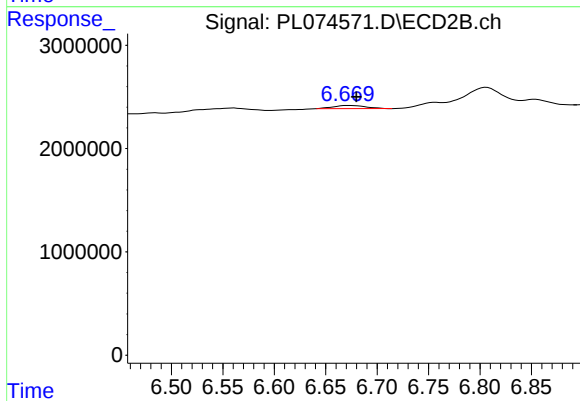

#6 beta-BHC


R.T.: 6.673 min
Delta R.T.: -0.007 min
Response: 681291
Conc: 0.60 ng/ml

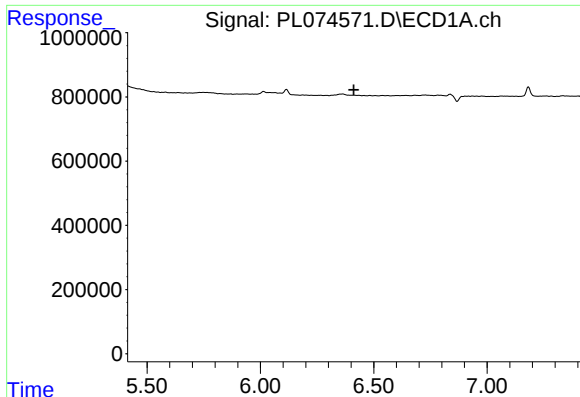

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

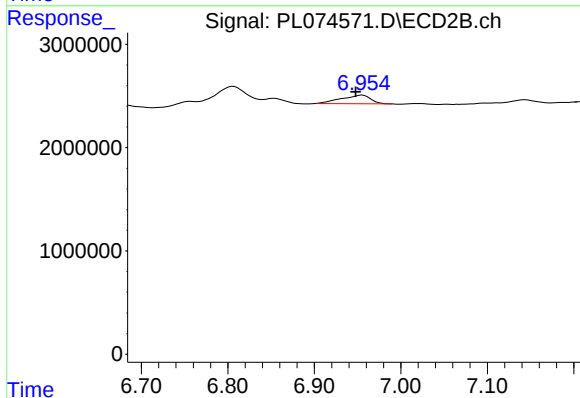


#7 delta-BHC

R.T.: 6.955 min
Delta R.T.: 0.007 min
Response: 1942836
Conc: 0.80 ng/ml

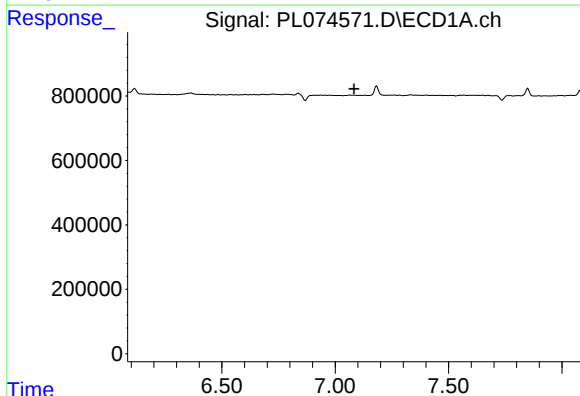


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.084 min
Response: 0
Conc: N.D.

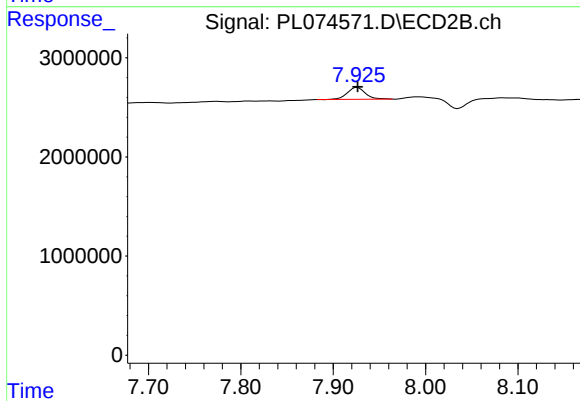

#8 Heptachlor epoxide


R.T.: 7.926 min
Delta R.T.: 0.000 min
Response: 1632577
Conc: 0.73 ng/ml

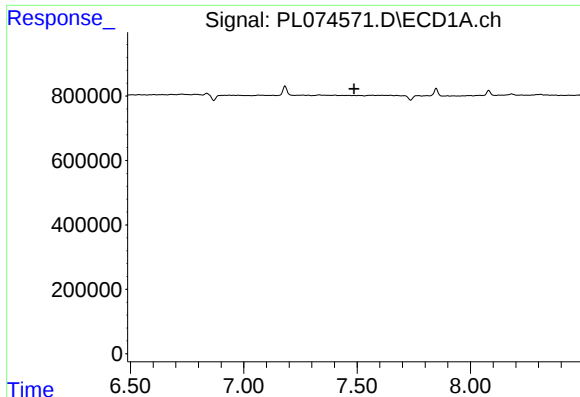

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

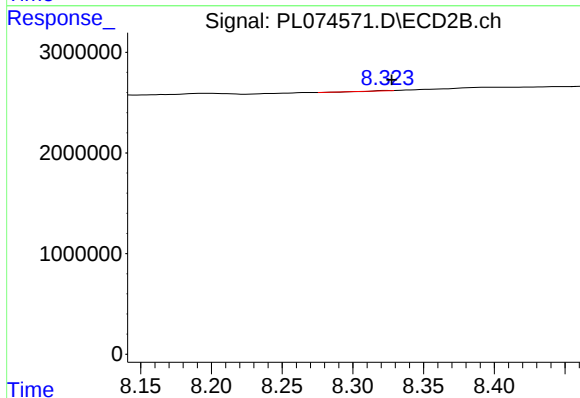


#9 Endosulfan I

R.T.: 8.324 min
Delta R.T.: -0.004 min
Response: 22
Conc: 0.00 ng/ml

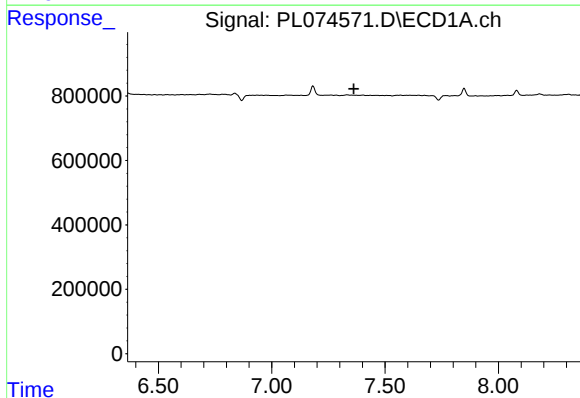


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

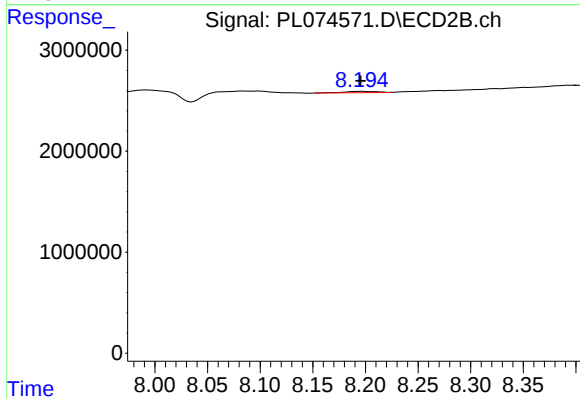

#10 gamma-Chlordane


R.T.: 8.197 min
Delta R.T.: 0.002 min
Response: 267058
Conc: 0.12 ng/ml

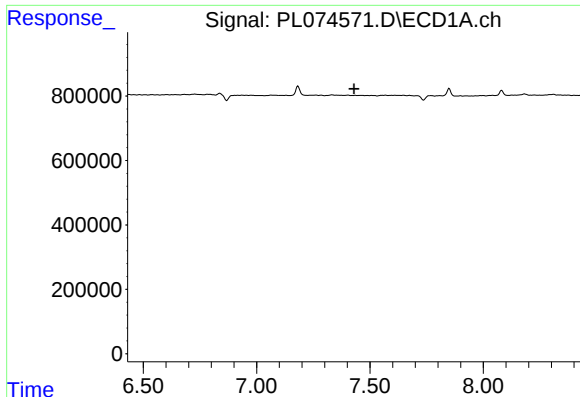

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

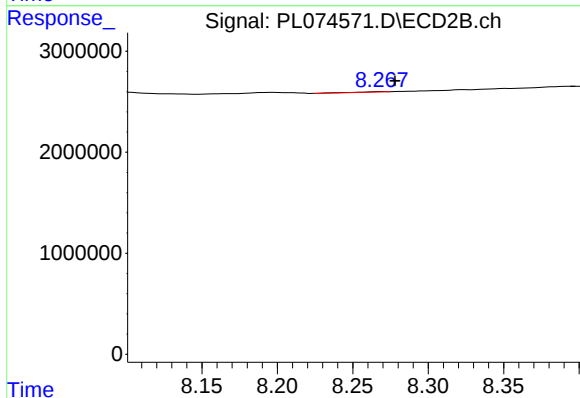


#11 alpha-Chlordane

R.T.: 8.270 min
Delta R.T.: -0.008 min
Response: 42220
Conc: 0.02 ng/ml

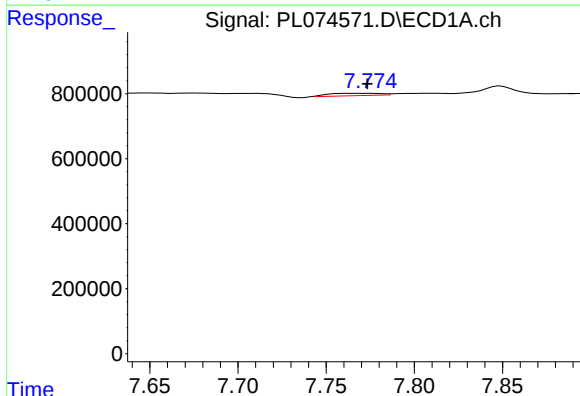


#13 Dieldrin

R.T.: 7.769 min
Delta R.T.: -0.005 min
Response: 151338
Conc: 0.35 ng/ml

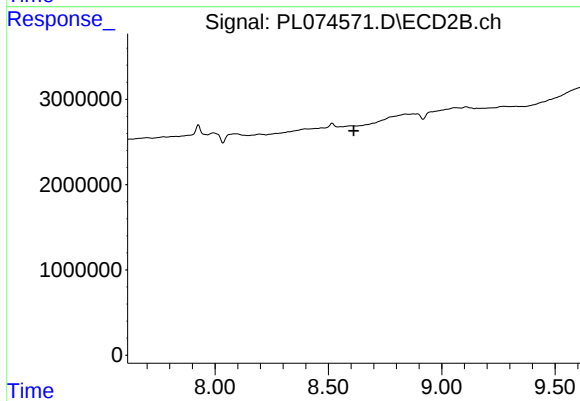

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.613 min
Response: 0
Conc: N.D.

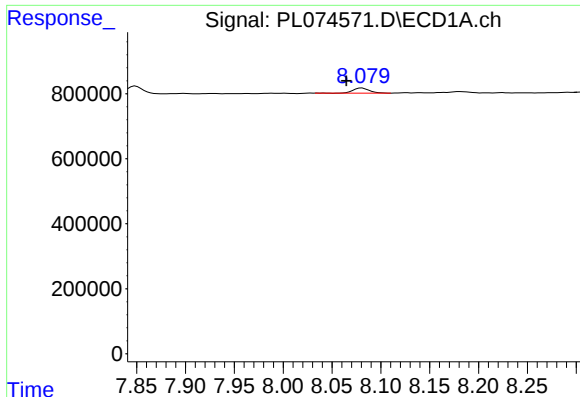

#14 Endrin


R.T.: 8.081 min
Delta R.T.: 0.016 min
Response: 177549
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

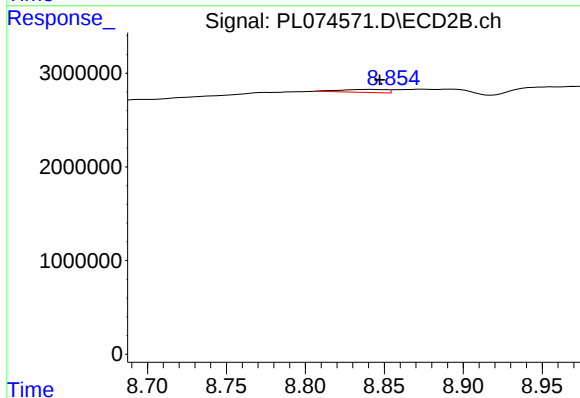


#14 Endrin

R.T.: 8.842 min
Delta R.T.: -0.005 min
Response: 640760
Conc: 0.38 ng/ml

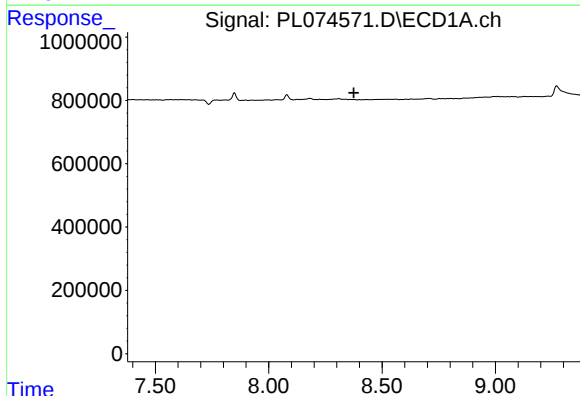


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

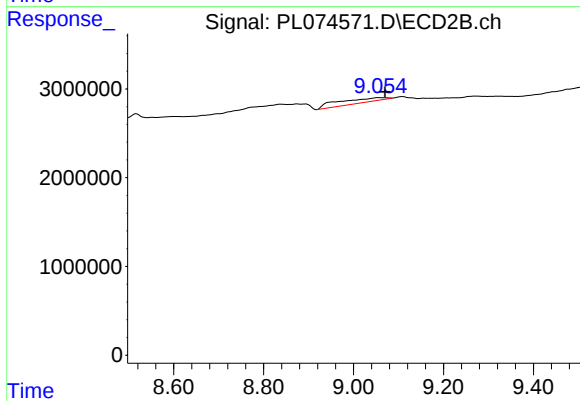

#15 Endosulfan II


R.T.: 9.055 min
Delta R.T.: -0.015 min
Response: 3666754
Conc: 2.11 ng/ml

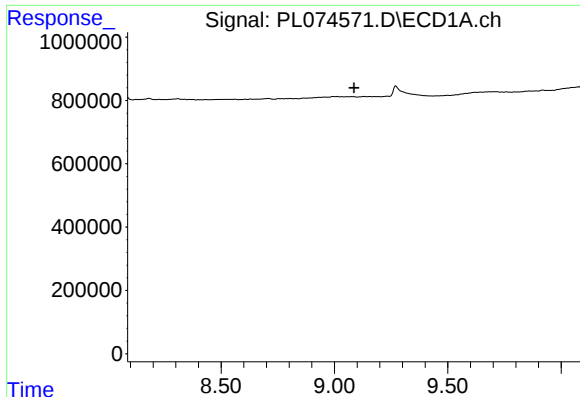

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

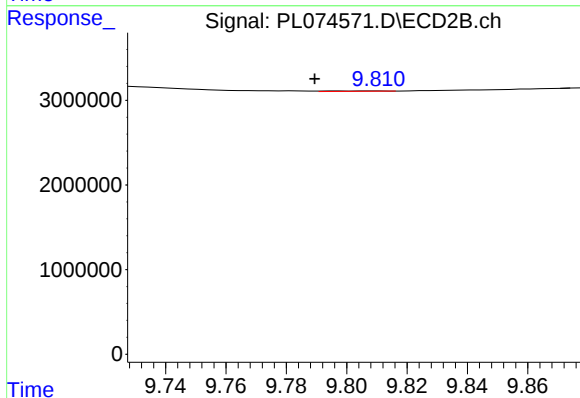


#20 Methoxychlor

R.T.: 9.797 min
Delta R.T.: 0.008 min
Response: 58402
Conc: 0.06 ng/ml

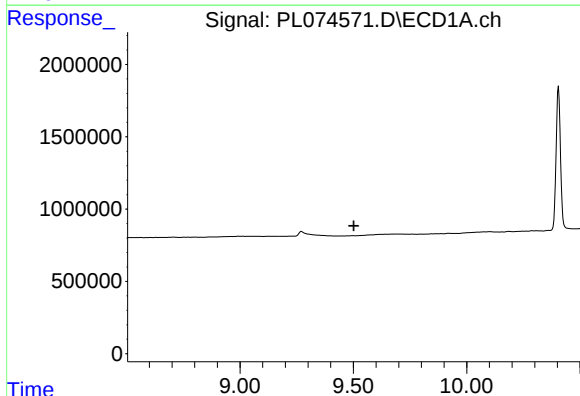


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

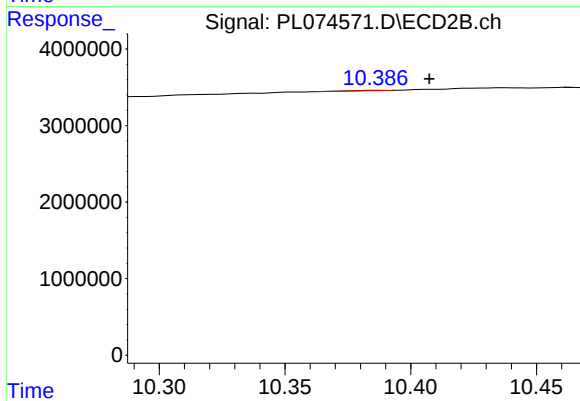

#22 Mirex


R.T.: 10.388 min
Delta R.T.: -0.020 min
Response: 52510
Conc: 0.04 ng/ml

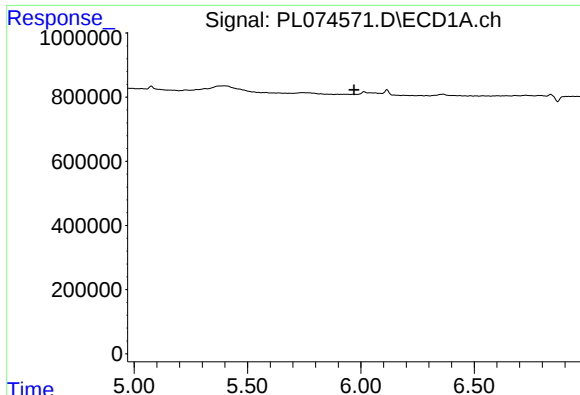

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

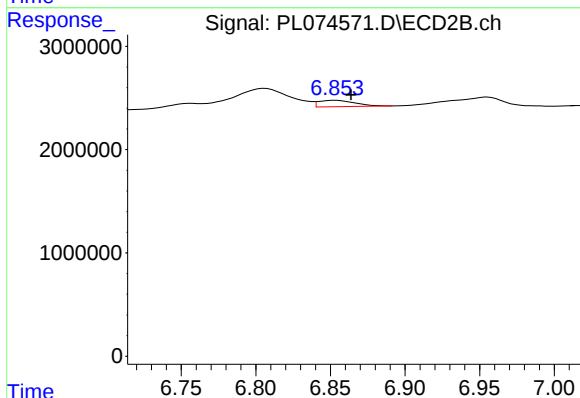


#23 Chlordane-1

R.T.: 6.854 min
Delta R.T.: -0.010 min
Response: 1047440
Conc: 13.13 ng/ml

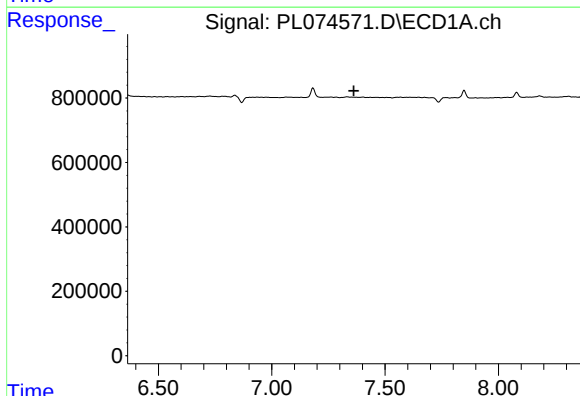


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

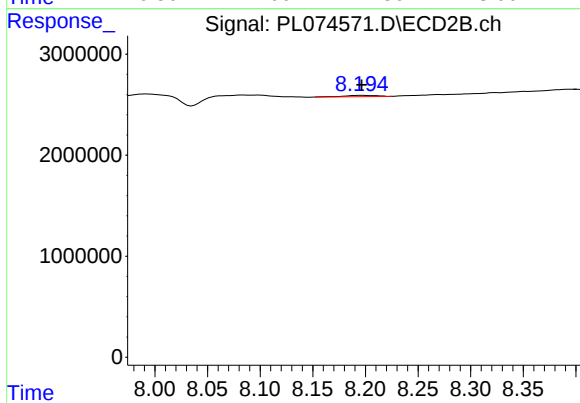

#25 Chlordane-3


R.T.: 8.197 min
Delta R.T.: 0.000 min
Response: 267058
Conc: 0.79 ng/ml

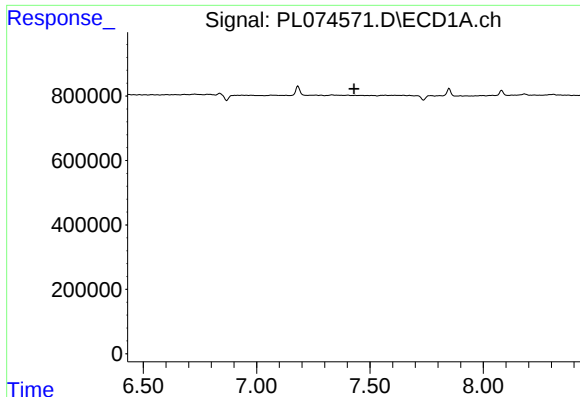

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

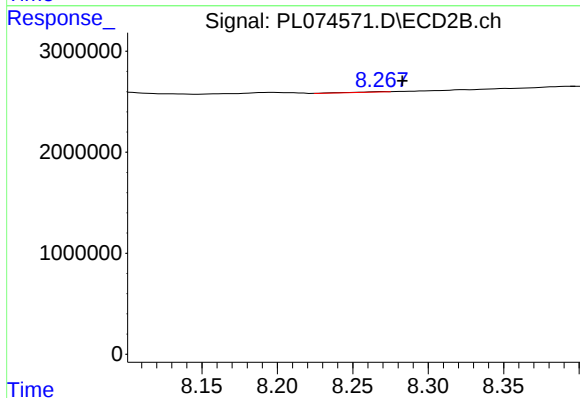


#26 Chlordane-4

R.T.: 8.270 min
Delta R.T.: -0.013 min
Response: 42220
Conc: 0.11 ng/ml

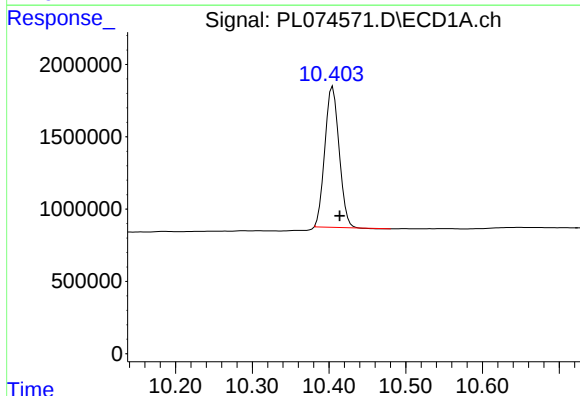

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.009 min
Response: 12535430
Conc: 24.11 ng/ml

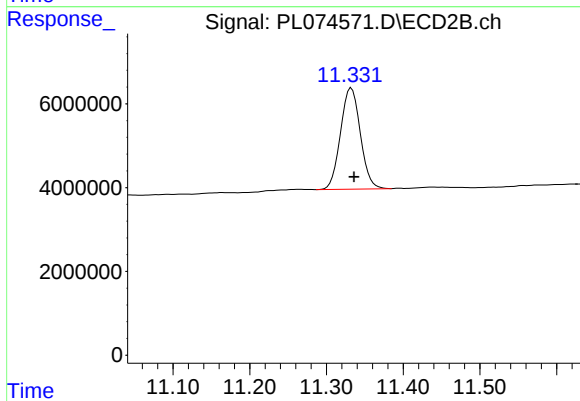

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: -0.004 min
Response: 43565875
Conc: 24.67 ng/ml