

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050523\
 Data File : PL082537.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 09:15
 Operator : AR\AJ
 Sample : PB152523BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB152523BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 21:09:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.643	50494036	53030129	18.903	22.890
28)	SA Decachlor...	8.741	7.754	42634394	48756608	22.332	21.361
Target Compounds							
23)	Chlordane-1	4.465	3.628	23763778	18964998	214.976	213.847
24)	Chlordane-2	4.992	4.201	27358586	24383914	229.803	217.436
25)	Chlordane-3	5.698	4.828	94083003	58568339	217.934	206.147
26)	Chlordane-4	5.777	4.889	113.1E6	61262095	217.617	205.297
27)	Chlordane-5	6.618	5.781	19942940	21101168	212.390	213.764



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050523\
Data File : PL082537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 09:15
Operator : AR\AJ
Sample : PB152523BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB152523BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 21:09:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

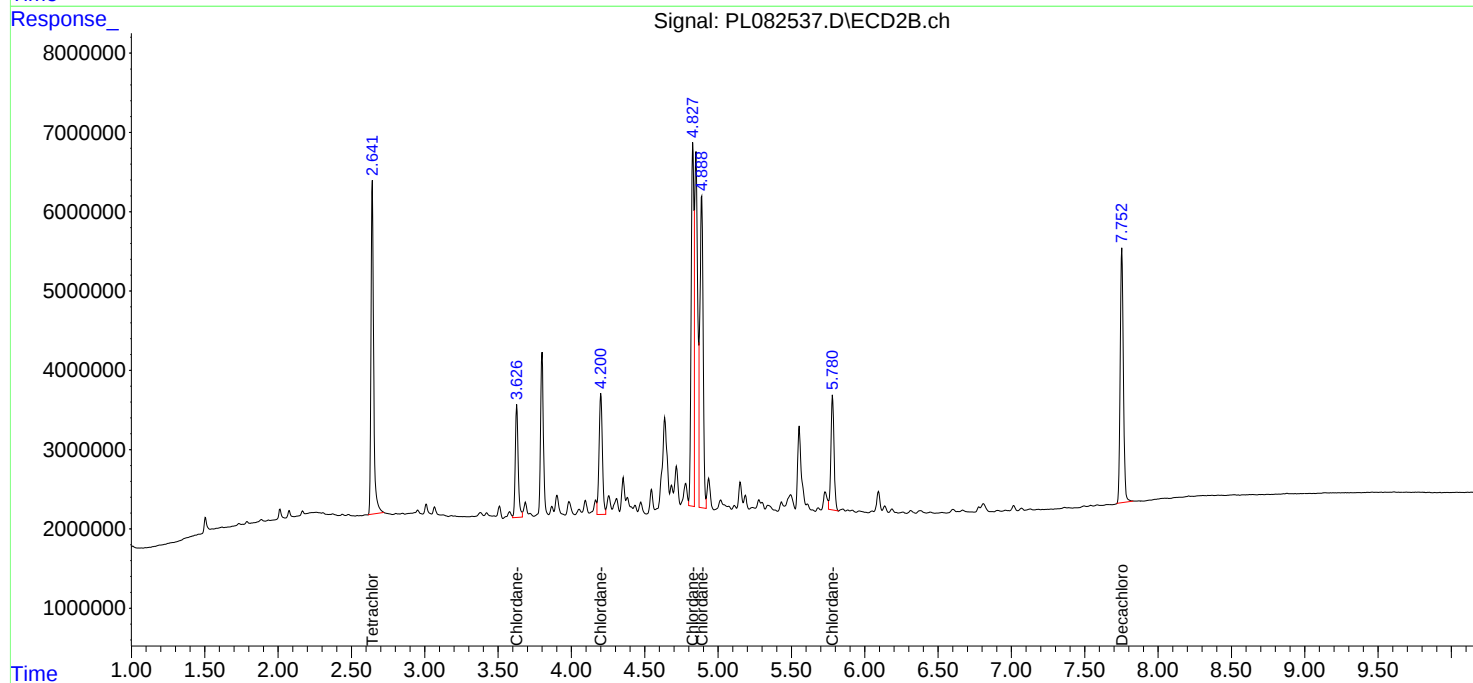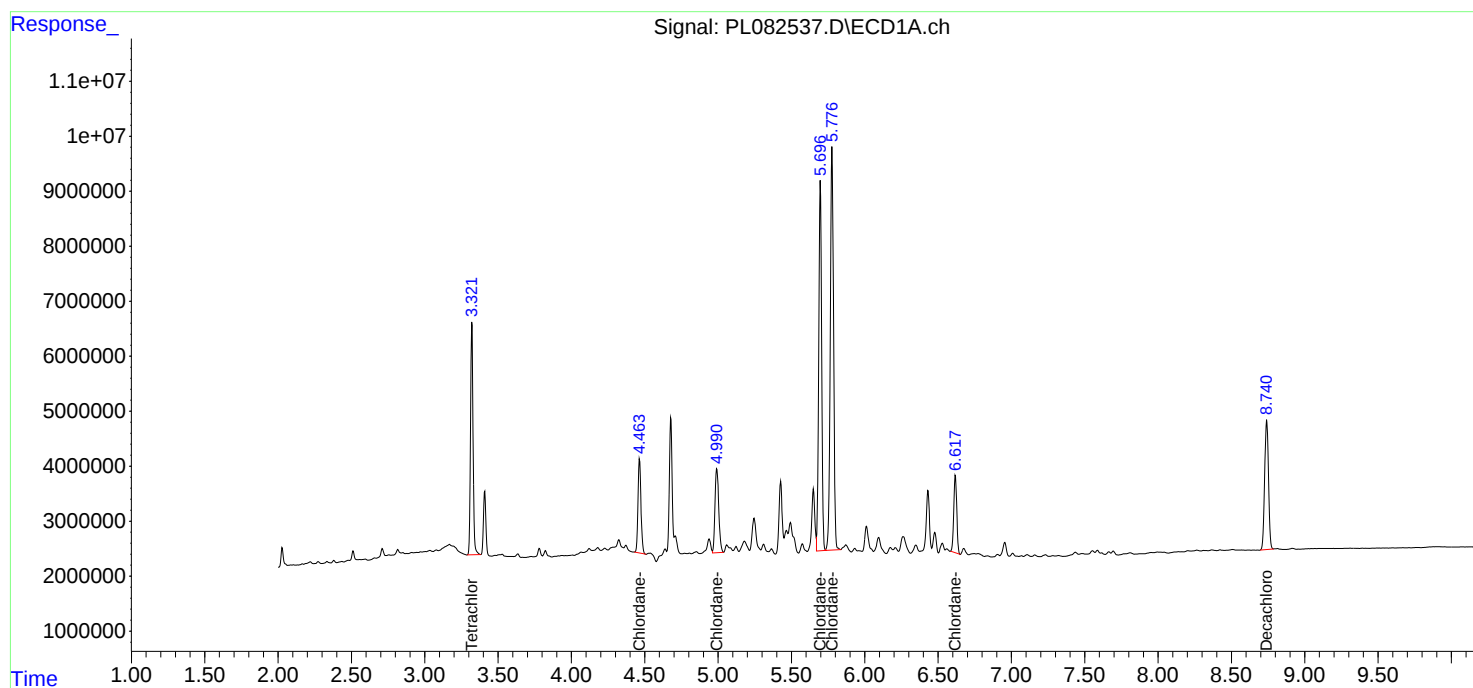


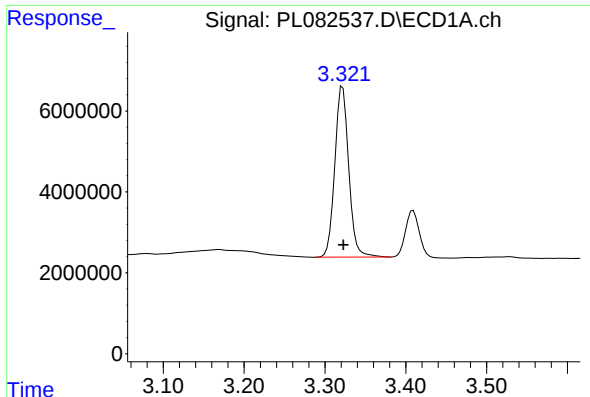

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.001 min
Response: 50494036
Conc: 18.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152523BS

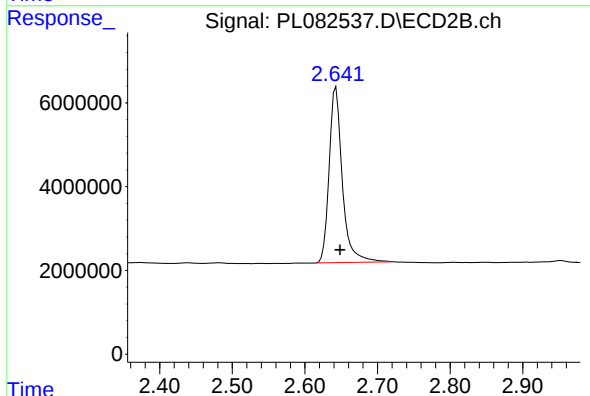


#1 Tetrachloro-m-xylene

R.T.: 2.643 min
Delta R.T.: -0.005 min
Response: 53030129
Conc: 22.89 ng/ml

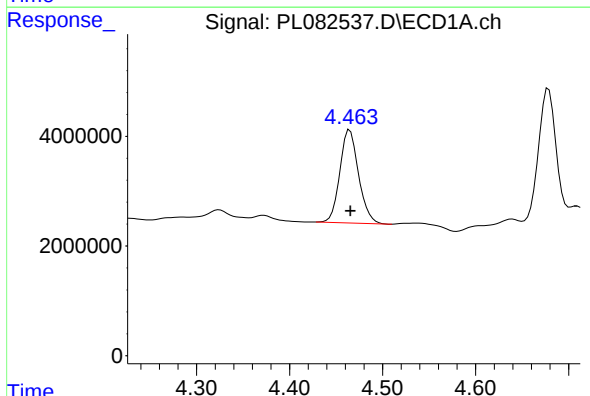


#23 Chlordane-1

R.T.: 4.465 min
Delta R.T.: 0.000 min
Response: 23763778
Conc: 214.98 ng/ml

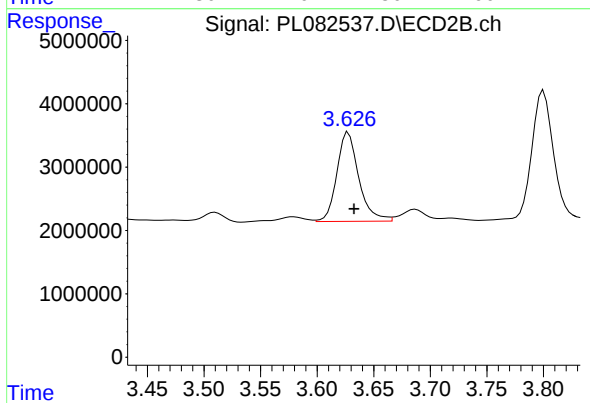

#23 Chlordane-1


R.T.: 3.628 min
Delta R.T.: -0.005 min
Response: 18964998
Conc: 213.85 ng/ml

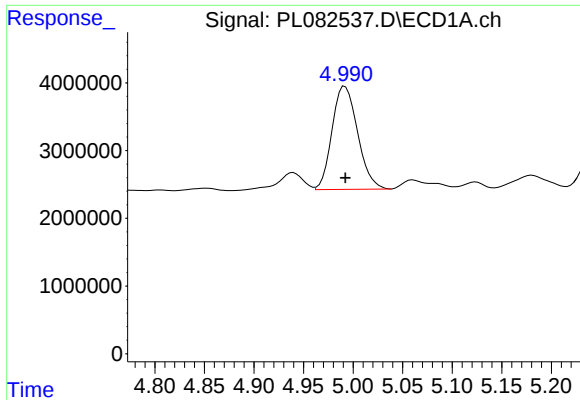

#24 Chlordane-2


R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 27358586
Conc: 229.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152523BS

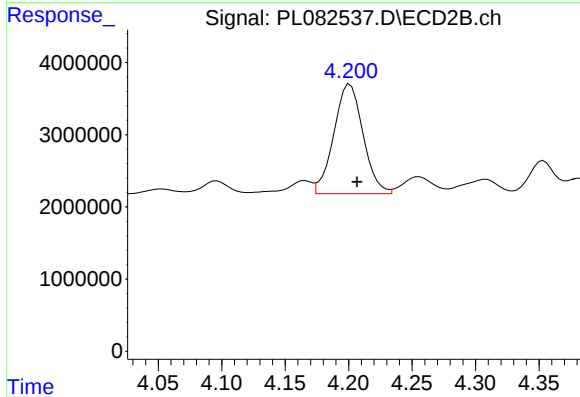


#24 Chlordane-2

R.T.: 4.201 min
Delta R.T.: -0.005 min
Response: 24383914
Conc: 217.44 ng/ml

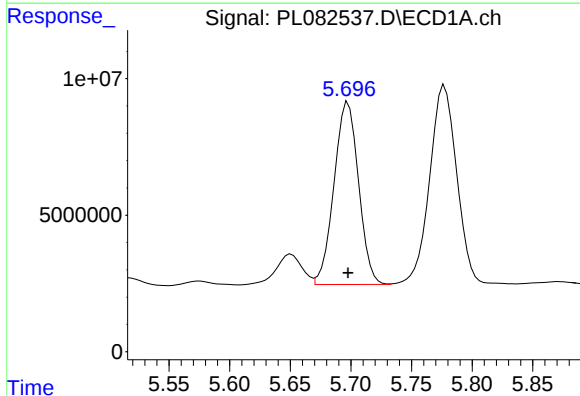


#25 Chlordane-3

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 94083003
Conc: 217.93 ng/ml

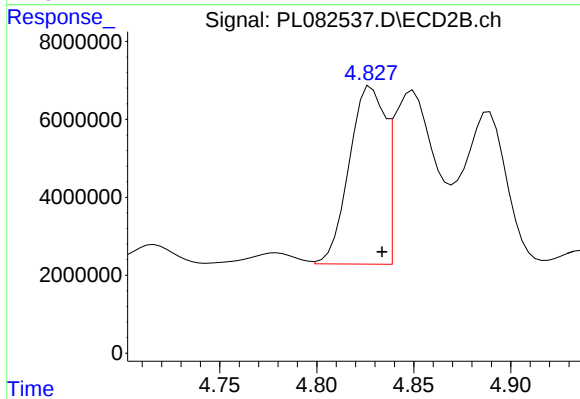

#25 Chlordane-3


R.T.: 4.828 min
Delta R.T.: -0.006 min
Response: 58568339
Conc: 206.15 ng/ml

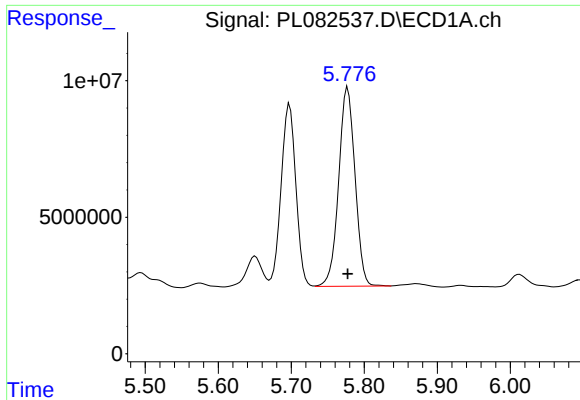

#26 Chlordane-4


R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 113142187
Conc: 217.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152523BS

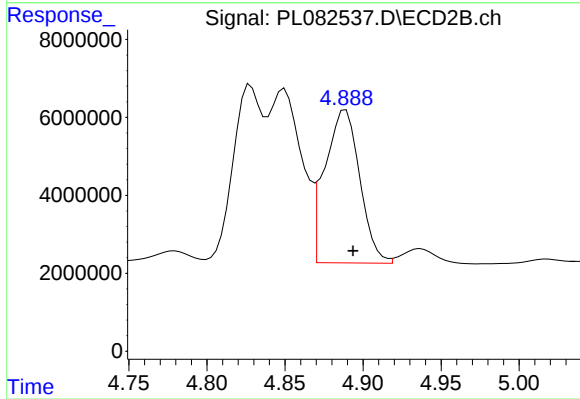


#26 Chlordane-4

R.T.: 4.889 min
Delta R.T.: -0.005 min
Response: 61262095
Conc: 205.30 ng/ml

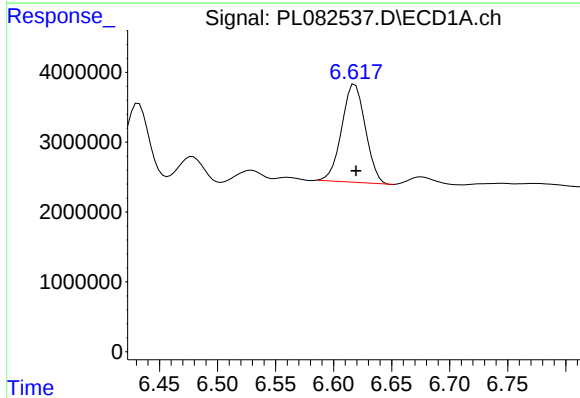


#27 Chlordane-5

R.T.: 6.618 min
Delta R.T.: 0.000 min
Response: 19942940
Conc: 212.39 ng/ml

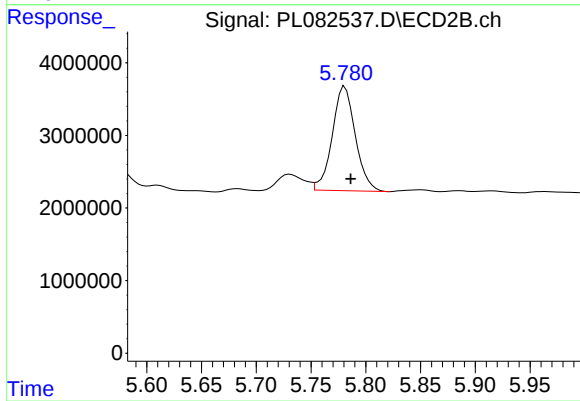

#27 Chlordane-5


R.T.: 5.781 min
Delta R.T.: -0.005 min
Response: 21101168
Conc: 213.76 ng/ml

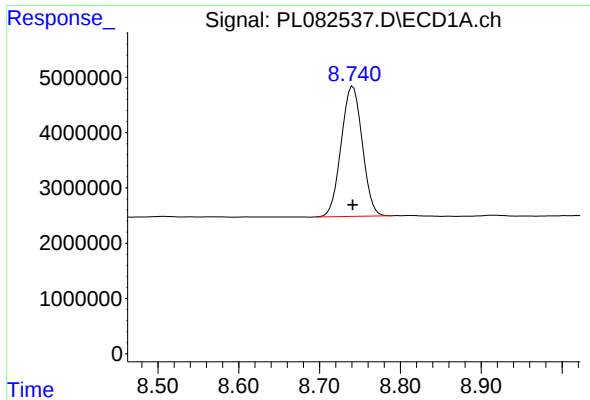

#28 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: 0.000 min
Response: 42634394
Conc: 22.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152523BS

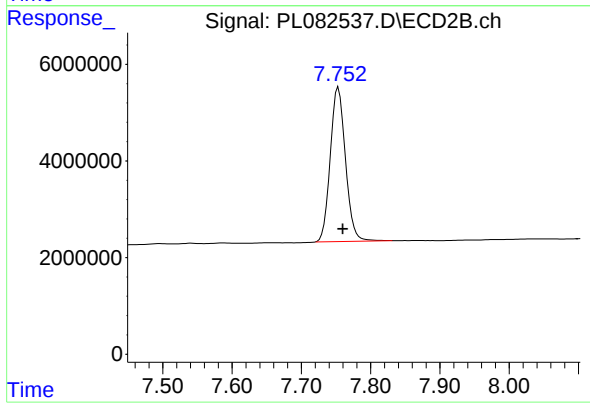

#28 Decachlorobiphenyl

R.T.: 7.754 min
Delta R.T.: -0.006 min
Response: 48756608
Conc: 21.36 ng/ml