

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050523\
 Data File : PL082557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 16:38
 Operator : AR\AJ
 Sample : 02618-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DSN001

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/08/2023
 Supervised By : Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 21:21:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	2.636	109.3E6	27637766	40.928m	11.930m#
2)	SA Decachlor...	8.737	7.752	33760864	35424952	17.684	15.520

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050523\
Data File : PL082557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 16:38
Operator : AR\AJ
Sample : 02618-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DSN001


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/08/2023
Supervised By : Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 21:21:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

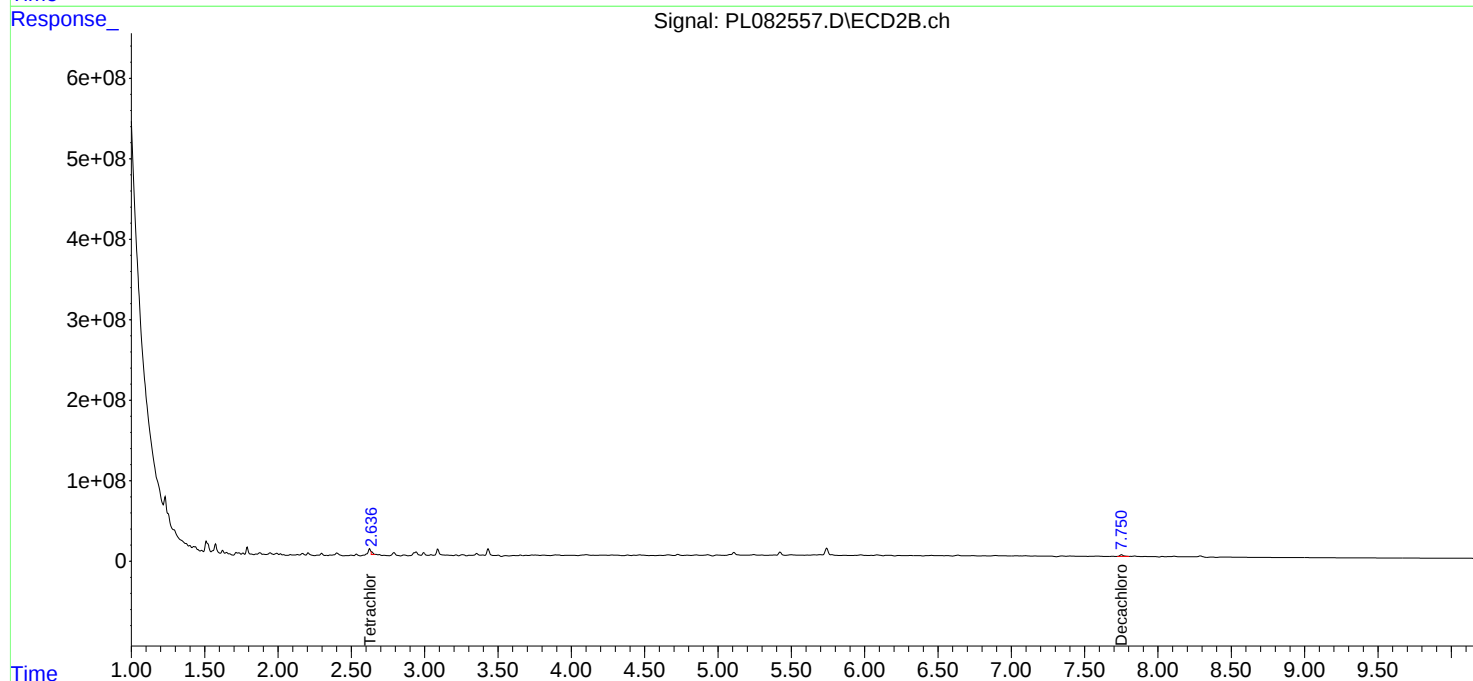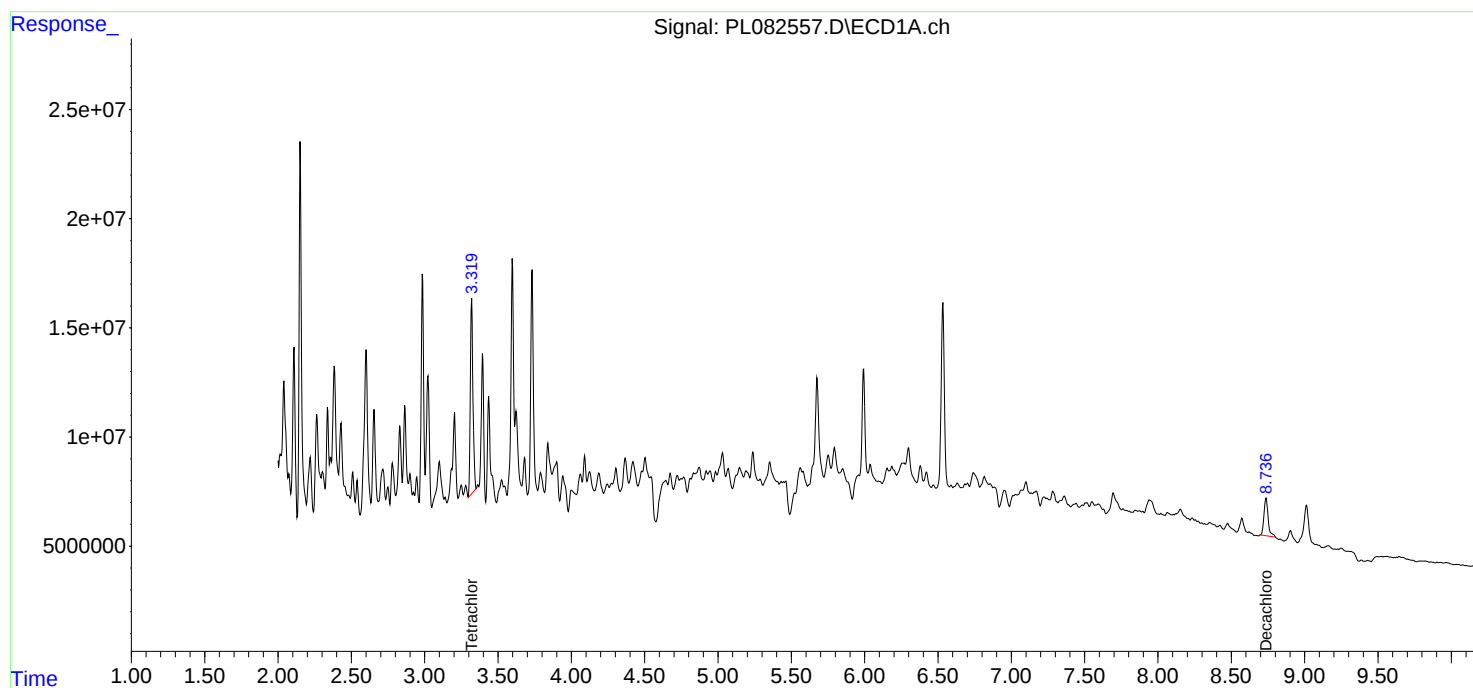

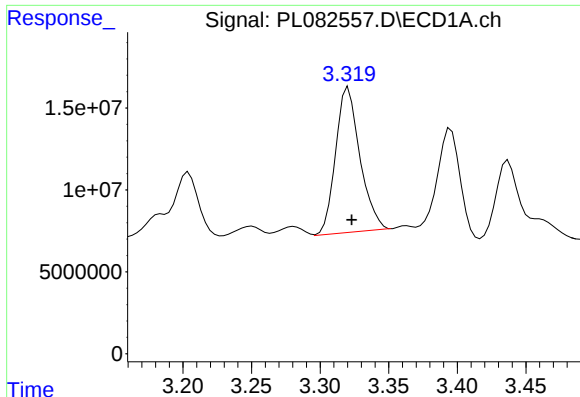


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: -0.004 min
Response: 109327737
Conc: 40.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
DSN001


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/08/2023
Supervised By :Ankita Jodhani 05/08/2023

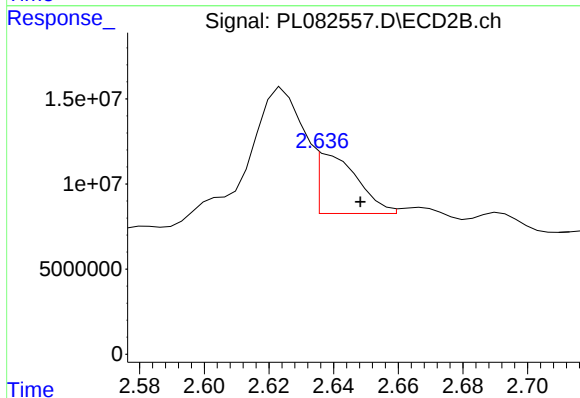


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: -0.013 min
Response: 27637766
Conc: 11.93 ng/ml m

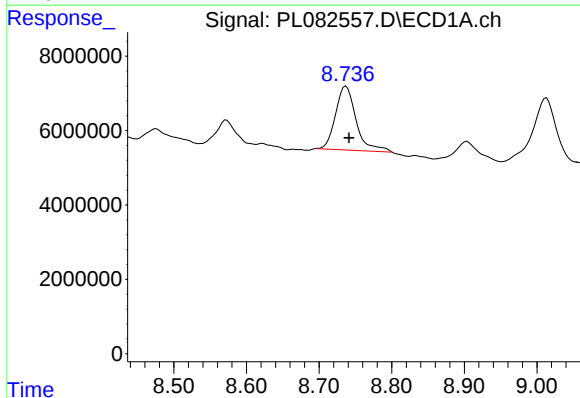

#28 Decachlorobiphenyl

R.T.: 8.737 min
Delta R.T.: -0.004 min
Response: 33760864
Conc: 17.68 ng/ml

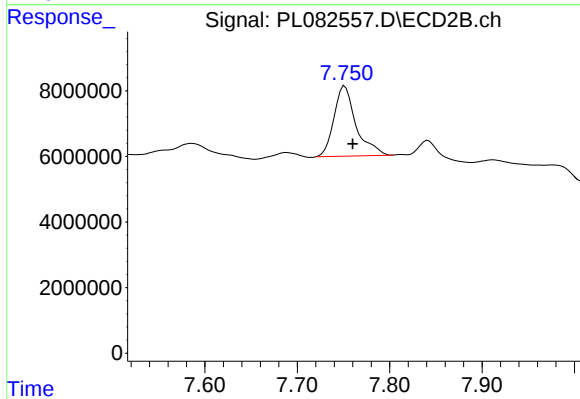

#28 Decachlorobiphenyl

R.T.: 7.752 min
Delta R.T.: -0.008 min
Response: 35424952
Conc: 15.52 ng/ml