

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050525\
 Data File : PL095526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2025 12:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 23:08:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.595	2.911	59815871	71341563	18.322	22.436
28)	SA Decachlor...	9.122	8.089	55963191	64602872	20.197	21.831
Target Compounds							
6)	B beta-BHC	0.000	4.018f	0	5723699	N.D.	2.757 #
8)	B Heptachlo...	5.729	0.000	50120729	0	12.514	N.D. #
10)	B gamma-Chl...	5.975f	0.000	45095297	0	11.055	N.D. #
14)	MA Endrin	0.000	5.814	0	7501225	N.D.	2.060 #
24)	Chlordane-2	0.000	4.502	0	22008214	N.D.	119.591 #
25)	Chlordane-3	5.975f	0.000	45095297	0	57.894	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050525\
Data File : PL095526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2025 12:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 23:08:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

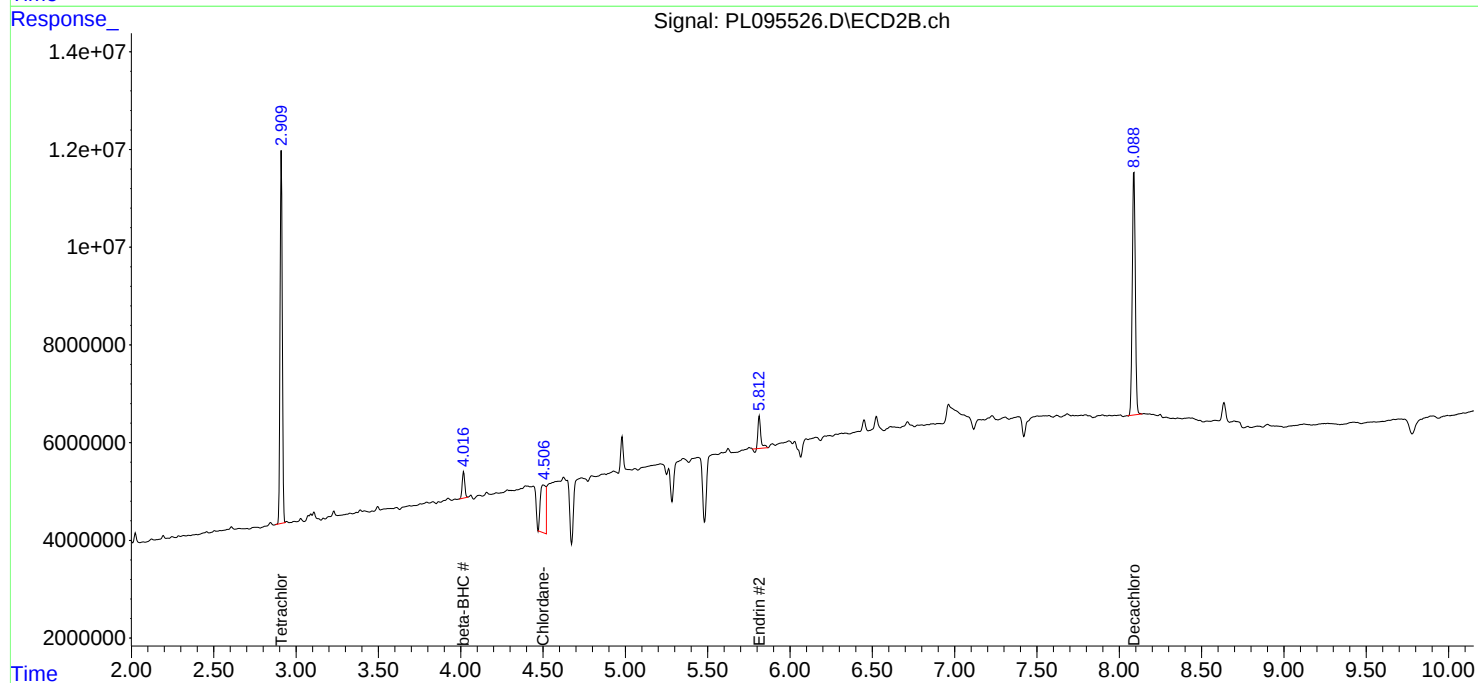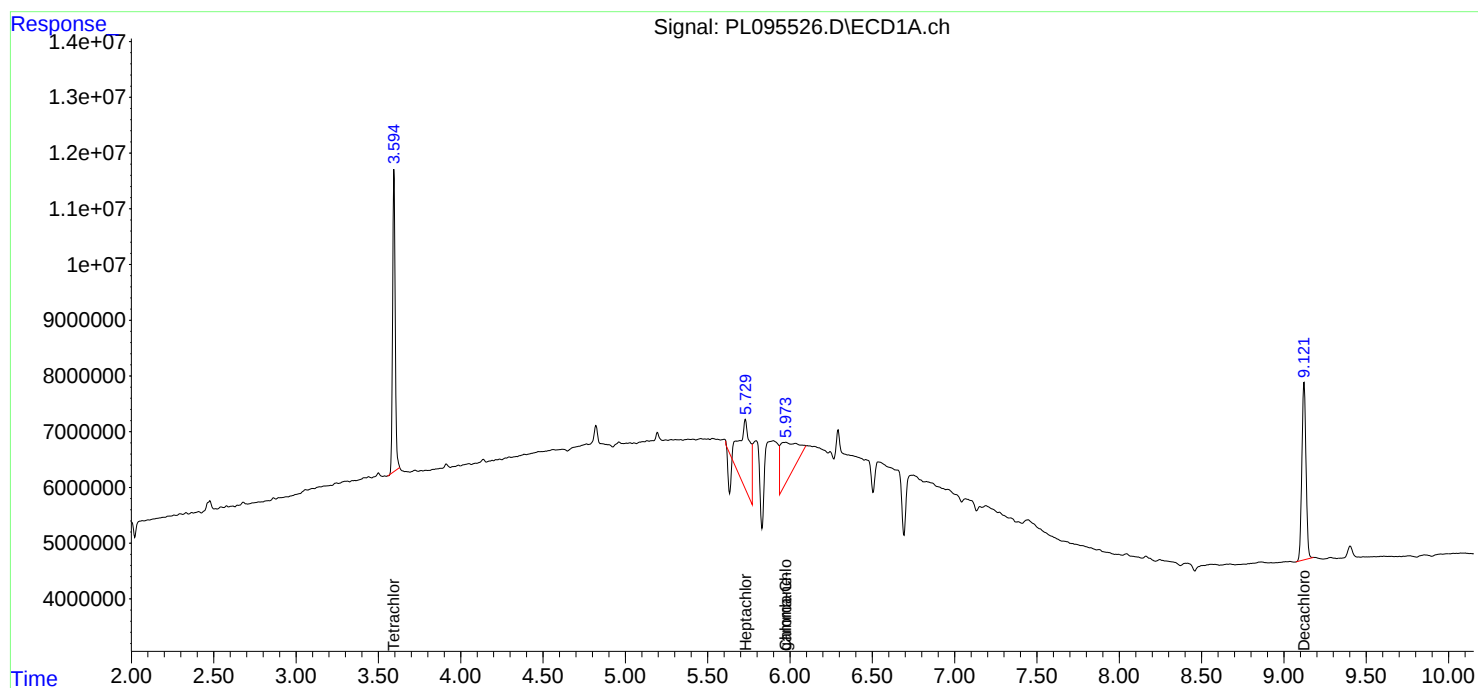


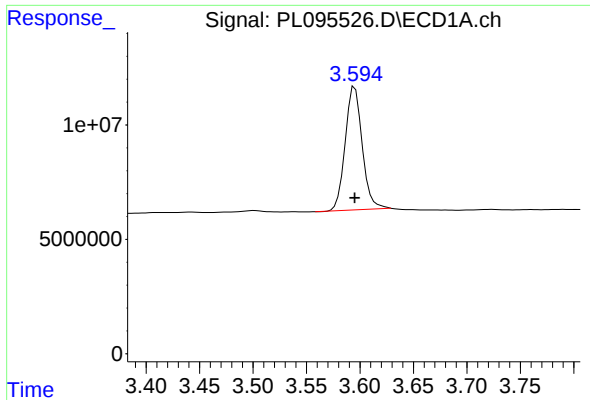

#1 Tetrachloro-m-xylene


R.T.: 3.595 min
Delta R.T.: 0.000 min
Response: 59815871
Conc: 18.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

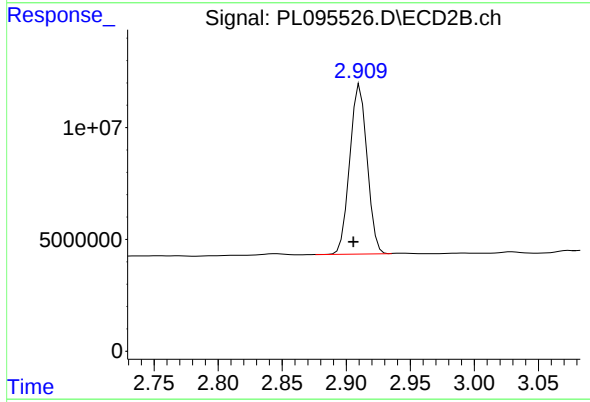


#1 Tetrachloro-m-xylene

R.T.: 2.911 min
Delta R.T.: 0.005 min
Response: 71341563
Conc: 22.44 ng/ml

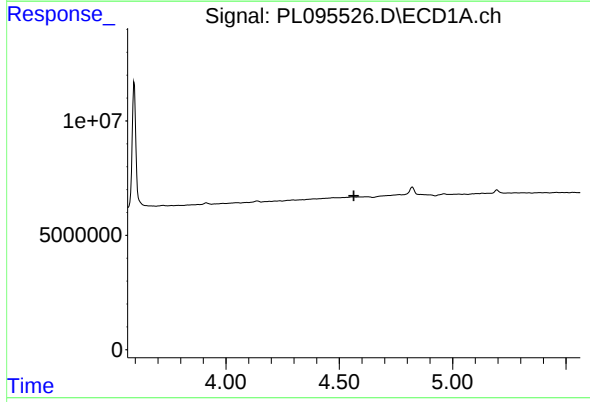


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.564 min
Response: 0
Conc: N.D.

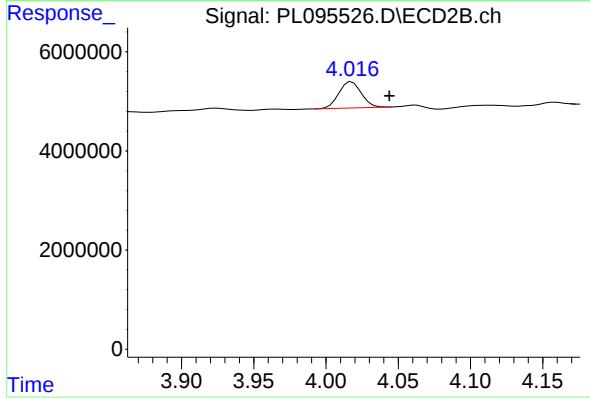

#6 beta-BHC


R.T.: 4.018 min
Delta R.T.: -0.026 min
Response: 5723699
Conc: 2.76 ng/ml

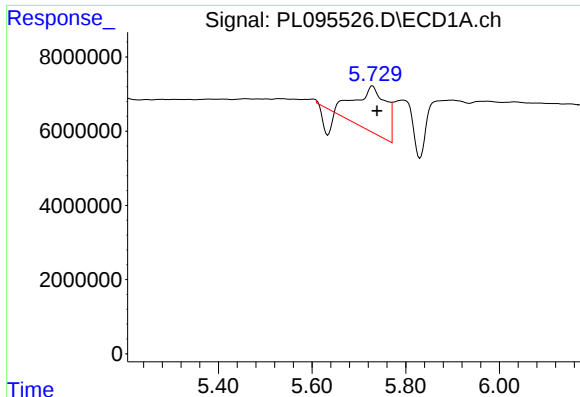

#8 Heptachlor epoxide


R.T.: 5.729 min
Delta R.T.: -0.010 min
Response: 50120729
Conc: 12.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

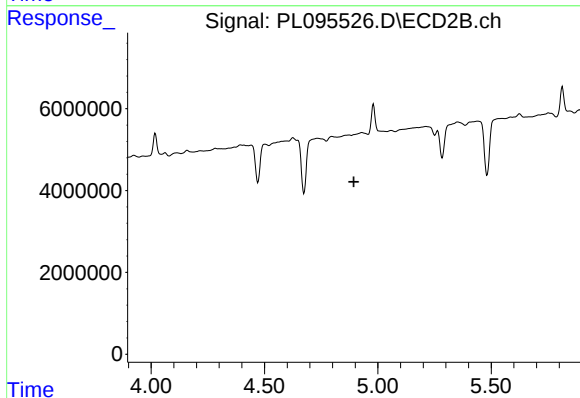


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.893 min
Response: 0
Conc: N.D.

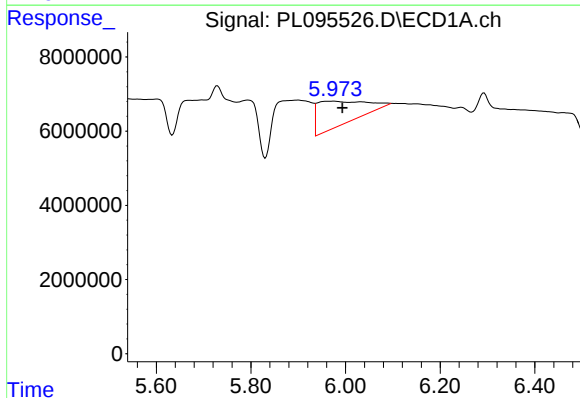


#10 gamma-Chlordane

R.T.: 5.975 min
Delta R.T.: -0.019 min
Response: 45095297
Conc: 11.05 ng/ml

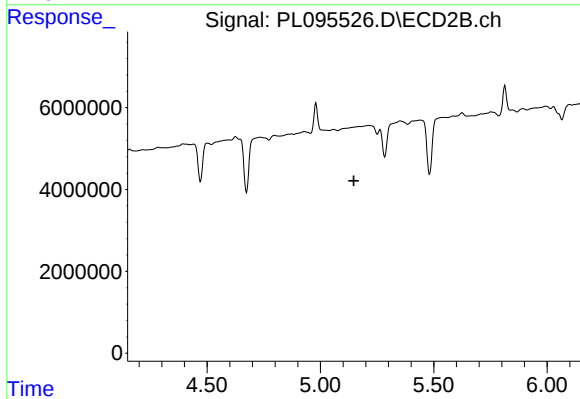

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.147 min
Response: 0
Conc: N.D.

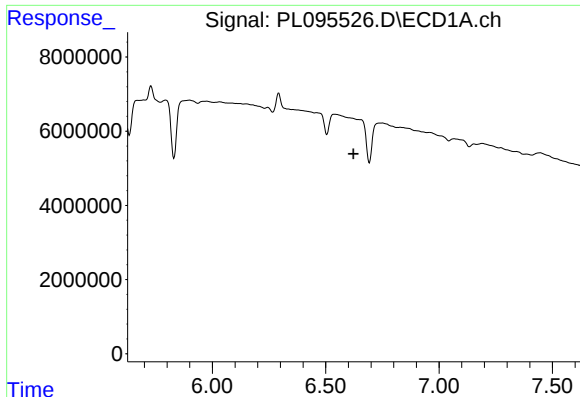

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.623 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

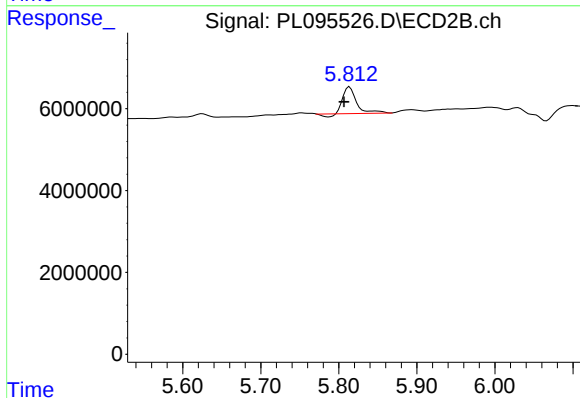


#14 Endrin

R.T.: 5.814 min
Delta R.T.: 0.007 min
Response: 7501225
Conc: 2.06 ng/ml

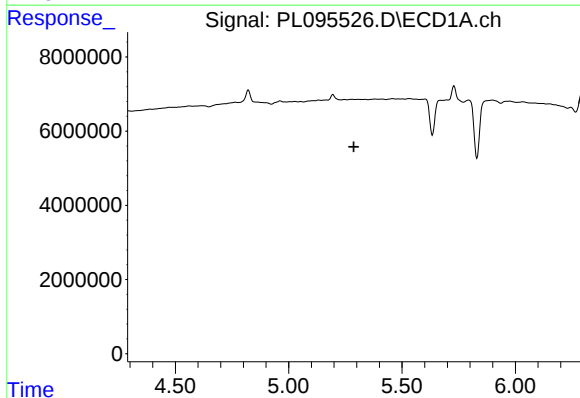


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.287 min
Response: 0
Conc: N.D.

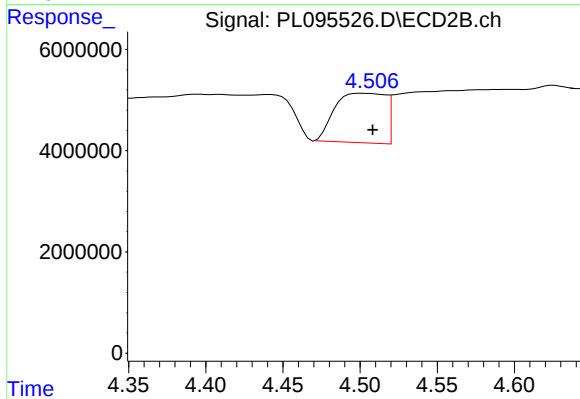

#24 Chlordane-2


R.T.: 4.502 min
Delta R.T.: -0.007 min
Response: 22008214
Conc: 119.59 ng/ml

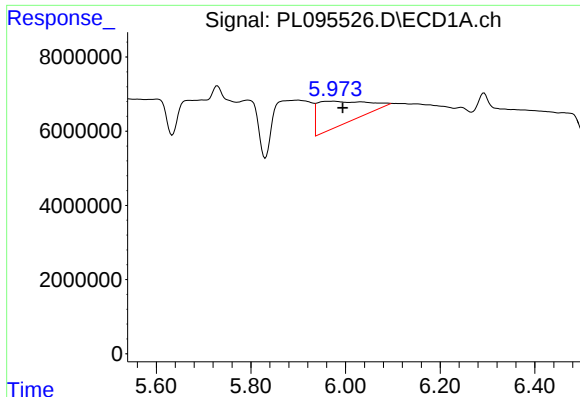

#25 Chlordane-3


R.T.: 5.975 min
Delta R.T.: -0.019 min
Response: 45095297
Conc: 57.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

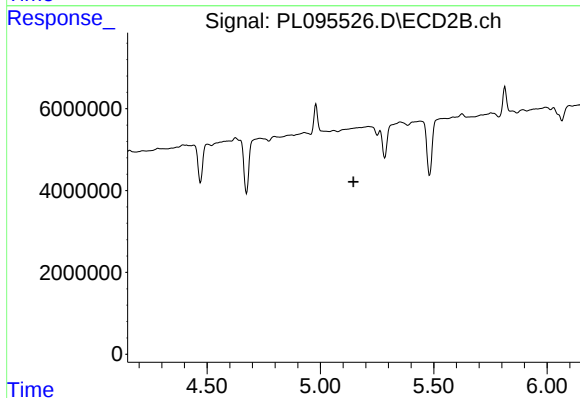


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.147 min
Response: 0
Conc: N.D.

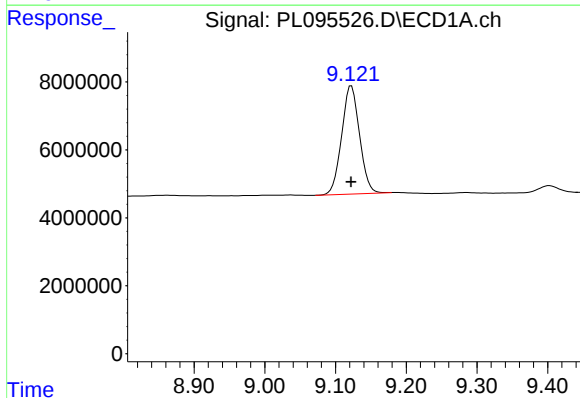

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: 0.000 min
Response: 55963191
Conc: 20.20 ng/ml

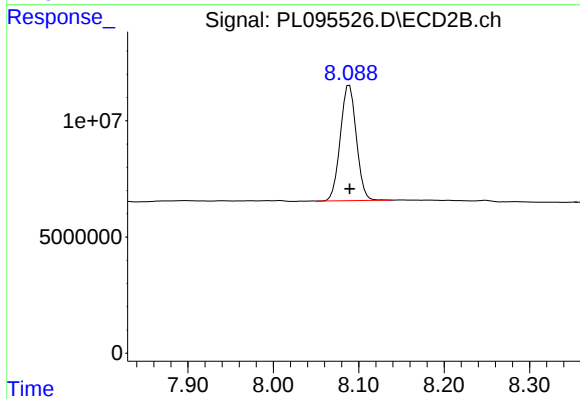

#28 Decachlorobiphenyl

R.T.: 8.089 min
Delta R.T.: 0.000 min
Response: 64602872
Conc: 21.83 ng/ml